

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092624\
 Data File : BF139551.D
 Acq On : 26 Sep 2024 16:56
 Operator : RC/JU
 Sample : PB163677BSD
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_F
ClientSampleId :

Quant Time: Sep 26 17:23:51 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091324.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Sep 14 02:58:23 2024
 Response via : Initial Calibration

Manual Integrations
APPROVED
 Reviewed By :Yogesh Patel

09/27/2024
 Supervised By :mohammad ahmed

Compound	R.T.	QI	on	Response	Conc	Units	Dev(Min)
Internal Standards							
1) 1,4-Dichlorobenzene-d4	6.881	152		72760	20.000	ng	0.00
21) Naphthalene-d8	8.157	136		272741	20.000	ng	# 0.00
39) Acenaphthene-d10	9.916	164		145233	20.000	ng	0.00
64) Phenanthrene-d10	11.404	188		254802	20.000	ng	# 0.00
76) Chrysene-d12	14.039	240		129364	20.000	ng	# 0.00
86) Perylene-d12	15.510	264		149417	20.000	ng	0.01
System Monitoring Compounds							
5) 2-Fluorophenol	5.504	112		444661	99.697	ng	0.01
7) Phenol-d6	6.510	99		570620	97.472	ng	0.00
23) Nitrobenzene-d5	7.445	82		548114	94.477	ng	0.00
42) 2,4,6-Tribromophenol	10.704	330		141745	91.674	ng	0.00
45) 2-Fluorobiphenyl	9.233	172		972090	93.875	ng	0.00
79) Terphenyl-d14	12.980	244		821007	104.171	ng	0.00
Target Compounds							
2) 1,4-Dioxane	2.734	88		81447	45.516	ng	Qvalue 95
3) Pyridine	3.475	79		216440	54.861	ng	96
4) n-Nitrosodimethylamine	3.440	42		159828	46.739	ng	# 81
6) Aniline	6.540	93		283068	64.072	ng	# 84
8) 2-Chlorophenol	6.663	128		249232	54.285	ng	99
9) Benzaldehyde	6.428	77		41003	12.123	ng	98
10) Phenol	6.528	94		322178	54.035	ng	99
11) bis(2-Chloroethyl)ether	6.616	93		238151	52.552	ng	99
12) 1,3-Dichlorobenzene	6.822	146		261284	50.041	ng	98
13) 1,4-Dichlorobenzene	6.898	146		268981	50.978	ng	99
14) 1,2-Dichlorobenzene	7.045	146		259443	52.037	ng	97
15) Benzyl Alcohol	7.022	79		236416	50.618	ng	94
16) 2,2'-oxybis(1-Chloropr...	7.151	45		442434	63.349	ng	95
17) 2-Methylphenol	7.134	107		195659	53.639	ng	98
18) Hexachloroethane	7.387	117		101781	50.644	ng	96
19) n-Nitroso-di-n-propyla...	7.292	70		185496	53.470	ng	97
20) 3+4-Methylphenols	7.287	107		249229	50.080	ng	# 88
22) Acetophenone	7.287	105		344526	48.319	ng	98
24) Nitrobenzene	7.463	77		288330	48.288	ng	97
25) Isophorone	7.698	82		497710	54.245	ng	99
26) 2-Nitrophenol	7.775	139		132576	56.990	ng	90
27) 2,4-Dimethylphenol	7.816	122		197543	64.376	ng	96
28) bis(2-Chloroethoxy)met...	7.910	93		287436	54.967	ng	99
29) 2,4-Dichlorophenol	8.022	162		202214	51.873	ng	99
30) 1,2,4-Trichlorobenzene	8.098	180		222475	48.980	ng	98
31) Naphthalene	8.181	128		738223	51.846	ng	99
32) Benzoic acid	7.939	122		139531	48.589	ng	90
33) 4-Chloroaniline	8.228	127		111447	25.585	ng	97
34) Hexachlorobutadiene	8.298	225		145127	47.029	ng	99
35) Caprolactam	8.598	113		65887m	54.944	ng	
36) 4-Chloro-3-methylphenol	8.716	107		222646	49.974	ng	96
37) 2-Methylnaphthalene	8.875	142		473163	52.354	ng	98
38) 1-Methylnaphthalene	8.975	142		436985	49.249	ng	100
40) 1,2,4,5-Tetrachloroben...	9.039	216		222215	51.627	ng	98
41) Hexachlorocyclopentadiene	9.022	237		271270	180.502	ng	100
43) 2,4,6-Trichlorophenol	9.151	196		149612	53.427	ng	100

09/28/2024

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092624\
 Data File : BF139551.D
 Acq On : 26 Sep 2024 16:56
 Operator : RC/JU
 Sample : PB163677BSD
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_F
ClientSampleId :

Quant Time: Sep 26 17:23:51 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091324.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Sep 14 02:58:23 2024
 Response via : Initial Calibration

Manual Integrations
APPROVED
 Reviewed By :Yogesh Patel

09/27/2024
 Supervised By :mohammad ahmed

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)	
44) 2,4,5-Trichlorophenol	9.198	196	157725	53.396	ng	98	
46) 1,1'-Biphenyl	9.339	154	578675	51.791	ng	99	
47) 2-Chloronaphthalene	9.363	162	435329	52.109	ng	99	
48) 2-Nitroaniline	9.457	65	160986	51.809	ng	99	
49) Acenaphthylene	9.781	152	711570	56.584	ng	100	
50) Dimethylphthalate	9.639	163	506674	53.154	ng	99	
51) 2,6-Dinitrotoluene	9.704	165	111190	52.654	ng	88	
52) Acenaphthene	9.951	154	503826	57.404	ng	100	
53) 3-Nitroaniline	9.869	138	76423	36.213	ng	93	
54) 2,4-Dinitrophenol	9.980	184	130283	110.721	ng	#	84
55) Dibenzofuran	10.122	168	639671	52.290	ng	95	
56) 4-Nitrophenol	10.033	139	159088	91.103	ng	#	83
57) 2,4-Dinitrotoluene	10.104	165	149772	52.534	ng	96	
58) Fluorene	10.463	166	500872	50.182	ng	99	
59) 2,3,4,6-Tetrachlorophenol	10.239	232	129469	52.985	ng	95	
60) Diethylphthalate	10.333	149	508572	51.700	ng	99	
61) 4-Chlorophenyl-phenyle...	10.457	204	244606	50.426	ng	94	
62) 4-Nitroaniline	10.486	138	109227	47.423	ng	#	86
63) Azobenzene	10.616	77	513577	53.082	ng	94	
65) 4,6-Dinitro-2-methylph...	10.516	198	81095	60.302	ng	87	
66) n-Nitrosodiphenylamine	10.575	169	428271	57.490	ng	99	
67) 4-Bromophenyl-phenylether	10.945	248	143411	56.796	ng	97	
68) Hexachlorobenzene	11.010	284	156858	52.931	ng	99	
69) Atrazine	11.104	200	130365	73.507	ng	99	
70) Pentachlorophenol	11.210	266	171897	96.670	ng	98	
71) Phenanthrene	11.427	178	675610	54.958	ng	100	
72) Anthracene	11.480	178	693397	57.690	ng	100	
73) Carbazole	11.633	167	588022	51.116	ng	99	
74) Di-n-butylphthalate	11.957	149	682832	53.285	ng	99	
75) Fluoranthene	12.616	202	625574	47.652	ng	99	
77) Benzidine	12.733	184	214055	115.493	ng	98	
78) Pyrene	12.845	202	626209	56.376	ng	100	
80) Butylbenzylphthalate	13.457	149	213997	56.601	ng	98	
81) Benzo(a)anthracene	14.027	228	479553	55.963	ng	100	
82) 3,3'-Dichlorobenzidine	13.992	252	117933	46.996	ng	99	
83) Chrysene	14.063	228	457887	58.081	ng	99	
84) Bis(2-ethylhexyl)phtha...	14.016	149	265524	55.206	ng	98	
85) Di-n-octyl phthalate	14.627	149	446308	63.009	ng	98	
87) Indeno(1,2,3-cd)pyrene	16.992	276	512497	57.683	ng	#	96
88) Benzo(b)fluoranthene	15.080	252	505200	54.823	ng	98	
89) Benzo(k)fluoranthene	15.110	252	401450	47.249	ng	#	98
90) Benzo(a)pyrene	15.451	252	448278	58.656	ng	99	
91) Dibenzo(a,h)anthracene	17.009	278	420404	57.262	ng	#	97
92) Benzo(g,h,i)perylene	17.445	276	383067	52.697	ng	97	

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092624\
 Data File : BF139551.D
 Acq On : 26 Sep 2024 16:56
 Operator : RC/JU
 Sample : PB163677BSD
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :

Quant Time: Sep 26 17:23:51 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091324.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Sep 14 02:58:23 2024
 Response via : Initial Calibration

Manual Integrations
APPROVED
 Reviewed By :Yogesh Patel

09/27/2024
 Supervised By :mohammad ahmed

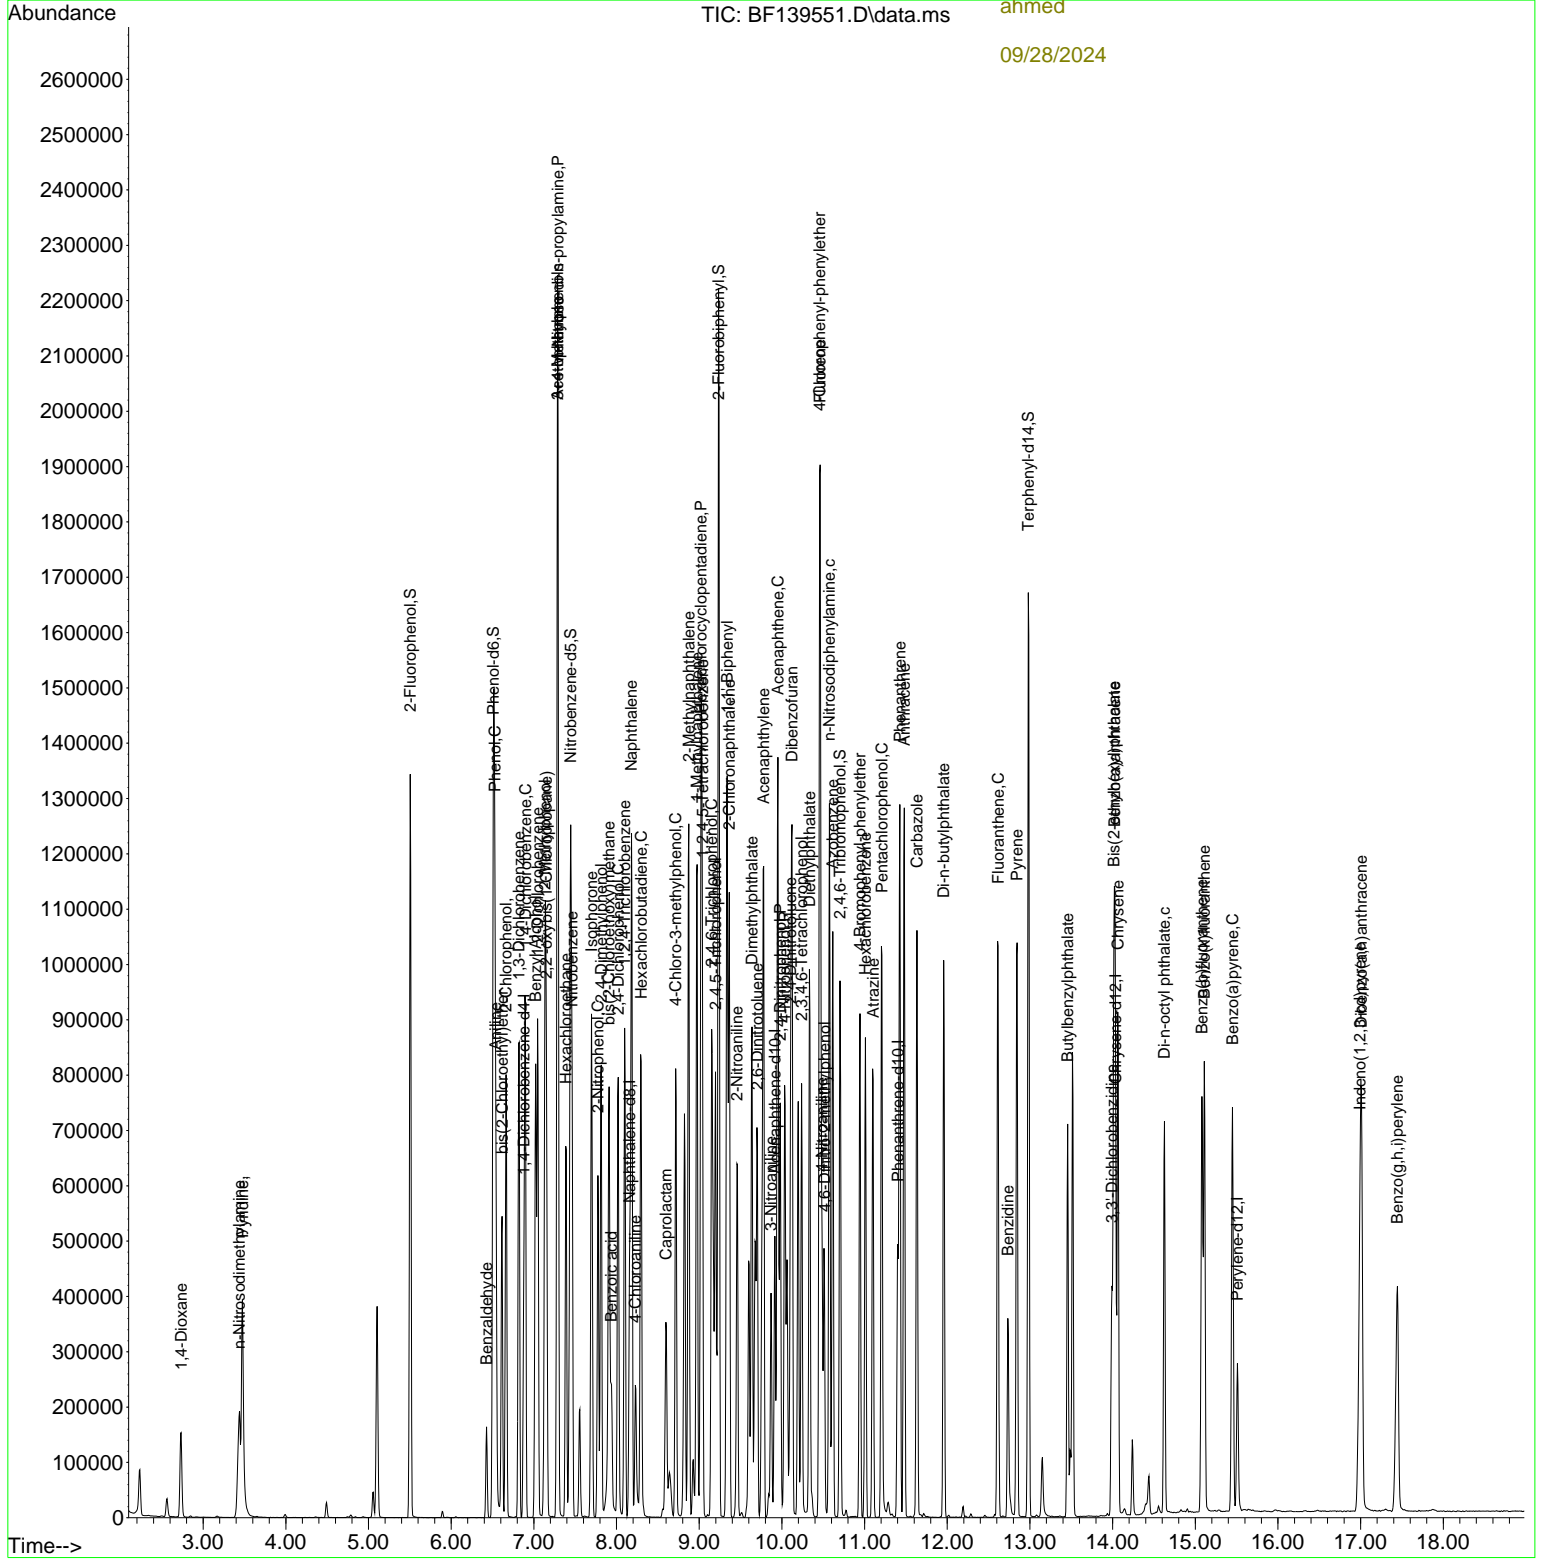

09/28/2024