
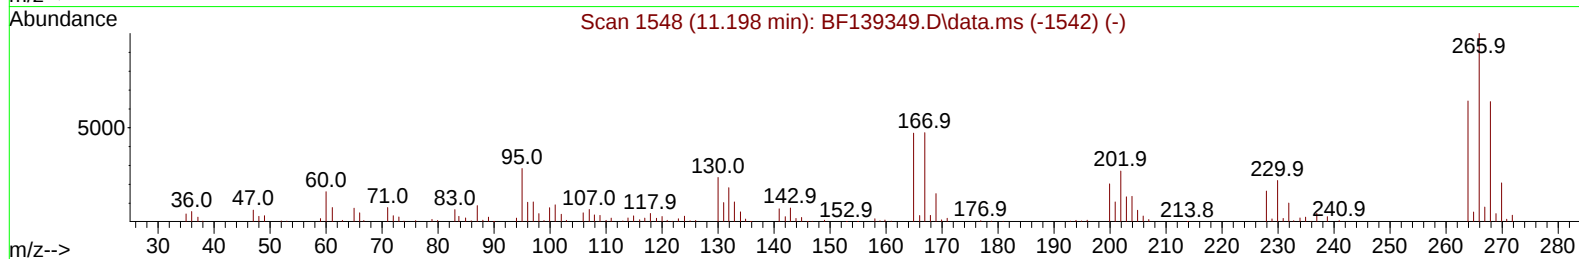
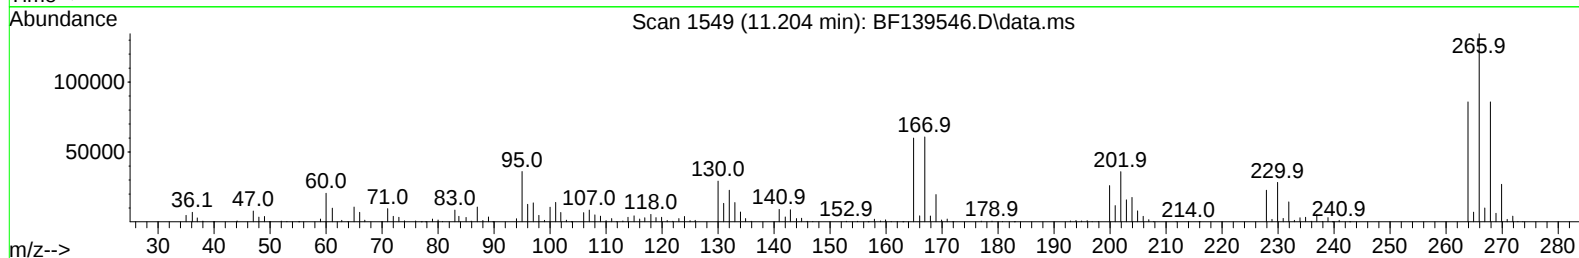


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092624\
Data File : BF139546.D
Acq On : 26 Sep 2024 14:26
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 26 15:03:33 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 14 02:58:23 2024
Response via : Initial Calibration

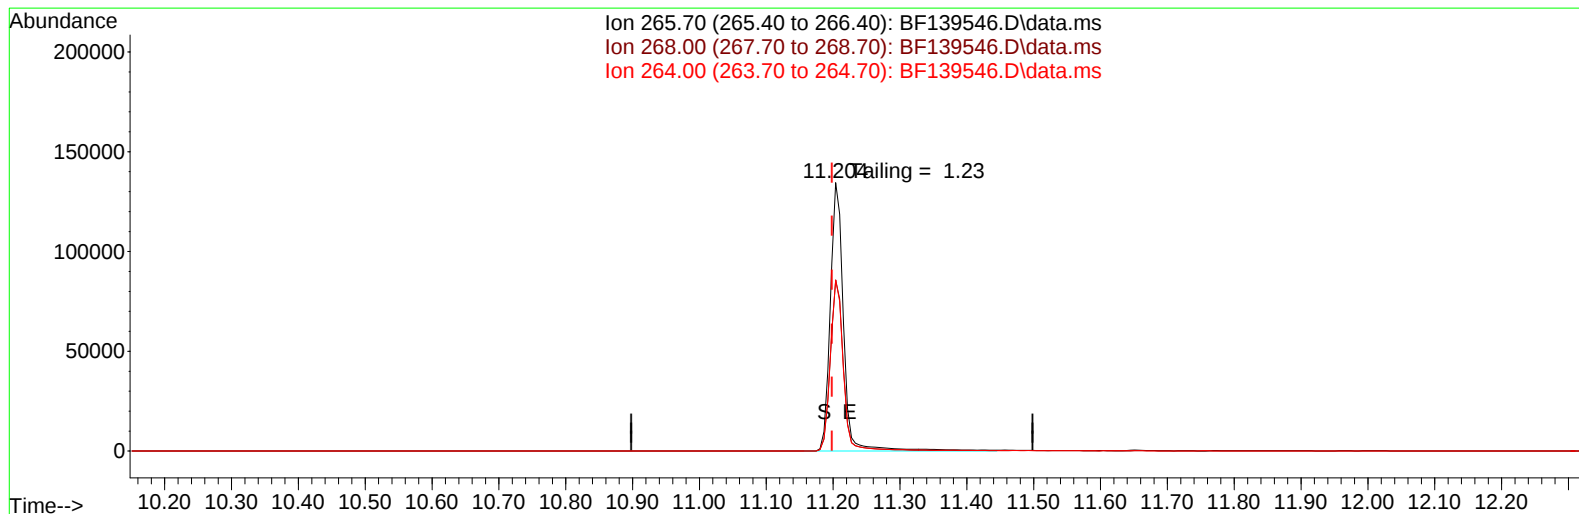

TIC: BF139546.D\data.ms

(70) Pentachlorophenol (C)




11.204min (+ 0.006) 28122.97 ng

response 182523

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.90	63.77
264.00	64.20	63.76
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092624\
Data File : BF139546.D
Acq On : 26 Sep 2024 14:26
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 26 15:03:33 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 14 02:58:23 2024
Response via : Initial Calibration

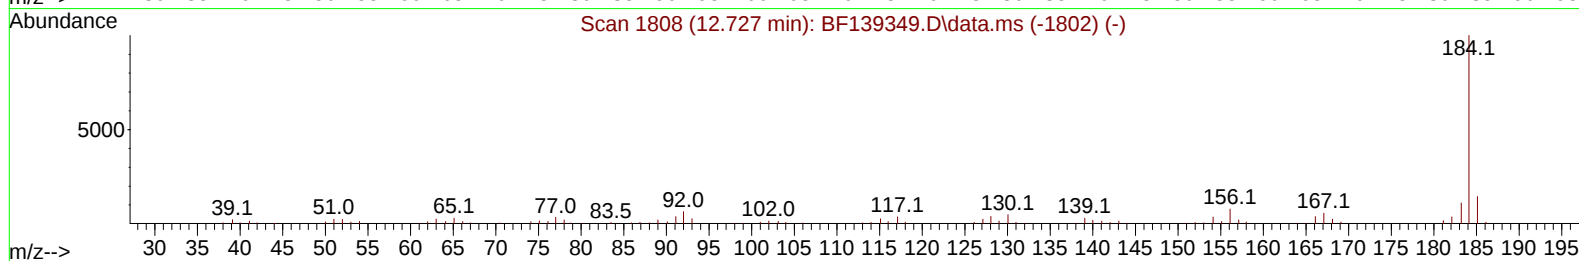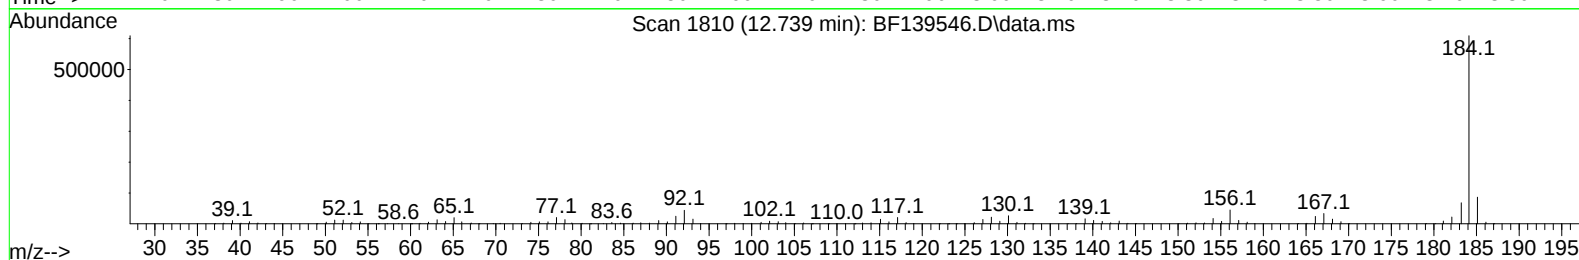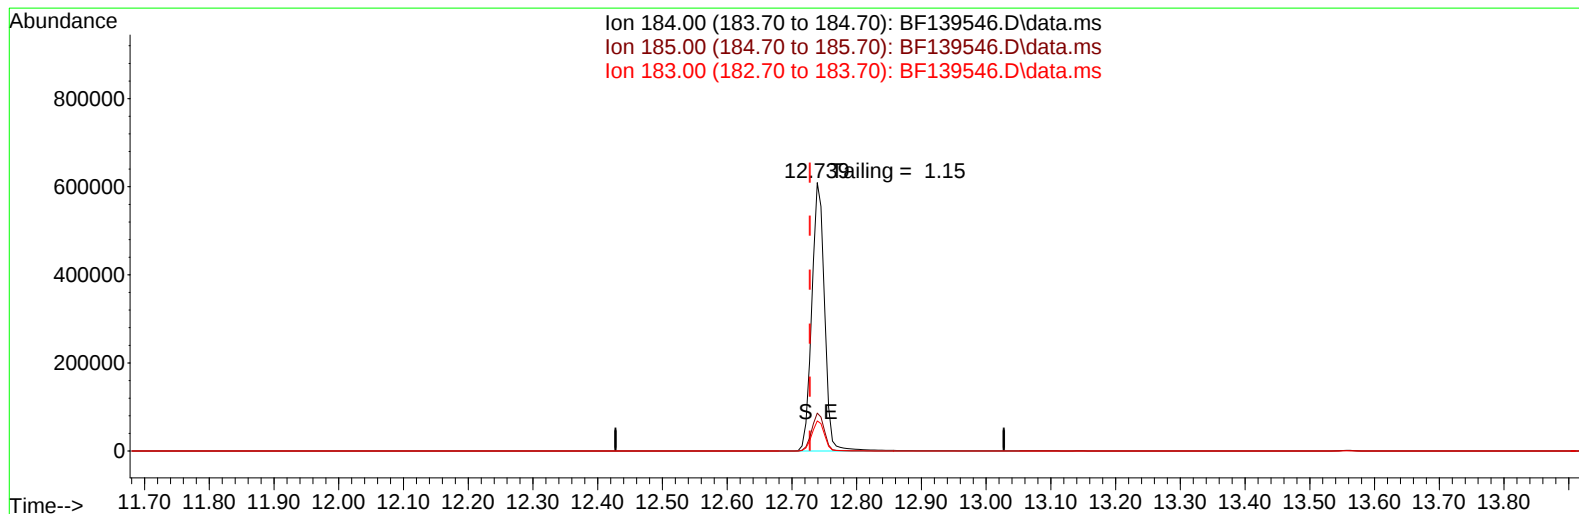

TIC: BF139546.D\data.ms

(77) Benzidine

12.739min (+ 0.012) 0.00 ng

response 839898

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.13
183.00	11.10	11.21
0.00	0.00	0.00