
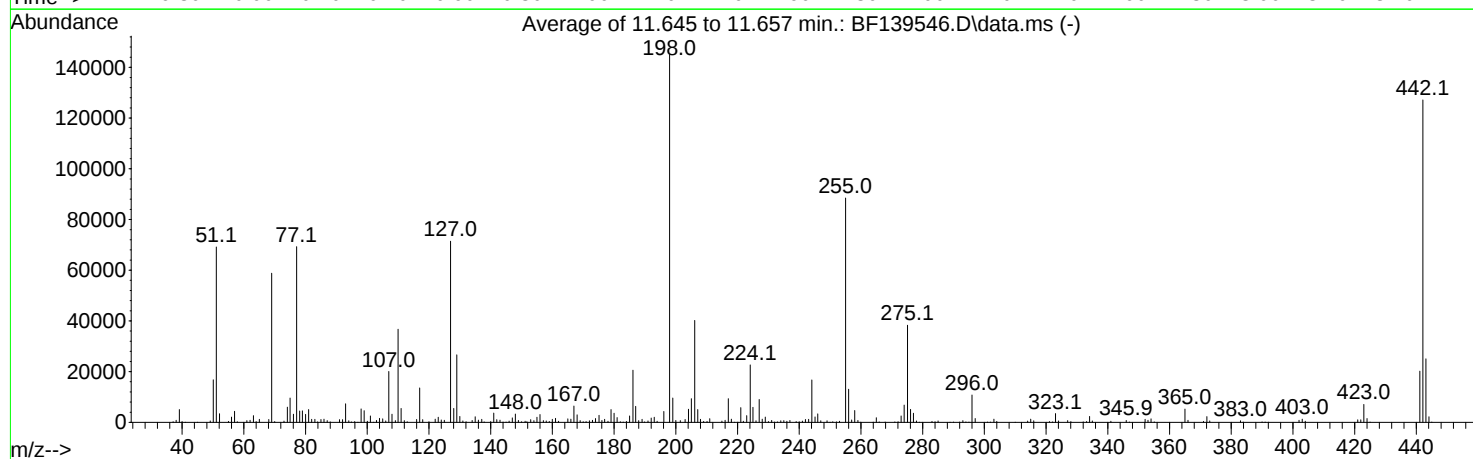


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092624\
Data File : BF139546.D
Acq On : 26 Sep 2024 14:26
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091324.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Sat Sep 14 02:58:23 2024

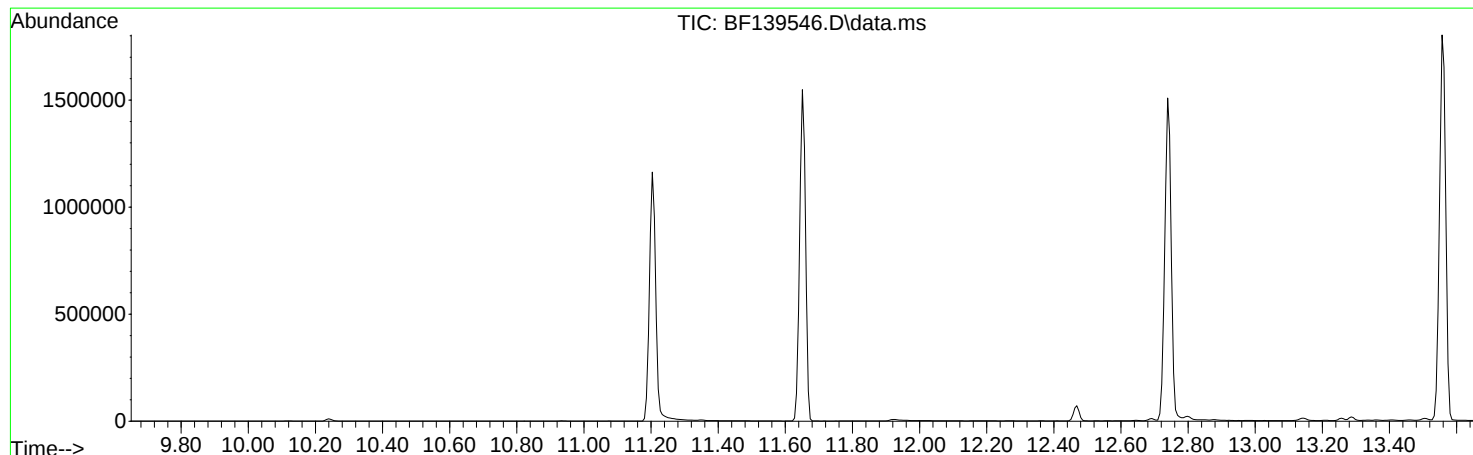




AutoFind: Scans 1624, 1625, 1626; Background Corrected with Scan 1618

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	47.7	69176	PASS
68	69	0.00	2	2.0	1152	PASS
69	198	0.00	100	40.5	58779	PASS
70	69	0.00	2	0.5	322	PASS
127	198	10	80	49.2	71405	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	145059	PASS
199	198	5	9	6.6	9584	PASS
275	198	10	60	26.4	38333	PASS
365	198	1	100	3.6	5257	PASS
441	198	0.01	100	13.9	20195	PASS
442	442	50	100	100.0	127139	PASS
443	442	15	24	19.7	25045	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092624\
Data File : BF139546.D
Acq On : 26 Sep 2024 14:26
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Sep 26 15:03:33 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 14 02:58:23 2024
Response via : Initial Calibration

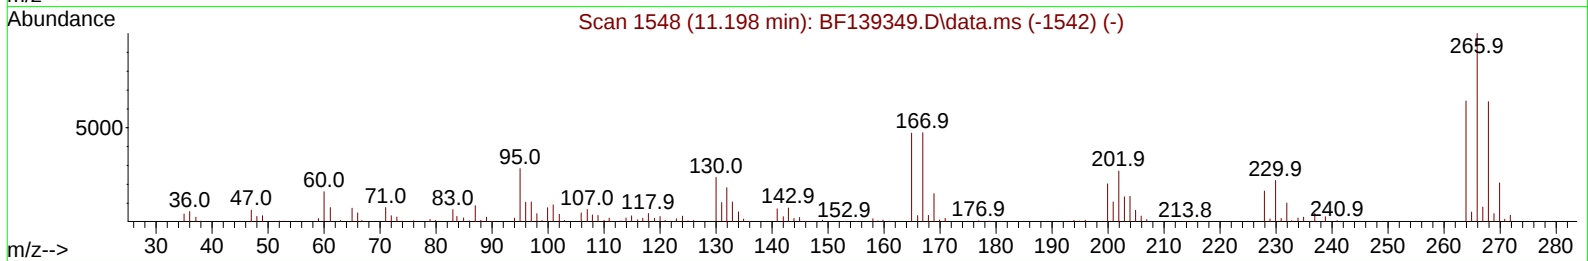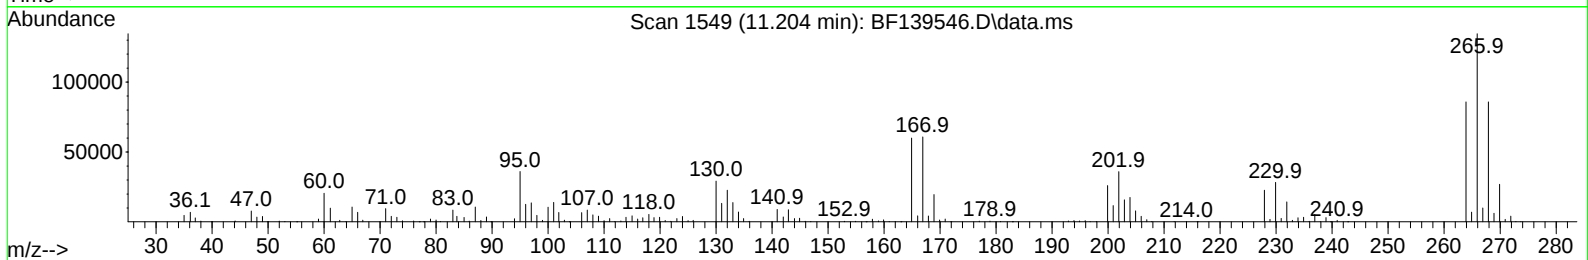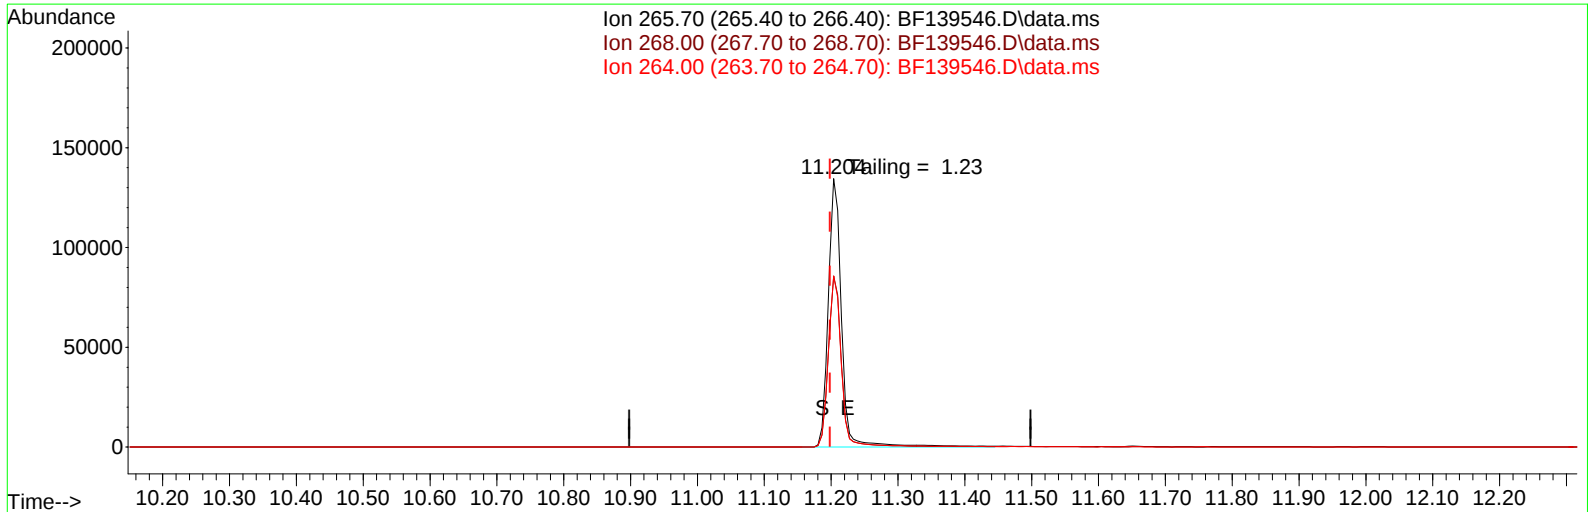

TIC: BF139546.D\data.ms

(70) Pentachlorophenol (C)

11.204min (+ 0.006) 28122.97 ng




response 182523

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.90	63.77
264.00	64.20	63.76
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092624\
Data File : BF139546.D
Acq On : 26 Sep 2024 14:26
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Sep 26 15:03:33 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091324.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 14 02:58:23 2024
Response via : Initial Calibration

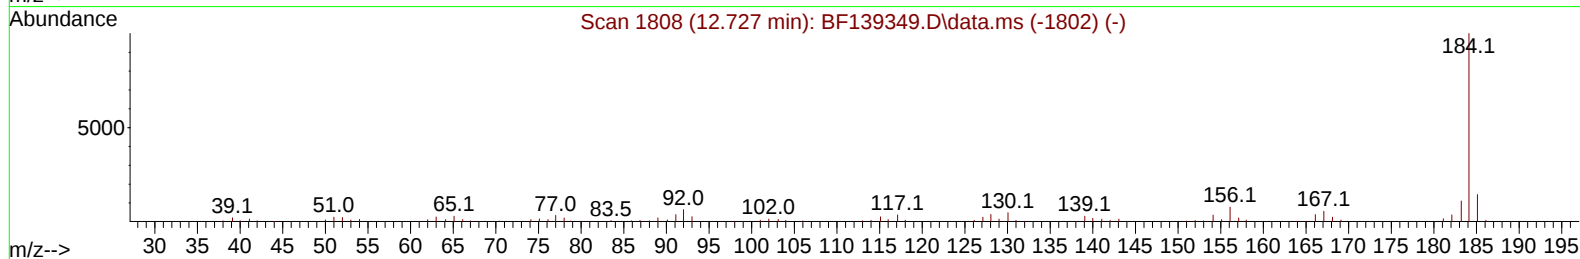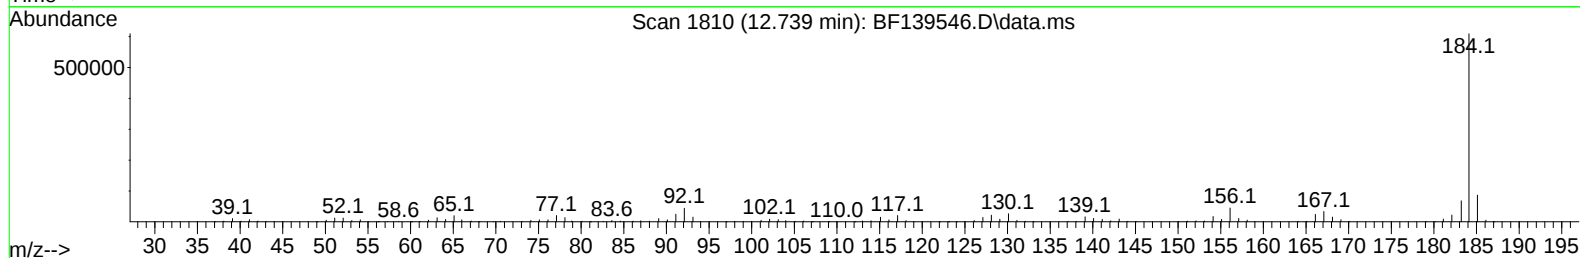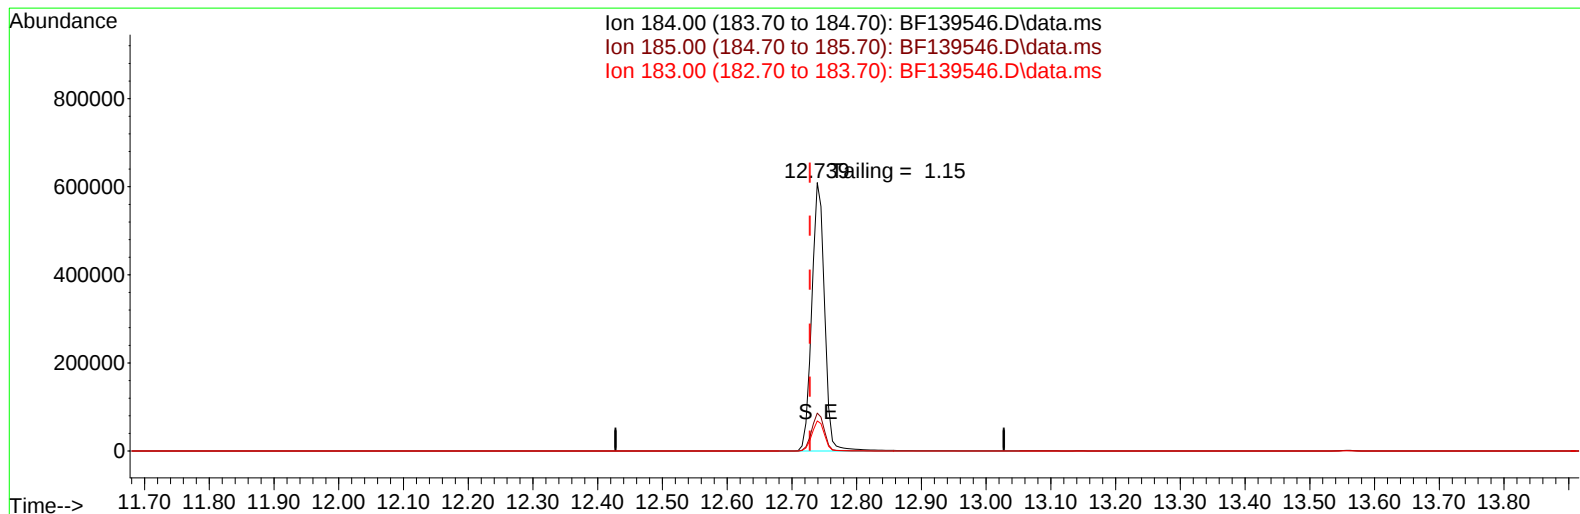

TIC: BF139546.D\data.ms

(77) Benzidine

12.739min (+ 0.012) 0.00 ng

response 839898

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.13
183.00	11.10	11.21
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/26/2024	BNA_F	<u>BF139546.D</u>
Compound Name	Response	Retention Time
DDT	448535	13.557
DDD	8495	13.286
DDE	148	12.921
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
8643	457178	1.89

Instrument :
BNA_F
ClientSampleId :
DFTPP