

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF092718\
 Data File : BF109399.D
 Acq On : 27 Sep 2018 20:35
 Operator : JU/SJ
 Sample : J5077-04 5X
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PARCEL-190-092418-2

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF092218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.887	473	476	481	rBV	10433	10132	1.26%	0.139%
2	5.310	544	548	556	rBV	360600	354964	44.03%	4.868%
3	6.334	719	722	735	rBV	396066	381290	47.29%	5.229%
4	6.469	742	745	749	rBV	460938	398812	49.47%	5.469%
5	6.704	782	785	789	rBV	760918	604898	75.03%	8.295%
6	6.863	808	812	815	rBV	370379	314913	39.06%	4.319%
7	7.263	876	880	888	rBV	269424	236768	29.37%	3.247%
8	7.987	999	1003	1010	rBV	936472	754485	93.58%	10.347%
9	9.063	1182	1186	1200	rBV	485199	415022	51.48%	5.691%
10	9.457	1250	1253	1263	rBV	121464	111323	13.81%	1.527%
11	9.733	1297	1300	1309	rBV	820344	772821	95.86%	10.598%
12	10.522	1430	1434	1446	rVB	185652	187888	23.30%	2.577%
13	11.210	1548	1551	1555	rBV	725696	687156	85.23%	9.423%
14	11.751	1639	1643	1647	rBV	10642	12198	1.51%	0.167%
15	12.416	1753	1756	1760	rBV	34469	30967	3.84%	0.425%
16	12.645	1790	1795	1798	rBV	32693	30850	3.83%	0.423%
17	12.792	1816	1820	1823	rBV	393582	325537	40.38%	4.464%
18	13.492	1935	1939	1941	rBV4	7084	9051	1.12%	0.124%
19	13.710	1974	1976	1978	rBV3	13141	13622	1.69%	0.187%
20	13.839	1993	1998	2001	rBV	860438	806224	100.00%	11.056%
21	13.863	2001	2002	2006	rVB	27011	17690	2.19%	0.243%
22	14.321	2077	2080	2082	rBV3	23200	22528	2.79%	0.309%
23	14.686	2139	2142	2147	rBV	44433	43059	5.34%	0.590%
24	14.845	2166	2169	2176	rBV	34990	69185	8.58%	0.949%
25	15.239	2231	2236	2240	rBV	560011	619301	76.82%	8.493%
26	15.551	2287	2289	2292	rBV3	18183	21684	2.69%	0.297%
27	15.680	2309	2311	2316	rVB2	30899	39702	4.92%	0.544%


Sum of corrected areas: 7292070

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF092718\
Data File : BF109399.D
Acq On : 27 Sep 2018 20:35
Operator : JU/SJ
Sample : J5077-04 5X
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PARCEL-190-092418-2

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF092218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

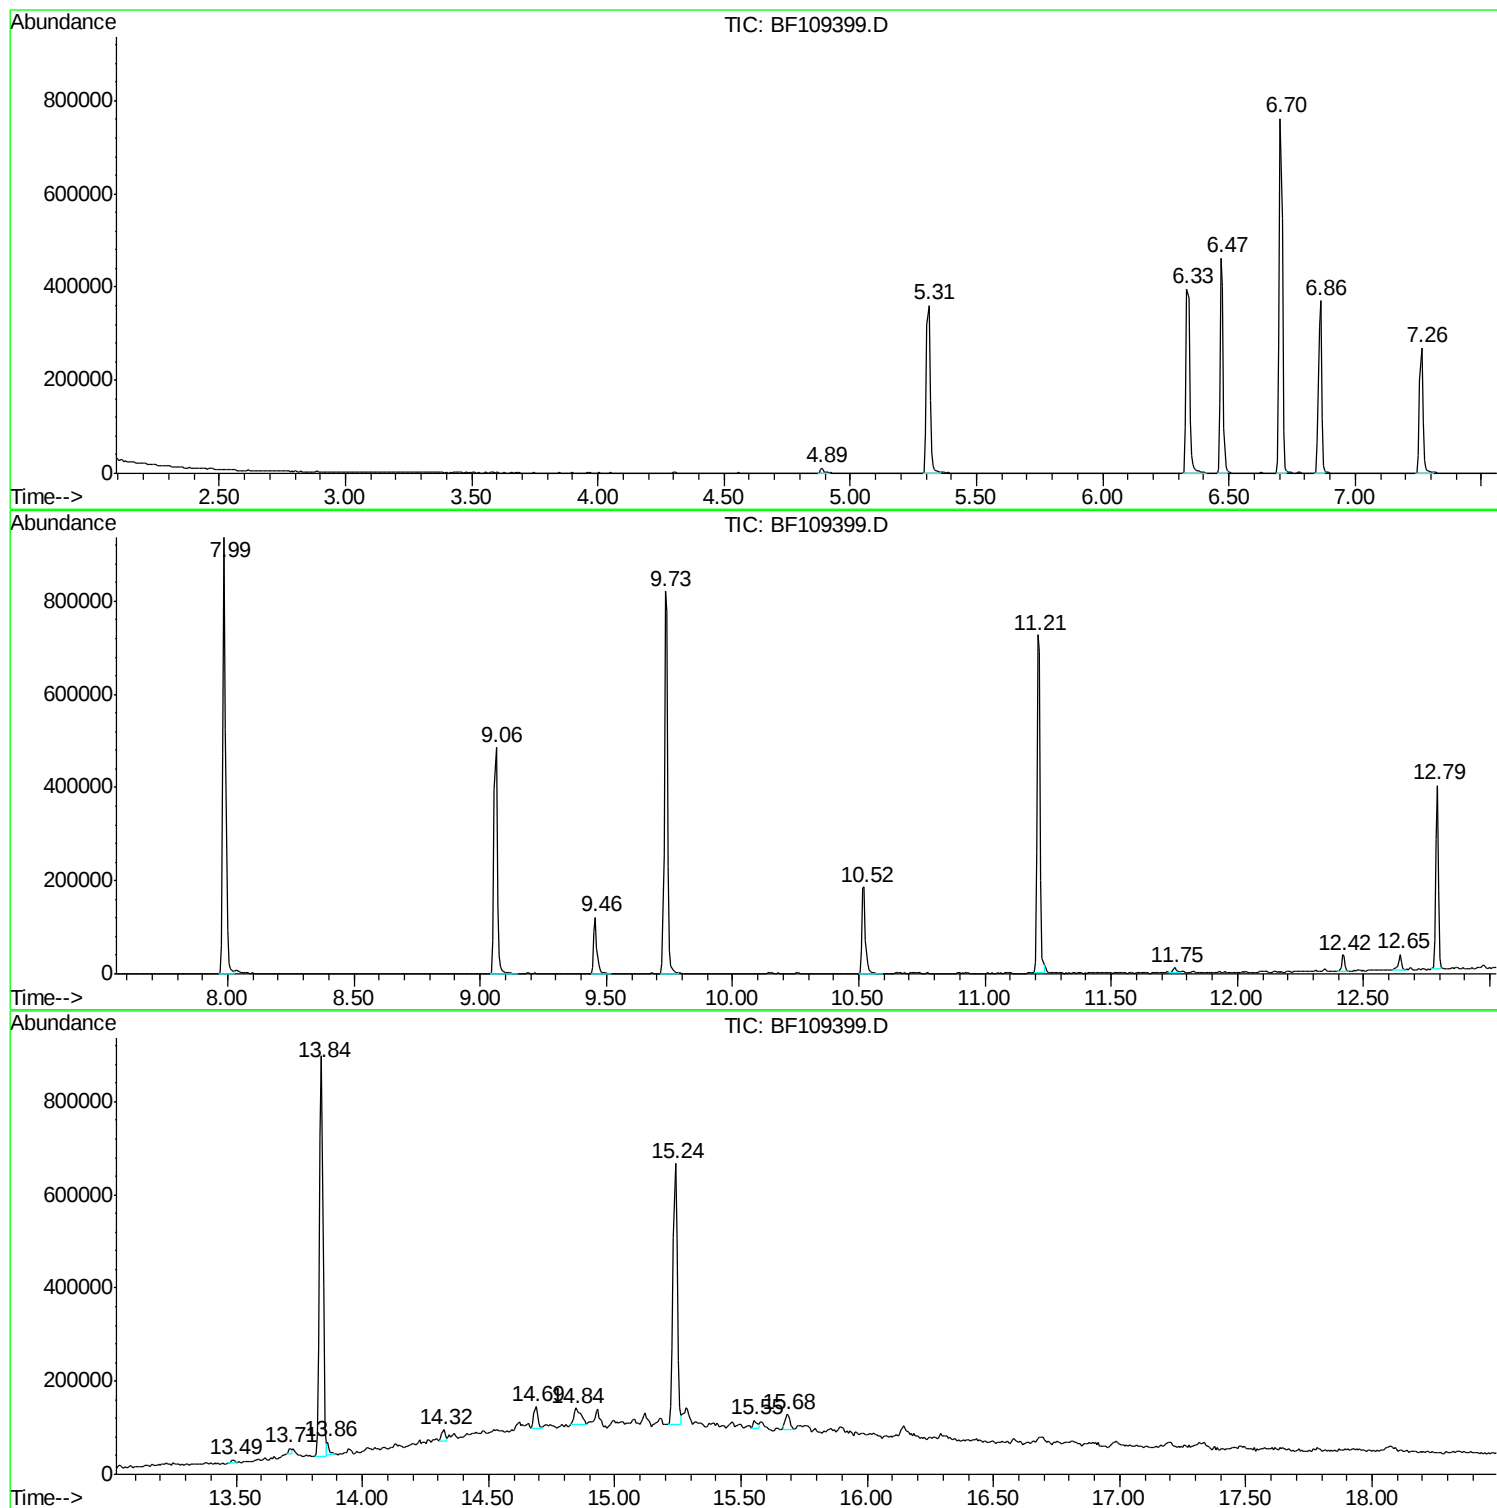

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF092718\
Data File : BF109399.D
Acq On : 27 Sep 2018 20:35
Operator : JU/SJ
Sample : J5077-04 5X
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PARCEL-190-092418-2










Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF092218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.47 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.47	13.19 ng	398812	1,4-Dichlorobenzene-d4	6.70

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	25
2		Bicyclo[4.2.0]octa-1,3,5-triene,...	132	C10H12	028749-81-7	9
3		1,3,4-Thiadiazole-2(3H)-thione, ...	132	C3H4N2S2	029490-19-5	9
4		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	9
5		4-Chloro-2-fluoro-pyrimidine	132	C4H2ClFN2	051422-00-5	9

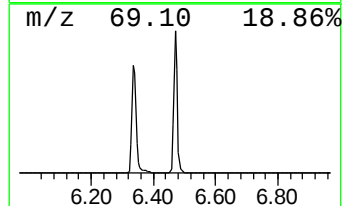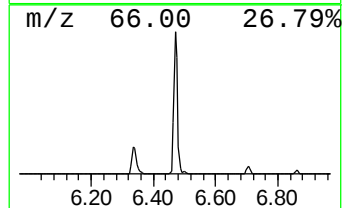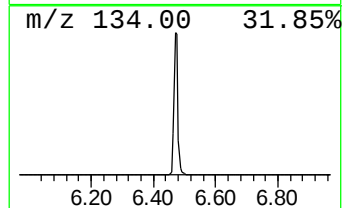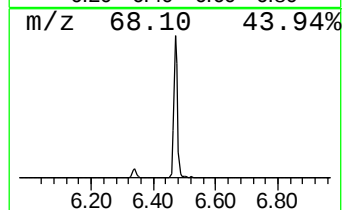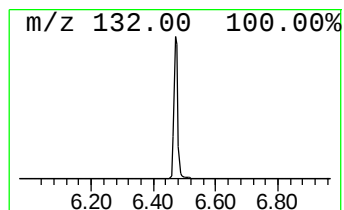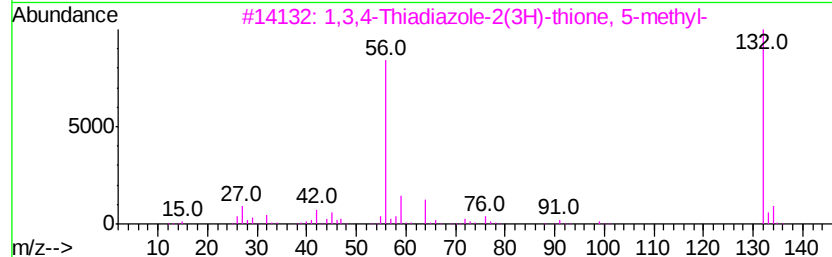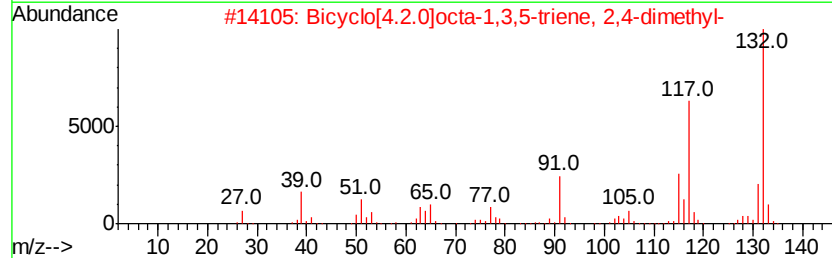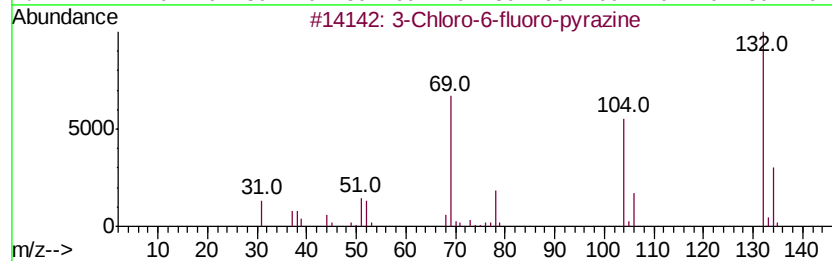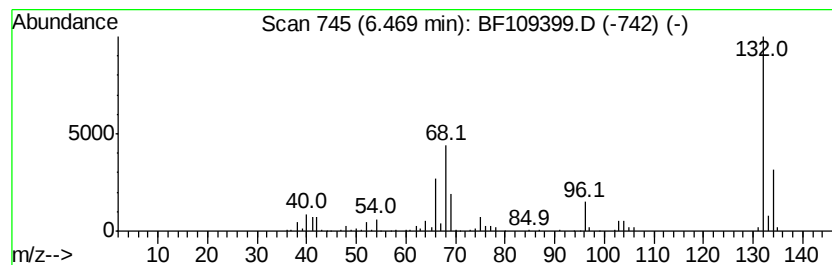

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF092718\
Data File : BF109399.D
Acq On : 27 Sep 2018 20:35
Operator : JU/SJ
Sample : J5077-04 5X
Misc :
ALS Vial : 22 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PARCEL-190-092418-2

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF092218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.47	6.47	13.2	ng	398812	1	6.70	604898	20.0