


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092718\
 Data File : BF109378.D
 Acq On : 27 Sep 2018 11:19
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF092218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Sep 22 13:32:18 2018

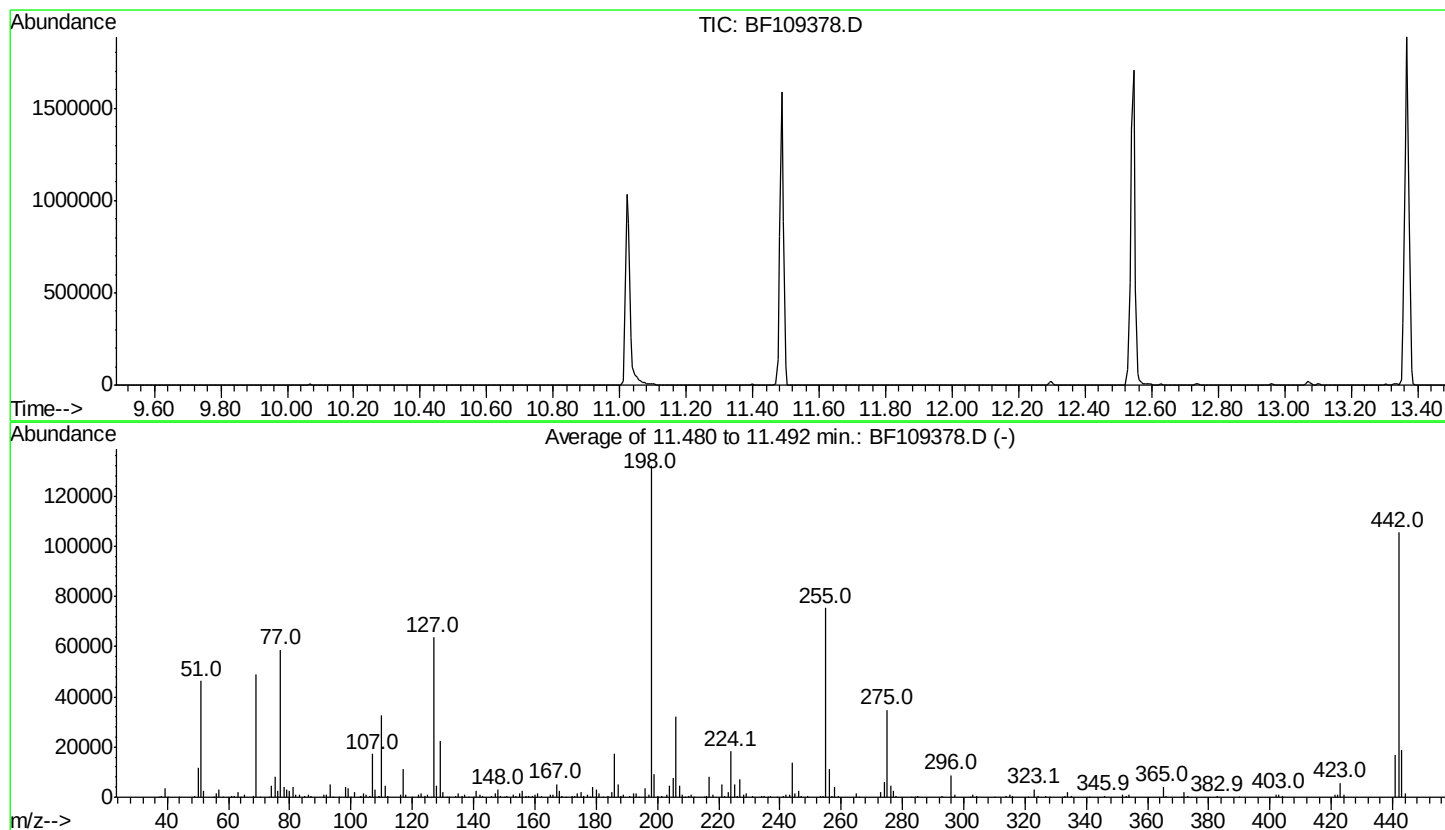

AutoFind: Scans 1597, 1598, 1599; Background Corrected with Scan 1592

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.0	46277	PASS
68	69	0.00	2	1.5	721	PASS
69	198	0.00	100	36.9	48749	PASS
70	69	0.00	2	0.2	115	PASS
127	198	10	80	48.2	63728	PASS
197	198	0.00	2	0.7	963	PASS
198	198	100	100	100.0	132093	PASS
199	198	5	9	6.9	9058	PASS
275	198	10	60	26.4	34858	PASS
365	198	1	100	3.2	4190	PASS
441	198	0.01	100	12.8	16943	PASS
442	198	50	100	79.8	105453	PASS
443	442	15	24	17.7	18701	PASS