
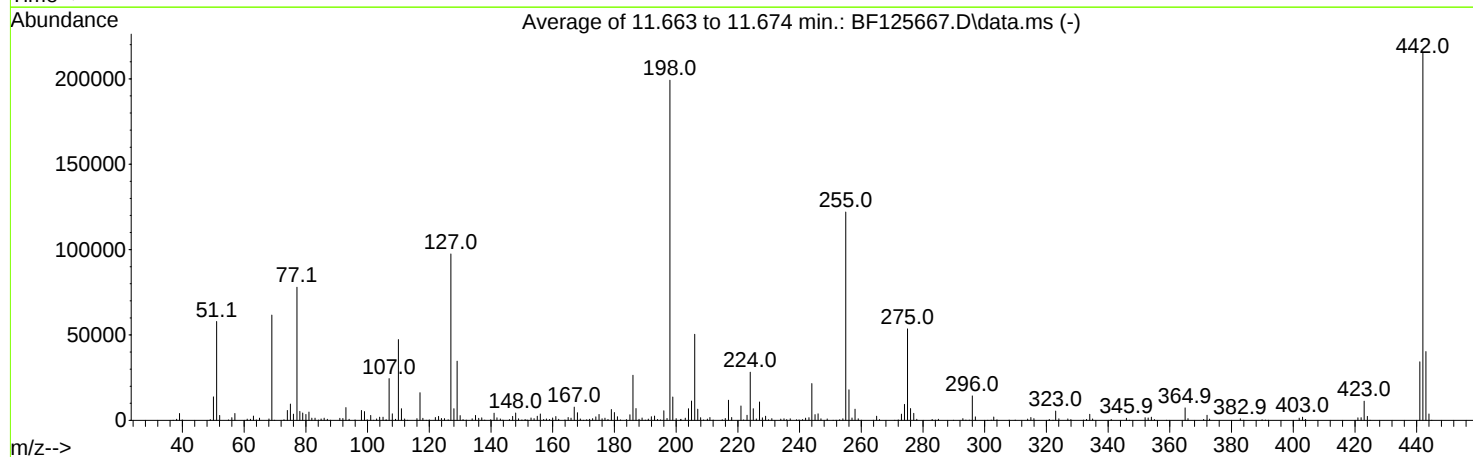


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092721\
 Data File : BF125667.D
 Acq On : 27 Sep 2021 12:02
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF092421.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Sep 24 15:38:32 2021

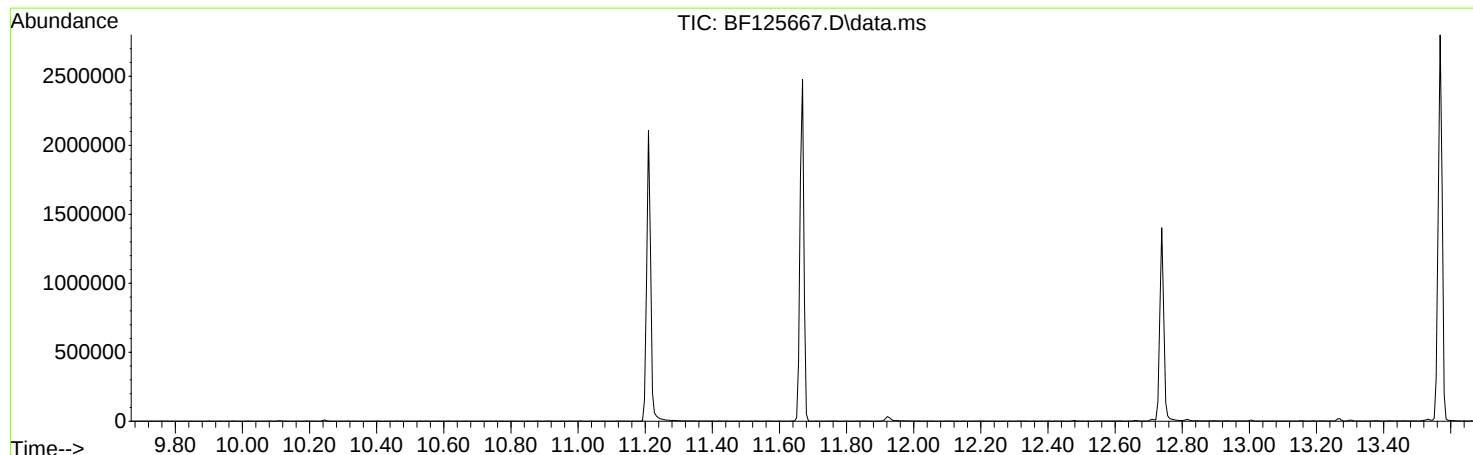




AutoFind: Scans 1628, 1629, 1630; Background Corrected with Scan 1623

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.1	57950	PASS
68	69	0.00	2	1.4	862	PASS
69	198	0.00	100	30.9	61648	PASS
70	69	0.00	2	0.2	108	PASS
127	198	10	80	48.9	97483	PASS
197	198	0.00	2	0.6	1129	PASS
198	198	100	100	100.0	199203	PASS
199	198	5	9	6.9	13675	PASS
275	198	10	60	26.9	53645	PASS
365	198	1	100	3.7	7301	PASS
441	198	0.01	100	17.2	34344	PASS
442	442	50	100	100.0	215445	PASS
443	442	15	24	18.7	40272	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092721\
 Data File : BF125667.D
 Acq On : 27 Sep 2021 12:02
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Sep 27 13:45:32 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF092421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 24 15:38:32 2021
 Response via : Initial Calibration

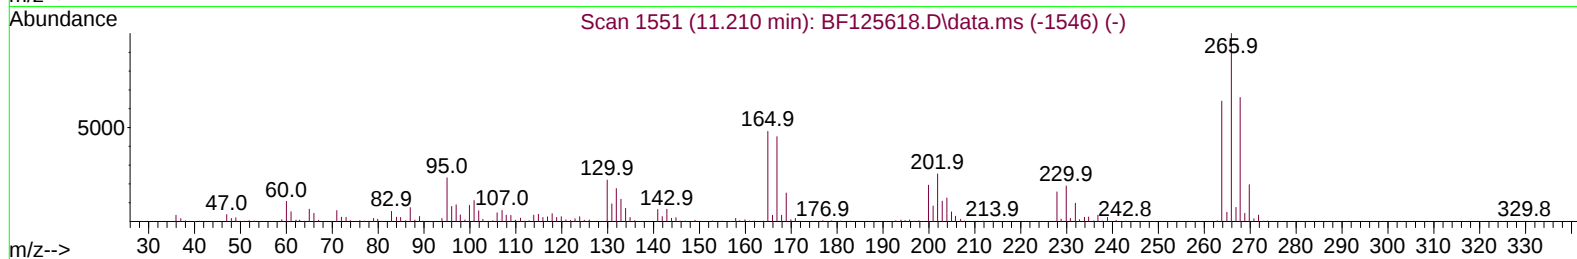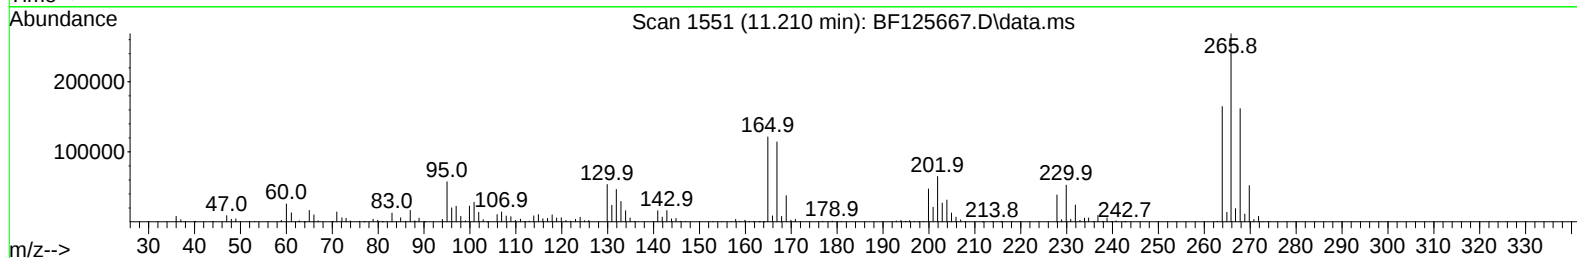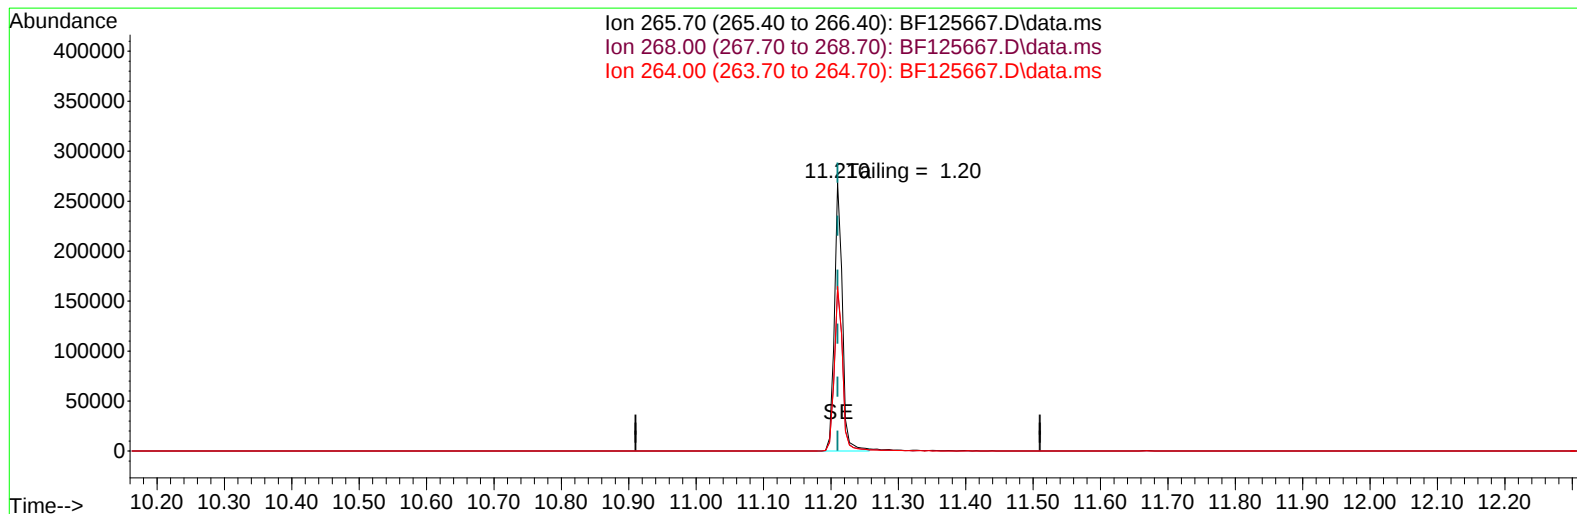

TIC: BF125667.D\data.ms

(70) Pentachlorophenol (C)

11.210min (-0.000) 47368.81 ng




response 224180

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	60.22
264.00	69.90	61.32
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092721\
Data File : BF125667.D
Acq On : 27 Sep 2021 12:02
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Sep 27 13:45:32 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF092421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 24 15:38:32 2021
Response via : Initial Calibration

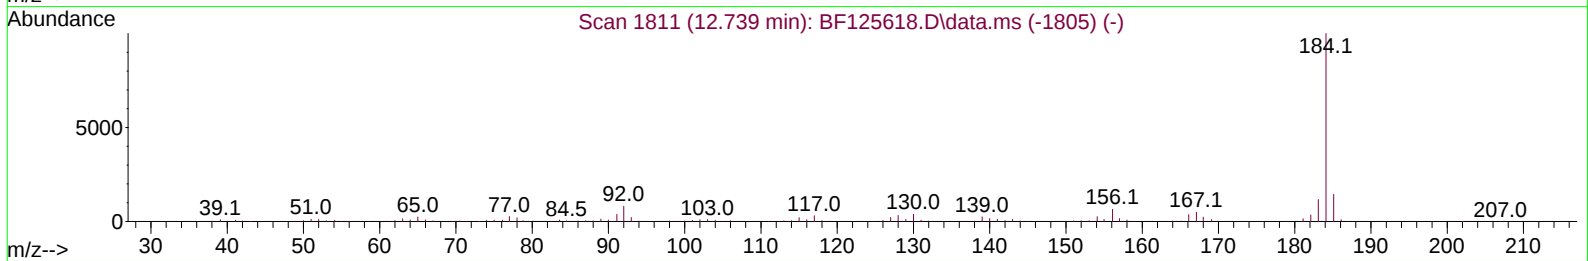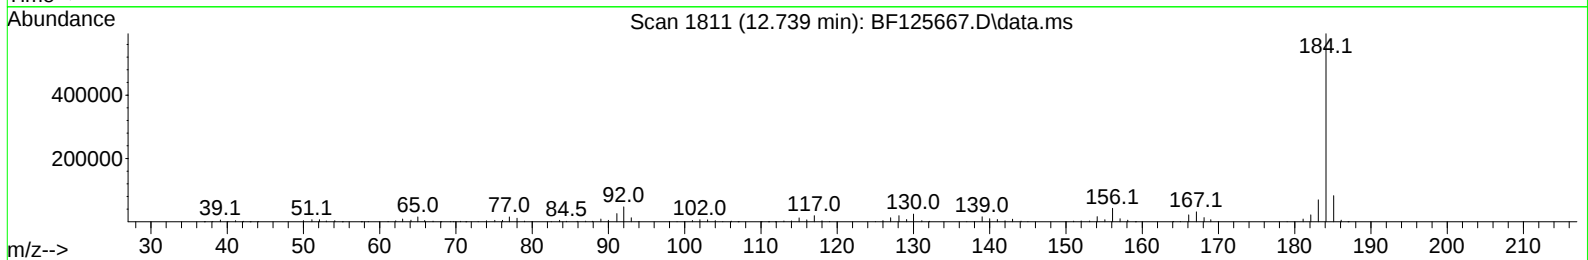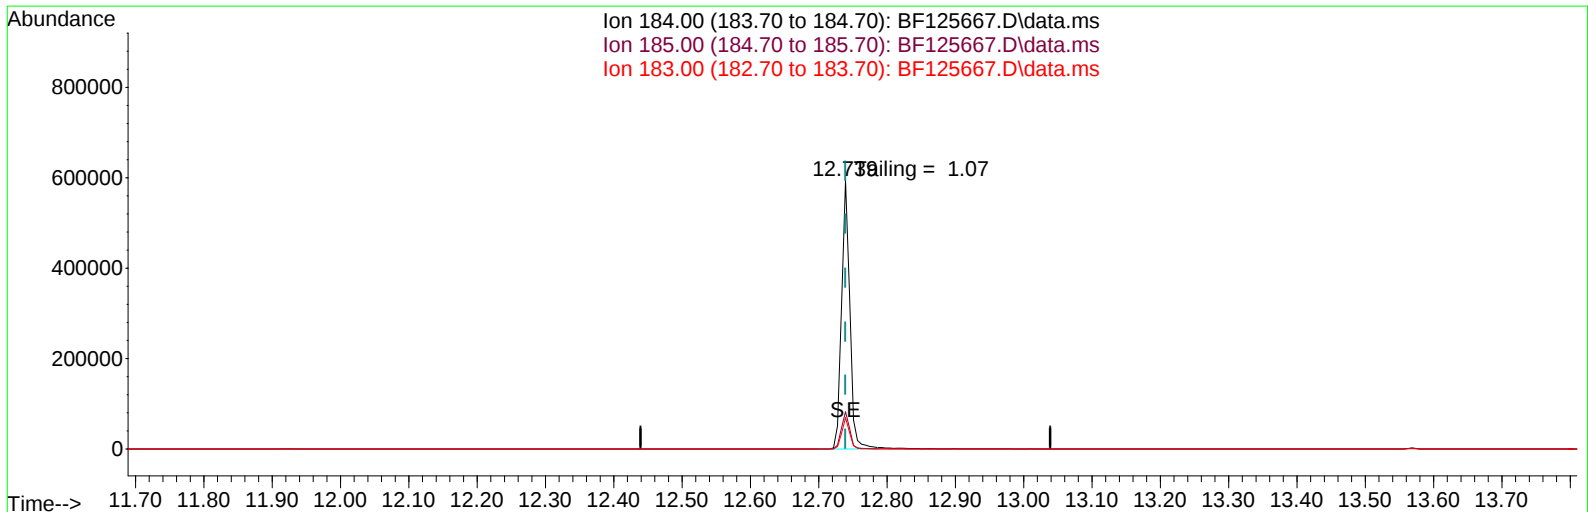

TIC: BF125667.D\data.ms

(77) Benzidine

12.739min (+ 0.000) 0.00 ng

response 505468

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	13.90
183.00	10.10	11.73
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/27/2021	BNA_F	<u>BF125667.D</u>
Compound Name	Response	Retention Time
DDT	454165	13.56
DDD	4151	13.26
DDE	539	12.93
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4690	458855	1.02