
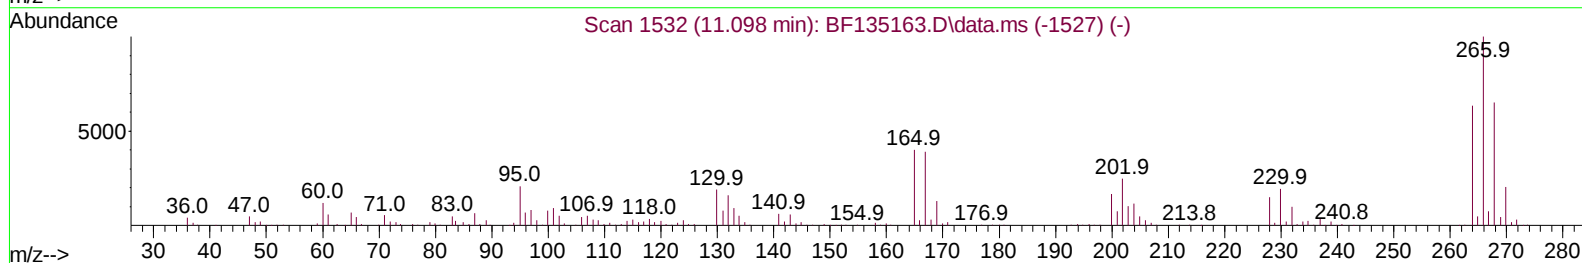
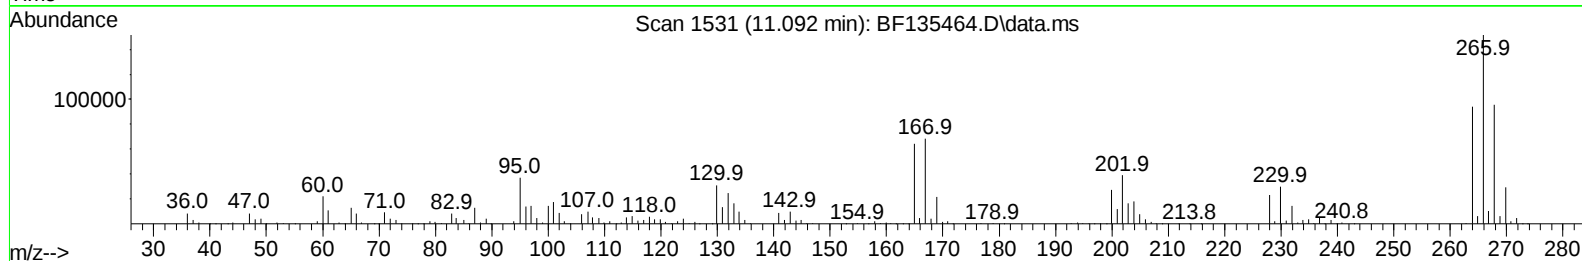


Quant Time: Sep 28 02:36:40 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 26 01:36:36 2023
Response via : Initial Calibration

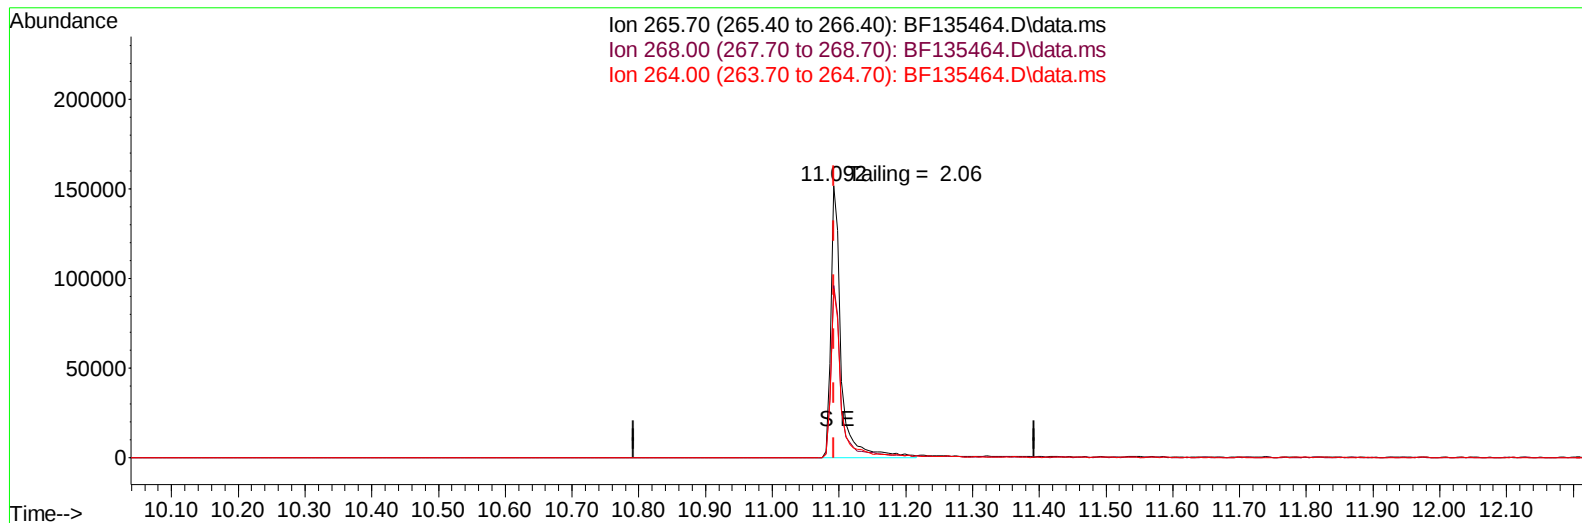

TIC: BF135464.D\data.ms




11.092min (-0.000) 34194.70 ng

response **163349**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.10	63.23
264.00	63.50	62.16
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092723\
Data File : BF135464.D
Acq On : 27 Sep 2023 10:31
Operator : CG\JU
Sample : DFTTP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 28 02:36:40 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Sep 26 01:36:36 2023
Response via : Initial Calibration

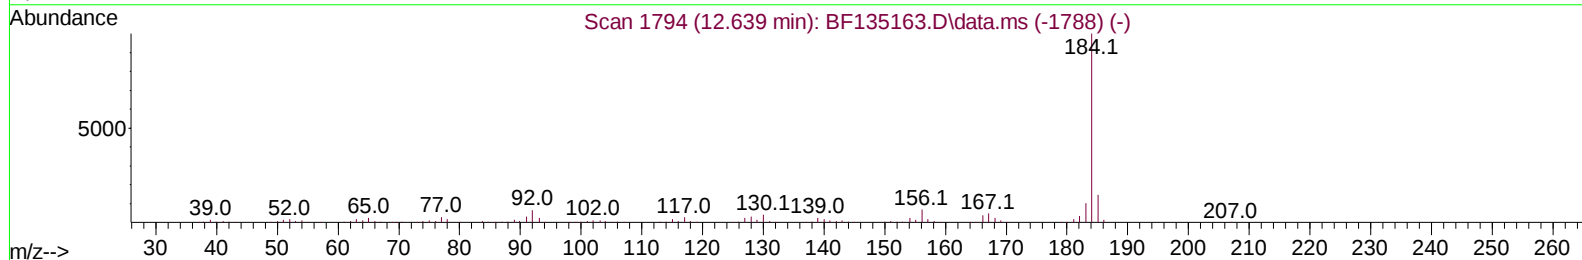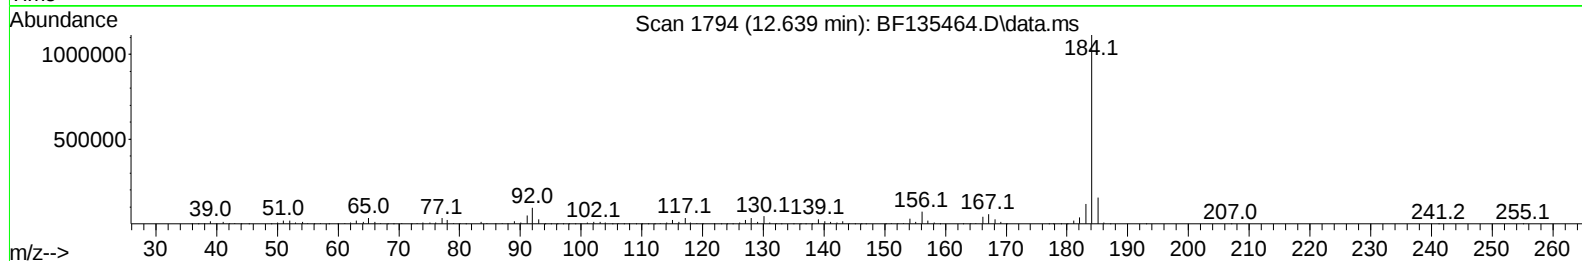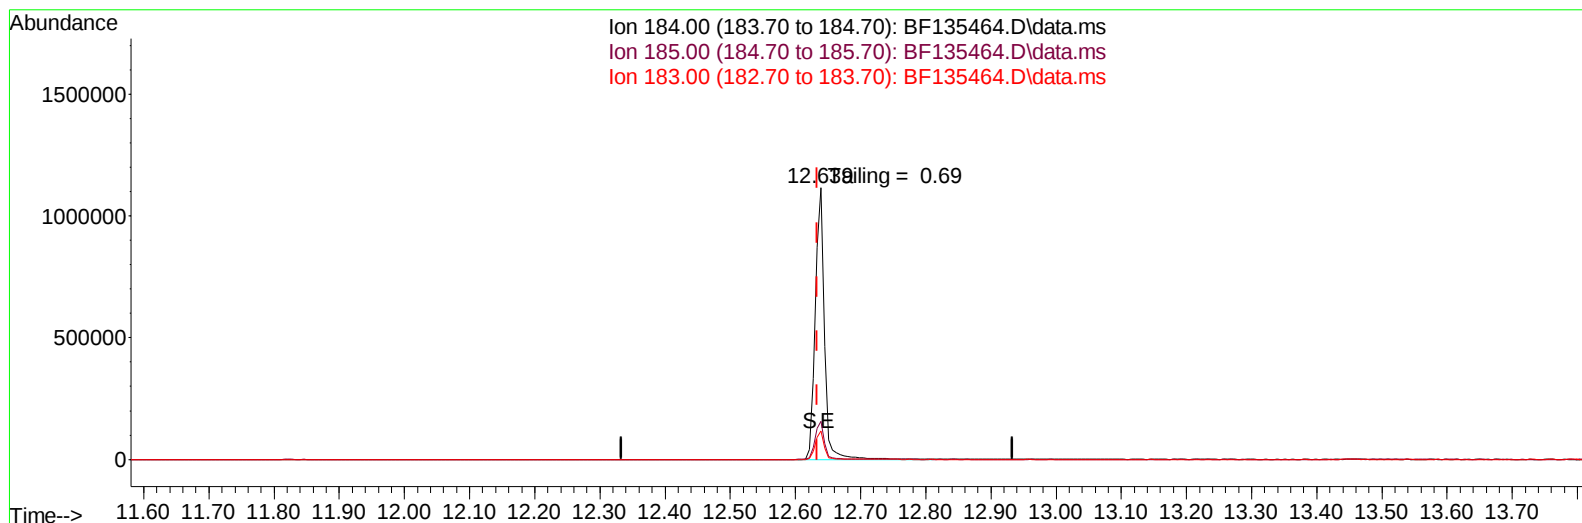

TIC: BF135464.D\data.ms

(77) Benzidine**12.639min (+ 0.006) 585013.69 ng****response 1078657**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.05
183.00	10.30	10.53
0.00	0.00	0.00