

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092723\
 Data File : BF135468.D
 Acq On : 27 Sep 2023 12:32
 Operator : CG\JU
 Sample : PB155755TB
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB155755TB

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF135468.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.398	558	563	577	rBV	4601754	4873014	96.60%	15.094%
2	6.404	729	734	737	rBV	4267020	4744769	94.06%	14.697%
3	6.751	790	793	804	rVB	1244014	1022120	20.26%	3.166%
4	7.322	884	890	893	rBV	3183386	3220316	63.84%	9.975%
5	8.034	1006	1011	1017	rBV	1406505	1325266	26.27%	4.105%
6	9.110	1189	1194	1198	rBV	4527808	5044625	100.00%	15.626%
7	9.786	1304	1309	1313	rBV	1458747	1419177	28.13%	4.396%
8	10.586	1440	1445	1467	rBV	2818833	2954201	58.56%	9.151%
9	11.280	1559	1563	1571	rBV	1612504	1449192	28.73%	4.489%
10	12.880	1830	1835	1839	rBV	3993600	4488489	88.98%	13.903%
11	13.939	2011	2015	2026	rBV	1006445	964717	19.12%	2.988%
12	15.410	2260	2265	2277	rBV	504966	777650	15.42%	2.409%




Sum of corrected areas: 32283536

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092723\
Data File : BF135468.D
Acq On : 27 Sep 2023 12:32
Operator : CG\JU
Sample : PB155755TB
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB155755TB

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

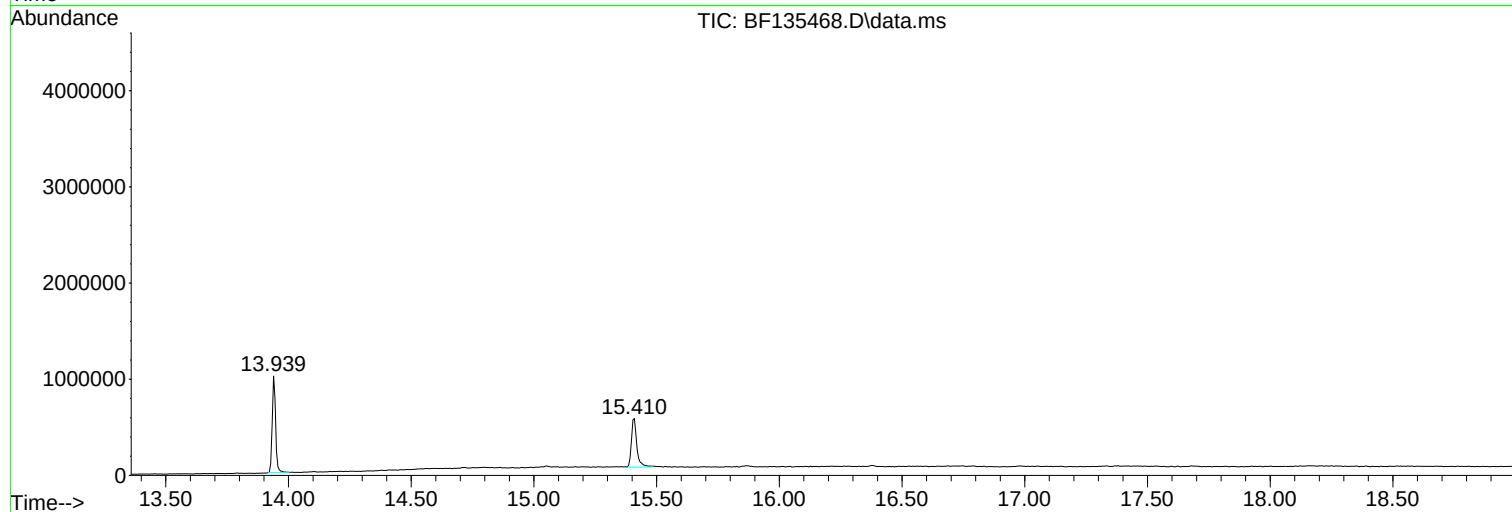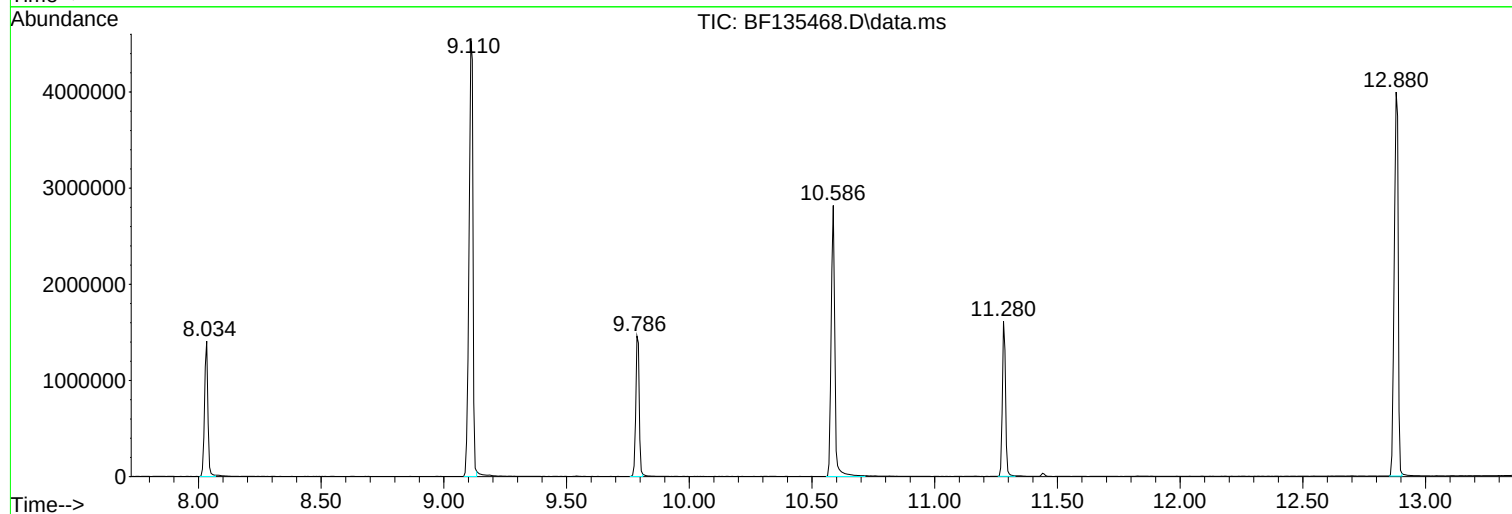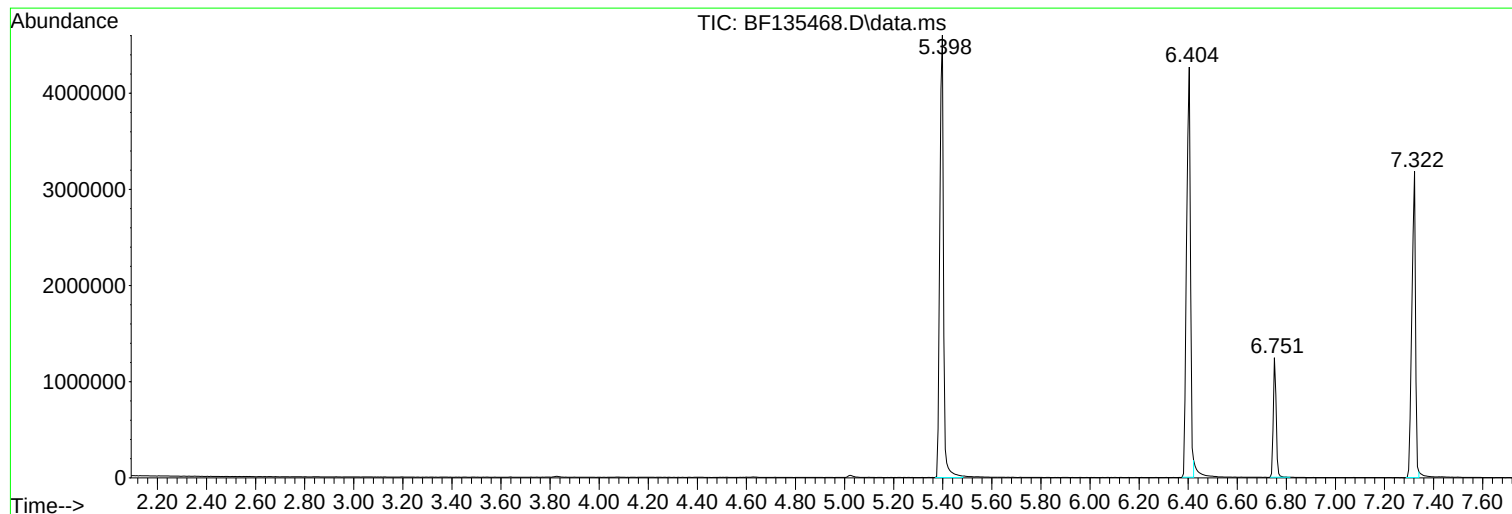

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092723\
Data File : BF135468.D
Acq On : 27 Sep 2023 12:32
Operator : CG\JU
Sample : PB155755TB
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB155755TB

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092723\
Data File : BF135468.D
Acq On : 27 Sep 2023 12:32
Operator : CG\JU
Sample : PB155755TB
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB155755TB

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------