

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092723\
 Data File : BF135469.D
 Acq On : 27 Sep 2023 13:03
 Operator : CG\JU
 Sample : PB155813TB
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB155813TB

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF135469.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.822	290	295	303	rVB	58321	87238	1.79%	0.286%
2	5.398	558	563	585	rBV	4341888	4786808	98.01%	15.671%
3	6.404	729	734	737	rBV	4185505	4590849	94.00%	15.029%
4	6.751	790	793	801	rVB	1059211	923887	18.92%	3.025%
5	7.322	885	890	893	rBV	2996742	3119540	63.87%	10.212%
6	8.033	1006	1011	1026	rBV	1242619	1228845	25.16%	4.023%
7	9.110	1189	1194	1198	rBV	4487113	4883996	100.00%	15.989%
8	9.786	1304	1309	1313	rBV	1403471	1272058	26.05%	4.164%
9	10.586	1441	1445	1448	rBV	2754427	2644951	54.16%	8.659%
10	11.280	1560	1563	1571	rBV	1454734	1267956	25.96%	4.151%
11	12.880	1830	1835	1839	rBV	3832751	4180576	85.60%	13.686%
12	13.939	2011	2015	2030	rBV	848086	863131	17.67%	2.826%
13	15.409	2260	2265	2281	rBV	459385	696754	14.27%	2.281%




Sum of corrected areas: 30546589

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092723\
Data File : BF135469.D
Acq On : 27 Sep 2023 13:03
Operator : CG\JU
Sample : PB155813TB
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB155813TB

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

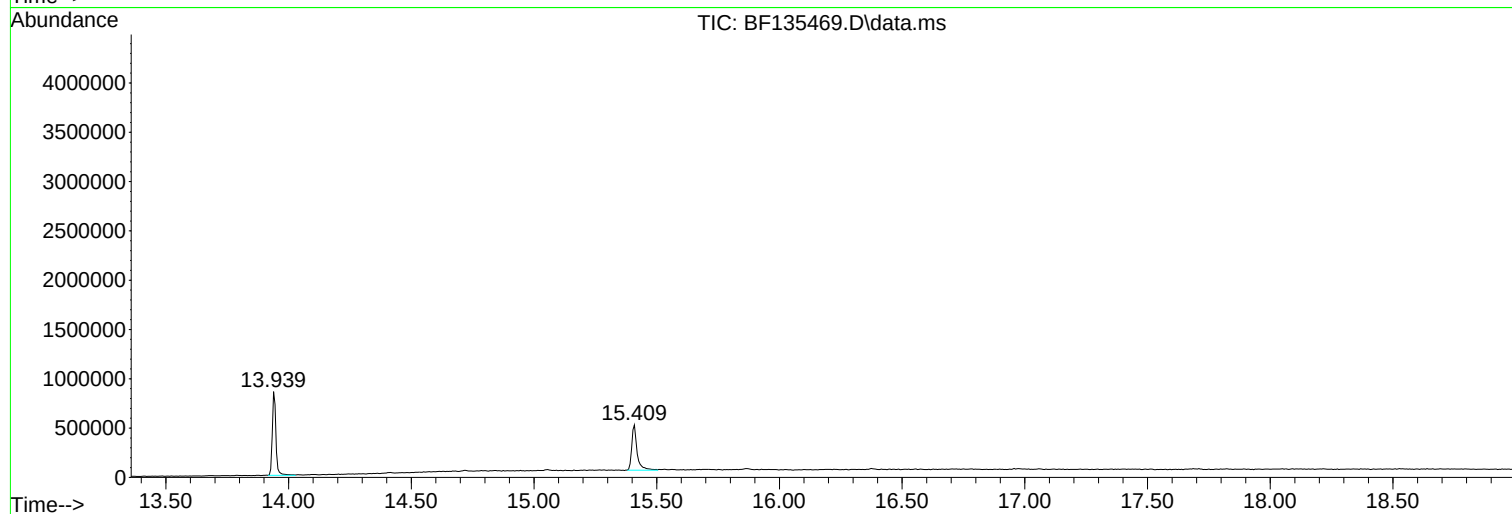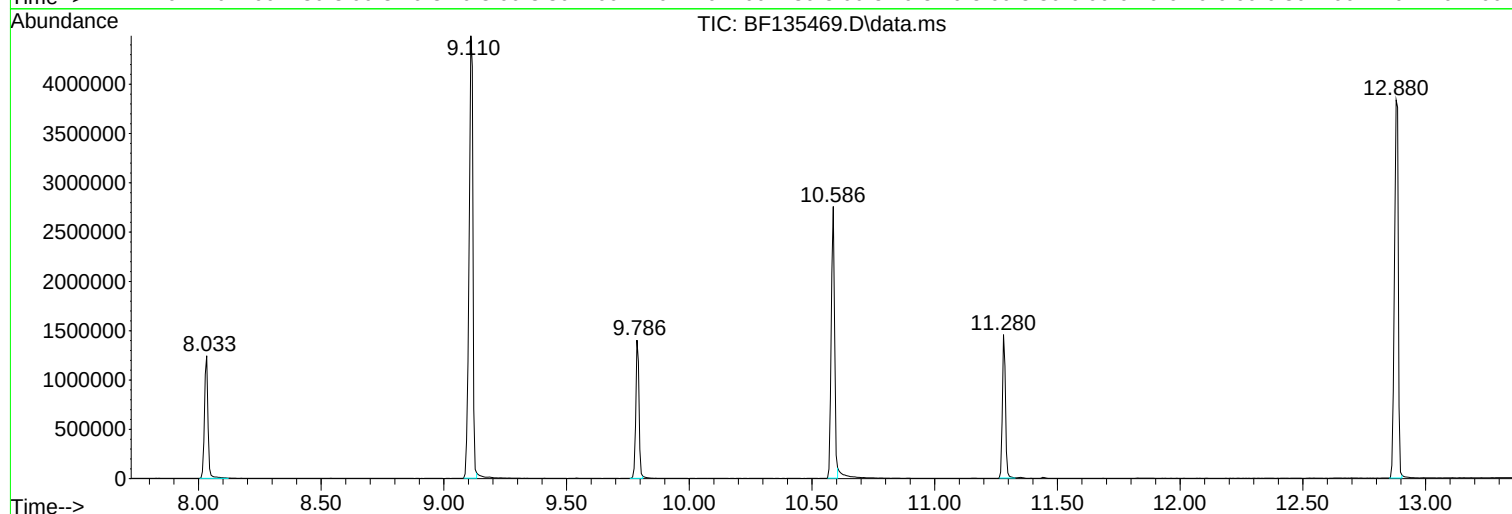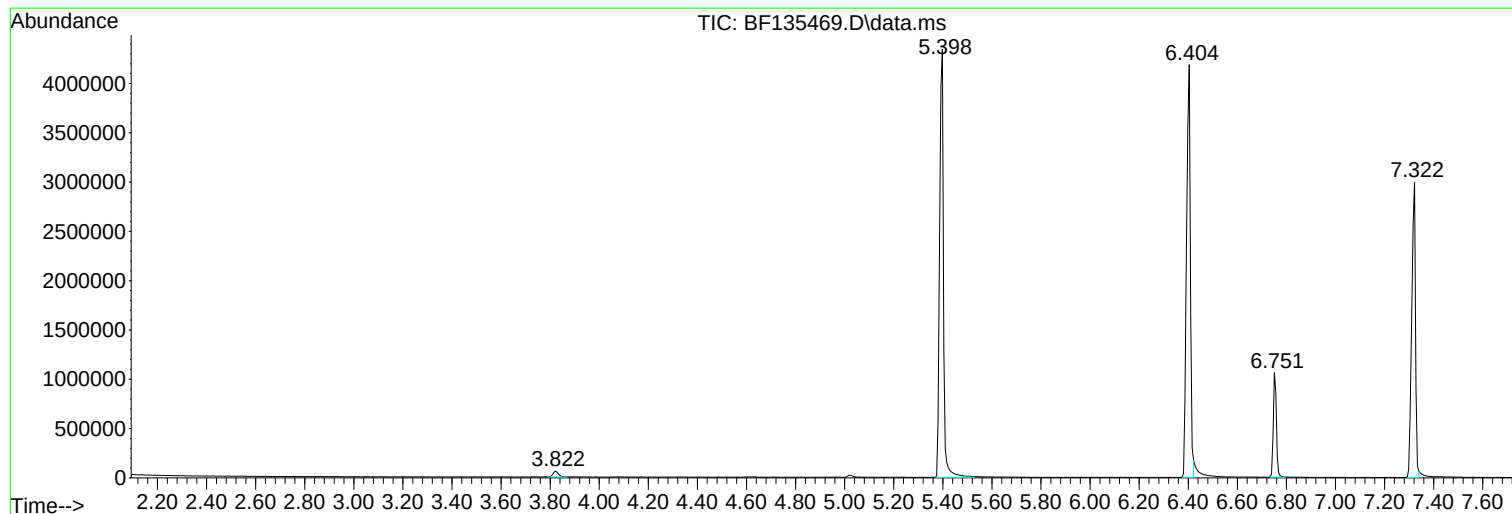

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092723\
Data File : BF135469.D
Acq On : 27 Sep 2023 13:03
Operator : CG\JU
Sample : PB155813TB
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB155813TB

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092723\
Data File : BF135469.D
Acq On : 27 Sep 2023 13:03
Operator : CG\JU
Sample : PB155813TB
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB155813TB

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------