

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092723\
 Data File : BF135478.D
 Acq On : 27 Sep 2023 18:04
 Operator : CG\JU
 Sample : 04566-11
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 FB-9-20

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF135478.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.751	278	283	287	rBV	33396	49437	1.28%	0.228%
2	4.975	488	491	507	rVB	79696	105525	2.74%	0.487%
3	5.387	557	561	571	rBV	1620103	1710124	44.35%	7.897%
4	6.398	730	733	752	rBV	941950	1058897	27.46%	4.890%
5	6.751	790	793	803	rBV	1270576	1077746	27.95%	4.977%
6	7.322	885	890	904	rBV	2460023	2540972	65.90%	11.734%
7	7.422	904	907	917	rVV	41853	70425	1.83%	0.325%
8	8.034	1007	1011	1030	rBV	1593379	1389567	36.04%	6.417%
9	8.286	1051	1054	1068	rVB	50574	109161	2.83%	0.504%
10	9.110	1189	1194	1198	rBV	3987043	3855938	100.00%	17.806%
11	9.786	1305	1309	1322	rVB	1447495	1373226	35.61%	6.341%
12	10.586	1441	1445	1461	rBV	1878322	2022139	52.44%	9.338%
13	11.280	1560	1563	1572	rBV	1330715	1248066	32.37%	5.763%
14	12.880	1830	1835	1838	rBV	3478283	3273687	84.90%	15.117%
15	13.939	2012	2015	2025	rVB	819638	787636	20.43%	3.637%
16	15.410	2260	2265	2276	rBV	728270	982923	25.49%	4.539%




Sum of corrected areas: 21655469

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092723\
Data File : BF135478.D
Acq On : 27 Sep 2023 18:04
Operator : CG\JU
Sample : 04566-11
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
FB-9-20

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

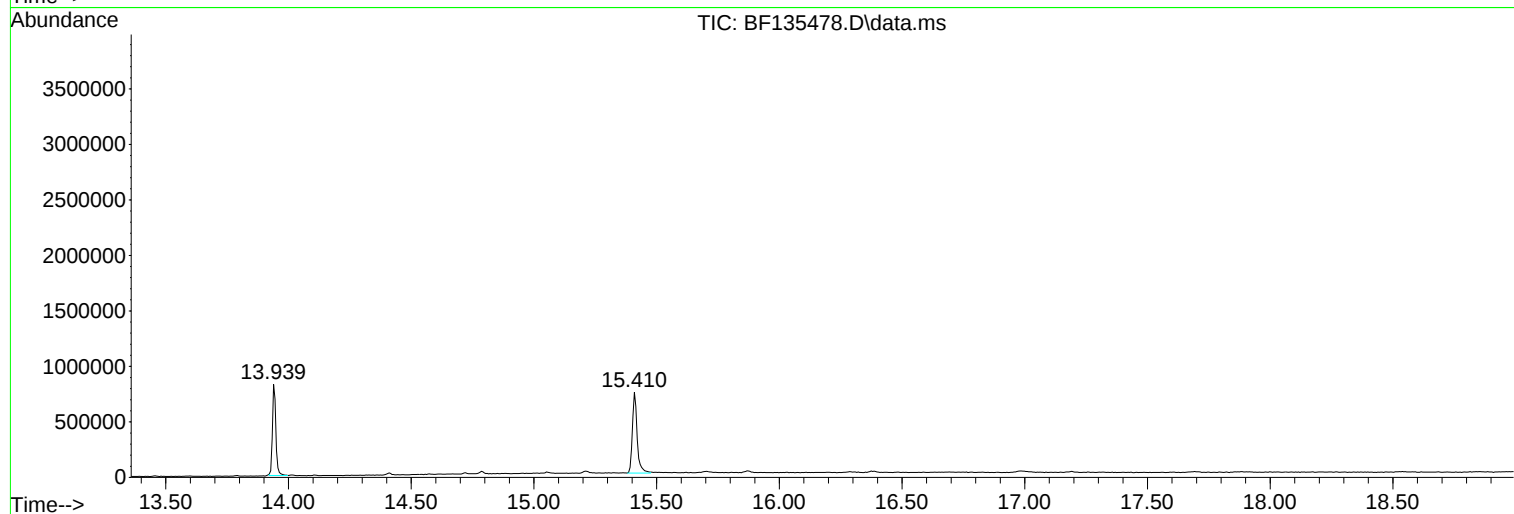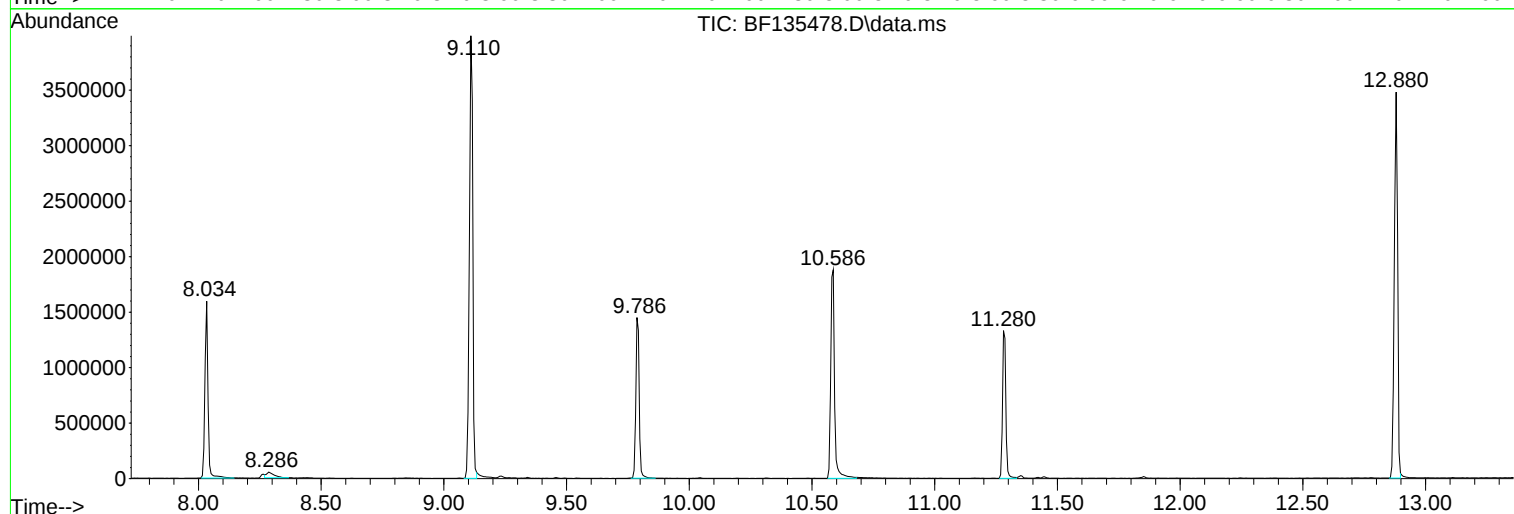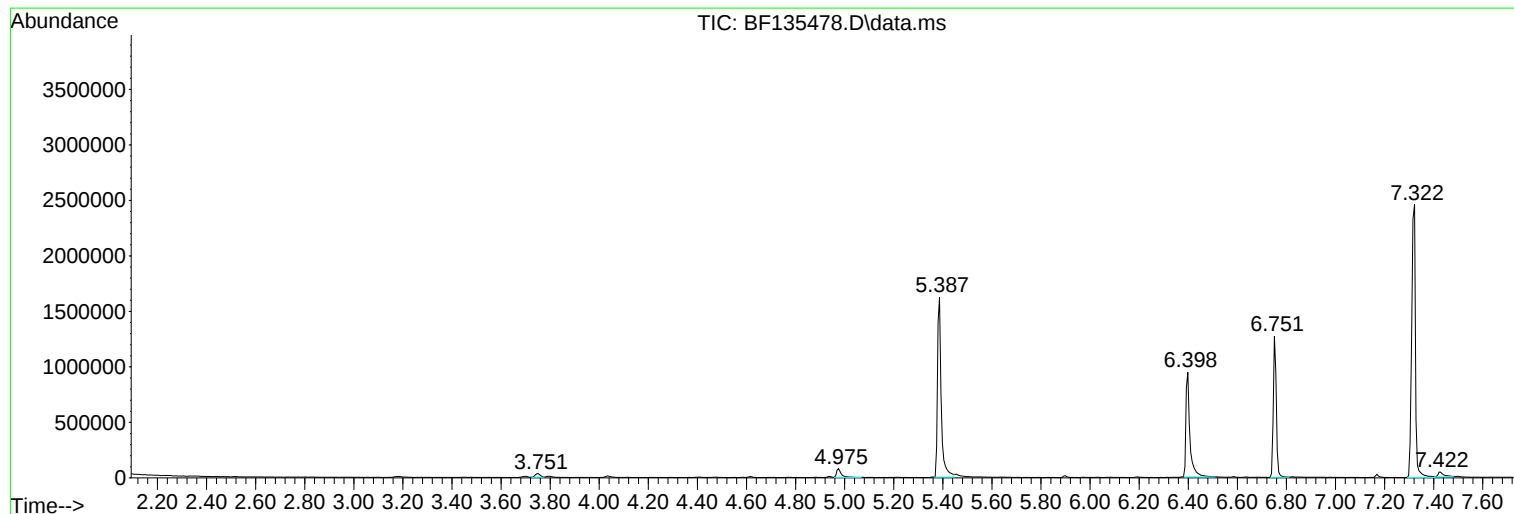

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092723\
Data File : BF135478.D
Acq On : 27 Sep 2023 18:04
Operator : CG\JU
Sample : 04566-11
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
FB-9-20

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092723\
Data File : BF135478.D
Acq On : 27 Sep 2023 18:04
Operator : CG\JU
Sample : 04566-11
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
FB-9-20

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------