


Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF092723\  
Data File : BF135464.D  
Acq On : 27 Sep 2023 10:31  
Operator : CG\JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF091123.M  
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
Last Update : Tue Sep 26 01:36:36 2023

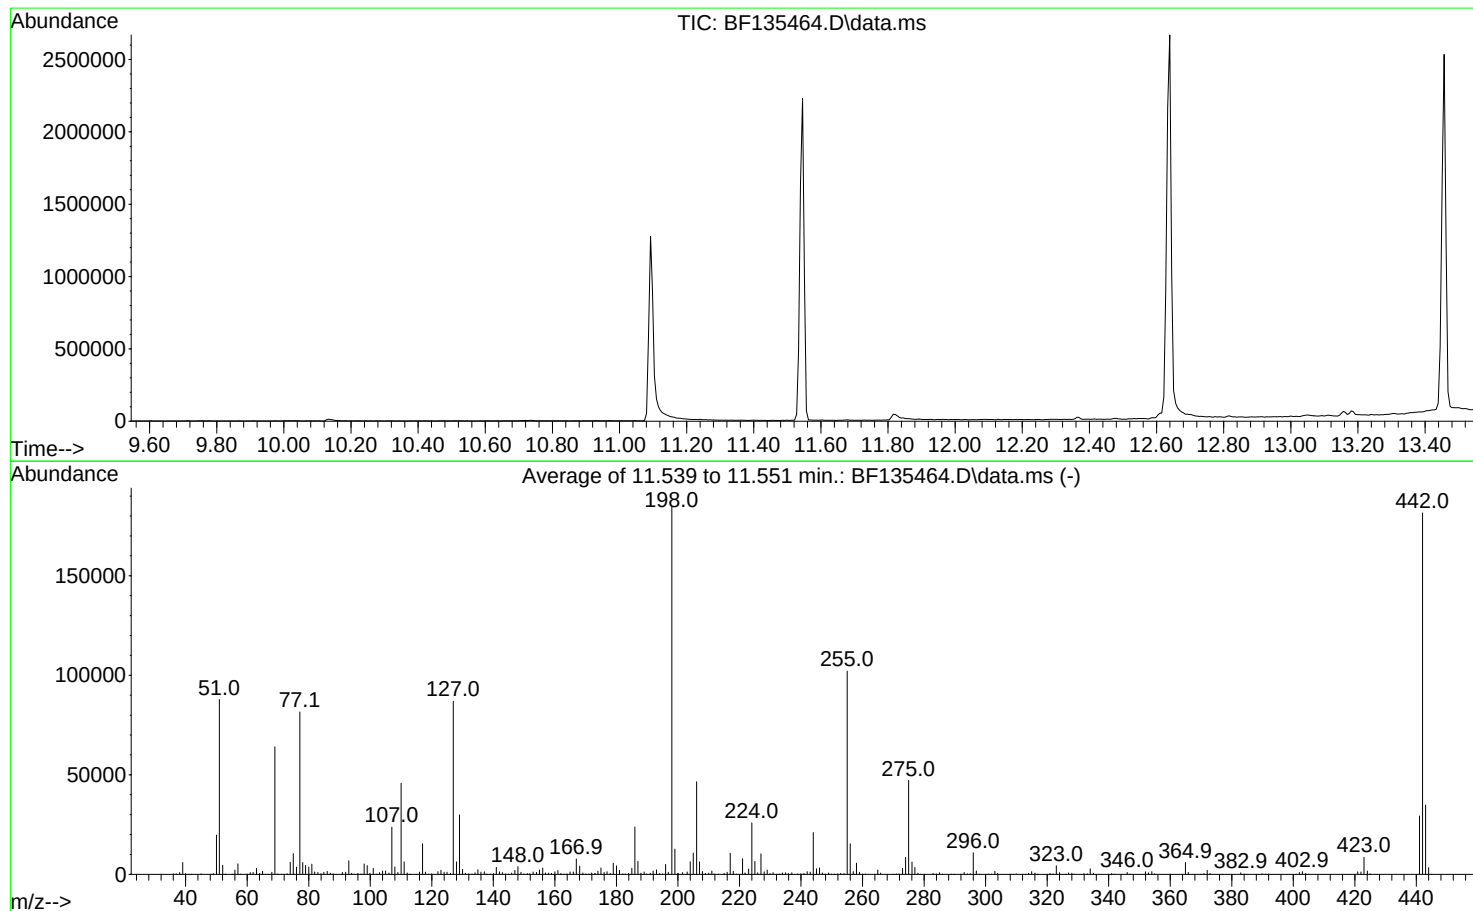




AutoFind: Scans 1607, 1608, 1609; Background Corrected with Scan 1602

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 47.6         | 87885      | PASS                |
| 68             | 69              | 0.00            | 2               | 1.7          | 1072       | PASS                |
| 69             | 198             | 0.00            | 100             | 34.7         | 64032      | PASS                |
| 70             | 69              | 0.00            | 2               | 0.3          | 196        | PASS                |
| 127            | 198             | 10              | 80              | 47.1         | 86952      | PASS                |
| 197            | 198             | 0.00            | 2               | 0.6          | 1024       | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 184779     | PASS                |
| 199            | 198             | 5               | 9               | 6.9          | 12676      | PASS                |
| 275            | 198             | 10              | 60              | 25.5         | 47147      | PASS                |
| 365            | 198             | 1               | 100             | 3.2          | 5923       | PASS                |
| 441            | 198             | 0.01            | 100             | 15.9         | 29352      | PASS                |
| 442            | 442             | 50              | 100             | 100.0        | 181584     | PASS                |
| 443            | 442             | 15              | 24              | 19.2         | 34803      | PASS                |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF092723\  
Data File : BF135464.D  
Acq On : 27 Sep 2023 10:31  
Operator : CG\JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP

Quant Time: Sep 28 02:36:40 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF091123.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Sep 26 01:36:36 2023  
Response via : Initial Calibration

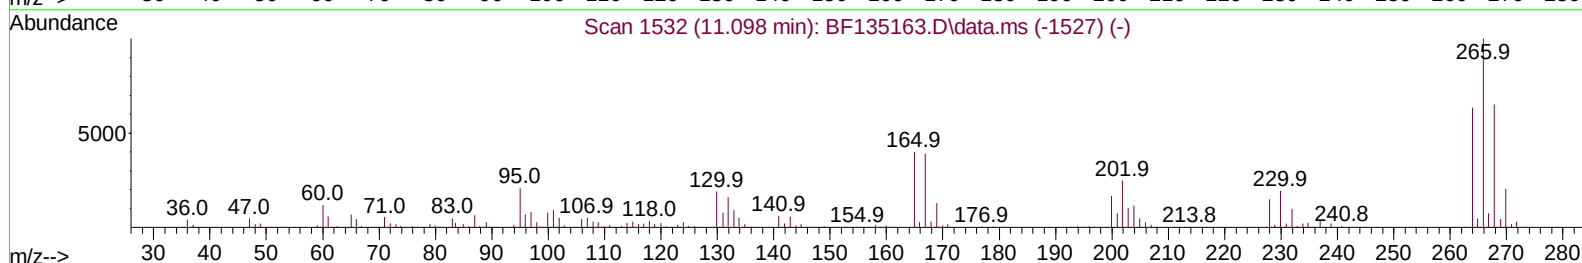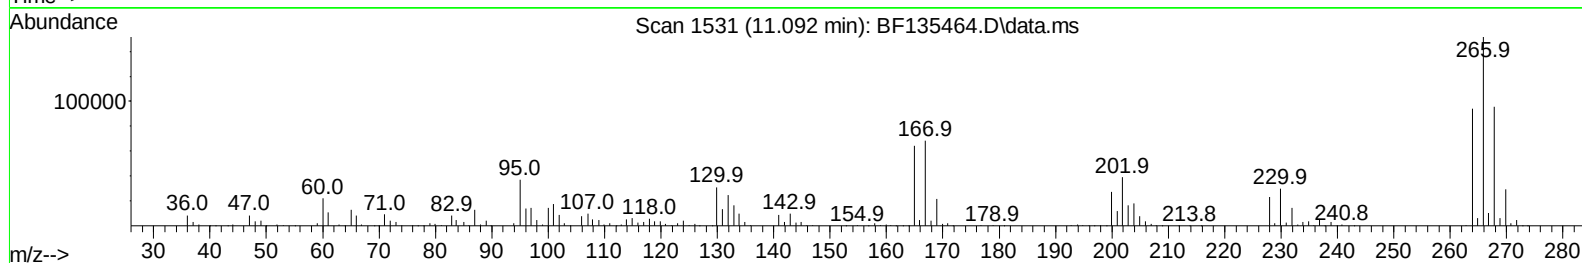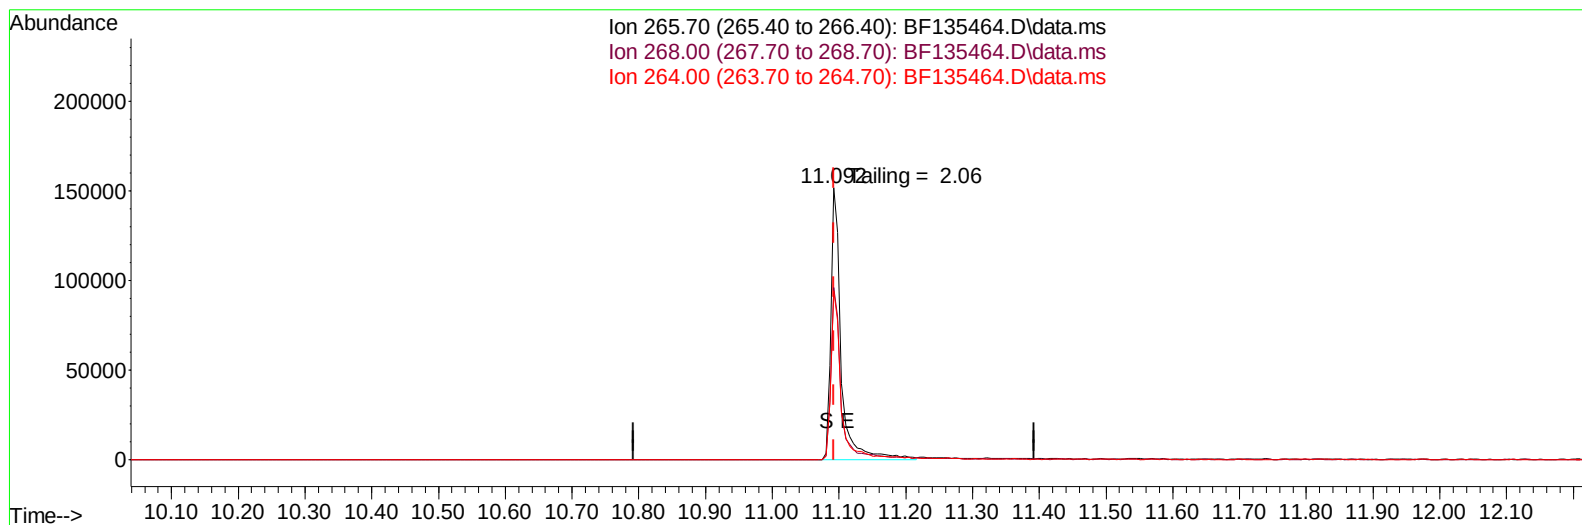

TIC: BF135464.D\data.ms

**(70) Pentachlorophenol (C)**

**11.092min (-0.000) 34194.70 ng**




**response 163349**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 65.10  | 63.23  |
| 264.00 | 63.50  | 62.16  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF092723\  
 Data File : BF135464.D  
 Acq On : 27 Sep 2023 10:31  
 Operator : CG\JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 DFTPP

Quant Time: Sep 28 02:36:40 2023  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF091123.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Tue Sep 26 01:36:36 2023  
 Response via : Initial Calibration

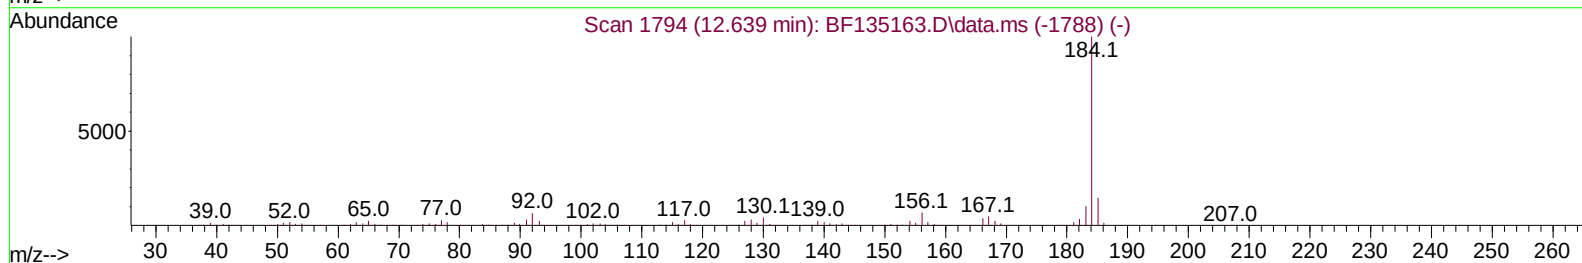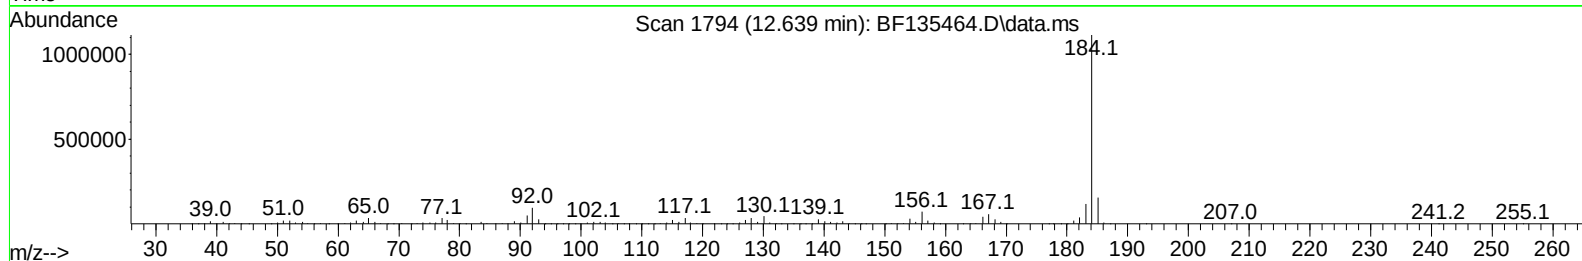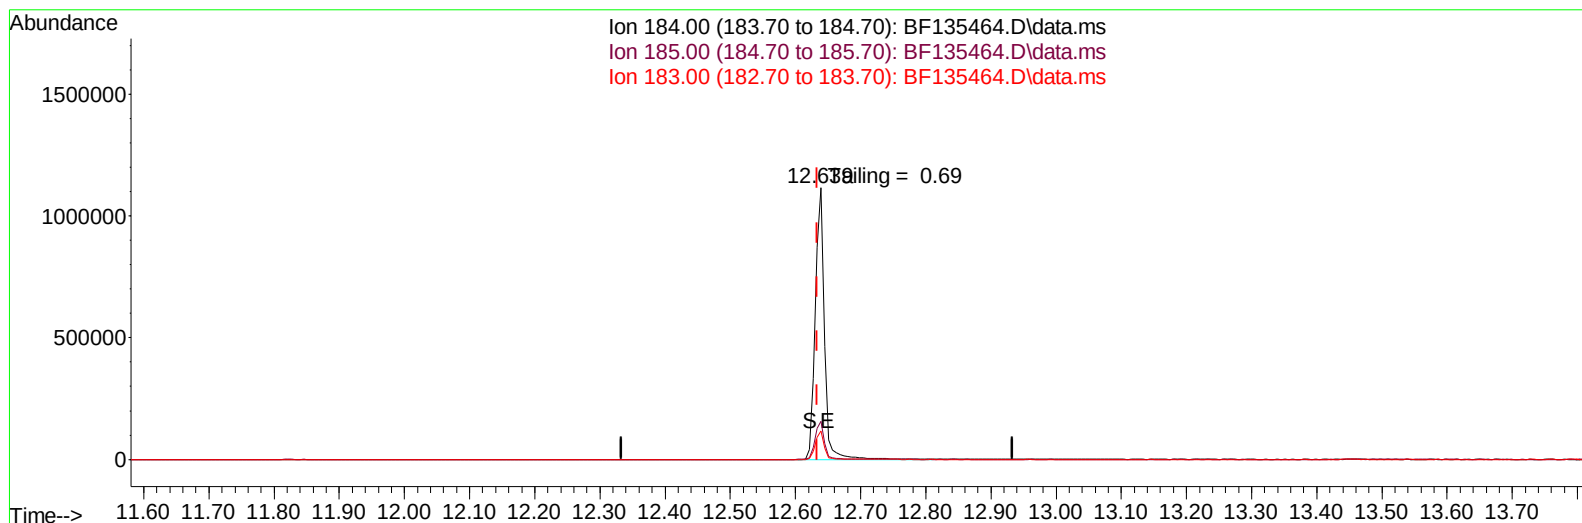

TIC: BF135464.D\data.ms

**(77) Benzidine****12.639min (+ 0.006) 585013.69 ng****response 1078657**

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 14.60  | 14.05  |
| 183.00 | 10.30  | 10.53  |
| 0.00   | 0.00   | 0.00   |

# DDT Breakdown

| Date          | Instrument Name  | DFTPP Data File    |
|---------------|------------------|--------------------|
| 9/27/2023     | BNA_F            | <u>BF135464.D</u>  |
|               |                  |                    |
|               |                  |                    |
| Compound Name | Response         | Retention Time     |
|               |                  |                    |
| DDT           | 415359           | 13.457             |
| DDD           | 11121            | 13.18              |
| DDE           | 1246             | 12.822             |
|               |                  |                    |
|               |                  |                    |
| SUM(DDD+DDE)  | SUM(DDT+DDD+DDE) | % Breakdown Of DDT |
|               |                  |                    |
| 12367         | 427726           | 2.89               |
|               |                  |                    |

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP