

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092822\
 Data File : BF130452.D
 Acq On : 28 Sep 2022 17:25
 Operator : CG\JU
 Sample : N4850-02
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 WC-14B-SP-2

Quant Time: Sep 29 02:16:13 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 28 02:59:31 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.645	152	101213	20.000	ng	0.00
21) Naphthalene-d8	7.928	136	396942	20.000	ng	# 0.00
39) Acenaphthene-d10	9.675	164	200862	20.000	ng	0.00
64) Phenanthrene-d10	11.157	188	311830	20.000	ng	# 0.00
76) Chrysene-d12	13.786	240	183136	20.000	ng	# 0.00
86) Perylene-d12	15.174	264	210645	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.263	112	690015	118.246	ng	0.02
7) Phenol-d6	6.287	99	774964	106.139	ng	0.00
23) Nitrobenzene-d5	7.210	82	592274	76.229	ng	0.00
42) 2,4,6-Tribromophenol	10.469	330	278525	144.715	ng	0.00
45) 2-Fluorobiphenyl	9.004	172	1137117	82.438	ng	0.00
79) Terphenyl-d14	12.745	244	1018181	92.096	ng	0.00
Target Compounds						
32) Benzoic acid	7.681	122	31183	8.098	ng	Qvalue 93
77) Benzidine	12.498	184	284877	53.586	ng	# 96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092822\
Data File : BF130452.D
Acq On : 28 Sep 2022 17:25
Operator : CG\JU
Sample : N4850-02
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
WC-14B-SP-2

Quant Time: Sep 29 02:16:13 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 28 02:59:31 2022
Response via : Initial Calibration




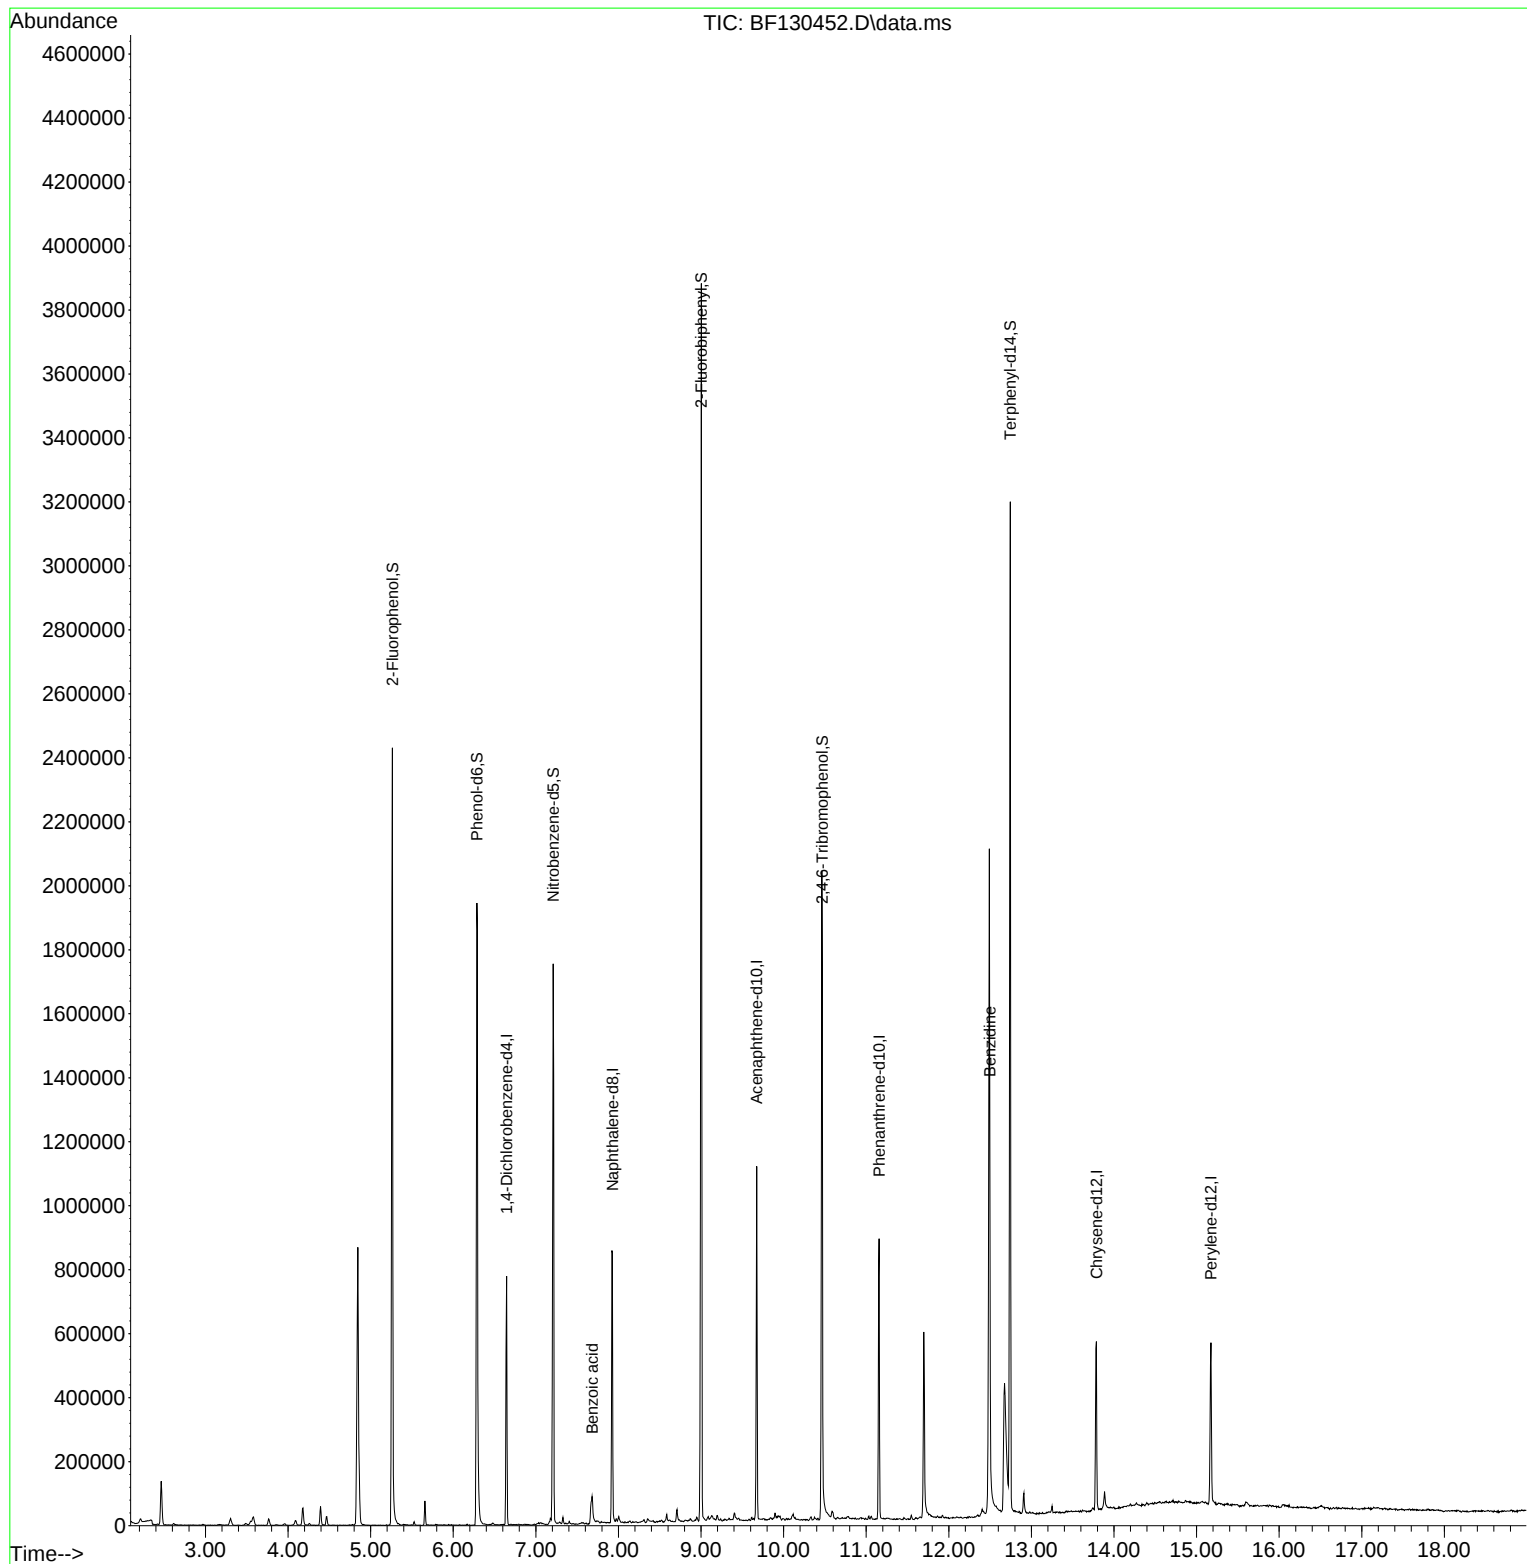




#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.645 min Scan# 71
Delta R.T. 0.000 min
Lab File: BF130452.D
Acq: 28 Sep 2022 17:25




Instrument :
BNA_F
ClientSampleId :
WC-14B-SP-2

Tgt Ion:152 Resp: 101213
Ion Ratio Lower Upper
152 100
150 155.1 122.8 184.2
115 62.2 53.8 80.8

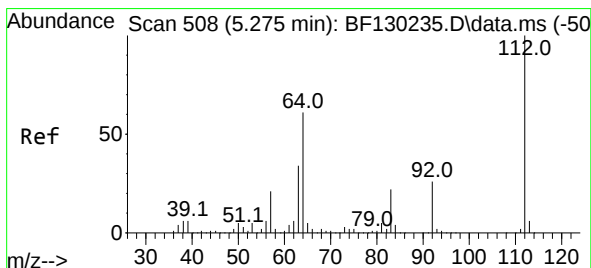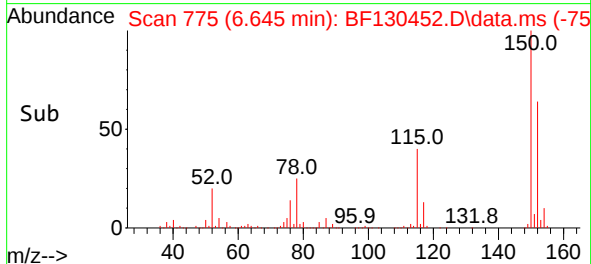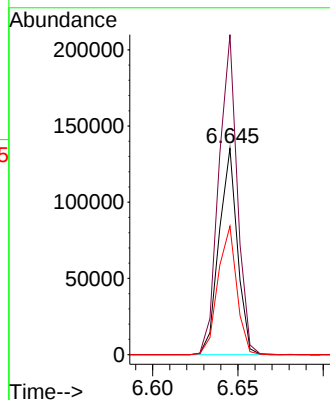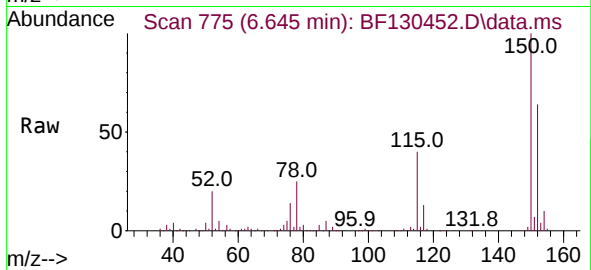

#5
2-Fluorophenol
Concen: 118.246 ng
RT: 5.263 min Scan# 540
Delta R.T. 0.018 min
Lab File: BF130452.D
Acq: 28 Sep 2022 17:25

Tgt Ion:112 Resp: 690015
Ion Ratio Lower Upper
112 100
64 55.3 51.4 77.0
63 29.8 28.8 43.2


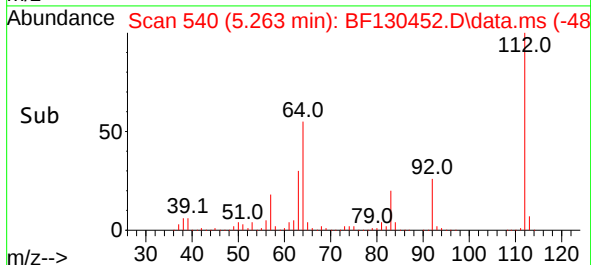
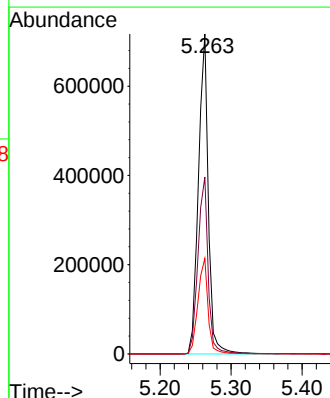
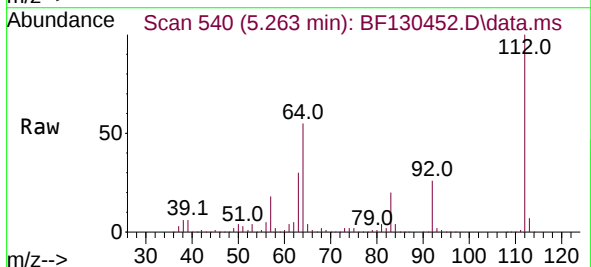




#7
Phenol-d6
Concen: 106.139 ng
RT: 6.287 min Scan# 71
Delta R.T. -0.006 min
Lab File: BF130452.D
Acq: 28 Sep 2022 17:25




Instrument :
BNA_F
ClientSampleId :
WC-14B-SP-2


Tgt Ion: 99 Resp: 774964
Ion Ratio Lower Upper
99 100
42 18.4 17.0 25.6
71 38.2 32.3 48.5

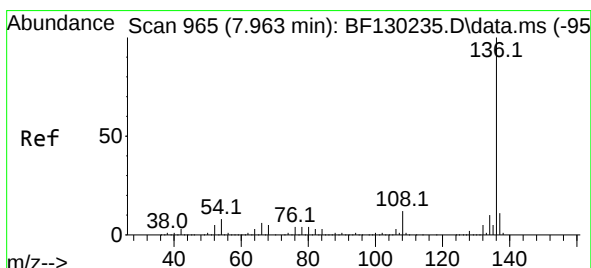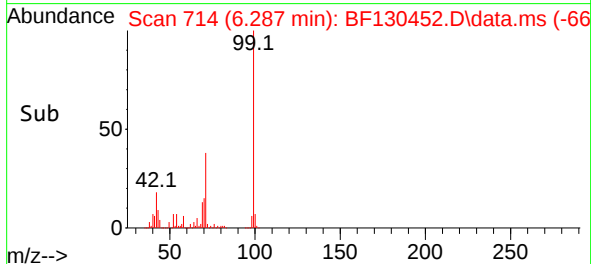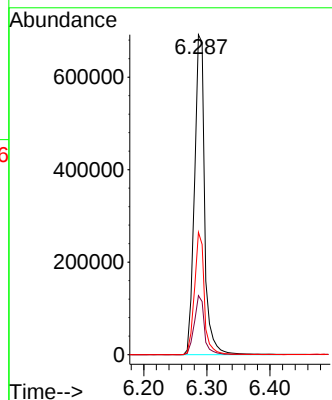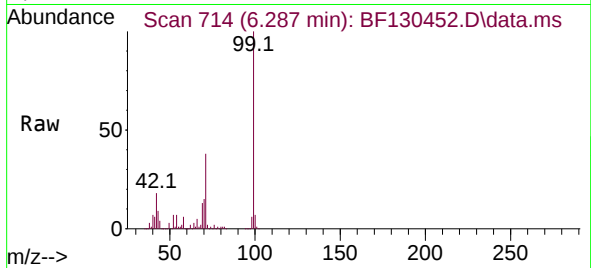

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 7.928 min Scan# 993
Delta R.T. -0.000 min
Lab File: BF130452.D
Acq: 28 Sep 2022 17:25

Tgt Ion: 136 Resp: 396942
Ion Ratio Lower Upper
136 100
137 10.5 9.1 13.7
54 6.2 7.1 10.7#
68 4.5 4.5 6.7

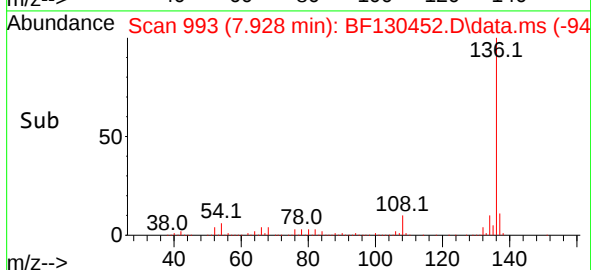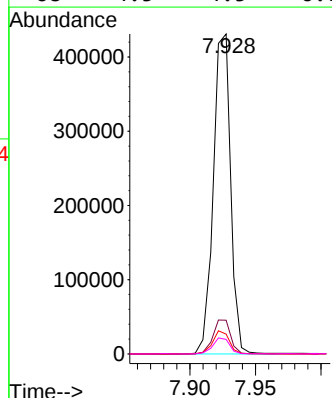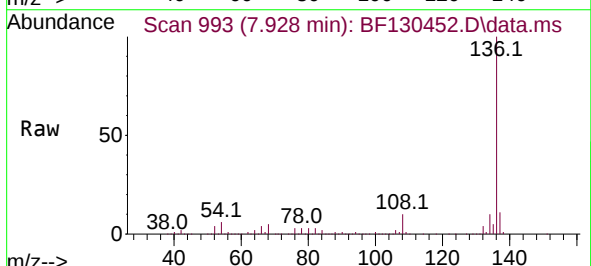

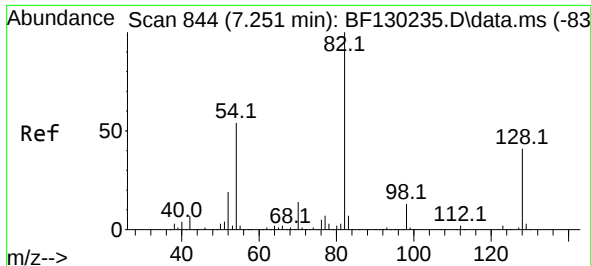

#23

Nitrobenzene-d5

Concen: 76.229 ng

RT: 7.210 min Scan# 81

Delta R.T. -0.006 min

Lab File: BF130452.D

Acq: 28 Sep 2022 17:25

Instrument :

BNA_F

ClientSampleId :

WC-14B-SP-2





Tgt Ion: 82 Resp: 592274

Ion Ratio Lower Upper

82 100

128 43.7 32.6 49.0

54 50.2 43.8 65.6

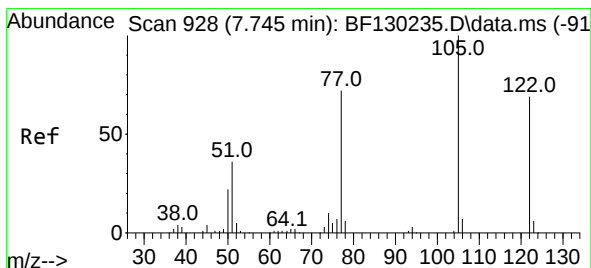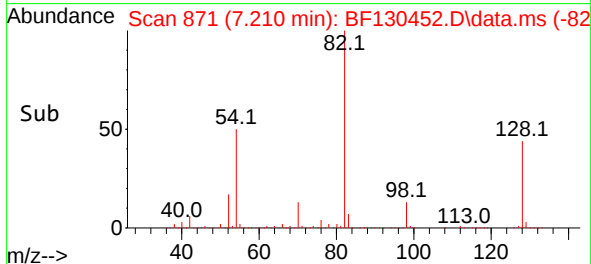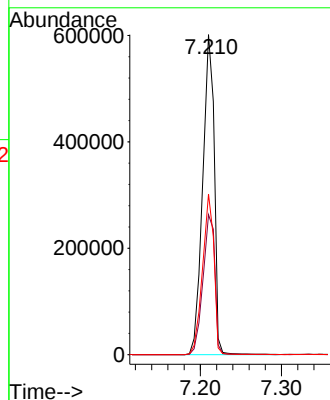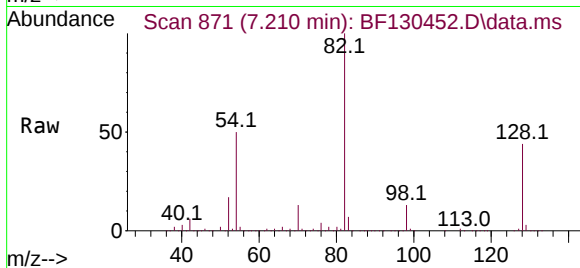

#32

Benzoic acid

Concen: 8.098 ng

RT: 7.681 min Scan# 951

Delta R.T. -0.053 min

Lab File: BF130452.D

Acq: 28 Sep 2022 17:25




Tgt Ion: 122 Resp: 31183


Ion Ratio Lower Upper

122 100

105 127.5 112.9 152.9

77 92.2 82.8 122.8


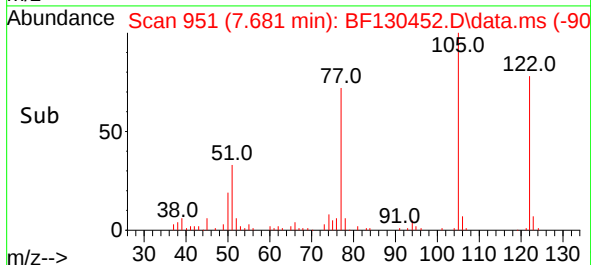
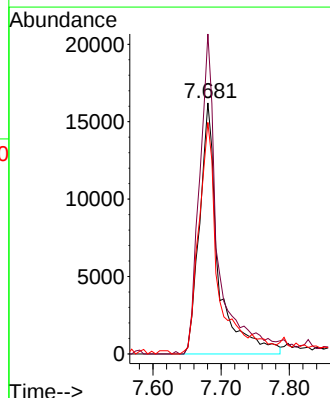
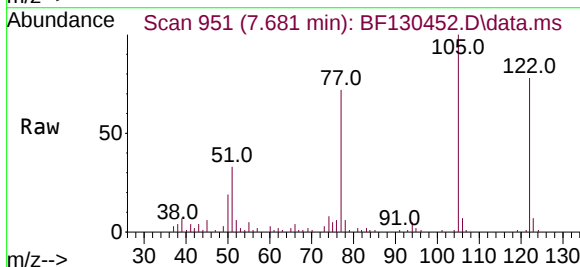


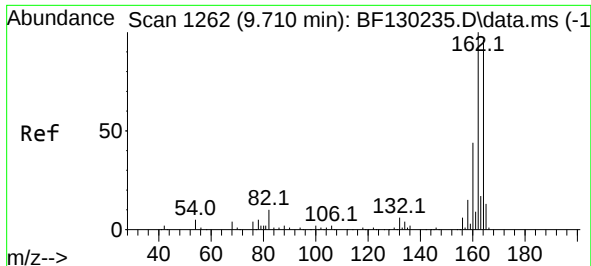

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 9.675 min Scan# 11
Delta R.T. -0.006 min
Lab File: BF130452.D
Acq: 28 Sep 2022 17:25




Instrument :
BNA_F
ClientSampleId :
WC-14B-SP-2


Tgt Ion:164 Resp: 200862
Ion Ratio Lower Upper
164 100
162 103.5 81.4 122.0
160 43.5 36.2 54.4

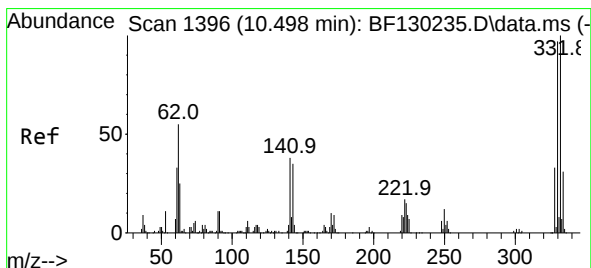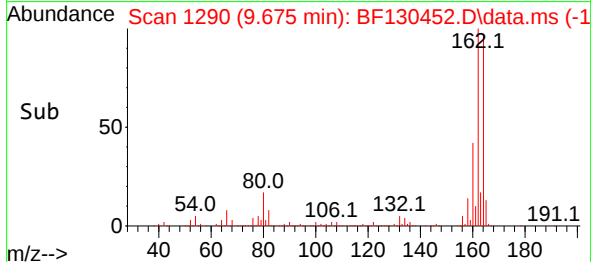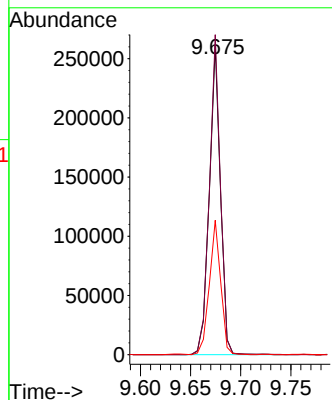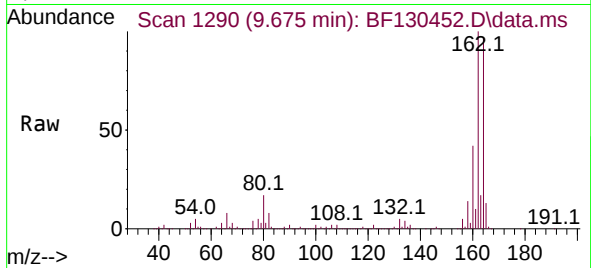

#42
2,4,6-Tribromophenol
Concen: 144.715 ng
RT: 10.469 min Scan# 1425
Delta R.T. -0.000 min
Lab File: BF130452.D
Acq: 28 Sep 2022 17:25

Tgt Ion:330 Resp: 278525
Ion Ratio Lower Upper
330 100
332 101.7 83.4 125.2
141 34.4 34.0 51.0

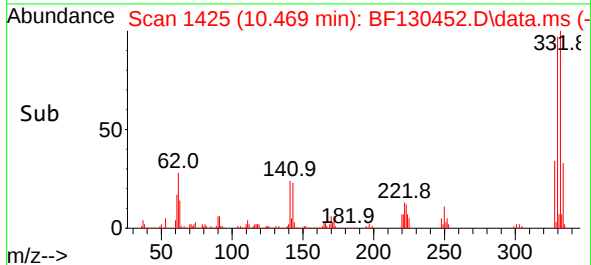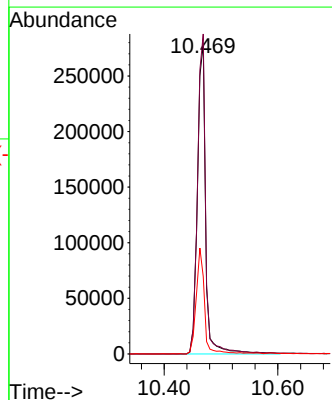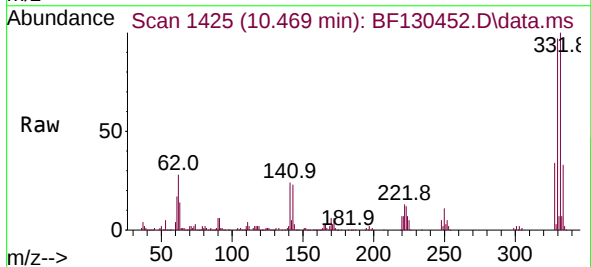

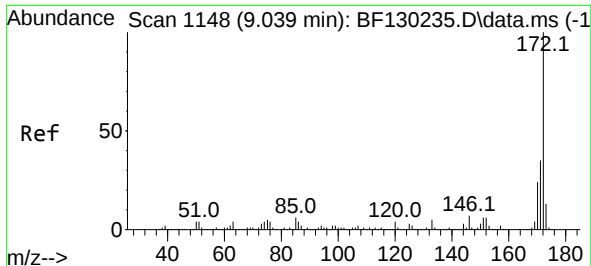

#45

2-Fluorobiphenyl

Concen: 82.438 ng

RT: 9.004 min Scan# 1176

Delta R.T. -0.006 min

Lab File: BF130452.D

Acq: 28 Sep 2022 17:25

Instrument :

BNA_F

ClientSampleId :

WC-14B-SP-2





Tgt Ion:172 Resp: 1137117

Ion Ratio Lower Upper

172 100

171 34.7 28.3 42.5

170 23.0 18.7 28.1

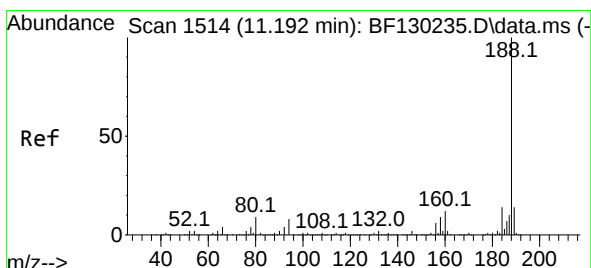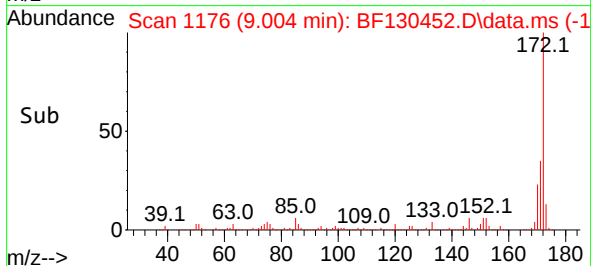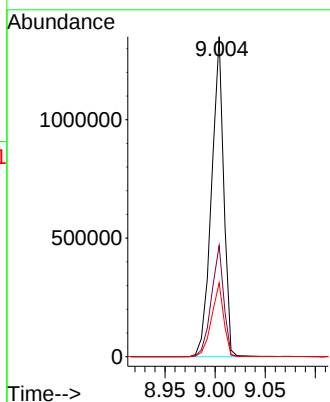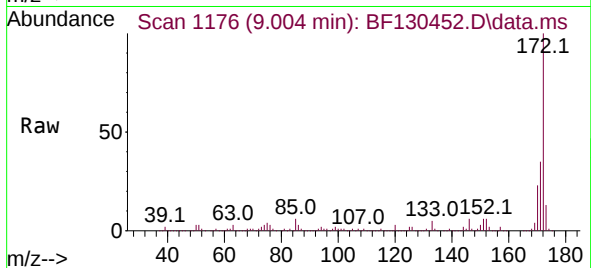

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 11.157 min Scan# 1542

Delta R.T. -0.000 min

Lab File: BF130452.D

Acq: 28 Sep 2022 17:25




Tgt Ion:188 Resp: 311830


Ion Ratio Lower Upper

188 100

94 7.3 7.4 11.2#

80 8.2 7.9 11.9


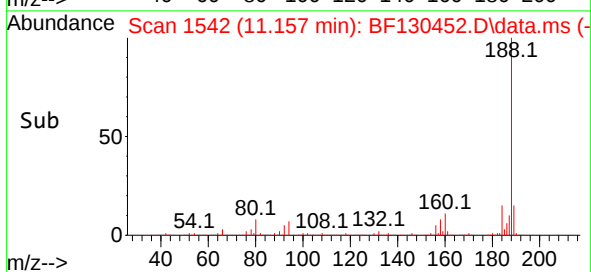
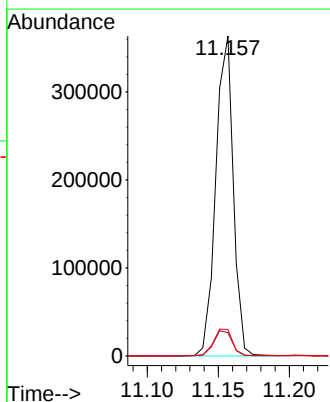
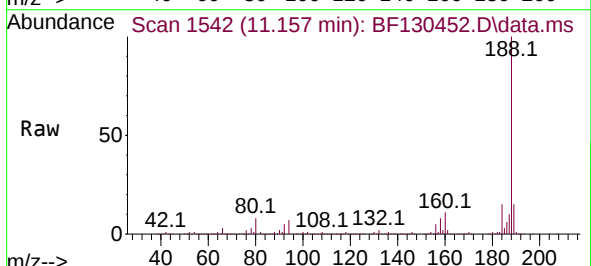


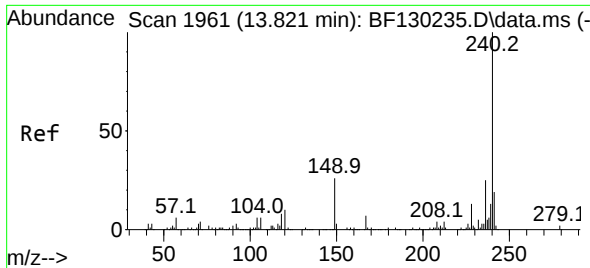

#76
Chrysene-d12
Concen: 20.000 ng
RT: 13.786 min Scan# 1961
Delta R.T. -0.006 min
Lab File: BF130452.D
Acq: 28 Sep 2022 17:25




Instrument :
BNA_F
ClientSampleId :
WC-14B-SP-2


Tgt Ion:240 Resp: 183136
Ion Ratio Lower Upper
240 100
120 8.7 8.7 13.1#
236 25.1 20.9 31.3

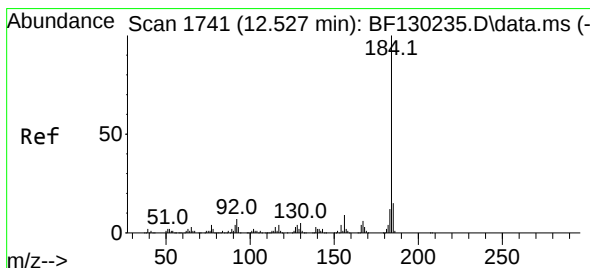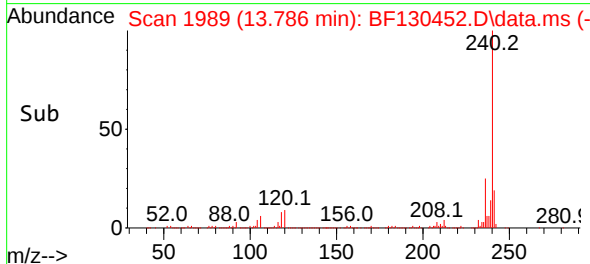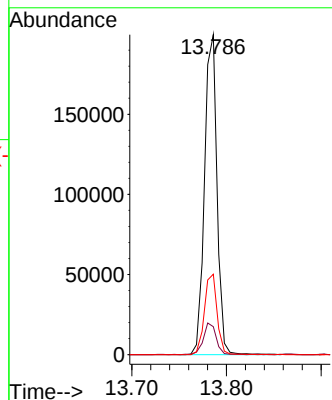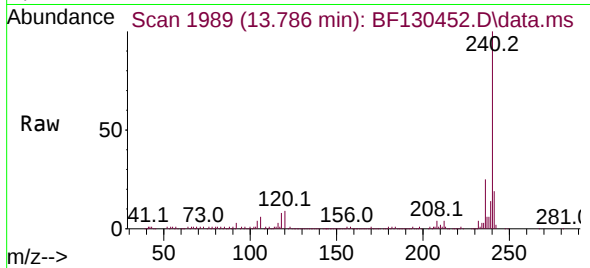

#77
Benzidine
Concen: 53.586 ng
RT: 12.498 min Scan# 1770
Delta R.T. -0.000 min
Lab File: BF130452.D
Acq: 28 Sep 2022 17:25

Tgt Ion:184 Resp: 284877
Ion Ratio Lower Upper
184 100
185 17.7 11.8 17.6#
183 11.3 9.1 13.7


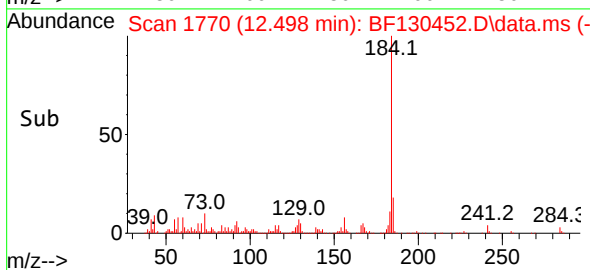
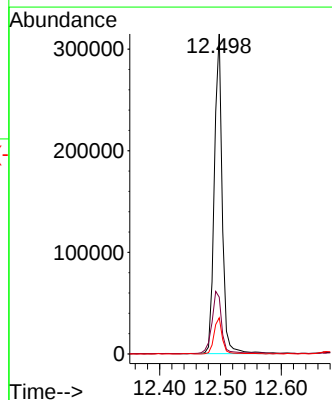
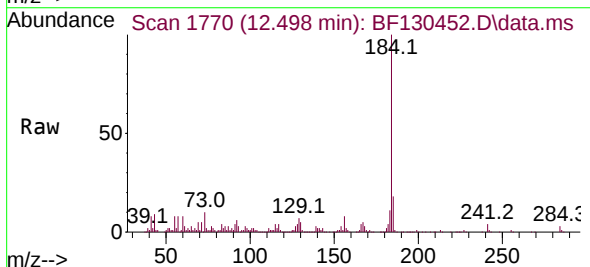


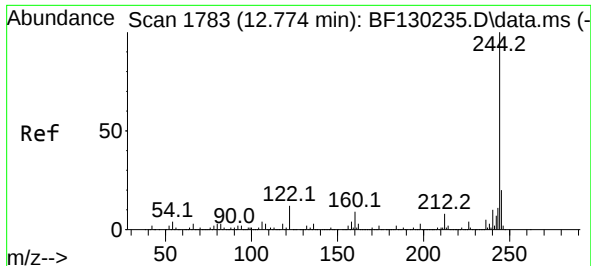

#79
 Terphenyl-d14
 Concen: 92.096 ng
 RT: 12.745 min Scan# 1812
 Delta R.T. -0.000 min
 Lab File: BF130452.D
 Acq: 28 Sep 2022 17:25

Instrument :
 BNA_F
 ClientSampleId :
 WC-14B-SP-2

Tgt Ion:244 Resp: 1018181
 Ion Ratio Lower Upper
 244 100
 212 6.9 5.9 8.9
 122 9.2 8.5 12.7

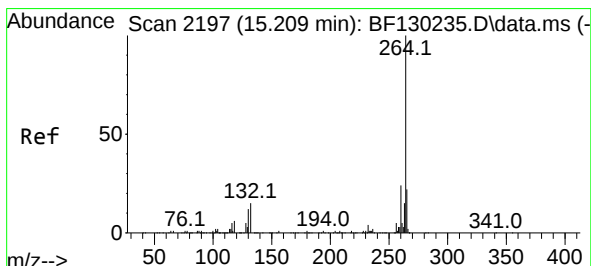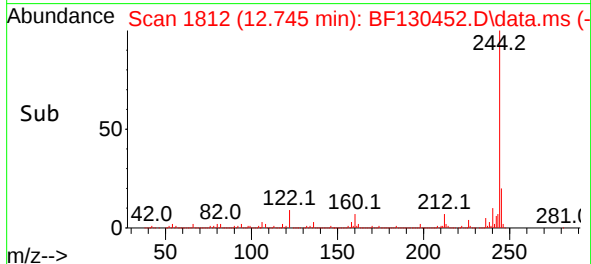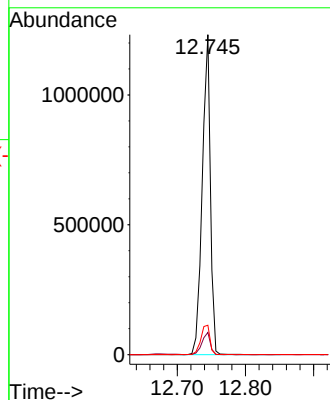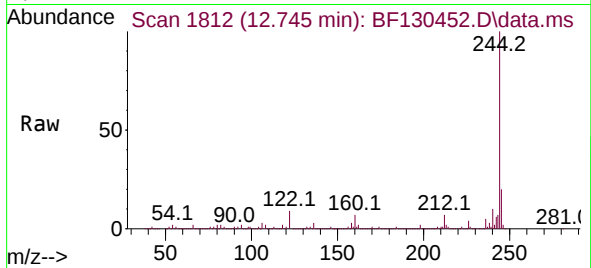

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.174 min Scan# 2225
 Delta R.T. -0.000 min
 Lab File: BF130452.D
 Acq: 28 Sep 2022 17:25

Tgt Ion:264 Resp: 210645
 Ion Ratio Lower Upper
 264 100
 260 23.4 19.3 28.9
 265 21.3 17.0 25.4

