

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092822\
 Data File : BF130443.D
 Acq On : 28 Sep 2022 12:10
 Operator : CG\JU
 Sample : PB147926BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB147926BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF130443.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.857	467	471	479	rBV	36873	49105	1.31%	0.221%
2	5.257	534	539	542	rBV	2901139	2895290	77.00%	13.012%
3	6.287	709	714	717	rBV	2658946	2878872	76.56%	12.938%
4	6.639	771	774	778	rBV	835447	725384	19.29%	3.260%
5	7.210	865	871	874	rBV	1833926	1931180	51.36%	8.679%
6	7.928	987	993	996	rBV	966813	962646	25.60%	4.326%
7	9.004	1170	1176	1179	rBV	4121530	3760358	100.00%	16.900%
8	9.675	1284	1290	1294	rBV	1289654	1087716	28.93%	4.888%
9	10.463	1418	1424	1428	rBV	2384398	2236528	59.48%	10.051%
10	11.157	1538	1542	1545	rBV	1261396	1016817	27.04%	4.570%
11	12.745	1807	1812	1815	rBV	3984733	3415740	90.84%	15.351%
12	13.786	1985	1989	1997	rBV	854182	734714	19.54%	3.302%
13	15.174	2220	2225	2229	rBV	488528	556534	14.80%	2.501%




Sum of corrected areas: 22250884

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092822\
Data File : BF130443.D
Acq On : 28 Sep 2022 12:10
Operator : CG\JU
Sample : PB147926BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB147926BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

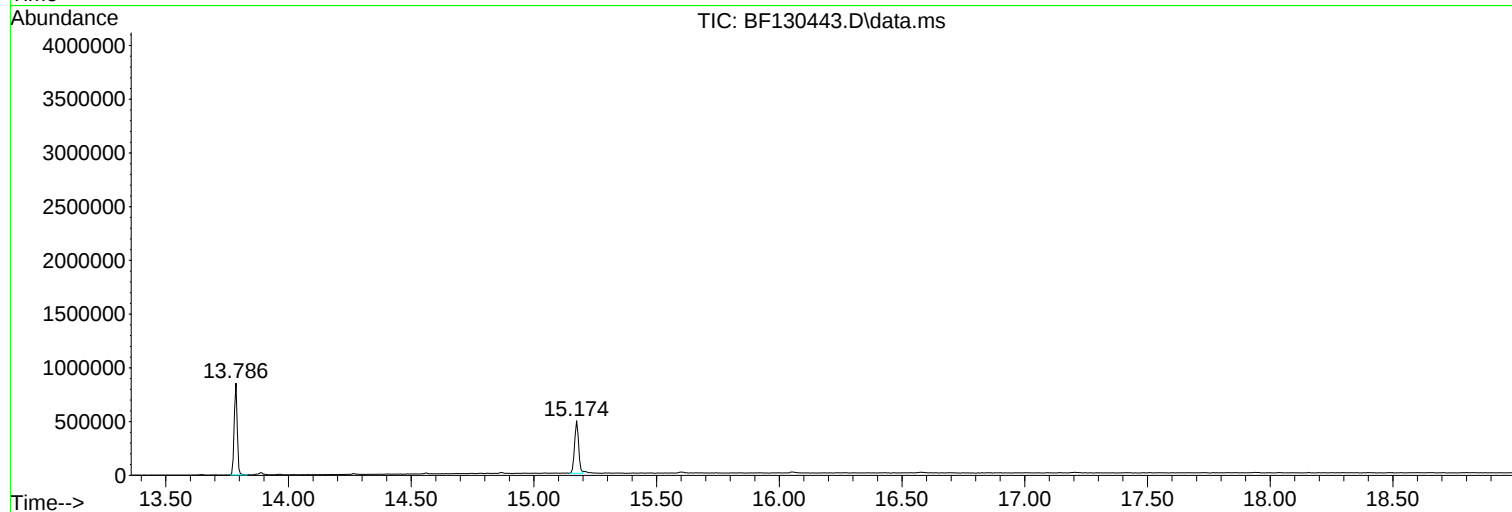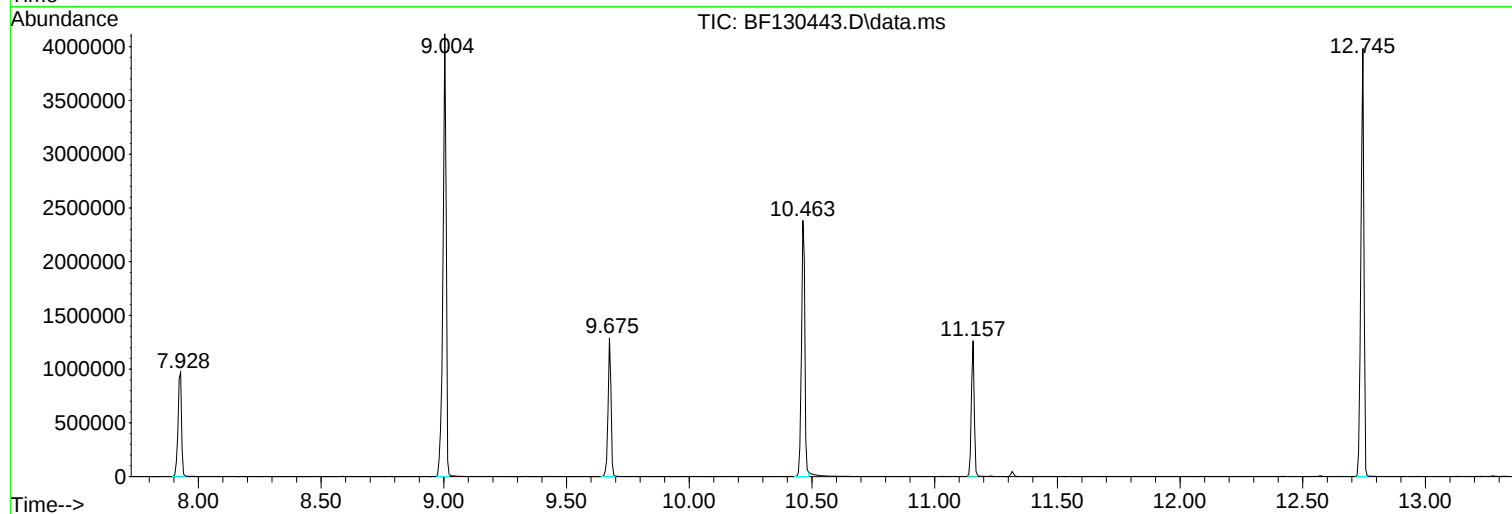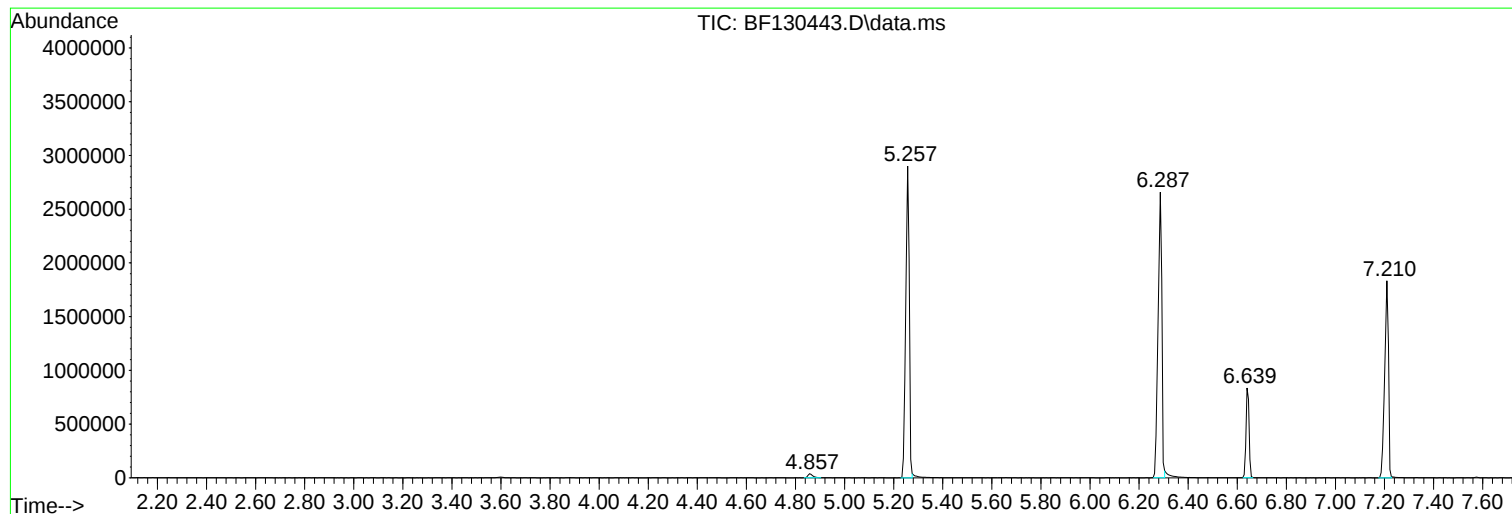

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092822\
Data File : BF130443.D
Acq On : 28 Sep 2022 12:10
Operator : CG\JU
Sample : PB147926BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB147926BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092822\
Data File : BF130443.D
Acq On : 28 Sep 2022 12:10
Operator : CG\JU
Sample : PB147926BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB147926BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------