

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092822\
 Data File : BF130459.D
 Acq On : 28 Sep 2022 21:33
 Operator : CG\JU
 Sample : N4826-01 5X
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 OK-03-092622

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF130459.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.534	241	246	252	rVB	5412	8811	1.38%	0.137%
2	4.816	461	464	468	rBV	25218	28666	4.51%	0.446%
3	5.246	534	537	551	rBV	324135	327818	51.53%	5.096%
4	6.287	710	714	730	rBV	300630	336574	52.90%	5.232%
5	6.646	772	775	779	rBV	636252	503707	79.17%	7.831%
6	7.210	867	871	881	rBV	220754	183031	28.77%	2.845%
7	7.928	989	993	999	rBV	723396	594283	93.41%	9.239%
8	8.016	1006	1008	1016	rVB7	6033	8456	1.33%	0.131%
9	8.739	1128	1131	1135	rVB2	8719	10573	1.66%	0.164%
10	9.004	1172	1176	1179	rBV	409797	311405	48.95%	4.841%
11	9.087	1185	1190	1193	rBV2	11844	13074	2.06%	0.203%
12	9.404	1242	1244	1247	rBV4	12569	11718	1.84%	0.182%
13	9.463	1251	1254	1257	rVB4	7936	10690	1.68%	0.166%
14	9.539	1263	1267	1273	rBV	47179	43810	6.89%	0.681%
15	9.616	1278	1280	1283	rBV	14623	11984	1.88%	0.186%
16	9.681	1287	1291	1294	rBV	717333	599967	94.30%	9.327%
17	9.787	1306	1309	1314	rVB7	6267	9967	1.57%	0.155%
18	9.839	1314	1318	1321	rBV6	5531	10392	1.63%	0.162%
19	9.881	1321	1325	1330	rVB8	6660	15481	2.43%	0.241%
20	9.992	1341	1344	1351	rVB7	9131	16007	2.52%	0.249%
21	10.110	1362	1364	1367	rBV2	15095	17356	2.73%	0.270%
22	10.222	1380	1383	1390	rVB5	12299	20617	3.24%	0.321%
23	10.334	1400	1402	1405	rVB3	12186	10379	1.63%	0.161%
24	10.463	1419	1424	1429	rBV	255428	232633	36.57%	3.617%
25	10.586	1442	1445	1449	rBV2	29436	39547	6.22%	0.615%
26	10.669	1456	1459	1461	rBV	20135	25016	3.93%	0.389%
27	10.698	1462	1464	1467	rVV3	16992	21187	3.33%	0.329%
28	10.728	1467	1469	1473	rVV4	9048	14464	2.27%	0.225%
29	10.798	1479	1481	1486	rVB6	8824	8927	1.40%	0.139%
30	10.845	1486	1489	1492	rVB5	12103	13997	2.20%	0.218%
31	10.886	1493	1496	1497	rBV	11071	10937	1.72%	0.170%
32	10.969	1508	1510	1514	rVB5	9660	9618	1.51%	0.150%
33	11.033	1519	1521	1523	rVV2	31572	25561	4.02%	0.397%
34	11.063	1523	1526	1529	rVB4	15145	18982	2.98%	0.295%
35	11.116	1532	1535	1539	rVV	18840	17038	2.68%	0.265%
36	11.157	1539	1542	1545	rVV	703152	636202	100.00%	9.890%

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092822\
 Data File : BF130459.D
 Acq On : 28 Sep 2022 21:33
 Operator : CG\JU
 Sample : N4826-01 5X
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 OK-03-092622

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	11.181	1545	1546	1551	rVV	86819	64752	10.18%	1.007%
38	11.233	1552	1555	1559	rVB	21763	20191	3.17%	0.314%
39	11.269	1559	1561	1565	rBV4	17217	17506	2.75%	0.272%
40	11.392	1579	1582	1587	rBV6	9560	15586	2.45%	0.242%
41	11.457	1591	1593	1596	rBV	25151	20224	3.18%	0.314%
42	11.557	1607	1610	1616	rVB6	10304	15334	2.41%	0.238%
43	11.663	1625	1628	1630	rBV	26824	23513	3.70%	0.366%
44	11.686	1630	1632	1636	rVV2	37384	37628	5.91%	0.585%
45	11.769	1643	1646	1648	rBV	43124	38728	6.09%	0.602%
46	11.792	1648	1650	1654	rVB	25813	21372	3.36%	0.332%
47	11.869	1660	1663	1665	rVB	28686	26132	4.11%	0.406%
48	11.892	1665	1667	1671	rBV5	8786	9329	1.47%	0.145%
49	11.957	1676	1678	1680	rVV2	15220	14337	2.25%	0.223%
50	11.980	1680	1682	1685	rVB4	15485	16645	2.62%	0.259%
51	12.104	1701	1703	1706	rVB3	17276	15855	2.49%	0.246%
52	12.133	1706	1708	1710	rBV2	17377	16853	2.65%	0.262%
53	12.210	1718	1721	1723	rBV	43365	40873	6.42%	0.635%
54	12.251	1724	1728	1733	rVB5	37566	62258	9.79%	0.968%
55	12.292	1733	1735	1739	rBV4	19820	25191	3.96%	0.392%
56	12.369	1745	1748	1751	rVB	117465	95537	15.02%	1.485%
57	12.463	1761	1764	1767	rBV2	25080	31705	4.98%	0.493%
58	12.592	1781	1786	1789	rBV	127722	139532	21.93%	2.169%
59	12.622	1789	1791	1794	rVB3	36766	38792	6.10%	0.603%
60	12.739	1808	1811	1819	rVB	390035	373354	58.68%	5.804%
61	13.027	1858	1860	1863	rBV2	24380	15951	2.51%	0.248%
62	13.322	1908	1910	1913	rBV3	31209	27014	4.25%	0.420%
63	13.792	1986	1990	1993	rBV	644794	592290	93.10%	9.208%
64	13.892	2005	2007	2011	rVB	63374	51340	8.07%	0.798%
65	15.186	2223	2227	2231	rBV	322254	385764	60.64%	5.997%




Sum of corrected areas: 6432461

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092822\
Data File : BF130459.D
Acq On : 28 Sep 2022 21:33
Operator : CG\JU
Sample : N4826-01 5X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OK-03-092622

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

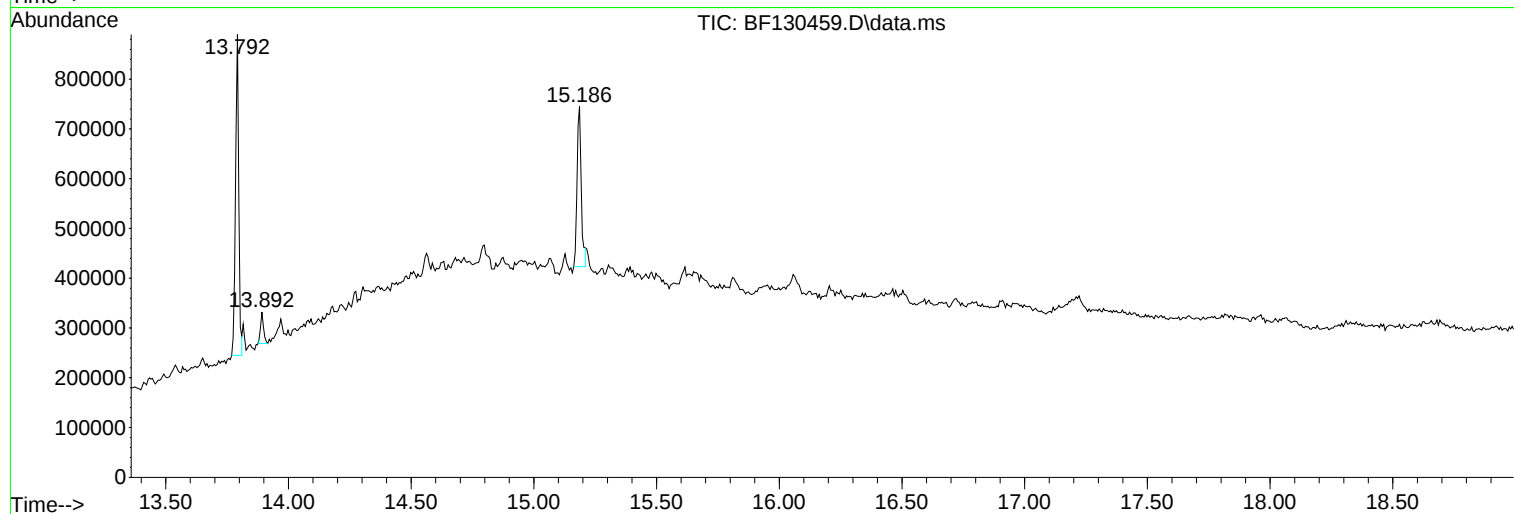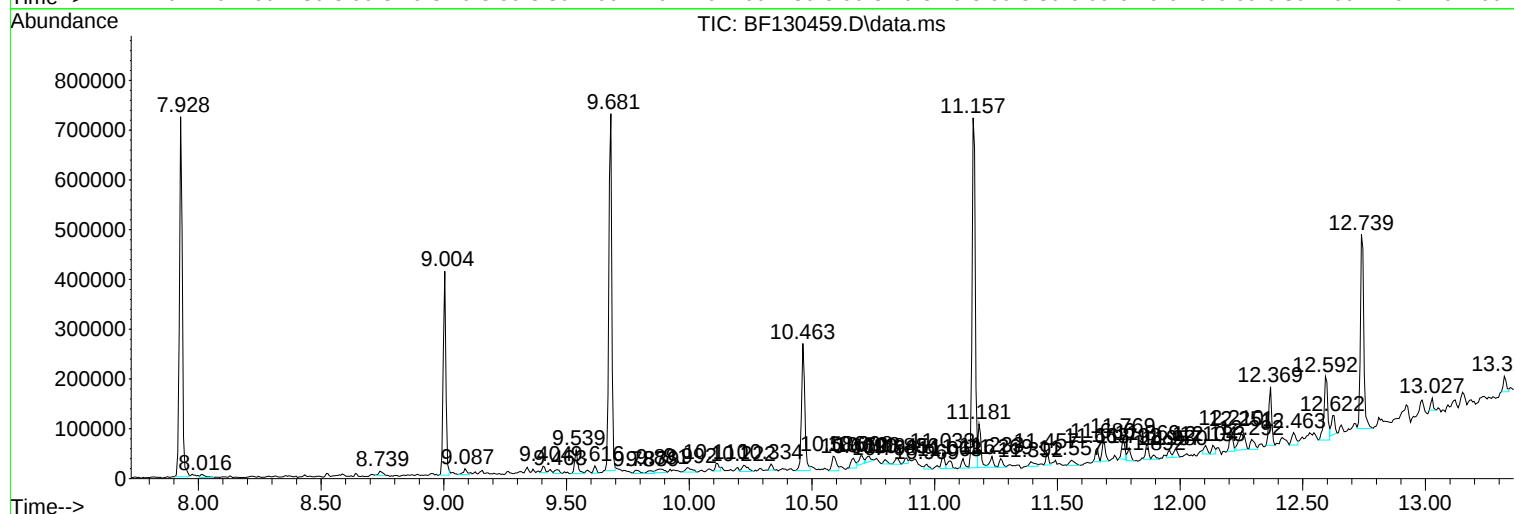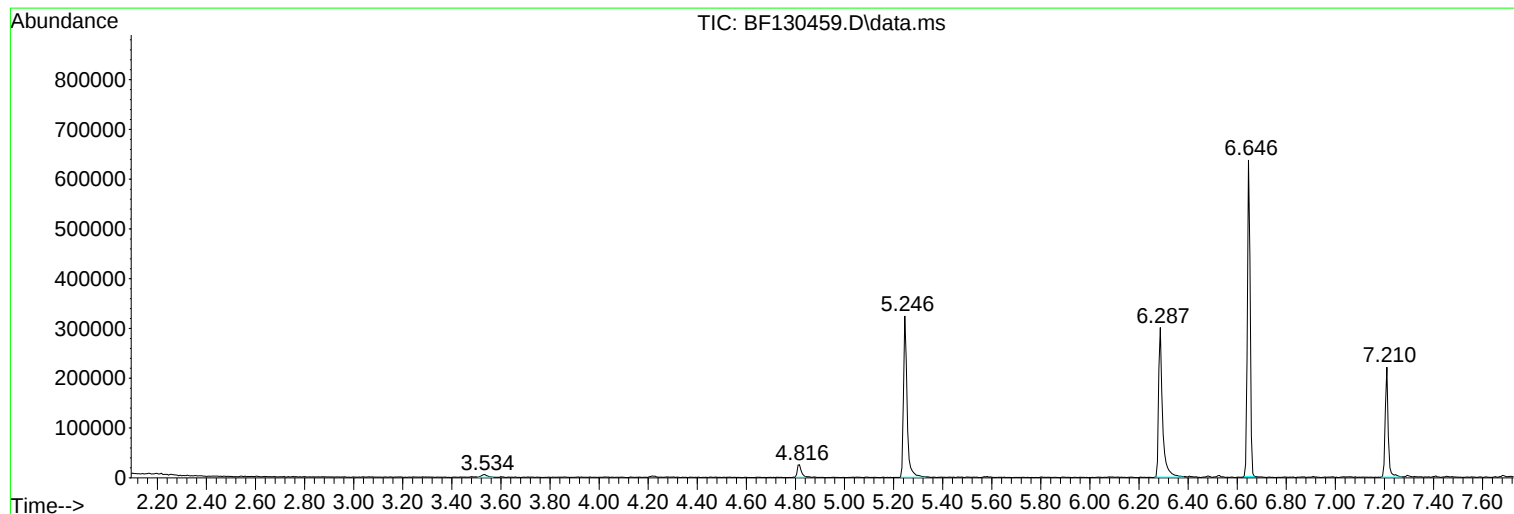

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092822\
Data File : BF130459.D
Acq On : 28 Sep 2022 21:33
Operator : CG\JU
Sample : N4826-01 5X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OK-03-092622

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092822\
Data File : BF130459.D
Acq On : 28 Sep 2022 21:33
Operator : CG\JU
Sample : N4826-01 5X
Misc :
ALS Vial : 20 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OK-03-092622

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------