
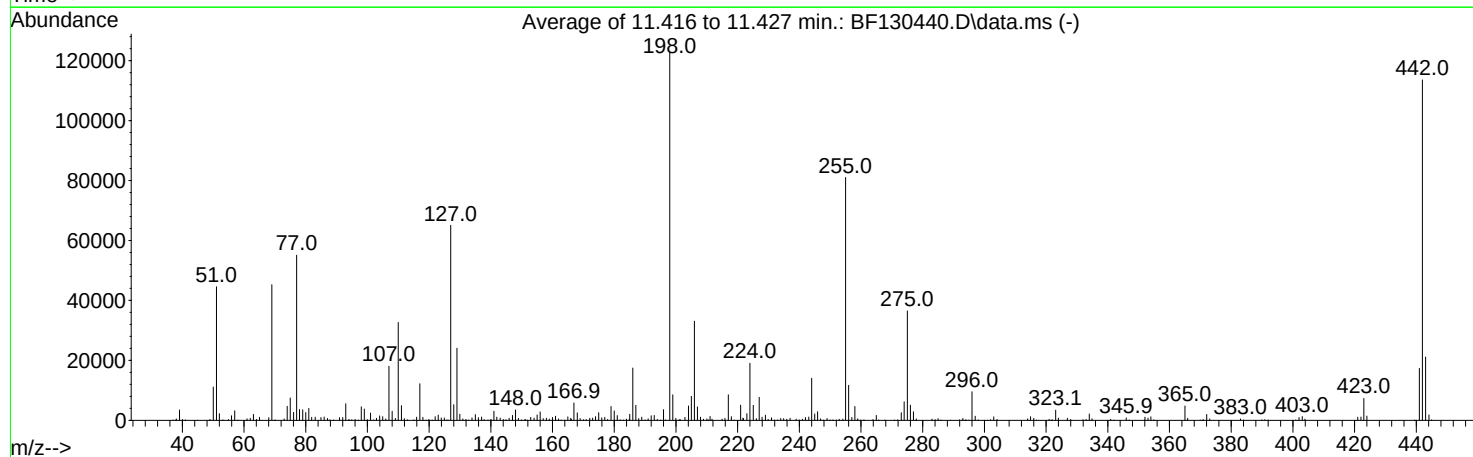


Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF092822\  
 Data File : BF130440.D  
 Acq On : 28 Sep 2022 10:04  
 Operator : CG\JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF091422.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Wed Sep 28 02:59:31 2022

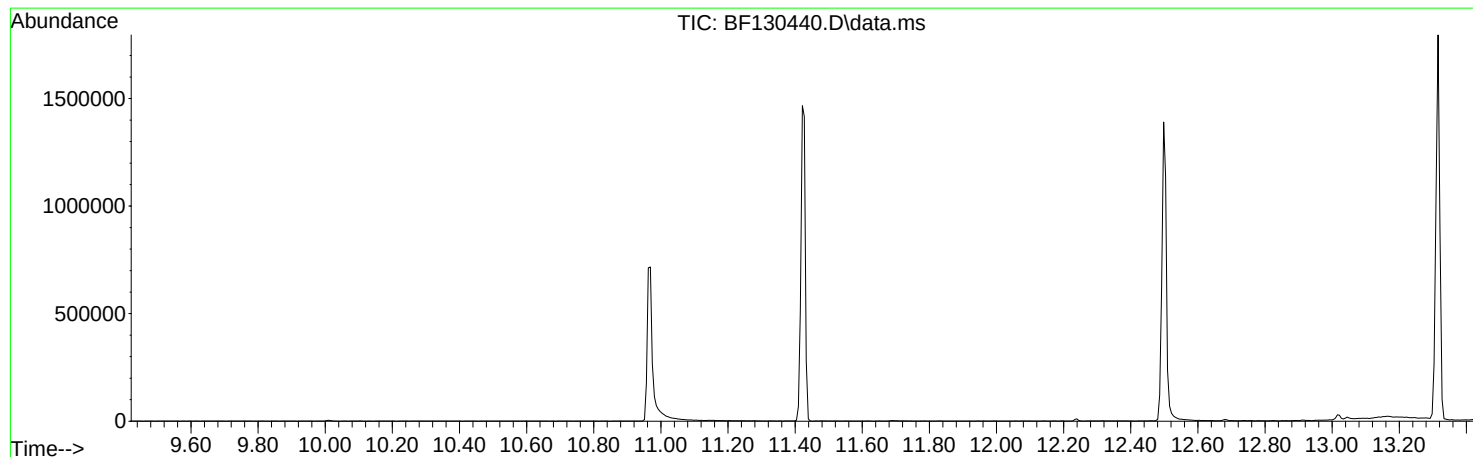




AutoFind: Scans 1586, 1587, 1588; Background Corrected with Scan 1581

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 51             | 198             | 10              | 80              | 36.3         | 44555      | PASS                |
| 68             | 69              | 0.00            | 2               | 1.9          | 869        | PASS                |
| 69             | 198             | 0.00            | 100             | 36.9         | 45240      | PASS                |
| 70             | 69              | 0.00            | 2               | 0.2          | 81         | PASS                |
| 127            | 198             | 10              | 80              | 53.0         | 65077      | PASS                |
| 197            | 198             | 0.00            | 2               | 0.1          | 116        | PASS                |
| 198            | 198             | 100             | 100             | 100.0        | 122749     | PASS                |
| 199            | 198             | 5               | 9               | 6.9          | 8518       | PASS                |
| 275            | 198             | 10              | 60              | 29.7         | 36476      | PASS                |
| 365            | 198             | 1               | 100             | 3.9          | 4764       | PASS                |
| 441            | 198             | 0.01            | 100             | 14.1         | 17308      | PASS                |
| 442            | 442             | 50              | 100             | 100.0        | 113565     | PASS                |
| 443            | 442             | 15              | 24              | 18.6         | 21105      | PASS                |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF092822\  
 Data File : BF130440.D  
 Acq On : 28 Sep 2022 10:04  
 Operator : CG\JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 DFTPP

Quant Time: Sep 29 05:26:36 2022  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF091422.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Wed Sep 28 02:59:31 2022  
 Response via : Initial Calibration

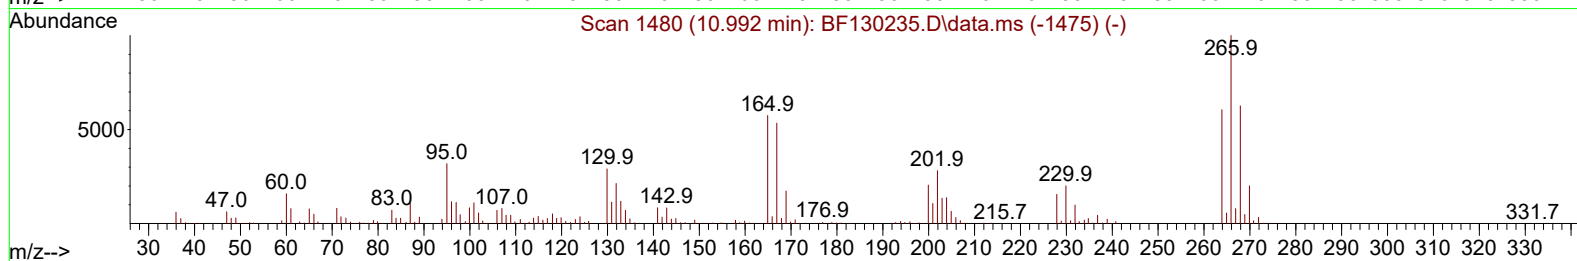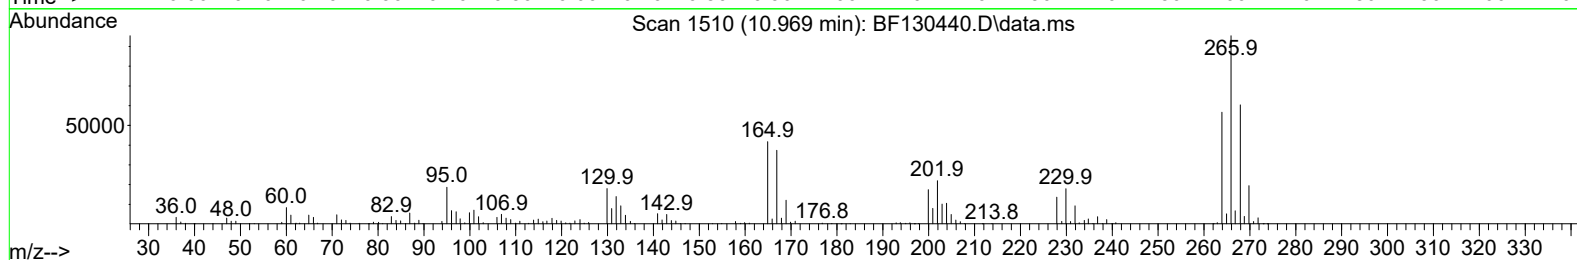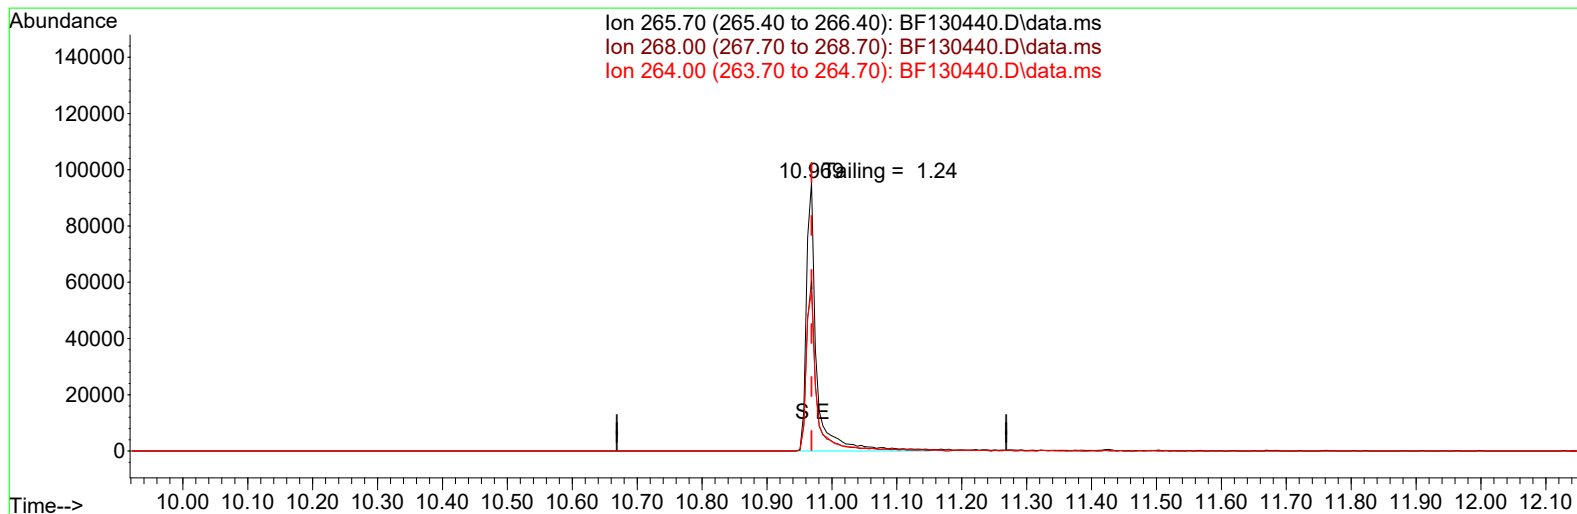

TIC: BF130440.D\data.ms

**(70) Pentachlorophenol (C)**

10.969min (-0.000) 26745.80 ng




response 105187

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 63.10  | 63.33  |
| 264.00 | 63.10  | 59.37  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF092822\  
Data File : BF130440.D  
Acq On : 28 Sep 2022 10:04  
Operator : CG\JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP

Quant Time: Sep 29 05:26:36 2022  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF091422.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Wed Sep 28 02:59:31 2022  
Response via : Initial Calibration

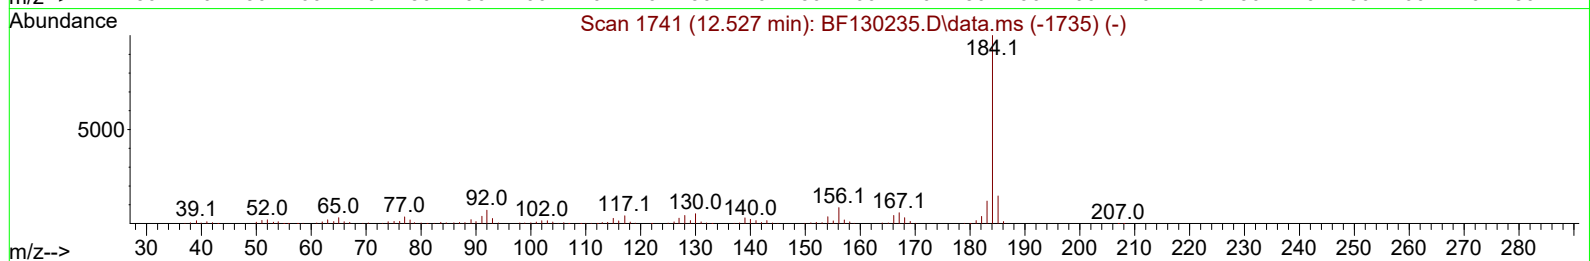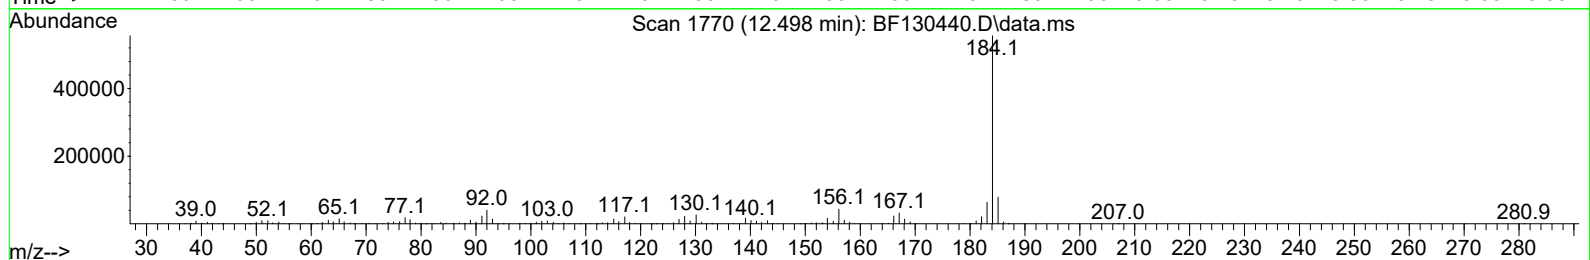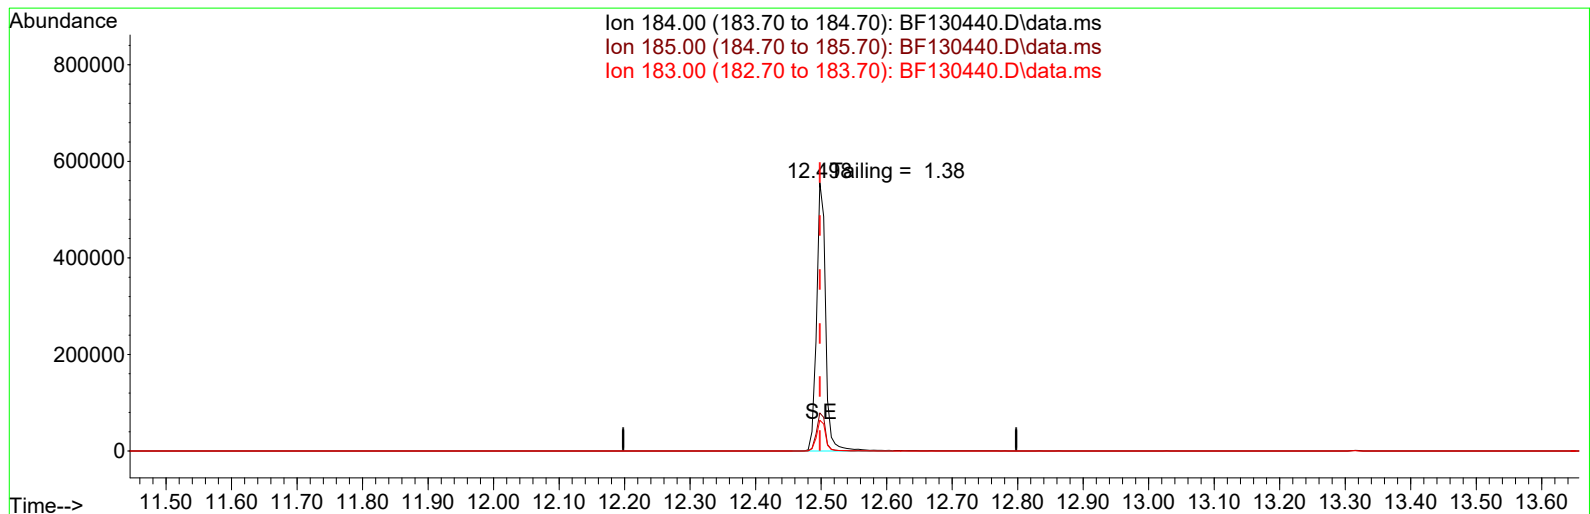

TIC: BF130440.D\data.ms

(77) Benzidine

12.498min (-0.000) 0.00 ng

response 534443

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 14.70  | 14.19  |
| 183.00 | 11.40  | 11.47  |
| 0.00   | 0.00   | 0.00   |

# DDT Breakdown

| Date          | Instrument Name  | DFTPP Data File    |
|---------------|------------------|--------------------|
| 9/28/2022     | BNA_F            | <u>BF130440.D</u>  |
|               |                  |                    |
|               |                  |                    |
| Compound Name | Response         | Retention Time     |
|               |                  |                    |
| DDT           | 280836           | 13.315             |
| DDD           | 6492             | 13.015             |
| DDE           | 906              | 12.68              |
|               |                  |                    |
|               |                  |                    |
| SUM(DDD+DDE)  | SUM(DDT+DDD+DDE) | % Breakdown Of DDT |
|               |                  |                    |
| 7398          | 288234           | 2.57               |
|               |                  |                    |

Instrument :  
BNA\_F  
ClientSampleId :  
DFTPP