
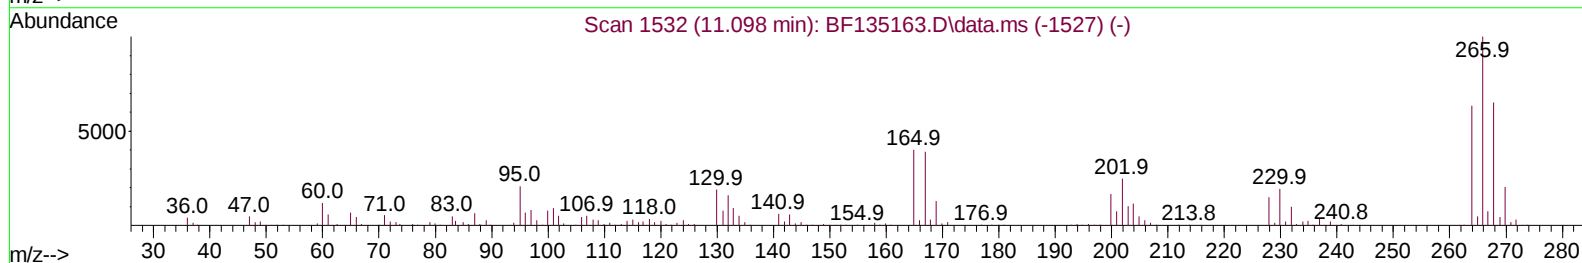
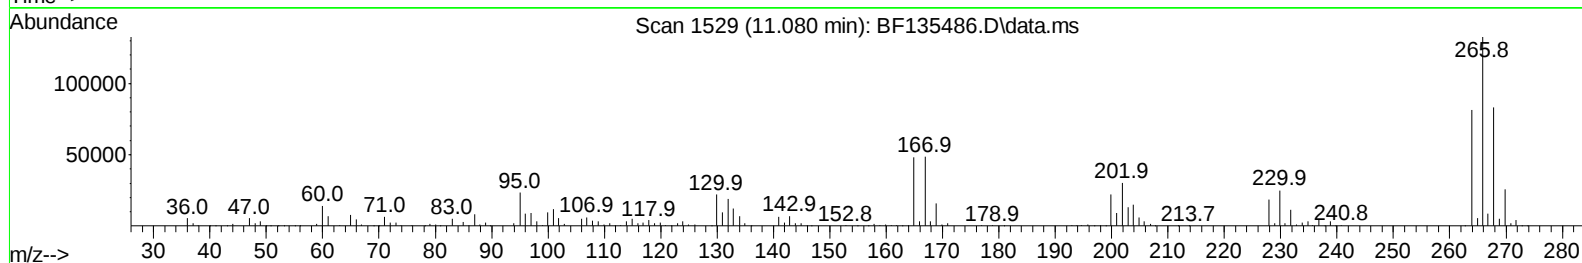


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092823\
Data File : BF135486.D
Acq On : 28 Sep 2023 11:25
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 29 02:01:13 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 28 19:03:19 2023
Response via : Initial Calibration

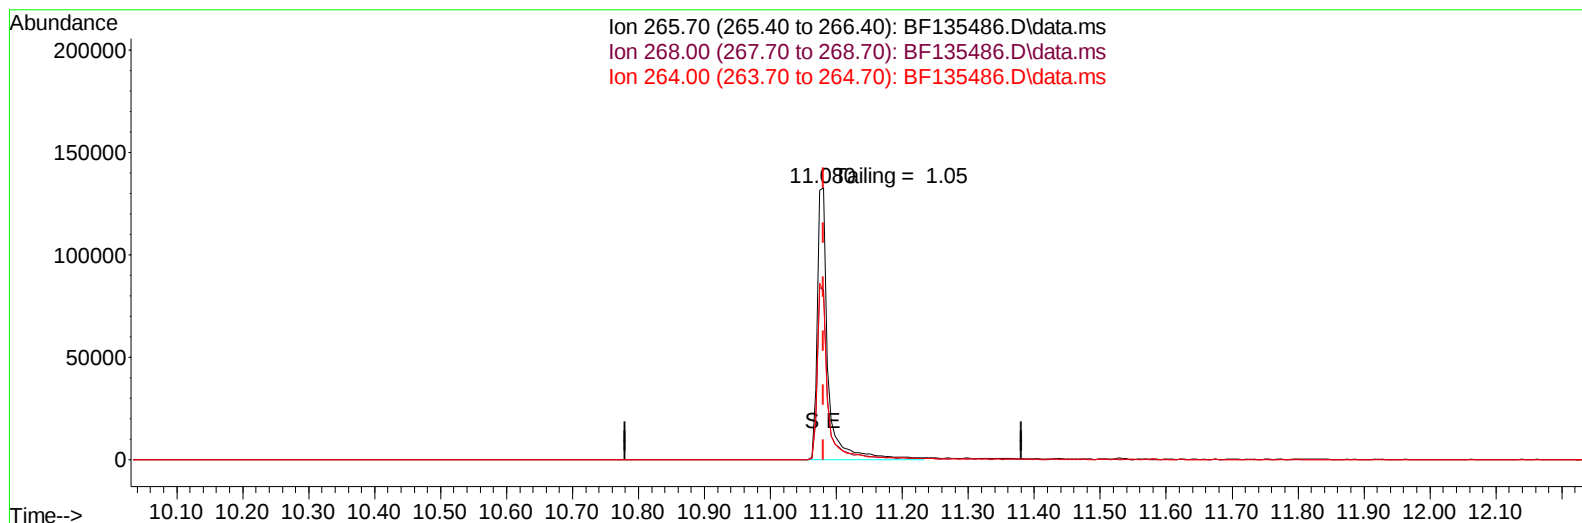




TIC: BF135486.D\data.ms

(70) Pentachlorophenol (C)**11.080min (-0.000) 30300.99 ng****response 152280**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.10	62.62
264.00	63.50	61.46
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092823\
Data File : BF135486.D
Acq On : 28 Sep 2023 11:25
Operator : CG\JU
Sample : DFTTP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 29 02:01:13 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 28 19:03:19 2023
Response via : Initial Calibration

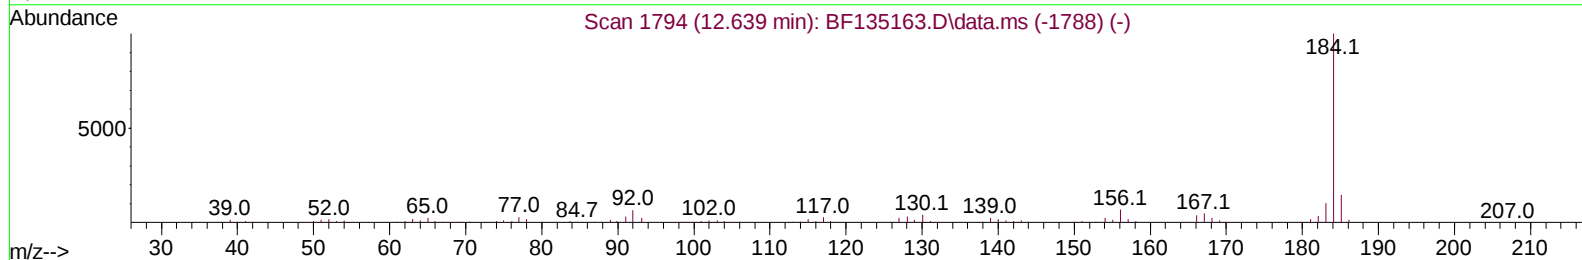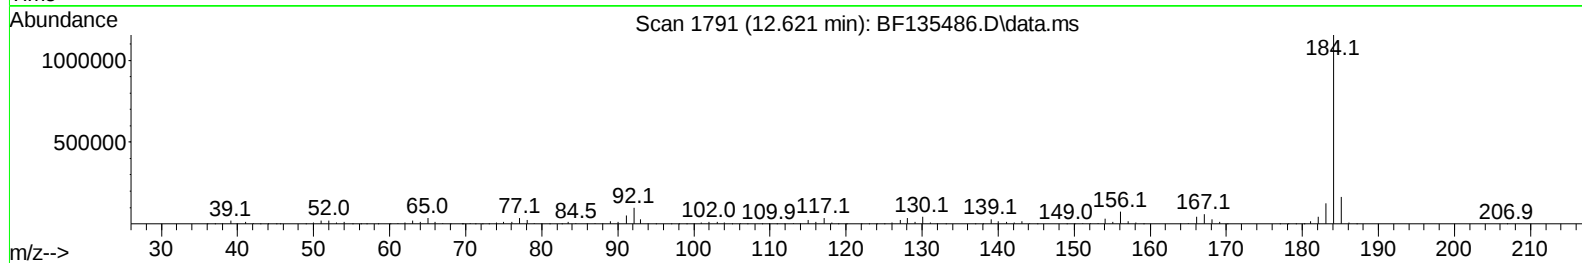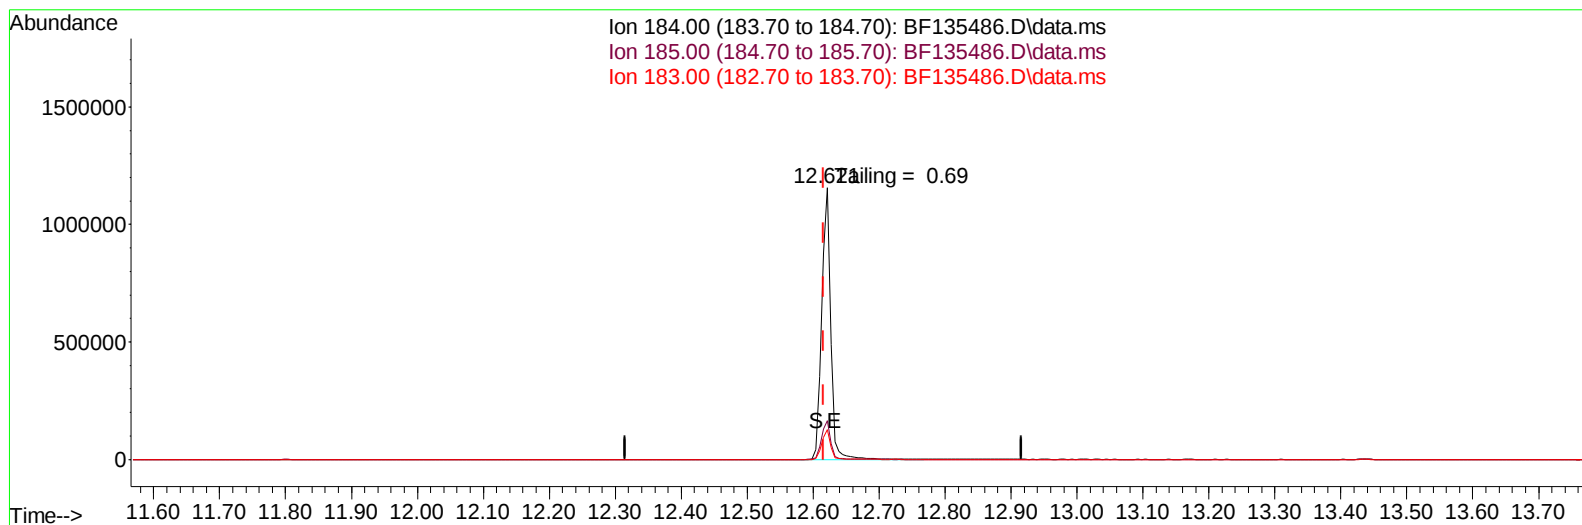

TIC: BF135486.D\data.ms

(77) Benzidine

12.621min (+ 0.006) 54084.06 ng

response 1108011

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.28
183.00	10.30	10.87
0.00	0.00	0.00