

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092823\
 Data File : BF135488.D
 Acq On : 28 Sep 2023 12:25
 Operator : CG\JU
 Sample : PB155836BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB155836BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF135488.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.387	556	561	581	rBV	4433227	4610761	96.46%	15.179%
2	6.393	727	732	735	rBV	4149784	4443491	92.96%	14.628%
3	6.745	788	792	799	rBV	965510	859817	17.99%	2.831%
4	7.310	883	888	891	rBV	2922071	3014266	63.06%	9.923%
5	8.022	1005	1009	1026	rBV	1252604	1125500	23.55%	3.705%
6	9.098	1187	1192	1196	rBV	4303357	4779849	100.00%	15.735%
7	9.775	1302	1307	1318	rBV	1325894	1209954	25.31%	3.983%
8	10.575	1438	1443	1446	rBV	2833297	2730097	57.12%	8.988%
9	11.269	1557	1561	1570	rBV	1444171	1269866	26.57%	4.180%
10	12.869	1828	1833	1836	rBV	4298311	4465777	93.43%	14.702%
11	13.921	2008	2012	2025	rBV	1003852	916535	19.17%	3.017%
12	14.086	2036	2040	2045	rBV	46063	47891	1.00%	0.158%
13	14.392	2088	2092	2096	rBV	56450	58922	1.23%	0.194%
14	14.698	2139	2144	2149	rBV	54816	61287	1.28%	0.202%
15	15.027	2195	2200	2203	rBV	42643	58926	1.23%	0.194%
16	15.380	2255	2260	2271	rBV	521444	723372	15.13%	2.381%




Sum of corrected areas: 30376311

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092823\
Data File : BF135488.D
Acq On : 28 Sep 2023 12:25
Operator : CG\JU
Sample : PB155836BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB155836BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

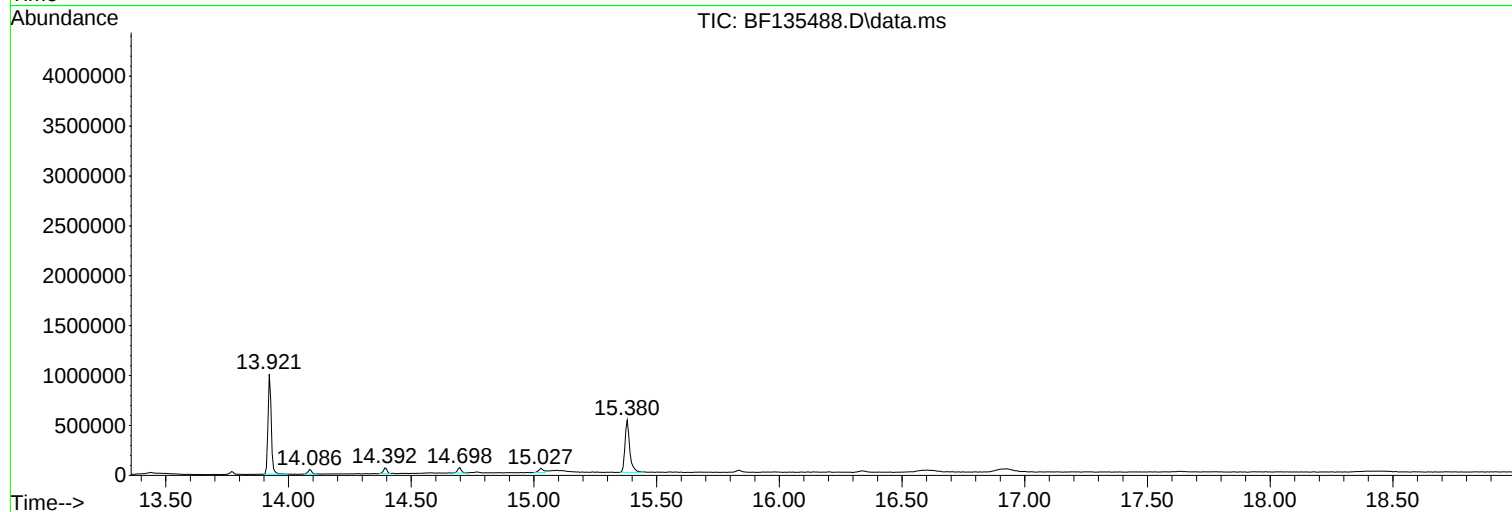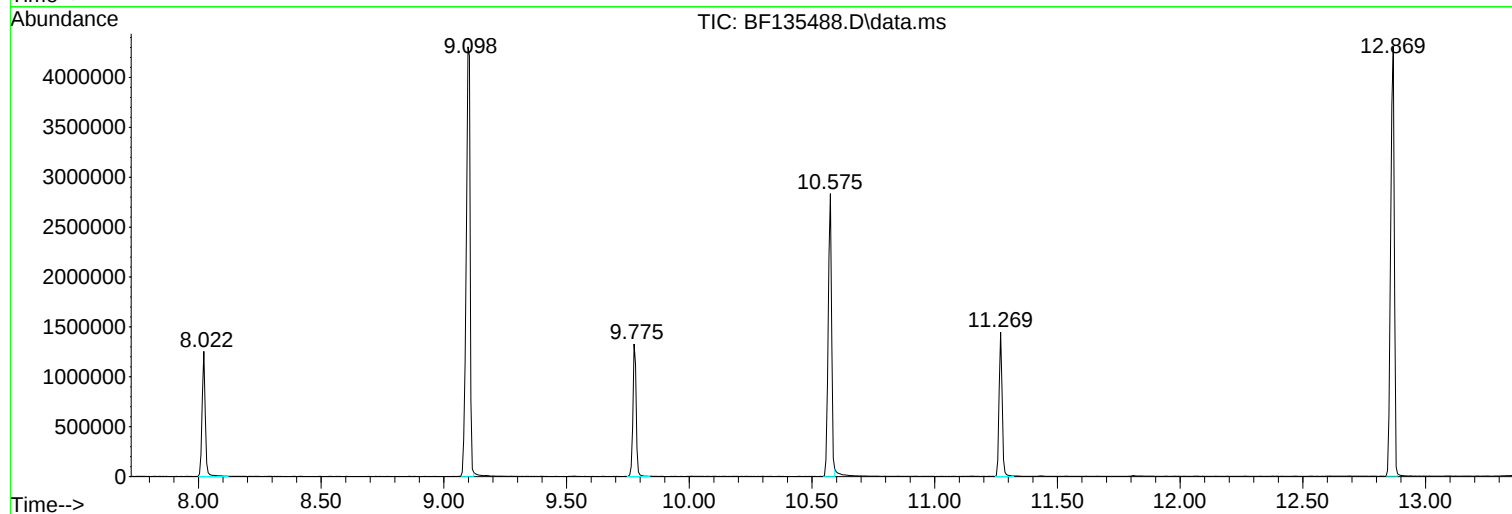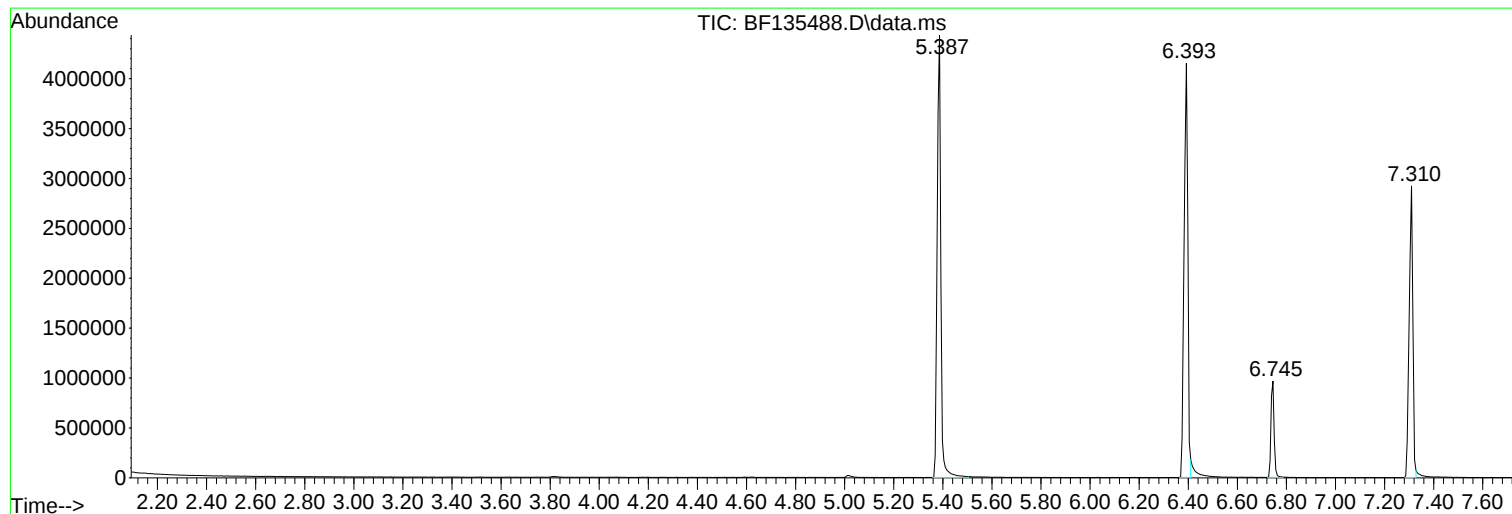

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092823\
Data File : BF135488.D
Acq On : 28 Sep 2023 12:25
Operator : CG\JU
Sample : PB155836BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB155836BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092823\
Data File : BF135488.D
Acq On : 28 Sep 2023 12:25
Operator : CG\JU
Sample : PB155836BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB155836BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------