


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092823\
Data File : BF135486.D
Acq On : 28 Sep 2023 11:25
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Sep 28 19:03:19 2023

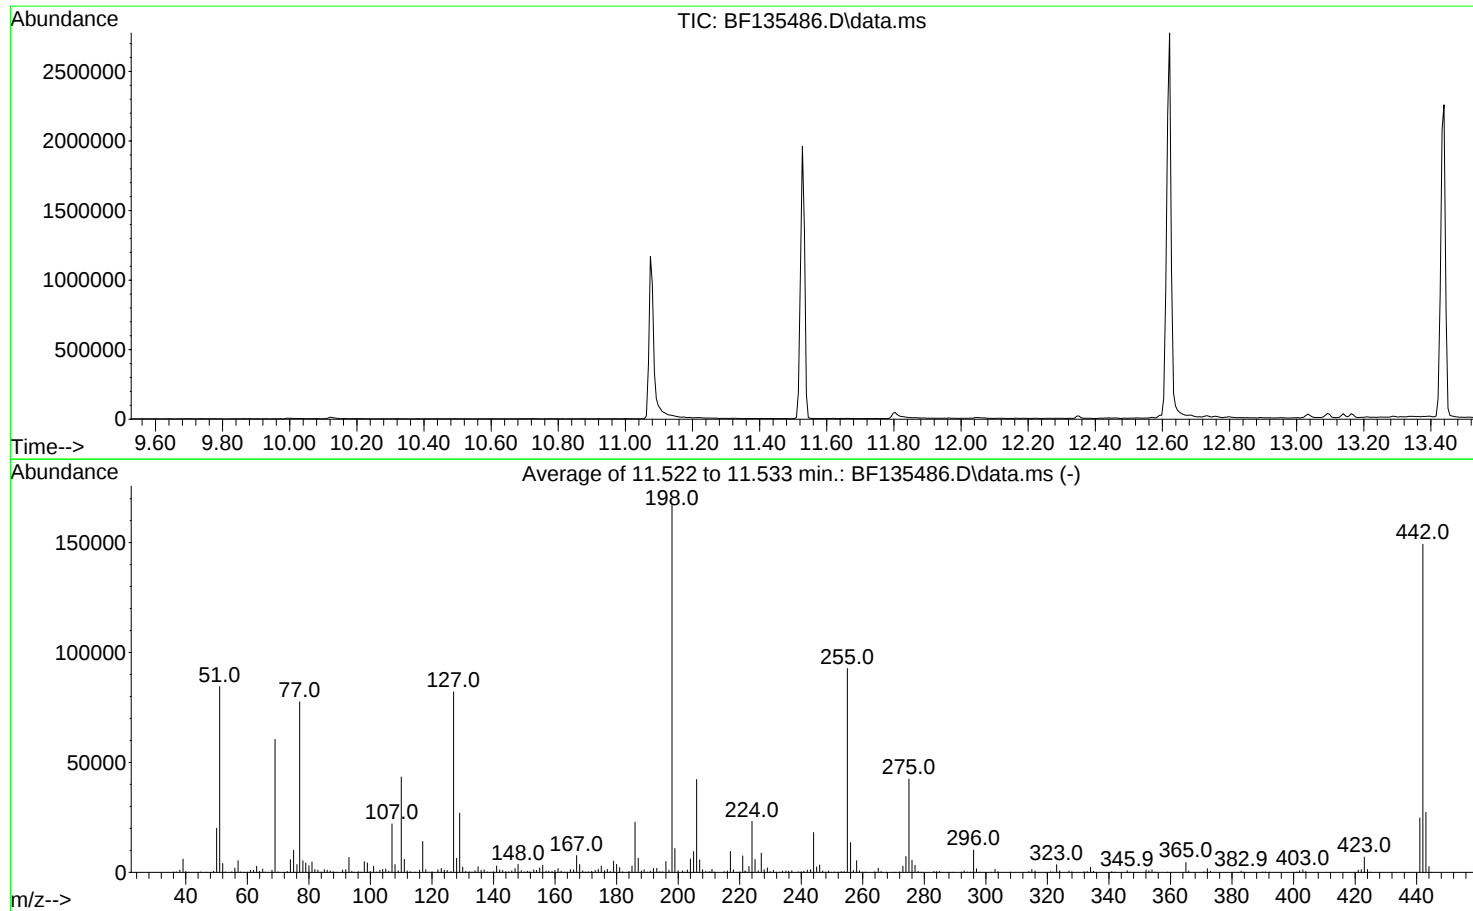




AutoFind: Scans 1604, 1605, 1606; Background Corrected with Scan 1599

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	50.5	84486	PASS
68	69	0.00	2	1.7	1043	PASS
69	198	0.00	100	36.2	60512	PASS
70	69	0.00	2	0.4	219	PASS
127	198	10	80	49.1	82149	PASS
197	198	0.00	2	0.6	967	PASS
198	198	100	100	100.0	167347	PASS
199	198	5	9	6.5	10883	PASS
275	198	10	60	25.4	42539	PASS
365	198	1	100	2.7	4534	PASS
441	198	0.01	100	14.8	24726	PASS
442	442	50	100	100.0	149267	PASS
443	442	15	24	18.3	27369	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092823\
Data File : BF135486.D
Acq On : 28 Sep 2023 11:25
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Sep 29 02:01:13 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 28 19:03:19 2023
Response via : Initial Calibration

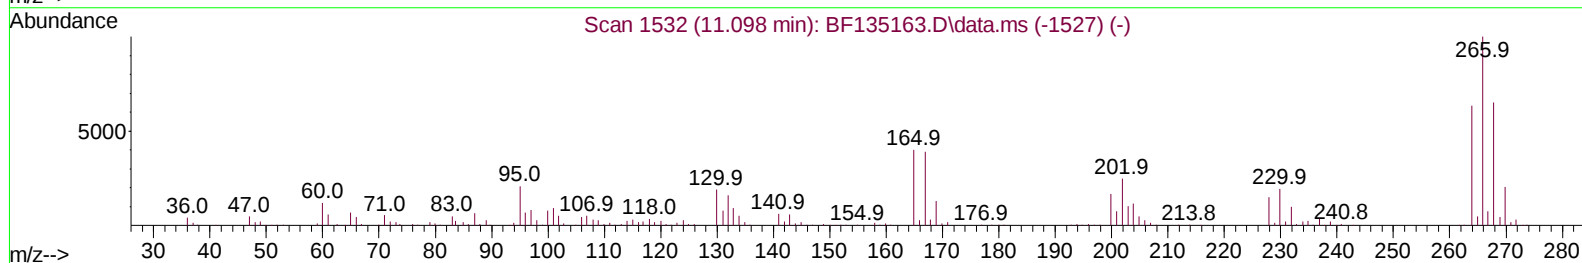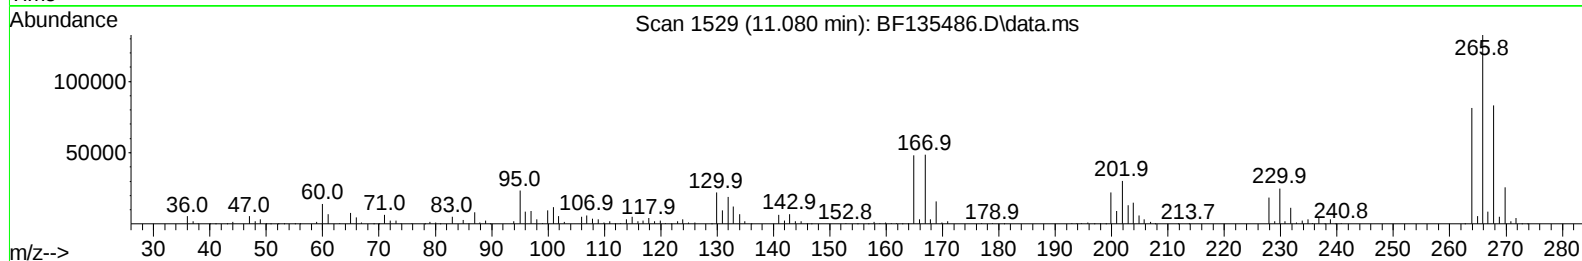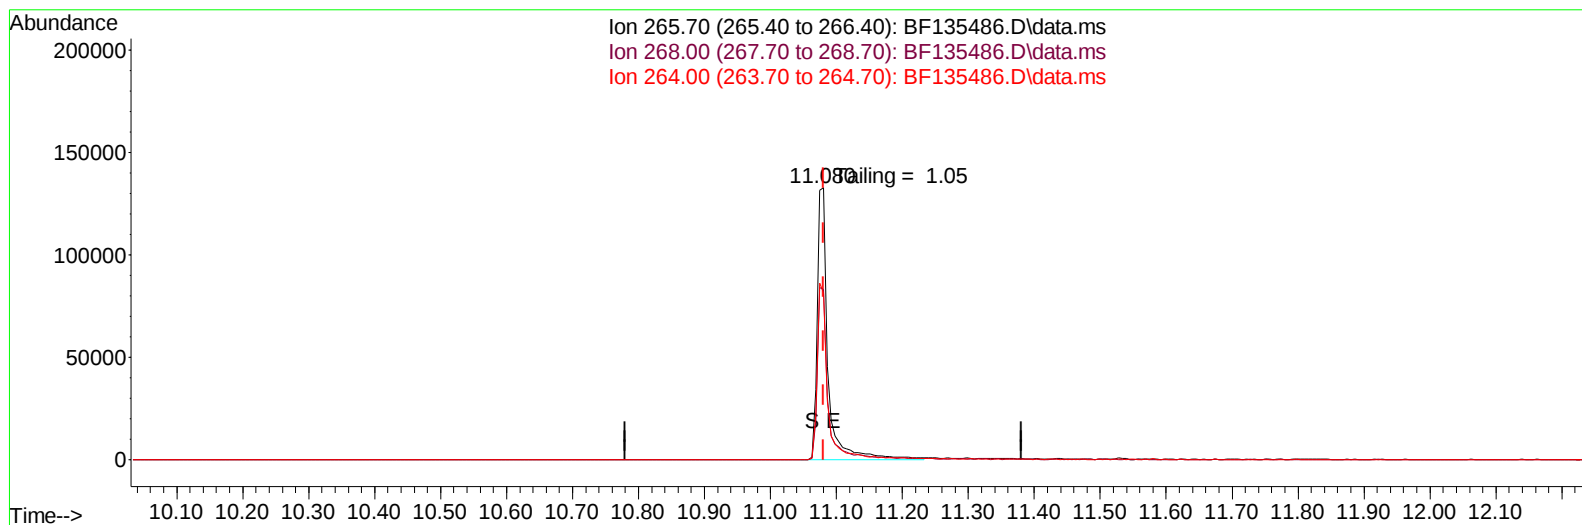

TIC: BF135486.D\data.ms

(70) Pentachlorophenol (C)

11.080min (-0.000) 30300.99 ng




response 152280

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.10	62.62
264.00	63.50	61.46
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092823\
Data File : BF135486.D
Acq On : 28 Sep 2023 11:25
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Sep 29 02:01:13 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Sep 28 19:03:19 2023
Response via : Initial Calibration

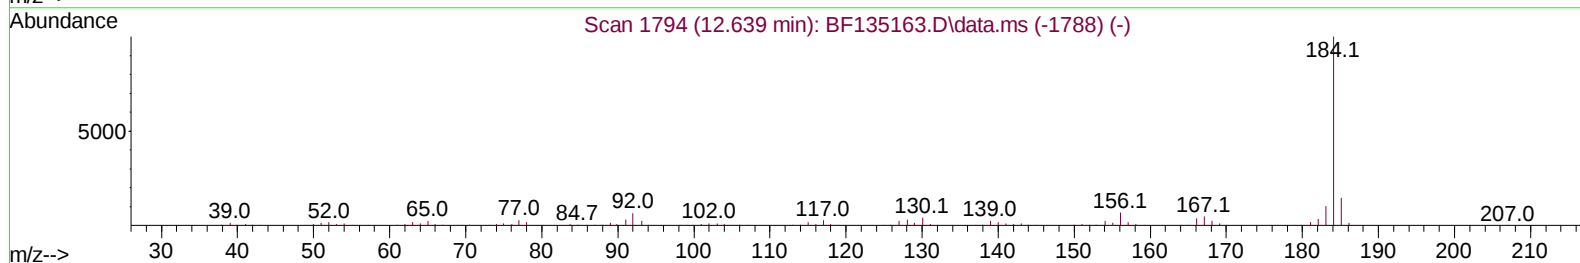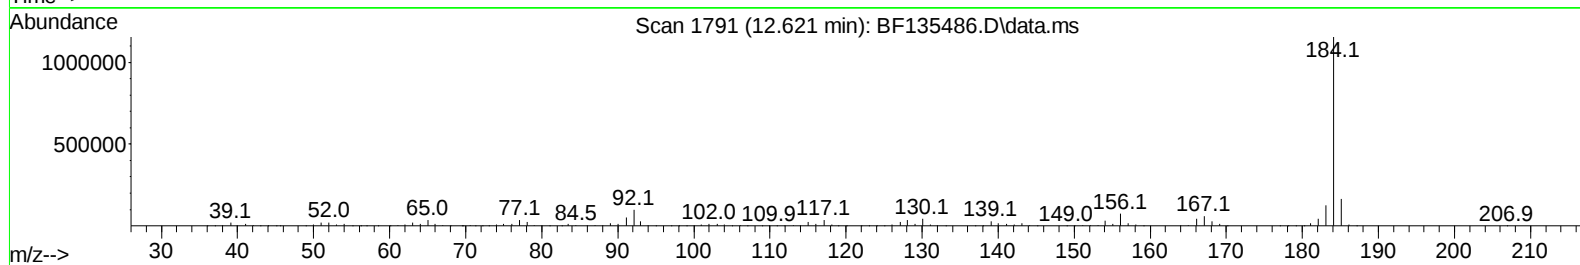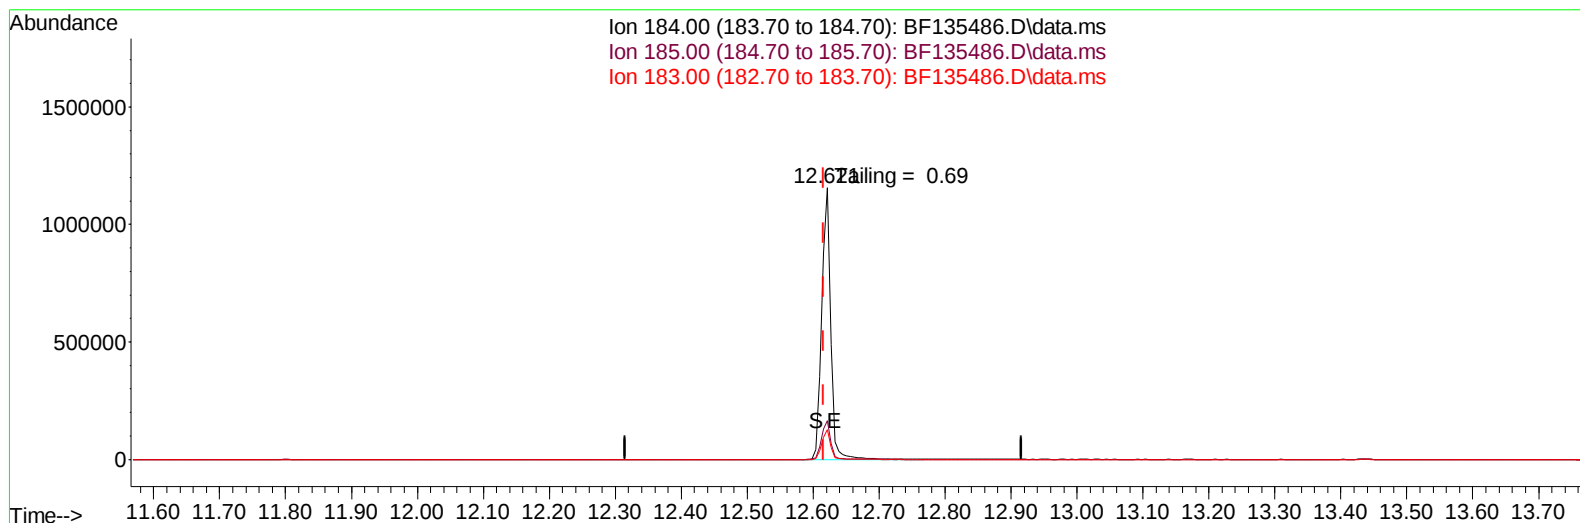

TIC: BF135486.D\data.ms

(77) Benzidine

12.621min (+ 0.006) 54084.06 ng

response 1108011

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.28
183.00	10.30	10.87
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/28/2023	BNA_F	<u>BF135486.D</u>
Compound Name	Response	Retention Time
DDT	431757	13.439
DDD	9230	13.139
DDE	998	12.798
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
10228	441985	2.31

Instrument :
BNA_F
ClientSampleId :
DFTPP