
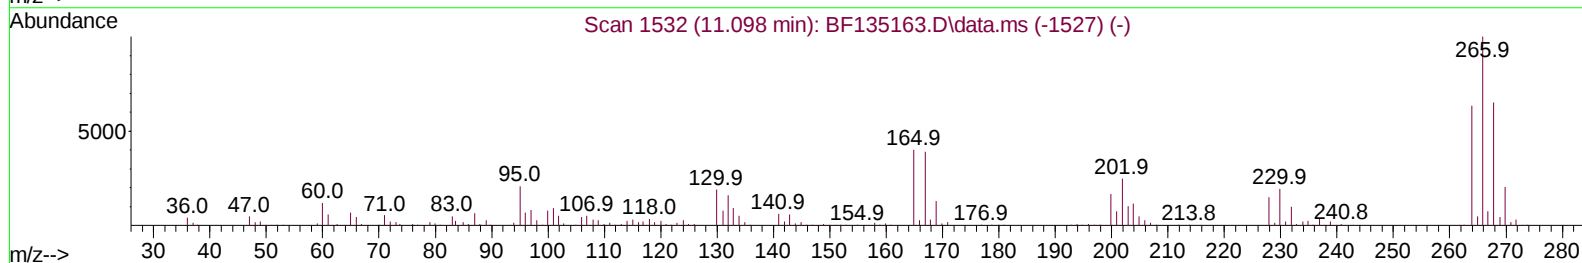
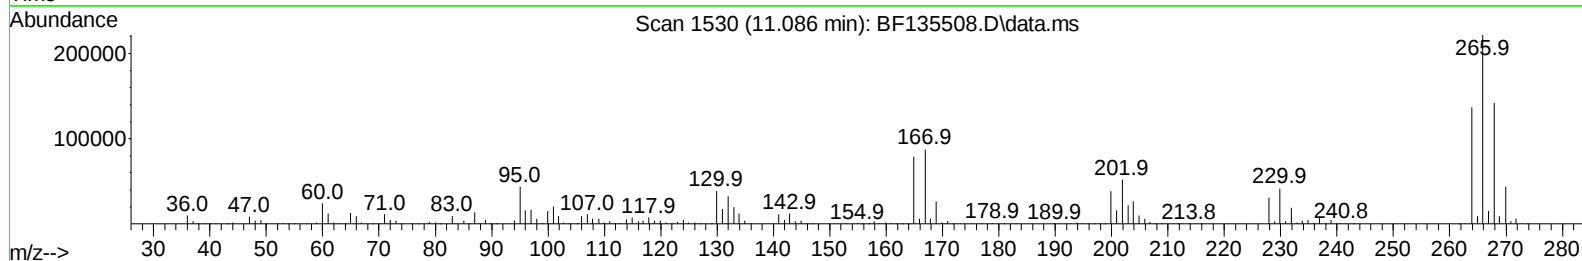


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092923\
Data File : BF135508.D
Acq On : 29 Sep 2023 09:03
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 30 01:18:26 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 30 00:12:20 2023
Response via : Initial Calibration

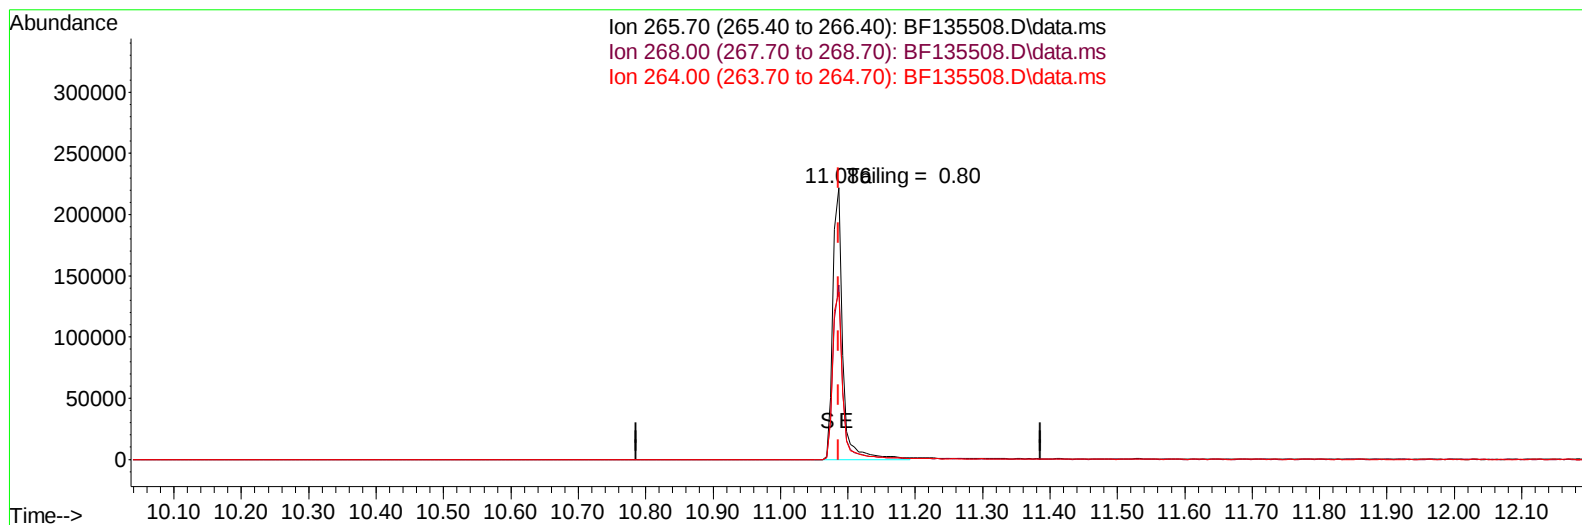

TIC: BF135508.D\data.ms

(70) Pentachlorophenol (C)




11.086min (-0.000) 180867.57 ng

response 224774

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.10	64.22
264.00	63.50	61.71
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092923\
Data File : BF135508.D
Acq On : 29 Sep 2023 09:03
Operator : CG\JU
Sample : DFTTP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Sep 30 01:18:26 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 30 00:12:20 2023
Response via : Initial Calibration

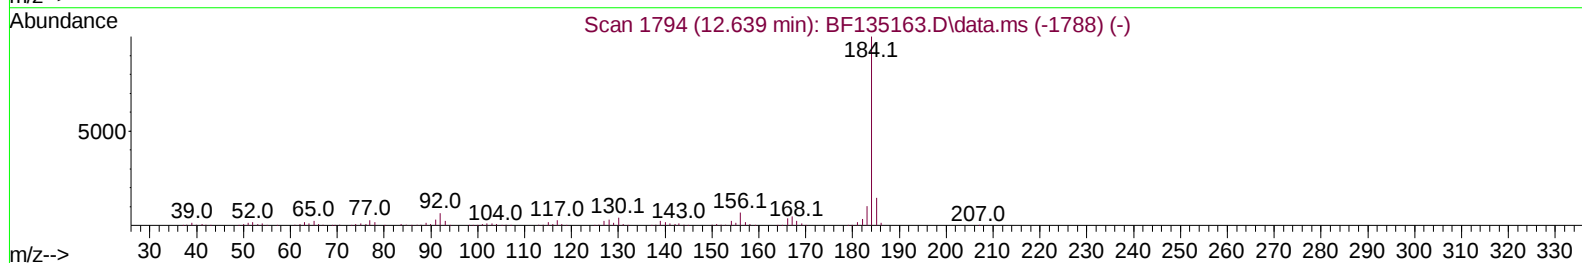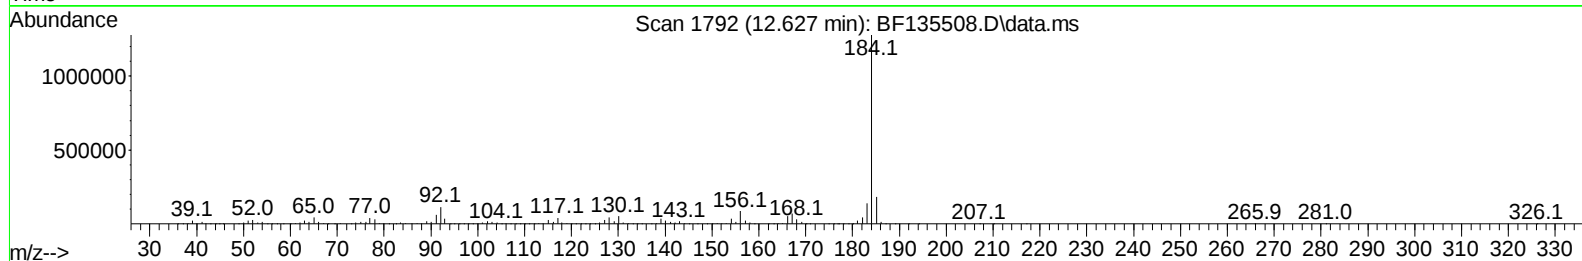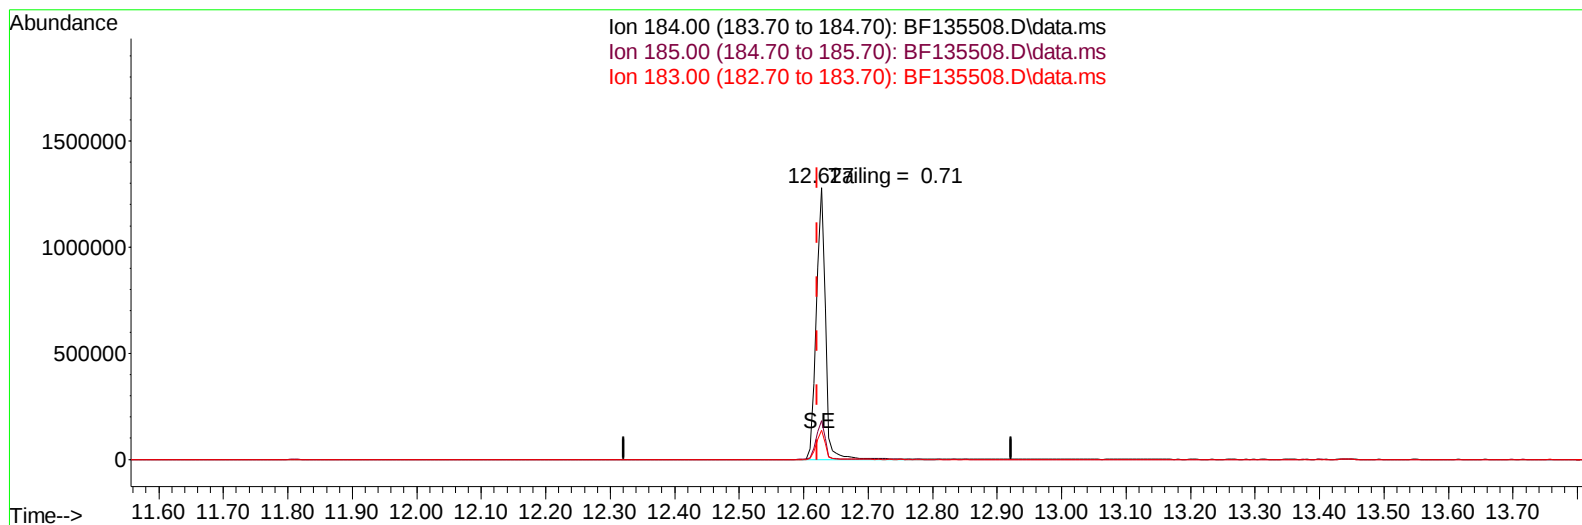

TIC: BF135508.D\data.ms

(77) Benzidine**12.627min (+ 0.006) 118584.32 ng****response 1275444**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.21
183.00	10.30	10.80
0.00	0.00	0.00