

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092923\
 Data File : BF135510.D
 Acq On : 29 Sep 2023 11:56
 Operator : CG\JU
 Sample : PB155928BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB155928BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF135510.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.393	558	562	584	rBV	4416360	4571274	95.32%	14.313%
2	6.398	728	733	736	rBV	4179460	4418902	92.15%	13.836%
3	6.745	788	792	803	rBV	1270726	1076230	22.44%	3.370%
4	7.310	883	888	891	rBV	2709942	3018280	62.94%	9.451%
5	8.022	1005	1009	1022	rBV	1523039	1478759	30.84%	4.630%
6	9.104	1187	1193	1196	rBV	4581529	4795531	100.00%	15.015%
7	9.781	1302	1308	1311	rBV	1625235	1512739	31.54%	4.737%
8	10.575	1439	1443	1458	rBV	2767798	2848249	59.39%	8.918%
9	11.275	1558	1562	1569	rBV	1694744	1572130	32.78%	4.923%
10	12.869	1828	1833	1837	rBV	4126360	4526781	94.40%	14.174%
11	13.927	2009	2013	2025	rBV	1265021	1184820	24.71%	3.710%
12	15.392	2257	2262	2275	rBV	641168	933672	19.47%	2.923%




Sum of corrected areas: 31937367

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092923\
Data File : BF135510.D
Acq On : 29 Sep 2023 11:56
Operator : CG\JU
Sample : PB155928BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB155928BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

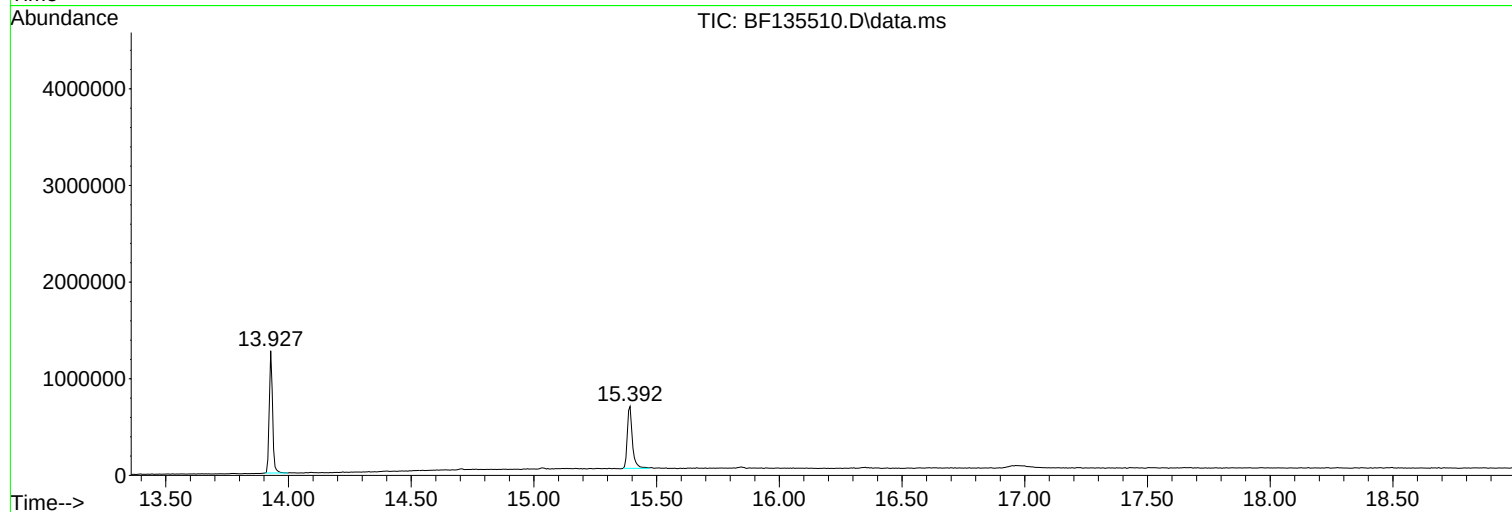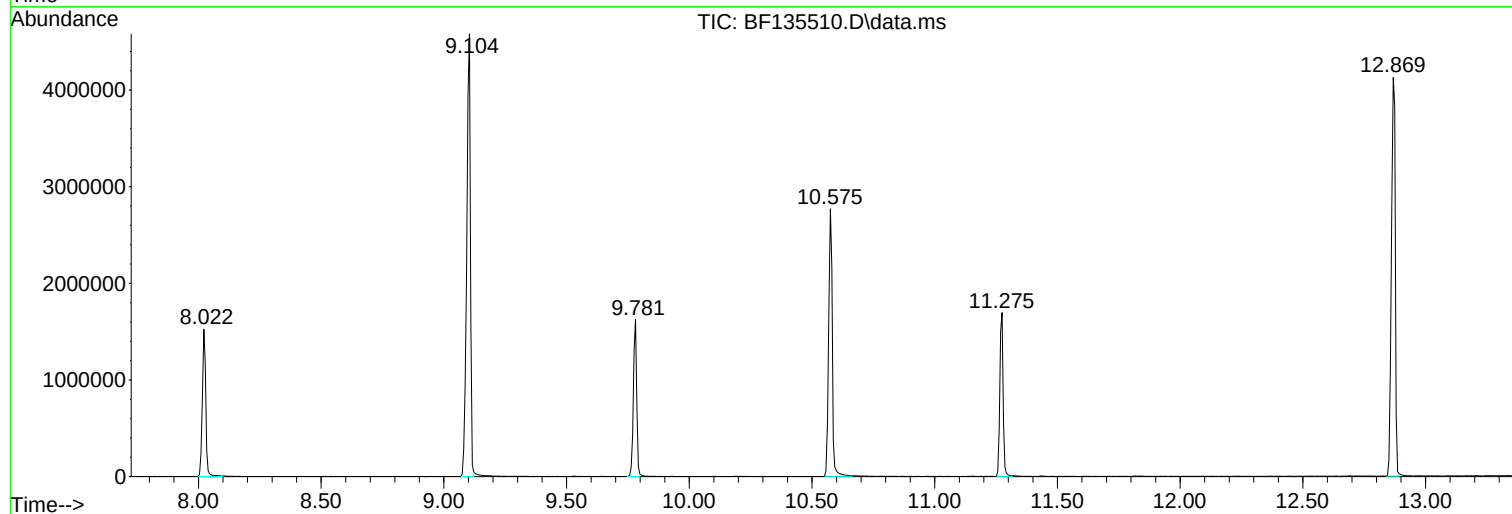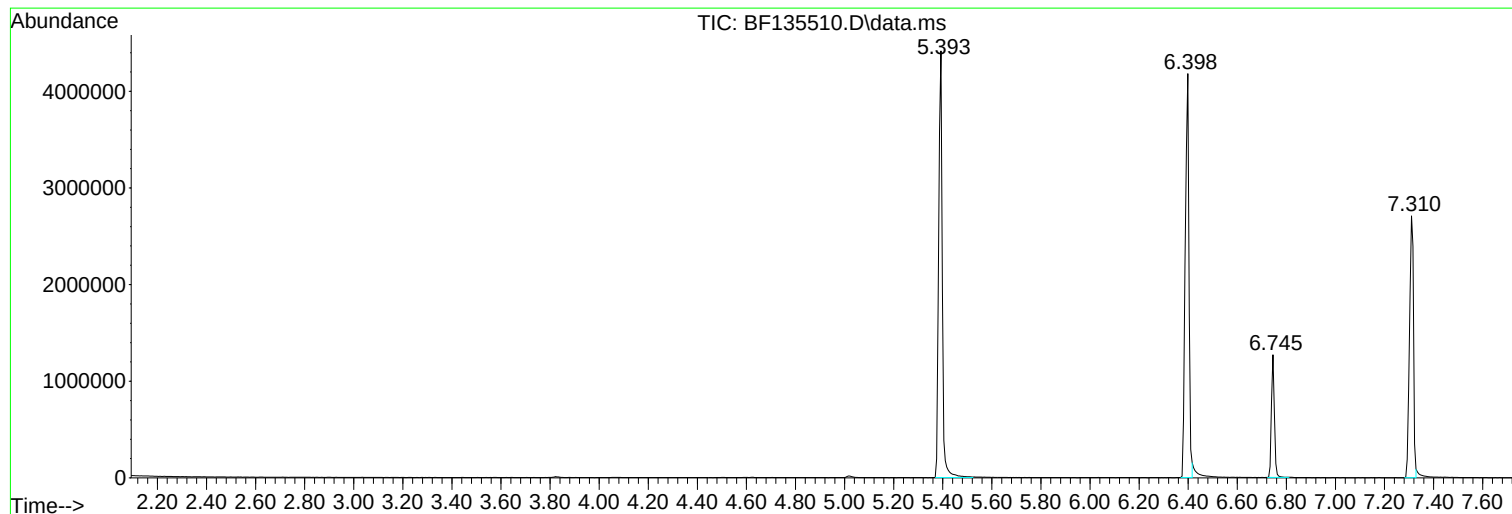

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092923\
Data File : BF135510.D
Acq On : 29 Sep 2023 11:56
Operator : CG\JU
Sample : PB155928BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB155928BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092923\
Data File : BF135510.D
Acq On : 29 Sep 2023 11:56
Operator : CG\JU
Sample : PB155928BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB155928BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------