

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092923\
Data File : BF135512.D
Acq On : 29 Sep 2023 12:58
Operator : CG\JU
Sample : PB155882TB
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB155882TB

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF135512.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.393	557	562	583	rBV	4044729	4340740	95.47%	14.571%
2	6.398	728	733	754	rBV	4013119	4326988	95.16%	14.525%
3	6.745	788	792	802	rBV	1097888	945868	20.80%	3.175%
4	7.310	883	888	905	rBV	2623732	2918247	64.18%	9.796%
5	8.022	1005	1009	1028	rBV	1294890	1244027	27.36%	4.176%
6	9.104	1187	1193	1196	rBV	4294887	4546840	100.00%	15.263%
7	9.781	1302	1308	1319	rBV	1464343	1344689	29.57%	4.514%
8	10.575	1439	1443	1461	rBV	2735899	2677250	58.88%	8.987%
9	11.275	1558	1562	1571	rBV	1470367	1405479	30.91%	4.718%
10	12.869	1828	1833	1836	rBV	4123178	4210275	92.60%	14.133%
11	13.927	2009	2013	2026	rVB	1085956	1012911	22.28%	3.400%
12	15.392	2257	2262	2275	rBV	566115	816530	17.96%	2.741%




Sum of corrected areas: 29789844

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092923\
Data File : BF135512.D
Acq On : 29 Sep 2023 12:58
Operator : CG\JU
Sample : PB155882TB
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB155882TB

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

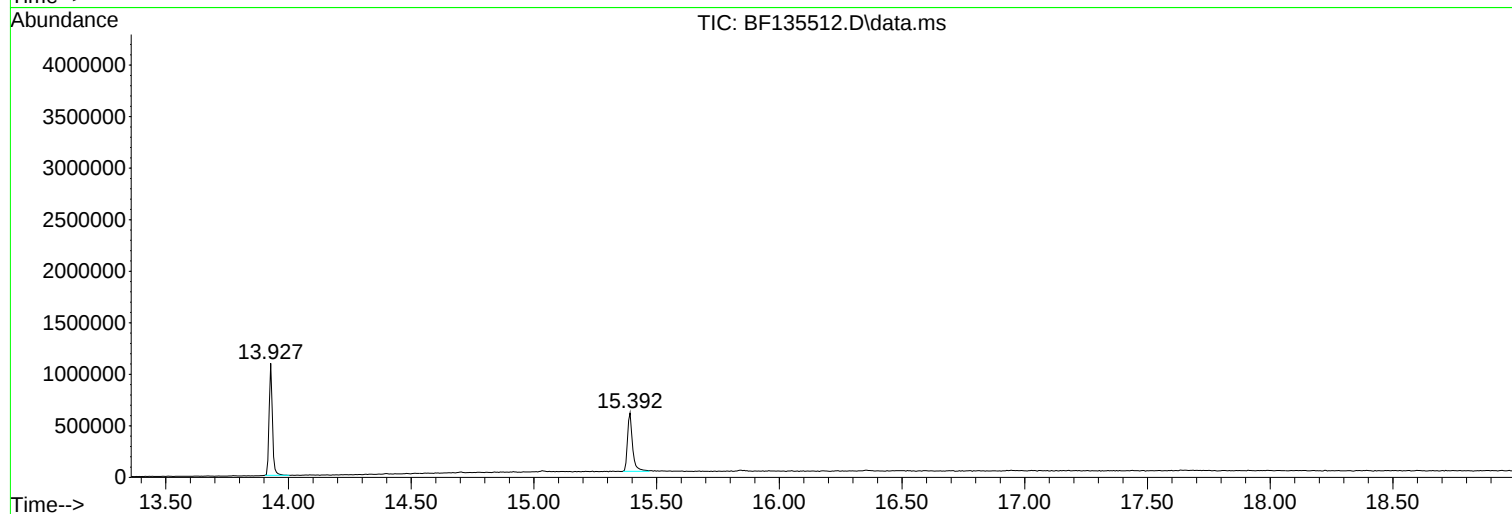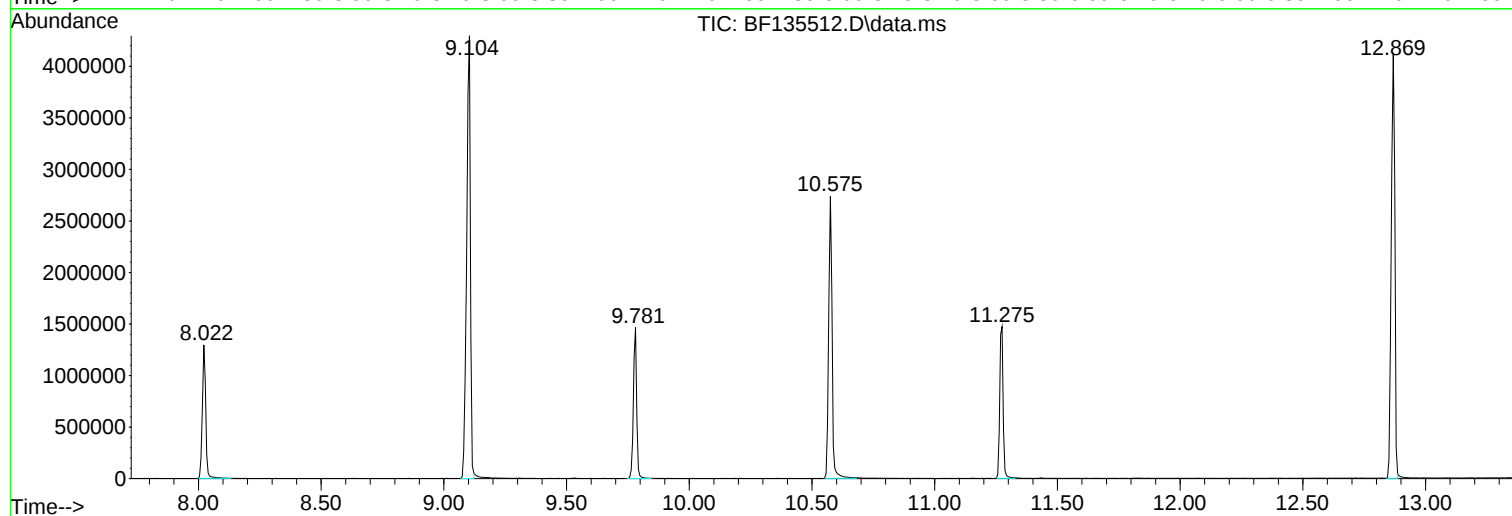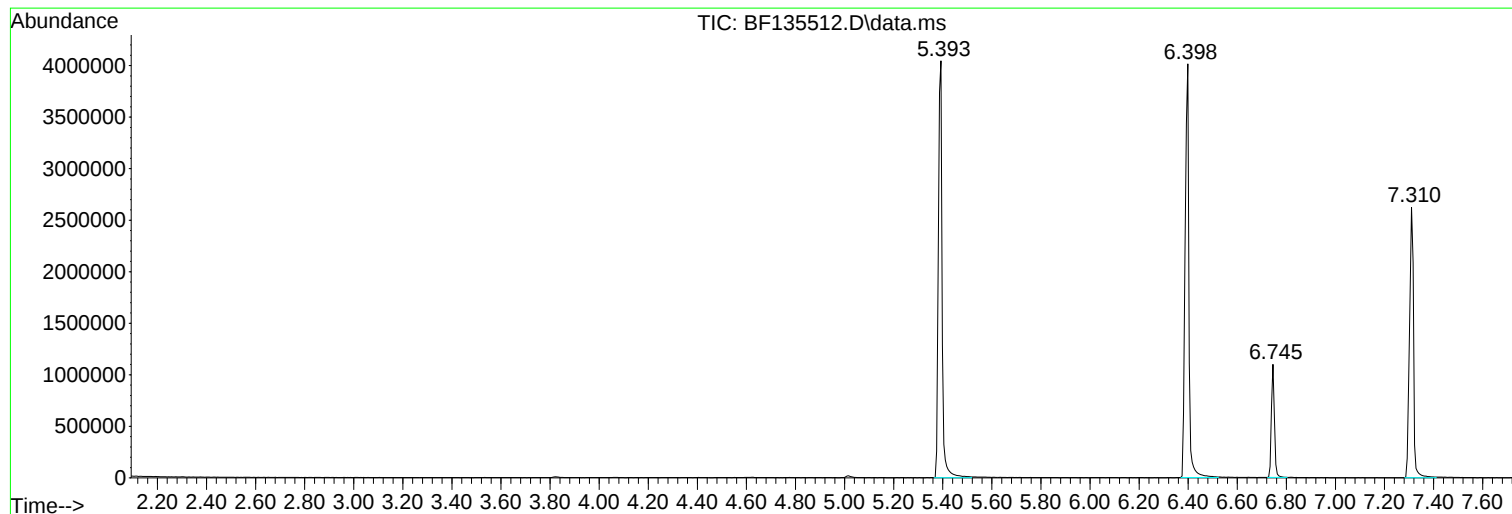

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092923\
Data File : BF135512.D
Acq On : 29 Sep 2023 12:58
Operator : CG\JU
Sample : PB155882TB
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB155882TB

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092923\
Data File : BF135512.D
Acq On : 29 Sep 2023 12:58
Operator : CG\JU
Sample : PB155882TB
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB155882TB

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------