


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092923\
Data File : BF135508.D
Acq On : 29 Sep 2023 09:03
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Sat Sep 30 00:12:20 2023



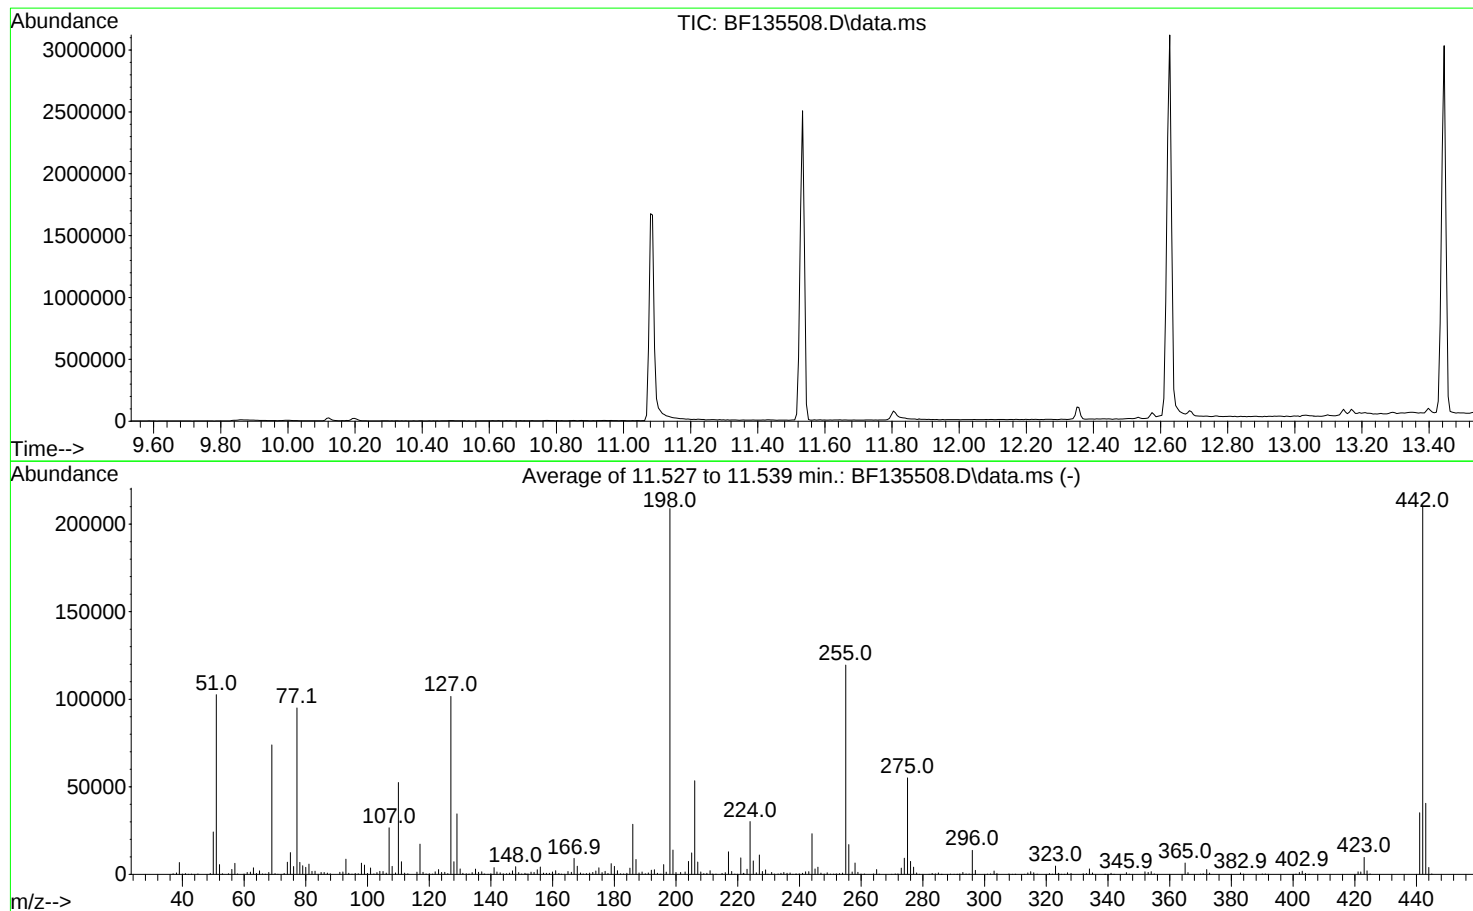


AutoFind: Scans 1605, 1606, 1607; Background Corrected with Scan 1599

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
51	198	10	80	49.1	102573	PASS
68	69	0.00	2	1.5	1139	PASS
69	198	0.00	100	35.4	73911	PASS
70	69	0.00	2	0.6	441	PASS
127	198	10	80	48.7	101643	PASS
197	198	0.00	2	0.6	1248	PASS
198	198	100	100	100.0	208853	PASS
199	198	5	9	6.7	13912	PASS
275	198	10	60	26.4	55061	PASS
365	198	1	100	3.1	6458	PASS
441	198	0.01	100	16.9	35200	PASS
442	442	50	100	100.0	210061	PASS
443	442	15	24	19.3	40571	PASS

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Sep 30 01:18:26 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 30 00:12:20 2023
Response via : Initial Calibration

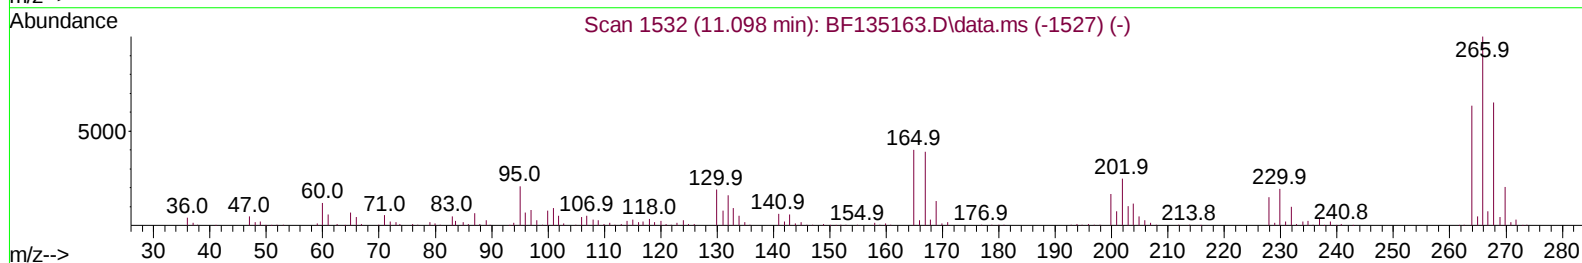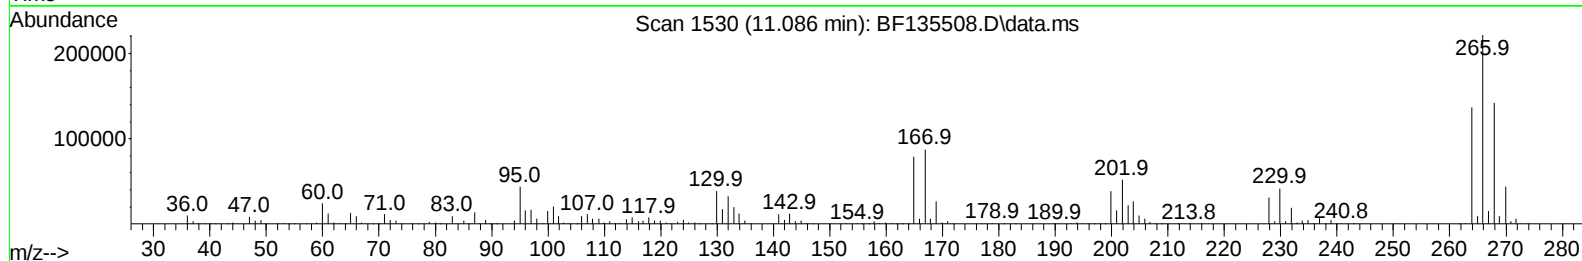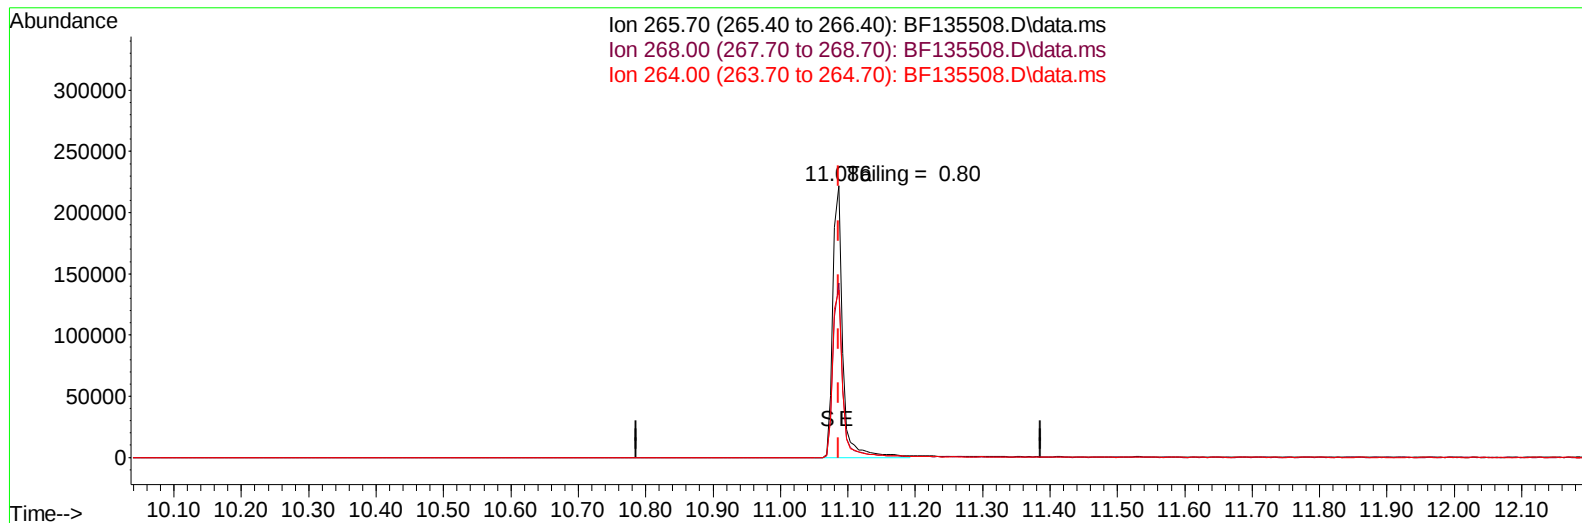

TIC: BF135508.D\data.ms

(70) Pentachlorophenol (C)

11.086min (-0.000) 180867.57 ng




response 224774

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.10	64.22
264.00	63.50	61.71
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF092923\
Data File : BF135508.D
Acq On : 29 Sep 2023 09:03
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Sep 30 01:18:26 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 30 00:12:20 2023
Response via : Initial Calibration

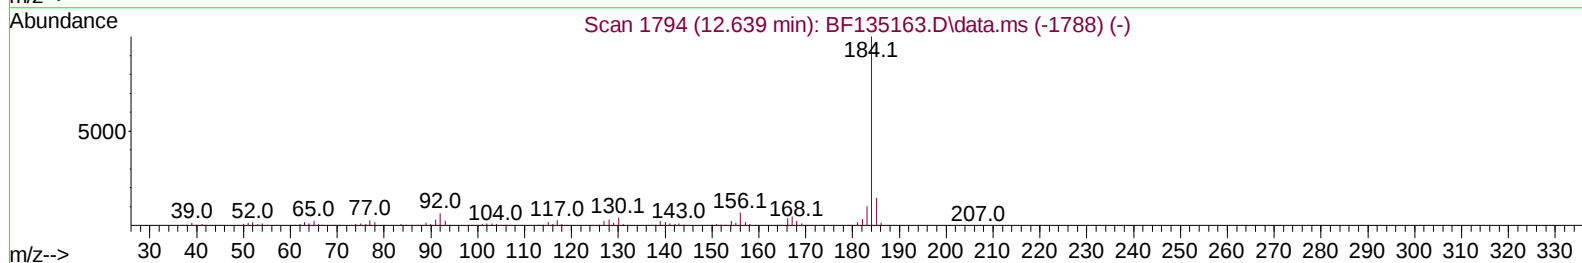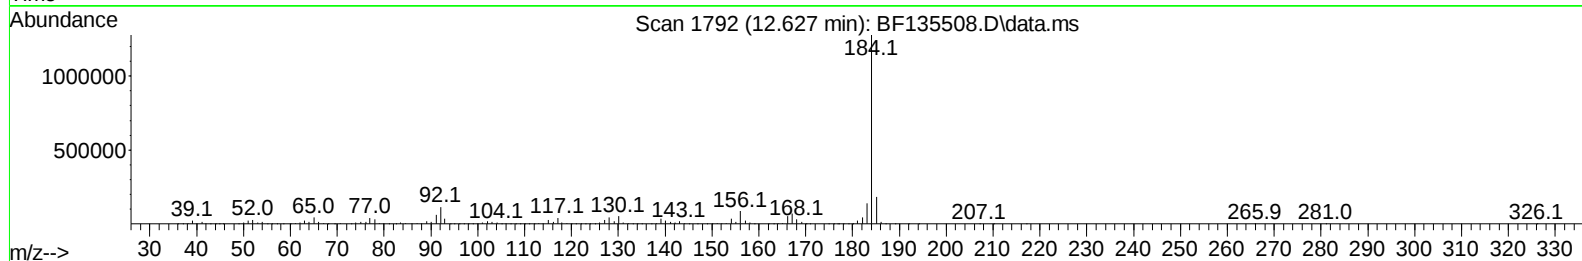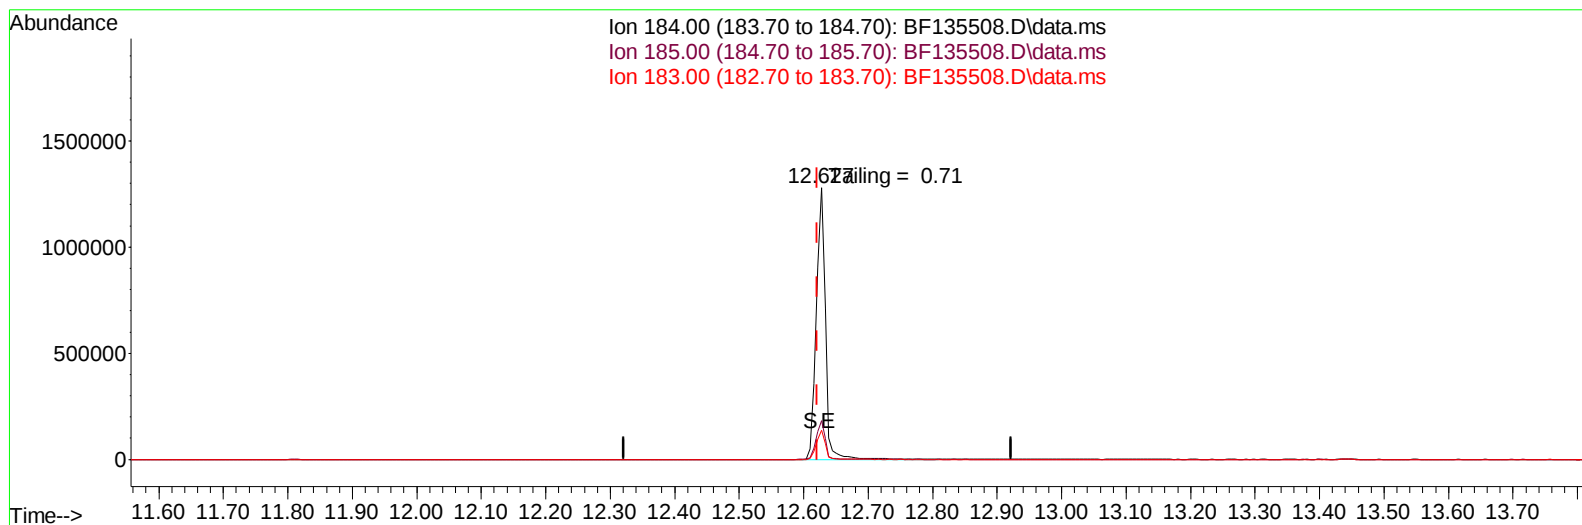

TIC: BF135508.D\data.ms

(77) Benzidine

12.627min (+ 0.006) 118584.32 ng

response 1275444

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.21
183.00	10.30	10.80
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
9/29/2023	BNA_F	<u>BF135508.D</u>
Compound Name	Response	Retention Time
DDT	529789	13.445
DDD	15501	13.145
DDE	720	12.804
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
16221	546010	2.97

Instrument :
BNA_F
ClientSampleId :
DFTPP