

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100121\
 Data File : BF125756.D
 Acq On : 1 Oct 2021 17:11
 Operator : JU/CG
 Sample : M4008-01
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 MW-SIDEWALK

Quant Time: Oct 02 03:12:25 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF092421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 24 15:38:32 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.887	152	214210	20.00	ng	0.00
21) Naphthalene-d8	8.169	136	878103	20.00	ng	# 0.00
39) Acenaphthene-d10	9.922	164	458942	20.00	ng	0.00
64) Phenanthrene-d10	11.404	188	778724	20.00	ng	# 0.00
76) Chrysene-d12	14.039	240	448916	20.00	ng	0.00
86) Perylene-d12	15.515	264	460794	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.504	112	810814	62.36	ng	0.00
7) Phenol-d6	6.504	99	1342001	76.78	ng	0.00
23) Nitrobenzene-d5	7.445	82	847623	67.33	ng	0.00
42) 2,4,6-Tribromophenol	10.704	330	97663	22.82	ng	-0.01
45) 2-Fluorobiphenyl	9.245	172	1729261	64.47	ng	0.00
79) Terphenyl-d14	12.992	244	1637925	63.19	ng	0.00


Target Compounds	Qvalue
-----	-----


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100121\
Data File : BF125756.D
Acq On : 1 Oct 2021 17:11
Operator : JU/CG
Sample : M4008-01
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
MW-SIDEWALK

Quant Time: Oct 02 03:12:25 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF092421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 24 15:38:32 2021
Response via : Initial Calibration




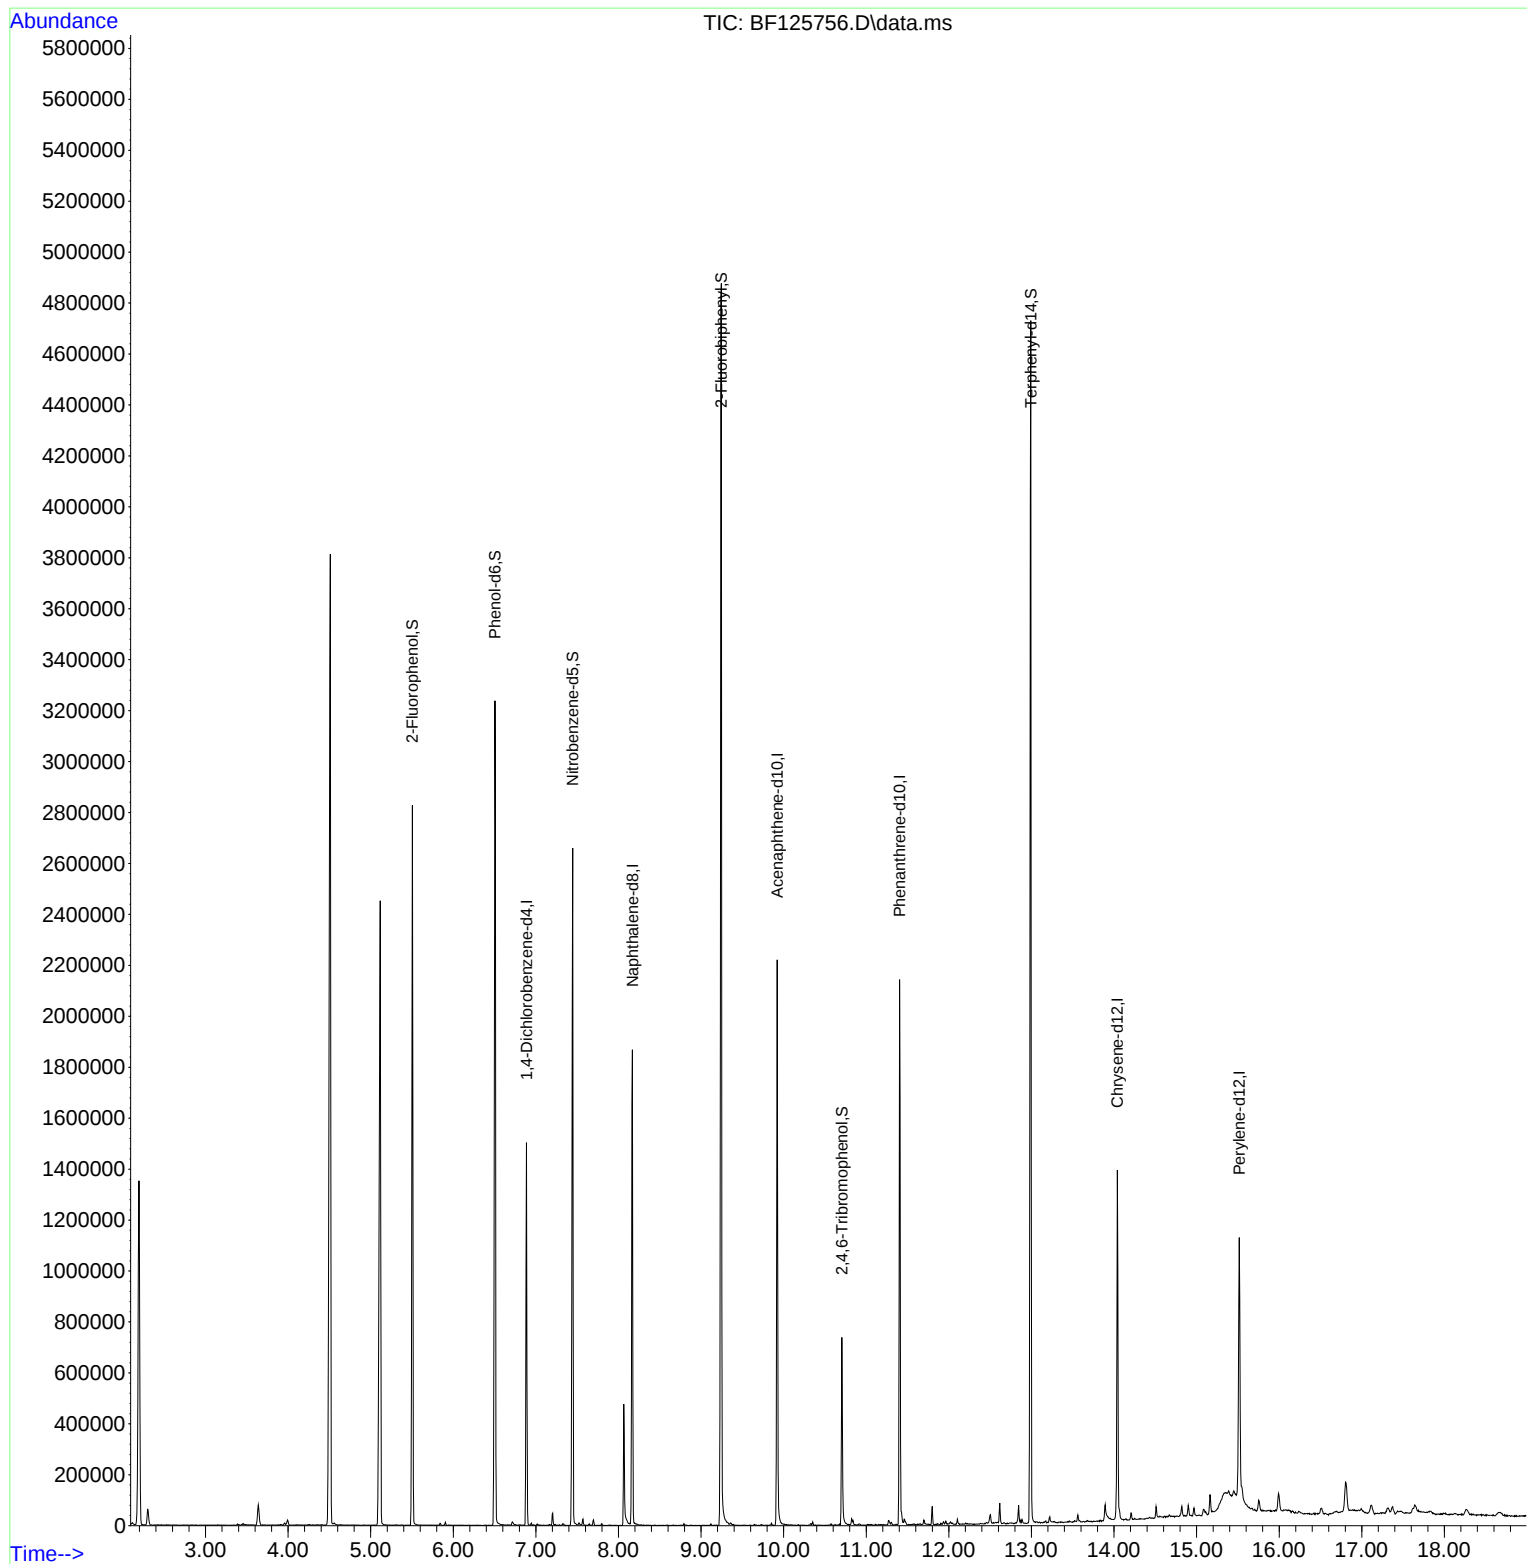


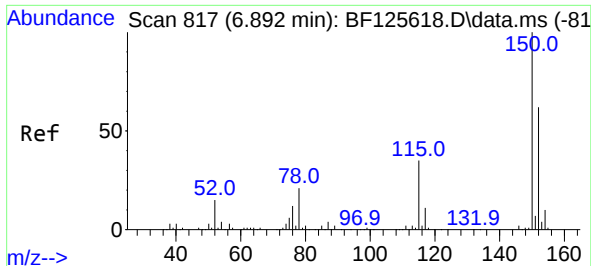

#1
1,4-Dichlorobenzene-d4
Concen: 20.00 ng
RT: 6.887 min Scan# 816
Delta R.T. -0.005 min
Lab File: BF125756.D
Acq: 1 Oct 2021 17:11




Instrument :
BNA_F
ClientSampleId :
MW-SIDEWALK


Tgt Ion:152 Resp: 214210
Ion Ratio Lower Upper
152 100
150 158.0 117.6 176.4
115 59.3 47.1 70.7

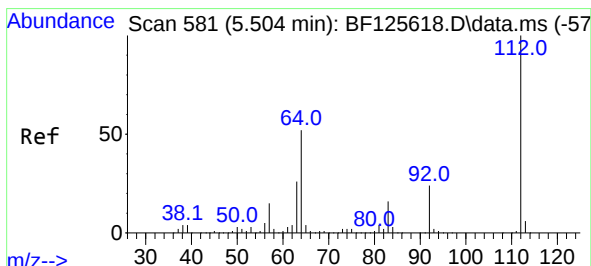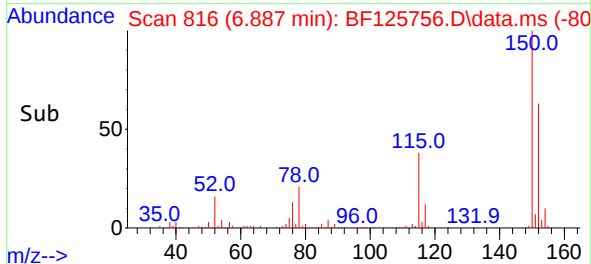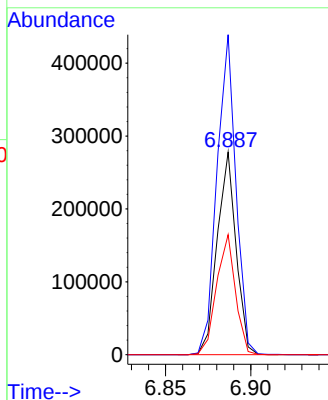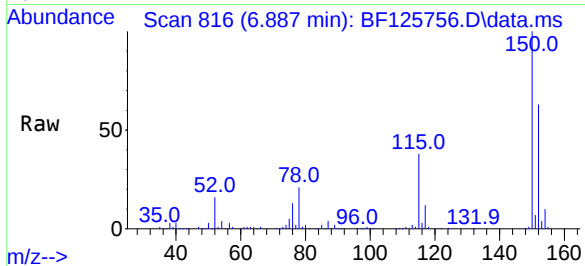

#5
2-Fluorophenol
Concen: 62.36 ng
RT: 5.504 min Scan# 581
Delta R.T. 0.000 min
Lab File: BF125756.D
Acq: 1 Oct 2021 17:11

Tgt Ion:112 Resp: 810814
Ion Ratio Lower Upper
112 100
64 51.6 44.2 66.2
63 25.2 26.2 39.2#


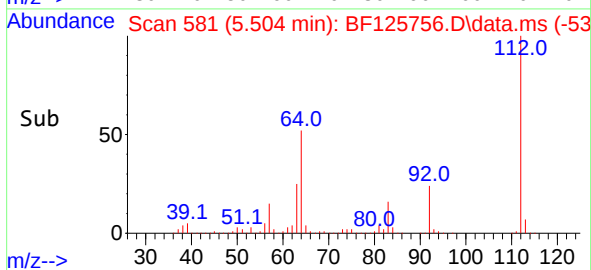
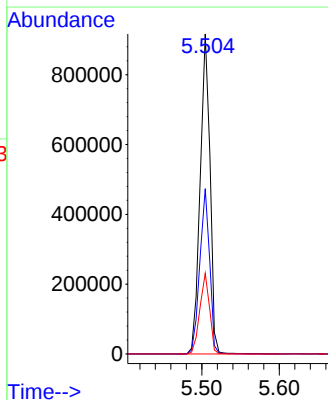
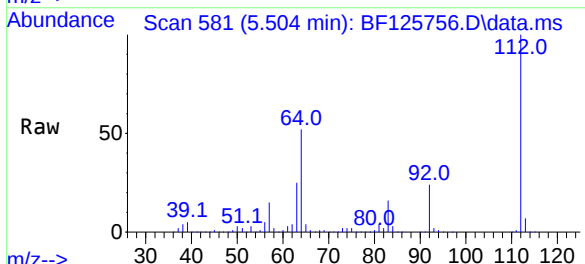


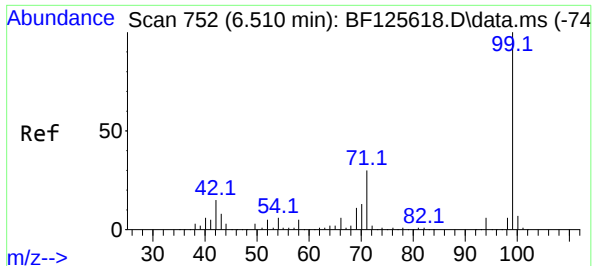

#7
Phenol-d6
Concen: 76.78 ng
RT: 6.504 min Scan# 751
Delta R.T. -0.006 min
Lab File: BF125756.D
Acq: 1 Oct 2021 17:11




Instrument :
BNA_F
ClientSampleId :
MW-SIDEWALK


Tgt Ion: 99 Resp: 1342001
Ion Ratio Lower Upper
99 100
42 14.3 23.5 35.3#
71 29.2 25.6 38.4

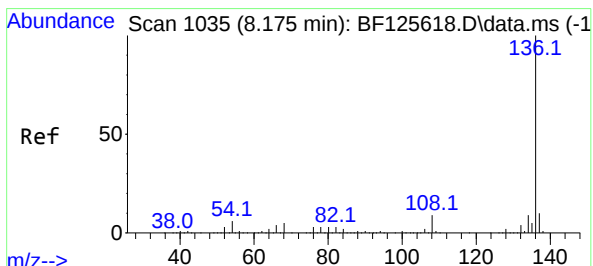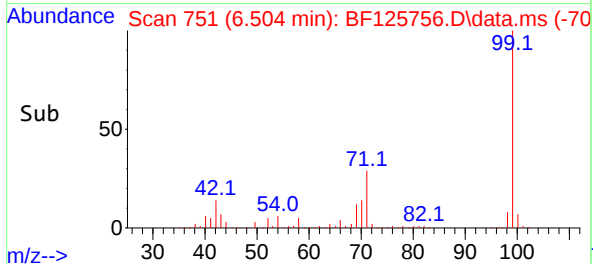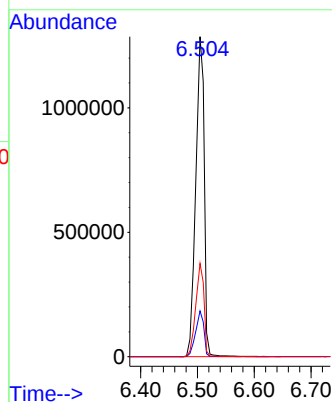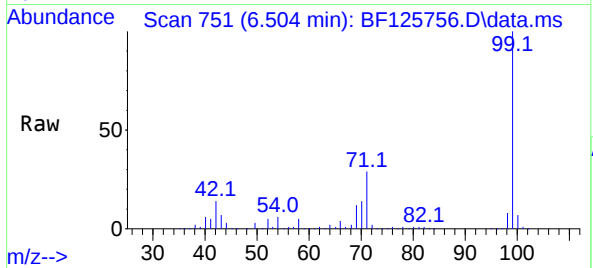

#21
Naphthalene-d8
Concen: 20.00 ng
RT: 8.169 min Scan# 1034
Delta R.T. -0.006 min
Lab File: BF125756.D
Acq: 1 Oct 2021 17:11

Tgt Ion: 136 Resp: 878103
Ion Ratio Lower Upper
136 100
137 10.3 9.8 14.6
54 5.9 6.4 9.6#
68 5.3 3.3 4.9#

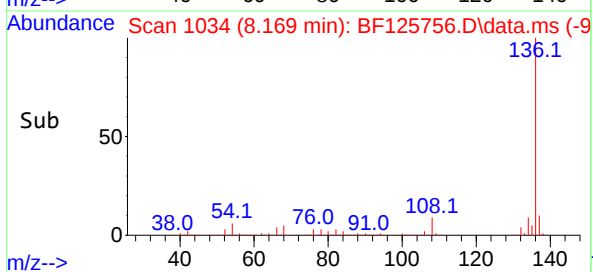
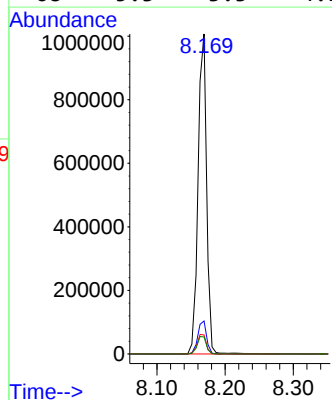
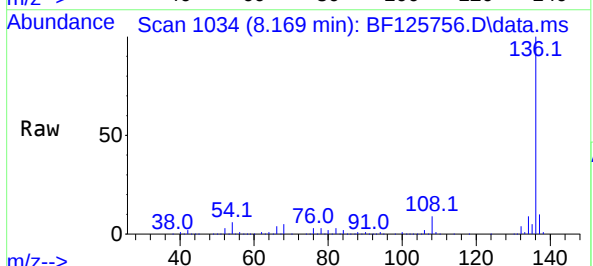


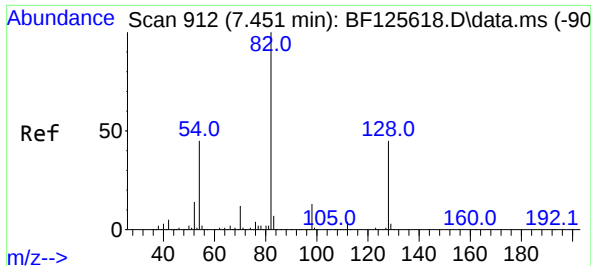

#23
Nitrobenzene-d5
Concen: 67.33 ng
RT: 7.445 min Scan# 911
Delta R.T. -0.006 min
Lab File: BF125756.D
Acq: 1 Oct 2021 17:11




Instrument :
BNA_F
ClientSampleId :
MW-SIDEWALK


Tgt Ion: 82 Resp: 847623
Ion Ratio Lower Upper
82 100
128 49.0 40.6 60.8
54 43.3 49.6 74.4#

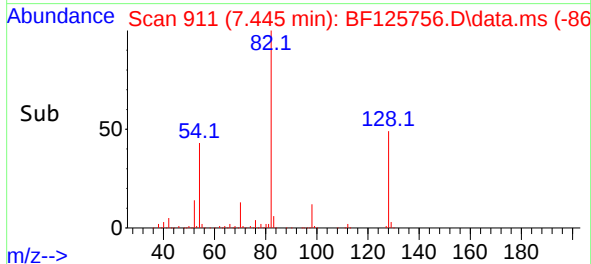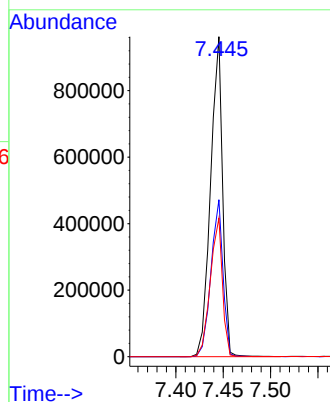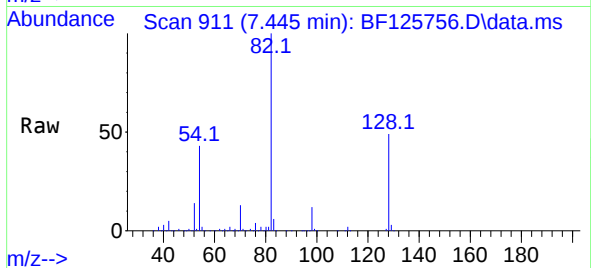

#39
Acenaphthene-d10
Concen: 20.00 ng
RT: 9.922 min Scan# 1332
Delta R.T. -0.006 min
Lab File: BF125756.D
Acq: 1 Oct 2021 17:11


Tgt Ion:164 Resp: 458942
Ion Ratio Lower Upper
164 100
162 103.2 81.3 121.9
160 45.1 38.0 57.0

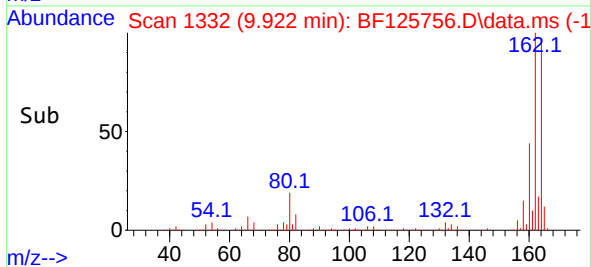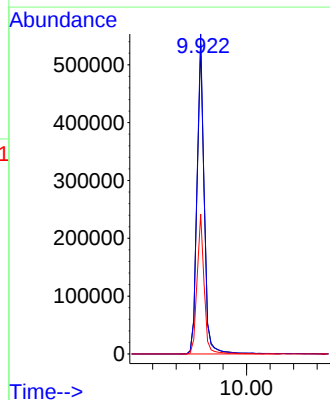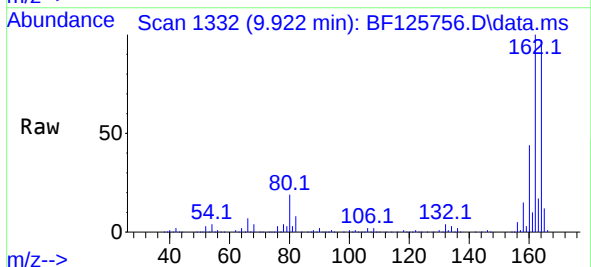



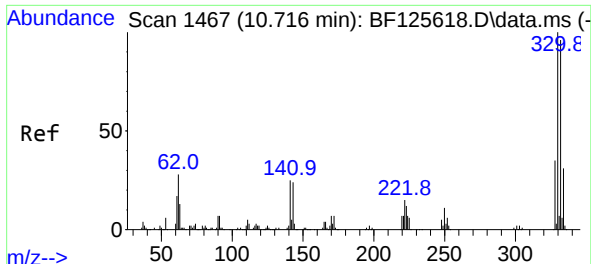


#42
2,4,6-Tribromophenol
Concen: 22.82 ng
RT: 10.704 min Scan# 1465
Delta R.T. -0.012 min
Lab File: BF125756.D
Acq: 1 Oct 2021 17:11


Instrument :
BNA_F
ClientSampleId :
MW-SIDEWALK

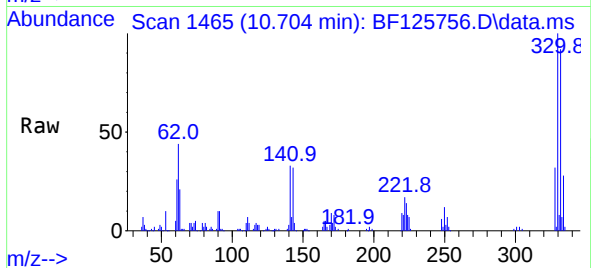



Tgt Ion:330 Resp: 97663
Ion Ratio Lower Upper
330 100
332 94.3 76.2 114.4
141 31.3 44.6 66.8#

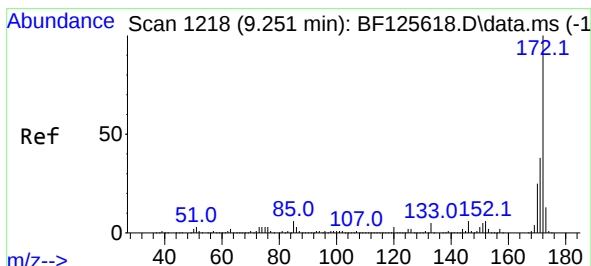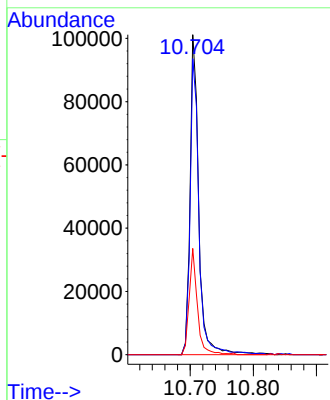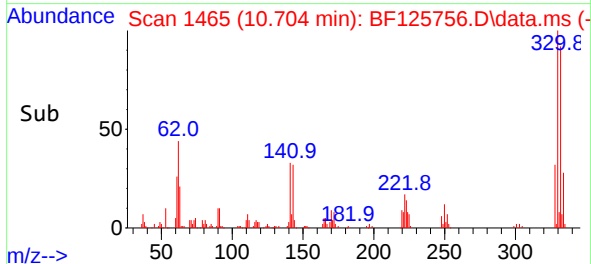

#45
2-Fluorobiphenyl
Concen: 64.47 ng
RT: 9.245 min Scan# 1217
Delta R.T. -0.006 min
Lab File: BF125756.D
Acq: 1 Oct 2021 17:11

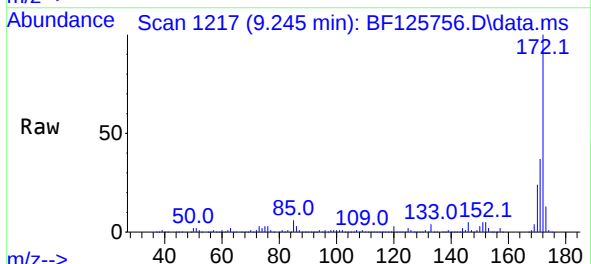

Tgt Ion:172 Resp: 1729261
Ion Ratio Lower Upper
172 100
171 36.7 26.5 39.7
170 24.1 18.8 28.2



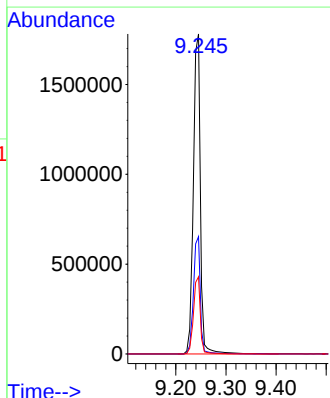
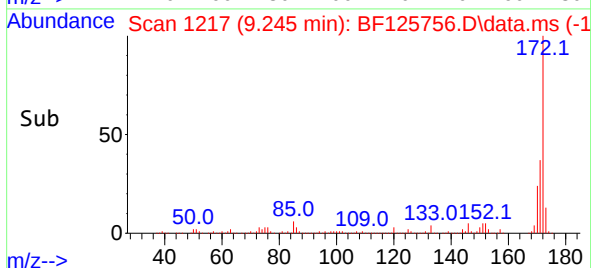




#64
Phenanthrene-d10
Concen: 20.00 ng
RT: 11.404 min Scan# 1584
Delta R.T. -0.006 min
Lab File: BF125756.D
Acq: 1 Oct 2021 17:11




Instrument :
BNA_F
ClientSampleId :
MW-SIDEWALK

Tgt Ion:188 Resp: 778724
Ion Ratio Lower Upper
188 100
94 10.4 6.7 10.1#
80 10.9 7.5 11.3

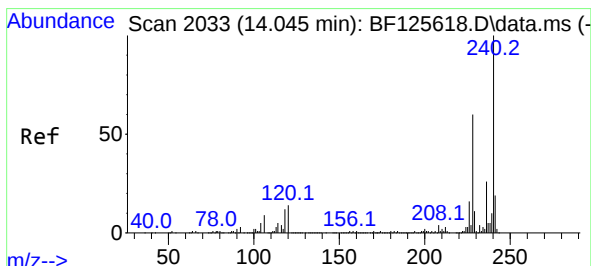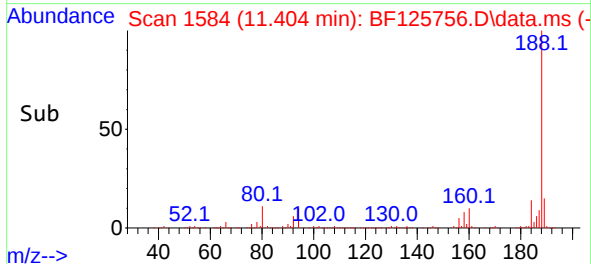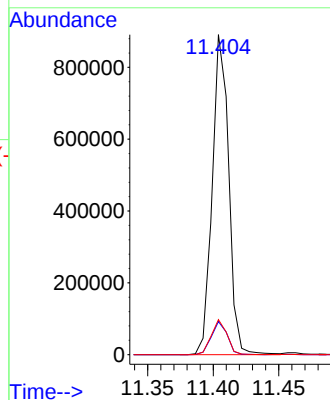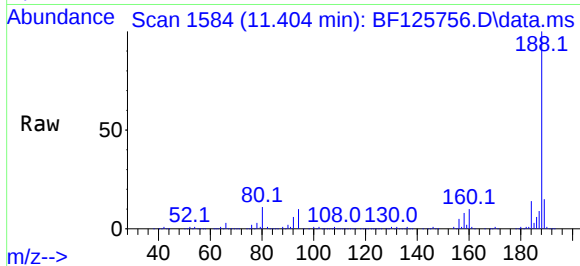

#76
Chrysene-d12
Concen: 20.00 ng
RT: 14.039 min Scan# 2032
Delta R.T. -0.006 min
Lab File: BF125756.D
Acq: 1 Oct 2021 17:11

Tgt Ion:240 Resp: 448916
Ion Ratio Lower Upper
240 100
120 13.5 10.8 16.2
236 25.0 21.6 32.4


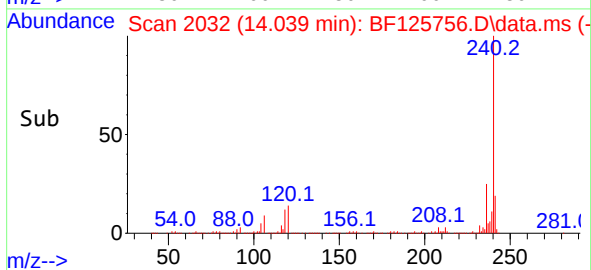
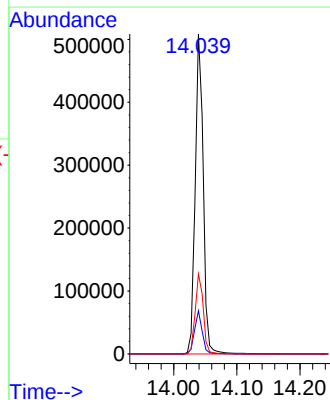
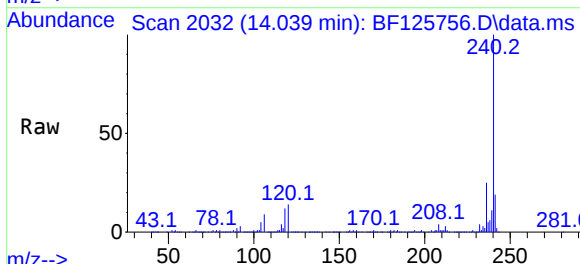




#79
Terphenyl-d14
Concen: 63.19 ng
RT: 12.992 min Scan# 1854
Delta R.T. 0.000 min
Lab File: BF125756.D
Acq: 1 Oct 2021 17:11

Instrument :
BNA_F
ClientSampleId :
MW-SIDEWALK

Tgt Ion:244 Resp: 1637925
Ion Ratio Lower Upper
244 100
212 6.5 5.9 8.9
122 11.4 9.0 13.4

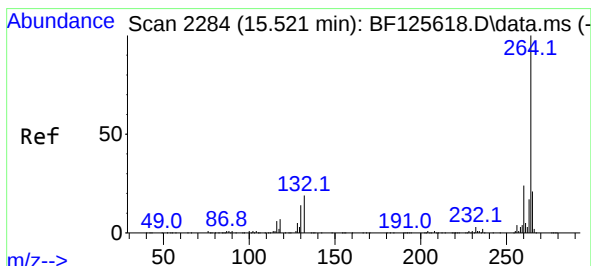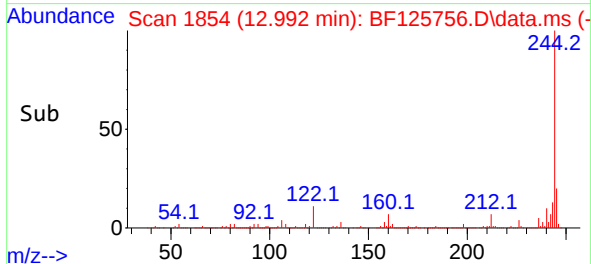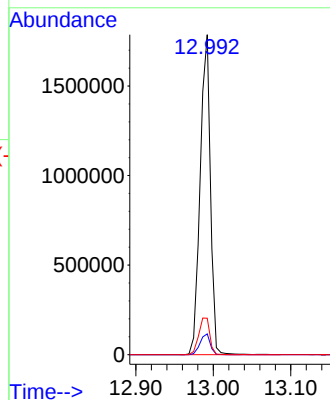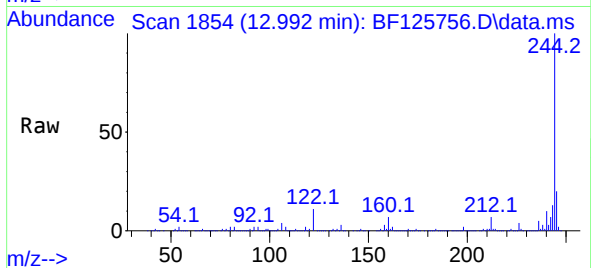

#86
Perylene-d12
Concen: 20.00 ng
RT: 15.515 min Scan# 2283
Delta R.T. -0.006 min
Lab File: BF125756.D
Acq: 1 Oct 2021 17:11

Tgt Ion:264 Resp: 460794
Ion Ratio Lower Upper
264 100
260 24.0 19.6 29.4
265 21.2 17.2 25.8

