

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF100121\  
 Data File : BF125745.D  
 Acq On : 1 Oct 2021 11:05  
 Operator : JU/CG  
 Sample : PB139493BS  
 Misc :  
 ALS Vial : 4 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 PB139493BS

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF092421.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF125745.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 2.240       | 17            | 26          | 34           | rVB      | 86585          | 120223        | 1.43%           | 0.046%        |
| 2         | 2.740       | 106           | 111         | 121          | rVB      | 362647         | 517472        | 6.15%           | 0.196%        |
| 3         | 3.446       | 223           | 231         | 237          | rBV      | 461406         | 897668        | 10.68%          | 0.340%        |
| 4         | 3.499       | 237           | 240         | 266          | rVB      | 470961         | 1272209       | 15.13%          | 0.482%        |
| 5         | 5.516       | 577           | 583         | 586          | rBV      | 5083880        | 5448214       | 64.80%          | 2.063%        |
| 6         | 6.440       | 736           | 740         | 743          | rBV      | 2270726        | 1875561       | 22.31%          | 0.710%        |
| 7         | 6.522       | 747           | 754         | 757          | rBV2     | 4493929        | 7641582       | 90.89%          | 2.893%        |
| 8         | 6.551       | 757           | 759         | 763          | rVV      | 2269491        | 1981020       | 23.56%          | 0.750%        |
| 9         | 6.622       | 767           | 771         | 774          | rVB      | 1859900        | 1662294       | 19.77%          | 0.629%        |
| 10        | 6.675       | 774           | 780         | 783          | rBV      | 2460235        | 2230467       | 26.53%          | 0.844%        |
| 11        | 6.834       | 803           | 807         | 810          | rBV      | 3058949        | 2581906       | 30.71%          | 0.978%        |
| 12        | 6.893       | 813           | 817         | 818          | rBV      | 1397271        | 1589012       | 18.90%          | 0.602%        |
| 13        | 6.910       | 818           | 820         | 823          | rVB      | 2954971        | 2285276       | 27.18%          | 0.865%        |
| 14        | 7.028       | 835           | 840         | 843          | rBV      | 2427890        | 2572479       | 30.60%          | 0.974%        |
| 15        | 7.057       | 843           | 845         | 849          | rVB      | 2814232        | 2539242       | 30.20%          | 0.961%        |
| 16        | 7.140       | 853           | 859         | 861          | rBV      | 2607577        | 2909690       | 34.61%          | 1.102%        |
| 17        | 7.163       | 861           | 863         | 867          | rVB      | 1555923        | 1689251       | 20.09%          | 0.640%        |
| 18        | 7.293       | 880           | 885         | 890          | rBV3     | 4891791        | 6627785       | 78.83%          | 2.509%        |
| 19        | 7.404       | 900           | 904         | 907          | rBV      | 2390507        | 2038324       | 24.24%          | 0.772%        |
| 20        | 7.451       | 907           | 912         | 914          | rVV      | 3226820        | 4171011       | 49.61%          | 1.579%        |
| 21        | 7.469       | 914           | 915         | 918          | rVB      | 2164309        | 1394179       | 16.58%          | 0.528%        |
| 22        | 7.563       | 928           | 931         | 935          | rBV      | 429677         | 364904        | 4.34%           | 0.138%        |
| 23        | 7.710       | 950           | 956         | 961          | rBV      | 2237371        | 2558316       | 30.43%          | 0.969%        |
| 24        | 7.787       | 964           | 969         | 971          | rBV      | 1758425        | 1605004       | 19.09%          | 0.608%        |
| 25        | 7.822       | 971           | 975         | 977          | rVB      | 3084153        | 2802396       | 33.33%          | 1.061%        |
| 26        | 7.916       | 980           | 991         | 994          | rBV      | 2357016        | 3040145       | 36.16%          | 1.151%        |
| 27        | 8.028       | 1004          | 1010        | 1013         | rBV      | 2564215        | 2473453       | 29.42%          | 0.936%        |
| 28        | 8.110       | 1019          | 1024        | 1028         | rVB      | 2825828        | 2851718       | 33.92%          | 1.080%        |
| 29        | 8.175       | 1029          | 1035        | 1036         | rBV      | 1953051        | 2092301       | 24.89%          | 0.792%        |
| 30        | 8.192       | 1036          | 1038        | 1041         | rVB      | 3984797        | 3513920       | 41.79%          | 1.330%        |
| 31        | 8.240       | 1041          | 1046        | 1049         | rBV      | 2205930        | 1965556       | 23.38%          | 0.744%        |
| 32        | 8.310       | 1054          | 1058        | 1062         | rVB      | 2612894        | 2512679       | 29.88%          | 0.951%        |
| 33        | 8.610       | 1104          | 1109        | 1111         | rBV      | 838796         | 958259        | 11.40%          | 0.363%        |
| 34        | 8.645       | 1111          | 1115        | 1122         | rVV2     | 210601         | 552463        | 6.57%           | 0.209%        |
| 35        | 8.722       | 1122          | 1128        | 1131         | rVB      | 2490075        | 2499120       | 29.72%          | 0.946%        |
| 36        | 8.834       | 1140          | 1147        | 1151         | rBV      | 1189108        | 1001671       | 11.91%          | 0.379%        |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF100121\  
 Data File : BF125745.D  
 Acq On : 1 Oct 2021 11:05  
 Operator : JU/CG  
 Sample : PB139493BS  
 Misc :  
 ALS Vial : 4 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 PB139493BS

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF092421.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

|    |        |      |      |      |      |         |         |         |        |
|----|--------|------|------|------|------|---------|---------|---------|--------|
| 37 | 8.887  | 1151 | 1156 | 1159 | rVV  | 4717081 | 4268135 | 50.76%  | 1.616% |
| 38 | 8.940  | 1161 | 1165 | 1168 | rVV  | 176759  | 171852  | 2.04%   | 0.065% |
| 39 | 8.987  | 1168 | 1173 | 1176 | rVV  | 4359107 | 4067905 | 48.38%  | 1.540% |
| 40 | 9.045  | 1176 | 1183 | 1187 | rVB2 | 4688977 | 6444600 | 76.65%  | 2.440% |
| 41 | 9.157  | 1197 | 1202 | 1205 | rBV  | 2621822 | 2629667 | 31.28%  | 0.996% |
| 42 | 9.198  | 1205 | 1209 | 1212 | rVV  | 2905046 | 2555041 | 30.39%  | 0.967% |
| 43 | 9.251  | 1212 | 1218 | 1221 | rVB  | 6875826 | 7115199 | 84.63%  | 2.694% |
| 44 | 9.351  | 1229 | 1235 | 1237 | rBV  | 4873177 | 4696245 | 55.86%  | 1.778% |
| 45 | 9.375  | 1237 | 1239 | 1242 | rVB  | 4186976 | 3184248 | 37.87%  | 1.206% |
| 46 | 9.469  | 1247 | 1255 | 1258 | rBV  | 2054002 | 2006066 | 23.86%  | 0.760% |
| 47 | 9.604  | 1274 | 1278 | 1280 | rVV  | 1588722 | 1322934 | 15.73%  | 0.501% |
| 48 | 9.651  | 1280 | 1286 | 1288 | rVV  | 3259217 | 3067553 | 36.48%  | 1.161% |
| 49 | 9.681  | 1288 | 1291 | 1293 | rVV  | 1553112 | 1522371 | 18.11%  | 0.576% |
| 50 | 9.710  | 1293 | 1296 | 1299 | rVV  | 2236252 | 1898194 | 22.58%  | 0.719% |
| 51 | 9.769  | 1299 | 1306 | 1307 | rVV  | 1239399 | 1306730 | 15.54%  | 0.495% |
| 52 | 9.792  | 1307 | 1310 | 1313 | rVB  | 4307965 | 3735032 | 44.42%  | 1.414% |
| 53 | 9.875  | 1320 | 1324 | 1327 | rVB  | 1675810 | 1458968 | 17.35%  | 0.552% |
| 54 | 9.928  | 1328 | 1333 | 1335 | rBV  | 2428889 | 2061014 | 24.51%  | 0.780% |
| 55 | 9.963  | 1335 | 1339 | 1341 | rVV  | 5084258 | 4861513 | 57.82%  | 1.841% |
| 56 | 9.981  | 1341 | 1342 | 1345 | rVV  | 2061795 | 1278923 | 15.21%  | 0.484% |
| 57 | 10.034 | 1345 | 1351 | 1354 | rVV  | 2416751 | 2577288 | 30.65%  | 0.976% |
| 58 | 10.075 | 1354 | 1358 | 1360 | rVV  | 915790  | 805738  | 9.58%   | 0.305% |
| 59 | 10.110 | 1360 | 1364 | 1366 | rVV  | 2172294 | 2165781 | 25.76%  | 0.820% |
| 60 | 10.134 | 1366 | 1368 | 1371 | rVB  | 4239027 | 3409986 | 40.56%  | 1.291% |
| 61 | 10.204 | 1376 | 1380 | 1384 | rBV  | 2720750 | 2335550 | 27.78%  | 0.884% |
| 62 | 10.251 | 1384 | 1388 | 1391 | rVB  | 2673912 | 2359599 | 28.06%  | 0.893% |
| 63 | 10.351 | 1398 | 1405 | 1408 | rBV  | 3292193 | 3147939 | 37.44%  | 1.192% |
| 64 | 10.475 | 1420 | 1426 | 1431 | rBV3 | 5318027 | 8407869 | 100.00% | 3.183% |
| 65 | 10.516 | 1431 | 1433 | 1437 | rVV  | 1220521 | 1084450 | 12.90%  | 0.411% |
| 66 | 10.586 | 1439 | 1445 | 1448 | rVV  | 4731156 | 4107796 | 48.86%  | 1.555% |
| 67 | 10.628 | 1448 | 1452 | 1455 | rVB  | 3487131 | 3015713 | 35.87%  | 1.142% |
| 68 | 10.716 | 1461 | 1467 | 1471 | rBV  | 4381786 | 4293924 | 51.07%  | 1.626% |
| 69 | 10.957 | 1503 | 1508 | 1511 | rBV  | 3164105 | 2565071 | 30.51%  | 0.971% |
| 70 | 11.028 | 1515 | 1520 | 1523 | rBV  | 3010555 | 2785661 | 33.13%  | 1.055% |
| 71 | 11.110 | 1527 | 1534 | 1537 | rBV  | 2995198 | 2678533 | 31.86%  | 1.014% |
| 72 | 11.216 | 1547 | 1552 | 1562 | rBV  | 3958352 | 3729174 | 44.35%  | 1.412% |
| 73 | 11.292 | 1562 | 1565 | 1571 | rVB2 | 147864  | 128274  | 1.53%   | 0.049% |
| 74 | 11.410 | 1581 | 1585 | 1587 | rBV  | 1991303 | 1977387 | 23.52%  | 0.749% |
| 75 | 11.439 | 1587 | 1590 | 1593 | rVV  | 5011597 | 4249016 | 50.54%  | 1.609% |
| 76 | 11.492 | 1593 | 1599 | 1602 | rVV  | 4755015 | 4305391 | 51.21%  | 1.630% |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF100121\  
 Data File : BF125745.D  
 Acq On : 1 Oct 2021 11:05  
 Operator : JU/CG  
 Sample : PB139493BS  
 Misc :  
 ALS Vial : 4 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 PB139493BS

Integration Parameters: rteint.p  
 Integrator: RTE  
 Smoothing : OFF Filtering: 5  
 Sampling : 1 Min Area: 1 % of largest Peak  
 Start Thrs: 0.2 Max Peaks: 100  
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >  
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF092421.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

|    |        |      |      |      |      |         |         |        |        |
|----|--------|------|------|------|------|---------|---------|--------|--------|
| 77 | 11.639 | 1620 | 1624 | 1627 | rVB  | 4097238 | 3625470 | 43.12% | 1.373% |
| 78 | 11.969 | 1676 | 1680 | 1684 | rBV  | 3727313 | 3166014 | 37.66% | 1.199% |
| 79 | 12.622 | 1787 | 1791 | 1795 | rBV  | 4155171 | 3854495 | 45.84% | 1.459% |
| 80 | 12.739 | 1807 | 1811 | 1815 | rBV  | 2564108 | 2365188 | 28.13% | 0.895% |
| 81 | 12.851 | 1825 | 1830 | 1834 | rBV  | 3981278 | 3881397 | 46.16% | 1.470% |
| 82 | 12.998 | 1850 | 1855 | 1858 | rBV  | 5849401 | 5758993 | 68.50% | 2.180% |
| 83 | 13.157 | 1878 | 1882 | 1888 | rBV  | 358049  | 358994  | 4.27%  | 0.136% |
| 84 | 13.469 | 1931 | 1935 | 1938 | rBV  | 2680268 | 2196161 | 26.12% | 0.832% |
| 85 | 13.498 | 1938 | 1940 | 1943 | rVV  | 468116  | 403091  | 4.79%  | 0.153% |
| 86 | 13.533 | 1943 | 1946 | 1949 | rVV  | 3004213 | 2416232 | 28.74% | 0.915% |
| 87 | 13.598 | 1953 | 1957 | 1961 | rVB  | 113723  | 93813   | 1.12%  | 0.036% |
| 88 | 13.998 | 2021 | 2025 | 2027 | rBV  | 1763428 | 1475060 | 17.54% | 0.558% |
| 89 | 14.033 | 2027 | 2031 | 2035 | rVV3 | 3502622 | 5996654 | 71.32% | 2.270% |
| 90 | 14.074 | 2035 | 2038 | 2041 | rVB  | 3722506 | 3015768 | 35.87% | 1.142% |
| 91 | 14.251 | 2064 | 2068 | 2075 | rBV  | 405201  | 378805  | 4.51%  | 0.143% |
| 92 | 14.451 | 2097 | 2102 | 2106 | rVB2 | 85543   | 105211  | 1.25%  | 0.040% |
| 93 | 14.639 | 2130 | 2134 | 2138 | rBV  | 2308082 | 2018341 | 24.01% | 0.764% |
| 94 | 15.092 | 2205 | 2211 | 2213 | rBV  | 2538652 | 2854304 | 33.95% | 1.081% |
| 95 | 15.121 | 2213 | 2216 | 2220 | rVB  | 2663827 | 2751154 | 32.72% | 1.042% |
| 96 | 15.463 | 2268 | 2274 | 2279 | rBV  | 2281838 | 2885512 | 34.32% | 1.093% |
| 97 | 15.521 | 2279 | 2284 | 2288 | rBV  | 968474  | 1154873 | 13.74% | 0.437% |
| 98 | 17.027 | 2528 | 2540 | 2553 | rBV2 | 2170744 | 5712587 | 67.94% | 2.163% |
| 99 | 17.468 | 2604 | 2615 | 2627 | rBV  | 1352163 | 3032496 | 36.07% | 1.148% |




Sum of corrected areas: 264119713

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF100121\  
Data File : BF125745.D  
Acq On : 1 Oct 2021 11:05  
Operator : JU/CG  
Sample : PB139493BS  
Misc :  
ALS Vial : 4 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
PB139493BS

Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF092421.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

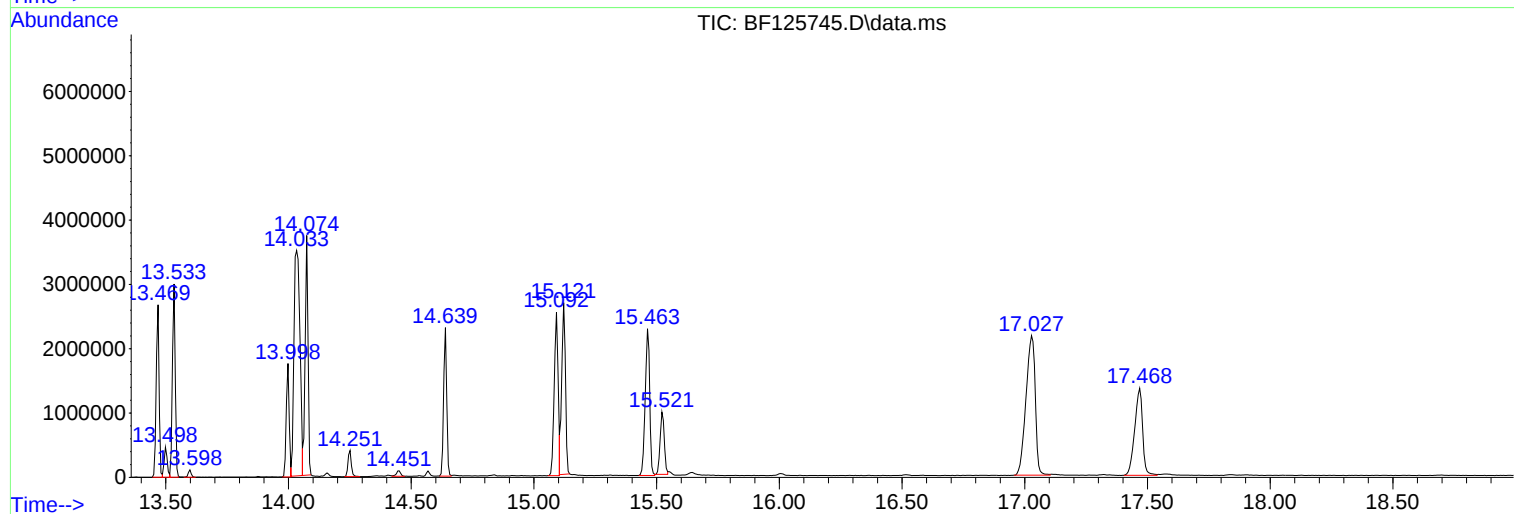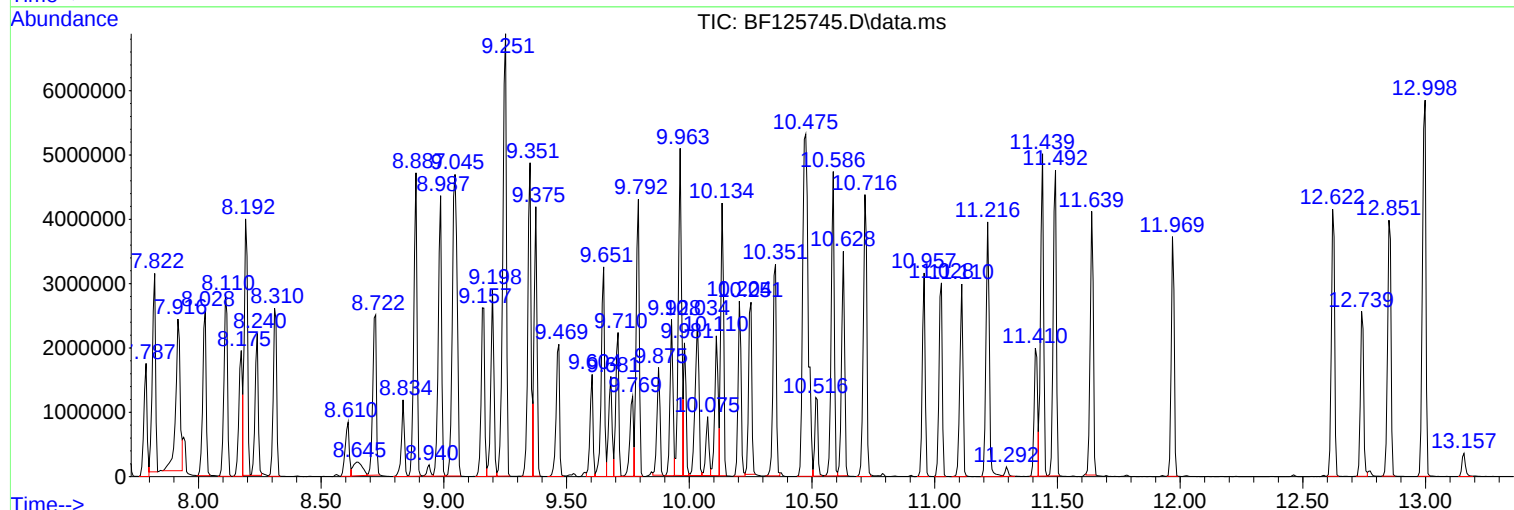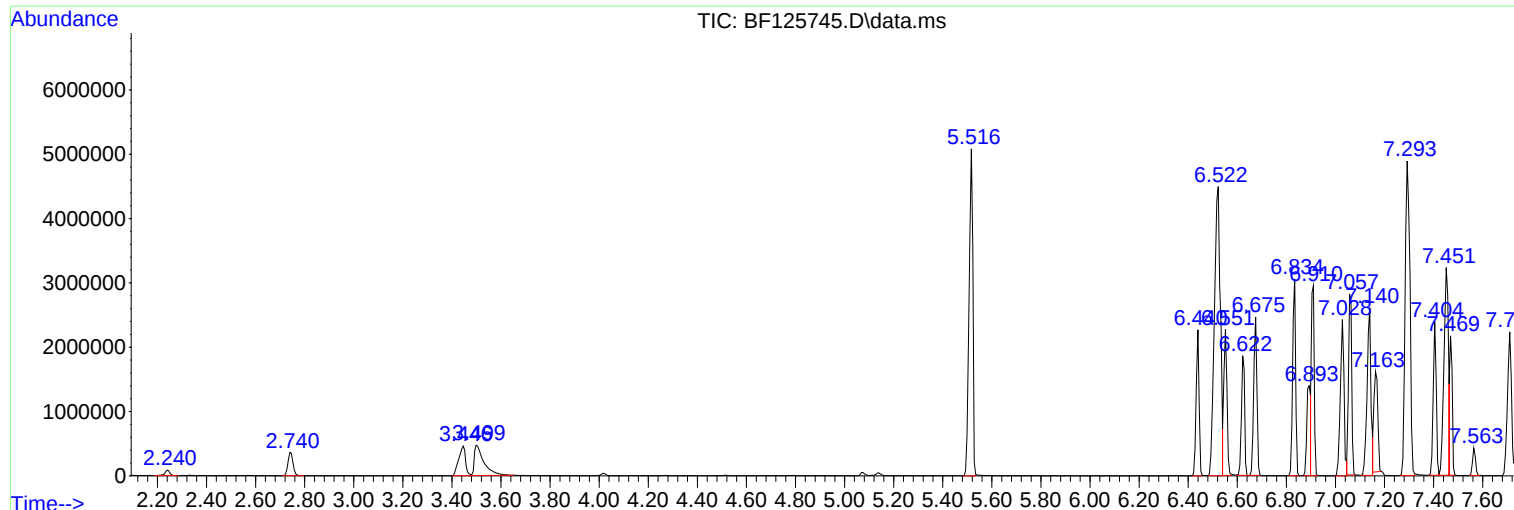

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF100121\  
Data File : BF125745.D  
Acq On : 1 Oct 2021 11:05  
Operator : JU/CG  
Sample : PB139493BS  
Misc :  
ALS Vial : 4 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
PB139493BS

Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF092421.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION










TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

\*\*\*\*\*

Peak Number 1 2-Methylindoline Concentration Rank 3

| R.T.  | EstConc | Area   | Relative to ISTD | R.T.  |
|-------|---------|--------|------------------|-------|
| 7.563 | 3.49 ng | 364904 | Naphthalene-d8   | 8.175 |

| Hit# | of | 5 | Tentative ID                        | MW  | MolForm   | CAS#        | Qual |
|------|----|---|-------------------------------------|-----|-----------|-------------|------|
| 1    |    |   | 2-Methylindoline                    | 133 | C9H11N    | 006872-06-6 | 47   |
| 2    |    |   | Ethanone, 1-phenyl-, o-(4-coumar... | 279 | C17H13NO3 | 034605-11-3 | 45   |
| 3    |    |   | Methanamine, N-(1-phenylethylide... | 133 | C9H11N    | 006907-71-7 | 33   |
| 4    |    |   | 1H-Benzimidazole                    | 118 | C7H6N2    | 000051-17-2 | 27   |
| 5    |    |   | Benzeneacetic acid, phenyl ester    | 212 | C14H12O2  | 000722-01-0 | 12   |

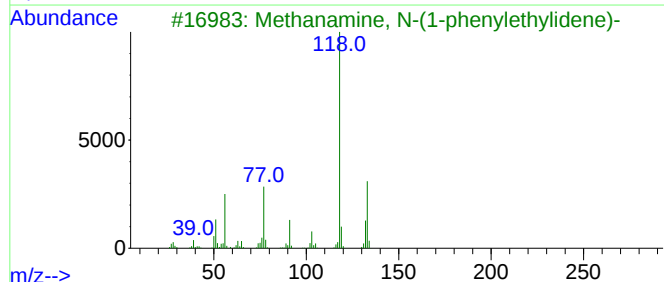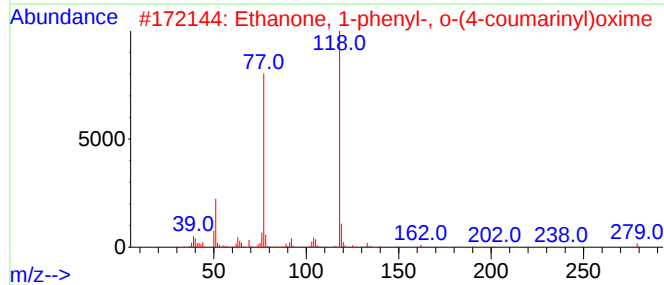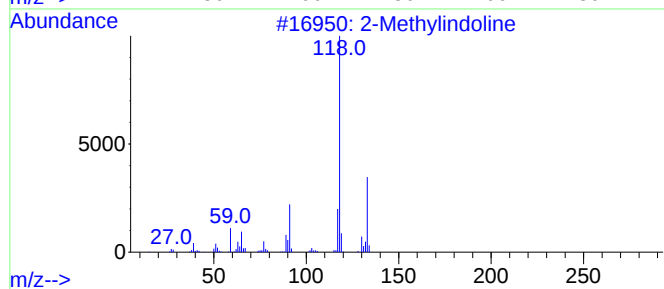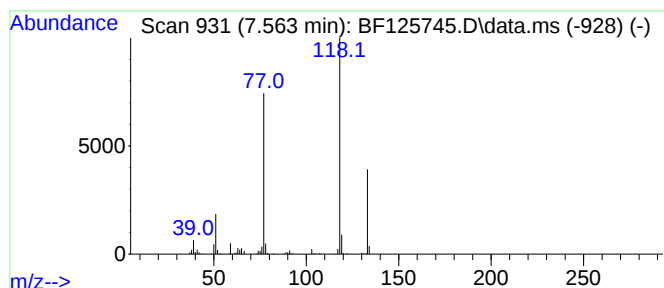

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF100121\  
Data File : BF125745.D  
Acq On : 1 Oct 2021 11:05  
Operator : JU/CG  
Sample : PB139493BS  
Misc :  
ALS Vial : 4 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
PB139493BS

Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF092421.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION










TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

\*\*\*\*\*

Peak Number 2 4-Chloroaniline, N-isopropy... Concentration Rank 1

| R.T.  | EstConc | Area    | Relative to ISTD | R.T.  |
|-------|---------|---------|------------------|-------|
| 8.834 | 9.57 ng | 1001670 | Naphthalene-d8   | 8.175 |

| Hit# | of | 5 | Tentative ID                        | MW  | MolForm   | CAS#         | Qual |
|------|----|---|-------------------------------------|-----|-----------|--------------|------|
| 1    |    |   | 4-Chloroaniline, N-isopropylidene   | 167 | C9H10ClN  | 040938-43-0  | 96   |
| 2    |    |   | 5-Aminopyrimidine, N-trimethylsi... | 167 | C7H13N3Si | 1000493-88-4 | 38   |
| 3    |    |   | Benzenamine, N,N-diethyl-4-fluoro-  | 167 | C10H14FN  | 000347-39-7  | 38   |
| 4    |    |   | 5-Chlorobenzimidazole               | 152 | C7H5ClN2  | 004887-82-5  | 38   |
| 5    |    |   | 4-Amino-2-chlorobenzonitrile        | 152 | C7H5ClN2  | 020925-27-3  | 38   |

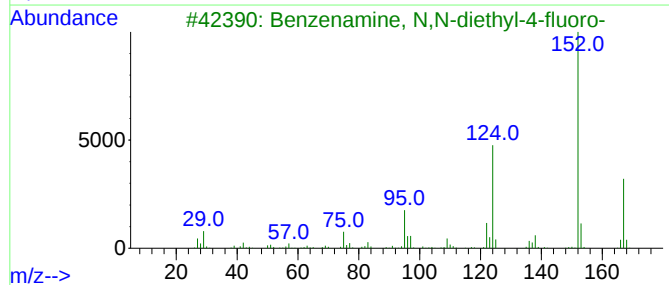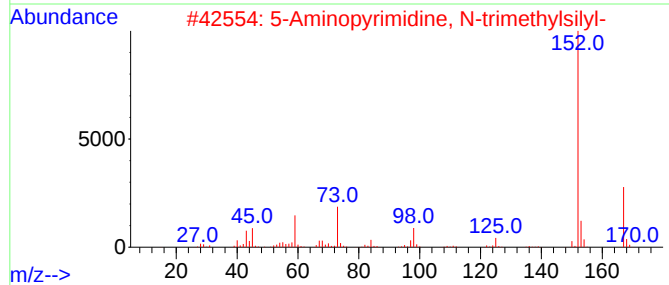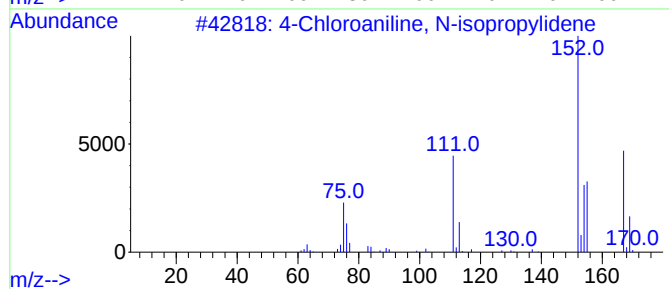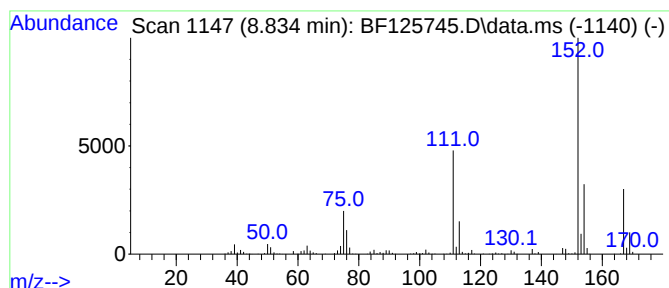

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF100121\  
Data File : BF125745.D  
Acq On : 1 Oct 2021 11:05  
Operator : JU/CG  
Sample : PB139493BS  
Misc :  
ALS Vial : 4 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
PB139493BS

Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF092421.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P










\*\*\*\*\*

Peak Number 3 Hexanedioic acid, bis(2-eth... Concentration Rank 2

| R.T.   | EstConc | Area    | Relative to ISTD | R.T.   |
|--------|---------|---------|------------------|--------|
| 13.533 | 8.06 ng | 2416230 | Chrysene-d12     | 14.051 |

| Hit# | of | 5 | Tentative ID                        | MW  | MolForm  | CAS#         | Qual |
|------|----|---|-------------------------------------|-----|----------|--------------|------|
| 1    |    |   | Hexanedioic acid, bis(2-ethylhex... | 370 | C22H42O4 | 000103-23-1  | 91   |
| 2    |    |   | Hexanedioic acid, dioctyl ester     | 370 | C22H42O4 | 000123-79-5  | 90   |
| 3    |    |   | Adipic acid, 2-ethylhexyl octyl ... | 370 | C22H42O4 | 1000324-48-6 | 90   |
| 4    |    |   | Hexanedioic acid, mono(2-ethylhe... | 258 | C14H26O4 | 004337-65-9  | 68   |
| 5    |    |   | Adipic acid, 2-ethylhexyl isobut... | 314 | C18H34O4 | 1010324-48-0 | 64   |

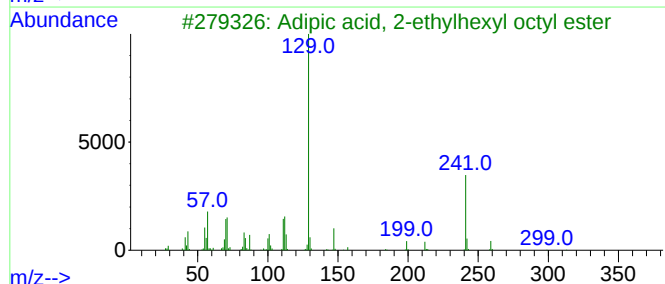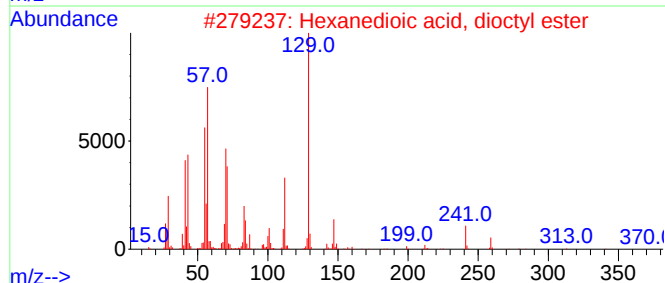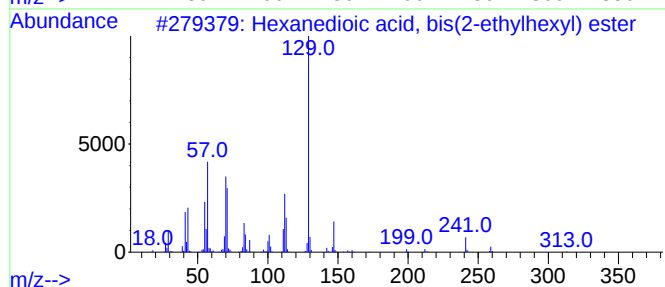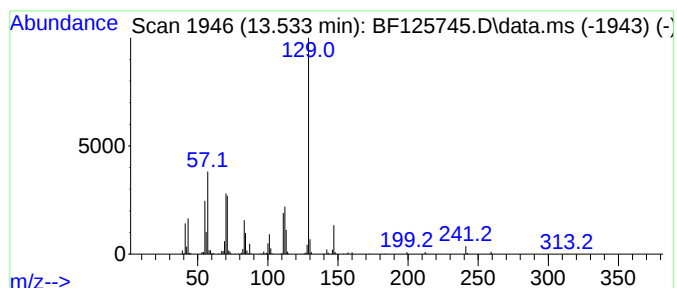

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF100121\  
Data File : BF125745.D  
Acq On : 1 Oct 2021 11:05  
Operator : JU/CG  
Sample : PB139493BS  
Misc :  
ALS Vial : 4 Sample Multiplier: 1

Instrument :  
BNA\_F  
ClientSampleId :  
PB139493BS

Quant Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF092421.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name   | RT     | EstConc | Units | Response | --Internal Standard-- |        |         |      |
|--------------------|--------|---------|-------|----------|-----------------------|--------|---------|------|
|                    |        |         |       |          | #                     | RT     | Resp    | Conc |
| 2-Methylindoline   | 7.563  | 3.5     | ng    | 364904   | 2                     | 8.175  | 2092300 | 20.0 |
| 4-Chloroaniline... | 8.834  | 9.6     | ng    | 1001670  | 2                     | 8.175  | 2092300 | 20.0 |
| Hexanedioic aci... | 13.533 | 8.1     | ng    | 2416230  | 5                     | 14.051 | 5996650 | 20.0 |