

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100121\
 Data File : BF125747.D
 Acq On : 1 Oct 2021 12:06
 Operator : JU/CG
 Sample : PB139485BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB139485BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF092421.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF125747.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.234	18	25	30	rVB	85708	114433	1.85%	0.308%
2	5.516	577	583	586	rBV	4555805	4524174	73.22%	12.195%
3	6.510	746	752	755	rBV	4264839	4861379	78.68%	13.104%
4	6.887	813	816	820	rVB	1580121	1264326	20.46%	3.408%
5	7.445	906	911	914	rBV	2944865	3133694	50.72%	8.447%
6	8.169	1029	1034	1037	rBV	2064239	1763705	28.54%	4.754%
7	9.245	1211	1217	1220	rBV	6690806	6178781	100.00%	16.655%
8	9.922	1328	1332	1345	rBV	2334207	2047618	33.14%	5.519%
9	10.710	1462	1466	1484	rBV	3790482	3573683	57.84%	9.633%
10	11.410	1581	1585	1588	rBV	2129185	1905799	30.84%	5.137%
11	12.992	1850	1854	1858	rBV	5436660	5407825	87.52%	14.577%
12	14.045	2029	2033	2046	rVB	1219857	1135699	18.38%	3.061%
13	15.521	2279	2284	2300	rBV	844485	1187834	19.22%	3.202%




Sum of corrected areas: 37098950

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100121\
Data File : BF125747.D
Acq On : 1 Oct 2021 12:06
Operator : JU/CG
Sample : PB139485BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB139485BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF092421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

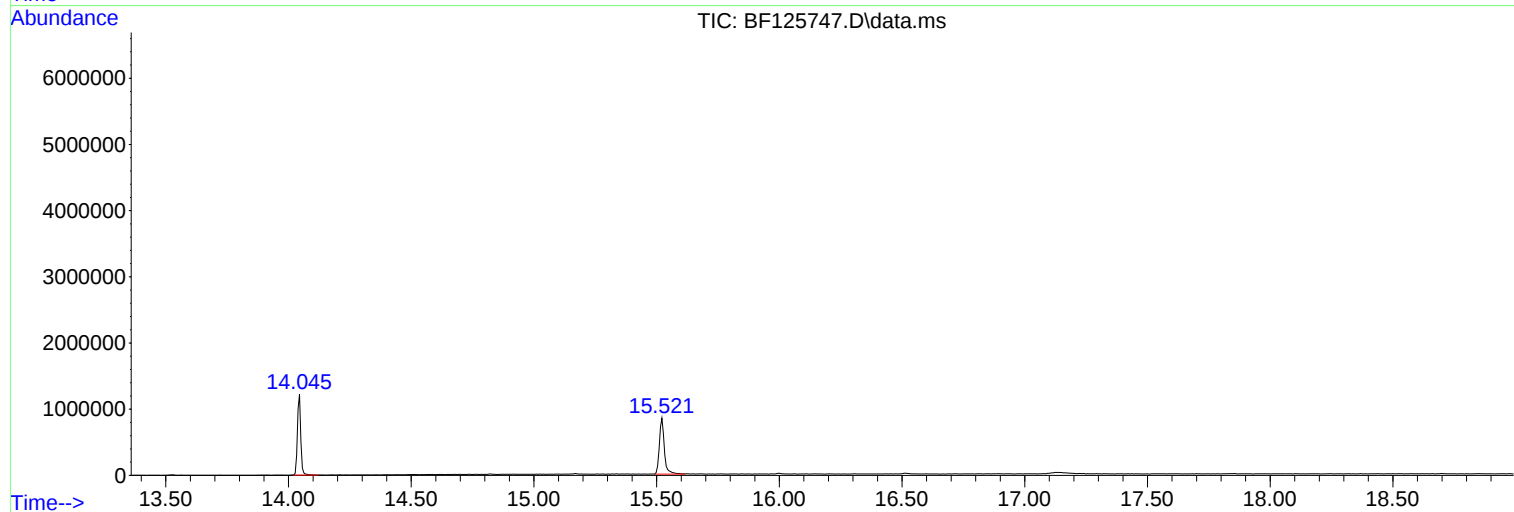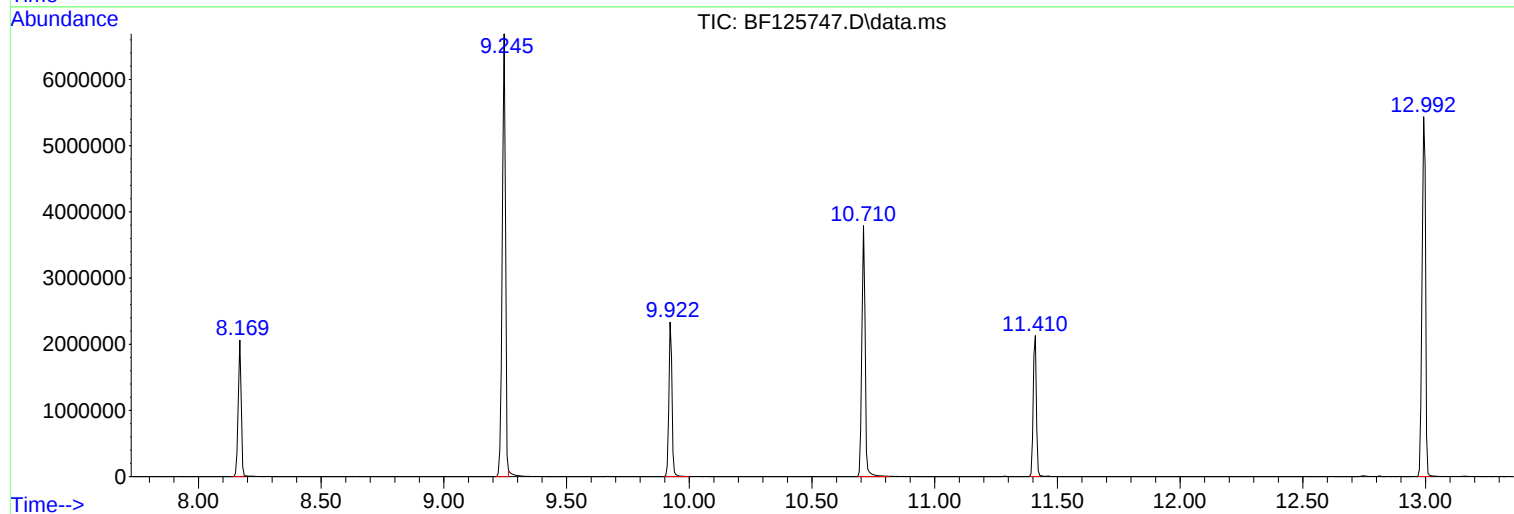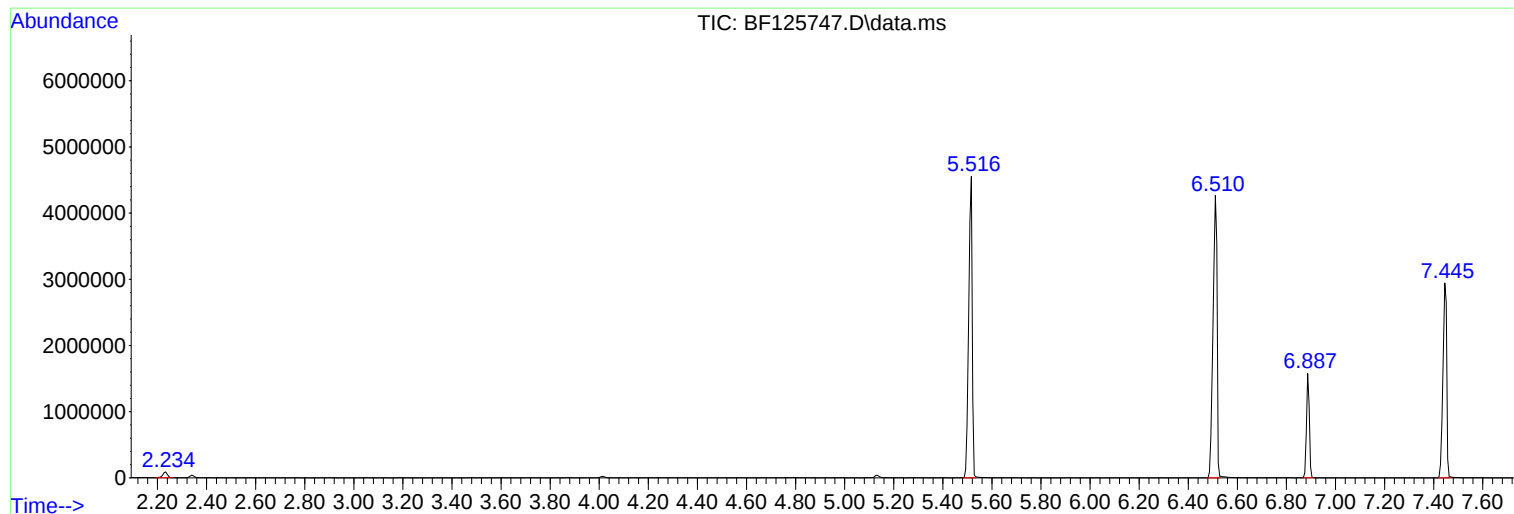

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100121\
Data File : BF125747.D
Acq On : 1 Oct 2021 12:06
Operator : JU/CG
Sample : PB139485BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB139485BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF092421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100121\
Data File : BF125747.D
Acq On : 1 Oct 2021 12:06
Operator : JU/CG
Sample : PB139485BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB139485BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF092421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------