

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100121\
 Data File : BF125750.D
 Acq On : 1 Oct 2021 13:42
 Operator : JU/CG
 Sample : PB139528BS
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB139528BS

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF092421.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF125750.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.763	110	115	128	rVB	452999	627974	6.73%	0.202%
2	3.469	226	235	240	rBV	537680	1112209	11.91%	0.358%
3	3.510	240	242	271	rVB	674143	1481032	15.86%	0.477%
4	5.134	511	518	530	rVB	883185	1393592	14.93%	0.448%
5	5.522	578	584	587	rBV	5575245	6304400	67.53%	2.028%
6	6.439	736	740	743	rBV	2239374	1788838	19.16%	0.576%
7	6.522	747	754	758	rBV2	4880488	9335297	100.00%	3.004%
8	6.551	758	759	766	rVV	2304346	1784321	19.11%	0.574%
9	6.628	767	772	775	rVB	2289622	2049194	21.95%	0.659%
10	6.675	776	780	784	rVV	2957358	2746072	29.42%	0.884%
11	6.833	803	807	810	rVB	3736475	3090153	33.10%	0.994%
12	6.892	813	817	818	rBV	1671147	1817124	19.47%	0.585%
13	6.910	818	820	823	rVB	3713155	2824374	30.25%	0.909%
14	7.033	835	841	843	rBV	2763908	3123769	33.46%	1.005%
15	7.063	843	846	849	rVB	3373921	3056127	32.74%	0.983%
16	7.139	853	859	861	rBV	3127635	3480147	37.28%	1.120%
17	7.163	861	863	867	rVB	1840510	2113049	22.64%	0.680%
18	7.292	879	885	891	rBV4	5432793	7981880	85.50%	2.568%
19	7.404	900	904	907	rBV	2654768	2465838	26.41%	0.793%
20	7.457	907	913	914	rVV	3817701	4660208	49.92%	1.499%
21	7.475	914	916	919	rVB	2701353	1905624	20.41%	0.613%
22	7.563	927	931	935	rBV	408104	373116	4.00%	0.120%
23	7.710	950	956	964	rBV	2246205	3166673	33.92%	1.019%
24	7.786	964	969	971	rBV	2257076	1985535	21.27%	0.639%
25	7.822	971	975	978	rVV	3760895	3536534	37.88%	1.138%
26	7.922	980	992	994	rVV	2935887	3797490	40.68%	1.222%
27	7.957	994	998	1000	rVV	705514	954435	10.22%	0.307%
28	8.028	1004	1010	1013	rBV	3413512	2980851	31.93%	0.959%
29	8.116	1019	1025	1028	rVB	3350579	3448311	36.94%	1.109%
30	8.175	1029	1035	1036	rBV	2453980	2494690	26.72%	0.803%
31	8.198	1036	1039	1041	rVB	4481130	4212351	45.12%	1.355%
32	8.239	1041	1046	1049	rBV	2650187	2188593	23.44%	0.704%
33	8.316	1054	1059	1062	rVB	3161705	3042472	32.59%	0.979%
34	8.616	1104	1110	1113	rBV	914205	1170159	12.53%	0.376%
35	8.657	1113	1117	1123	rVV2	231723	629721	6.75%	0.203%
36	8.722	1123	1128	1131	rVB	3287878	2991286	32.04%	0.962%

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100121\
 Data File : BF125750.D
 Acq On : 1 Oct 2021 13:42
 Operator : JU/CG
 Sample : PB139528BS
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB139528BS

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : OFF Filtering: 5
 Sampling : 1 Min Area: 1 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF092421.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	8.833	1140	1147	1150	rBV	1412579	1240247	13.29%	0.399%
38	8.886	1150	1156	1159	rVV	5460114	5050257	54.10%	1.625%
39	8.986	1168	1173	1176	rVV	5401675	4800739	51.43%	1.545%
40	9.045	1176	1183	1187	rVB3	5165331	7229789	77.45%	2.326%
41	9.163	1197	1203	1205	rBV	3335575	3314458	35.50%	1.066%
42	9.180	1205	1206	1207	rVV	1272787	845322	9.06%	0.272%
43	9.204	1207	1210	1213	rVV	3057756	2995852	32.09%	0.964%
44	9.251	1213	1218	1221	rVB	7798108	8026818	85.98%	2.583%
45	9.351	1229	1235	1237	rBV	5997537	5421176	58.07%	1.744%
46	9.375	1237	1239	1242	rVB	4732089	3980508	42.64%	1.281%
47	9.469	1246	1255	1258	rBV	2593988	2390014	25.60%	0.769%
48	9.604	1274	1278	1281	rVV	1856005	1616537	17.32%	0.520%
49	9.651	1281	1286	1288	rVV	3789108	3560935	38.14%	1.146%
50	9.680	1288	1291	1293	rVV	1689352	1803147	19.32%	0.580%
51	9.710	1293	1296	1299	rVB	2786502	2311185	24.76%	0.744%
52	9.769	1299	1306	1307	rBV	1574706	1445508	15.48%	0.465%
53	9.792	1307	1310	1313	rVB	5156499	4427358	47.43%	1.424%
54	9.880	1321	1325	1328	rVB	1914258	1770404	18.96%	0.570%
55	9.927	1328	1333	1336	rBV	2828020	2534891	27.15%	0.816%
56	9.963	1336	1339	1341	rVV	5638911	5531787	59.26%	1.780%
57	9.986	1341	1343	1346	rVV	2526938	1794888	19.23%	0.577%
58	10.039	1346	1352	1355	rVV	2826998	2950656	31.61%	0.949%
59	10.074	1355	1358	1361	rVV	954692	873245	9.35%	0.281%
60	10.116	1361	1365	1366	rVV	2625401	2436999	26.11%	0.784%
61	10.133	1366	1368	1372	rVB	4526982	4123966	44.18%	1.327%
62	10.210	1376	1381	1384	rBV	2941091	2759683	29.56%	0.888%
63	10.251	1384	1388	1391	rVB	3371345	2769845	29.67%	0.891%
64	10.351	1398	1405	1408	rBV	4093919	3698819	39.62%	1.190%
65	10.469	1419	1425	1429	rBV2	5922130	9084152	97.31%	2.923%
66	10.498	1429	1430	1431	rVV	1642781	676825	7.25%	0.218%
67	10.521	1431	1434	1437	rVV	1739989	1361125	14.58%	0.438%
68	10.586	1438	1445	1448	rVV	5210277	4746840	50.85%	1.527%
69	10.627	1448	1452	1455	rVB	4018947	3496626	37.46%	1.125%
70	10.721	1461	1468	1471	rBV	4788364	4722739	50.59%	1.519%
71	10.957	1504	1508	1511	rBV	3756780	2996877	32.10%	0.964%
72	11.027	1515	1520	1523	rVB	3665452	3243231	34.74%	1.043%
73	11.110	1529	1534	1537	rBV	3166527	3035413	32.52%	0.977%
74	11.216	1548	1552	1563	rBV	4469799	4335412	46.44%	1.395%
75	11.416	1581	1586	1587	rBV	2273039	2269796	24.31%	0.730%
76	11.439	1587	1590	1593	rVV	5621470	4899955	52.49%	1.576%

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100121\
 Data File : BF125750.D
 Acq On : 1 Oct 2021 13:42
 Operator : JU/CG
 Sample : PB139528BS
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB139528BS

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF092421.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

77	11.492	1593	1599	1602	rVV	5514521	4873684	52.21%	1.568%
78	11.639	1620	1624	1628	rVB	4207142	4137715	44.32%	1.331%
79	11.968	1677	1680	1684	rVB	3953087	3476930	37.24%	1.119%
80	12.627	1787	1792	1795	rBV	4533130	4251243	45.54%	1.368%
81	12.739	1807	1811	1815	rBV	1661150	1490334	15.96%	0.479%
82	12.851	1826	1830	1834	rVB	4196635	4250104	45.53%	1.367%
83	12.998	1850	1855	1858	rBV	5933316	5944617	63.68%	1.913%
84	13.157	1878	1882	1888	rBV	354154	373748	4.00%	0.120%
85	13.468	1931	1935	1938	rBV	2761291	2399132	25.70%	0.772%
86	13.533	1942	1946	1949	rVB	3202898	2655767	28.45%	0.854%
87	13.998	2021	2025	2027	rBV	2258527	1892720	20.27%	0.609%
88	14.039	2027	2032	2036	rVV3	3699938	6928988	74.22%	2.229%
89	14.074	2036	2038	2042	rVB	3776421	3214148	34.43%	1.034%
90	14.639	2130	2134	2138	rBV	2799680	2438411	26.12%	0.785%
91	15.092	2205	2211	2213	rBV	2910689	3476366	37.24%	1.118%
92	15.121	2213	2216	2220	rVV	3114395	3394973	36.37%	1.092%
93	15.462	2268	2274	2279	rBV	2731588	3542402	37.95%	1.140%
94	15.521	2279	2284	2288	rVV	1089844	1433148	15.35%	0.461%
95	15.556	2288	2290	2298	rVB	269339	279881	3.00%	0.090%
96	15.998	2359	2365	2372	rBV	232402	359448	3.85%	0.116%
97	16.515	2446	2453	2462	rBV	217904	381577	4.09%	0.123%
98	17.033	2526	2541	2550	rBV3	2544850	6928072	74.21%	2.229%
99	17.115	2550	2555	2565	rVB	143423	320481	3.43%	0.103%
100	17.468	2604	2615	2628	rBV	1661029	3681798	39.44%	1.185%

Sum of corrected areas: 310813150

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100121\
Data File : BF125750.D
Acq On : 1 Oct 2021 13:42
Operator : JU/CG
Sample : PB139528BS
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB139528BS









Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF092421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.134	15.34 ng	1393590	1,4-Dichlorobenzene-d4	6.892

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	56		
2	Propane, 2-methyl-2-(1-methyleth...	116	C7H16O	017348-59-3	23		
3	Acetic acid, cyano-, 1,1-dimethy...	141	C7H11NO2	001116-98-9	17		
4	1-Propen-2-ol, acetate	100	C5H8O2	000108-22-5	10		
5	5-Hexen-2-one	98	C6H10O	000109-49-9	9		

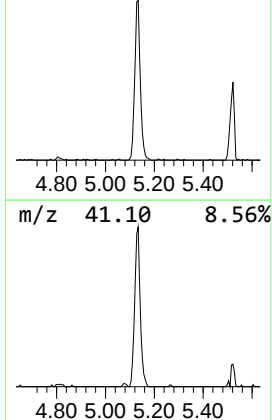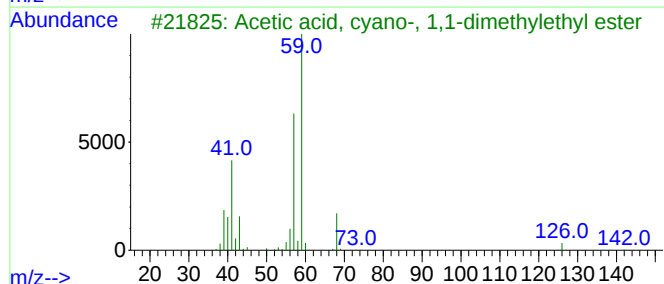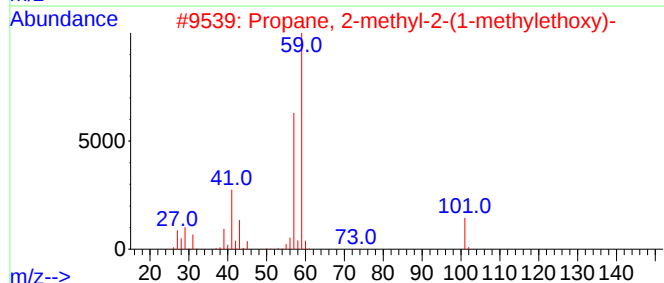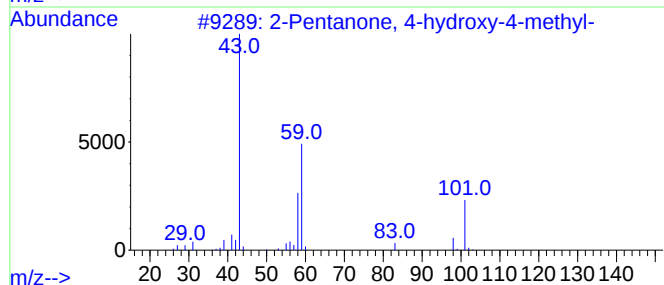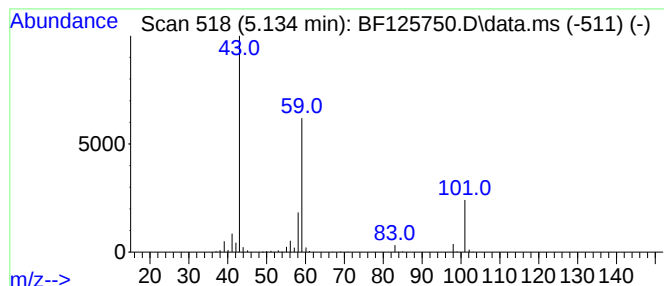

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100121\
Data File : BF125750.D
Acq On : 1 Oct 2021 13:42
Operator : JU/CG
Sample : PB139528BS
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB139528BS










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF092421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 3-Nitro-5-([(Z)-(1-phenylet... Concentration Rank 7

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.563	2.99 ng	373116	Naphthalene-d8	8.175

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			3-Nitro-5-([(Z)-(1-phenylethylidene)amino]oxy)benzylamine	300	C15H12N2O5	1000387-80-7	53
2			Methanamine, N-(1-phenylethylidene)-	133	C9H11N	006907-71-7	53
3			2-Methylindoline	133	C9H11N	006872-06-6	47
4			Ethanone, 1-phenyl-, o-(4-coumar...	279	C17H13NO3	034605-11-3	38
5			1H-Benzimidazole	118	C7H6N2	000051-17-2	27

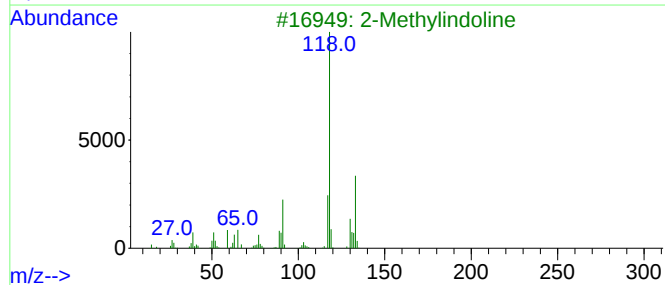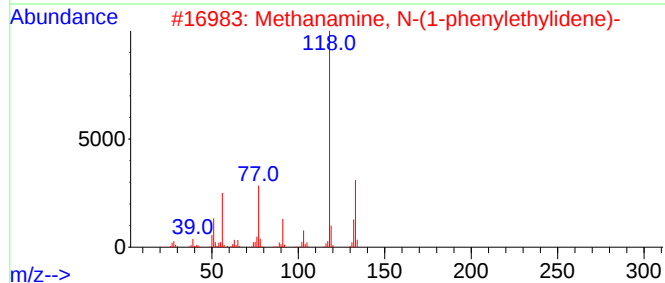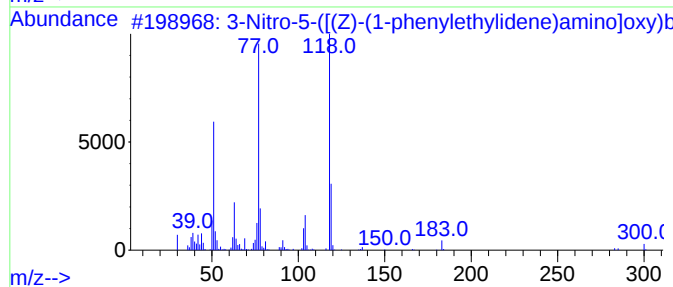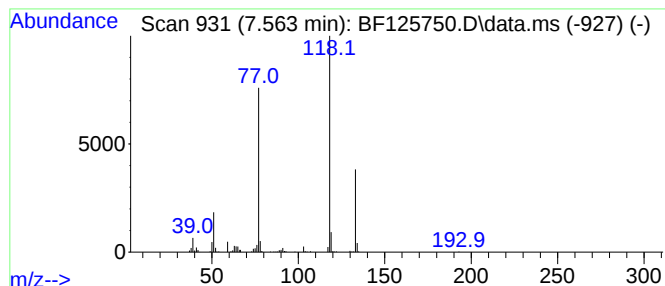

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100121\
Data File : BF125750.D
Acq On : 1 Oct 2021 13:42
Operator : JU/CG
Sample : PB139528BS
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB139528BS










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF092421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 3 4-Chloroaniline, N-isopropy... Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
8.833	9.94 ng	1240250	Naphthalene-d8	8.175

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			4-Chloroaniline, N-isopropylidene	167	C9H10ClN	040938-43-0	94
2			Benzonitrile, 2-amino-5-chloro-	152	C7H5ClN2	005922-60-1	38
3			Benzenamine, N,N-diethyl-4-fluoro-	167	C10H14FN	000347-39-7	38
4			4-Amino-2-chlorobenzonitrile	152	C7H5ClN2	020925-27-3	38
5			5-Aminopyrimidine, N-trimethylsi...	167	C7H13N3Si	1000493-88-4	38

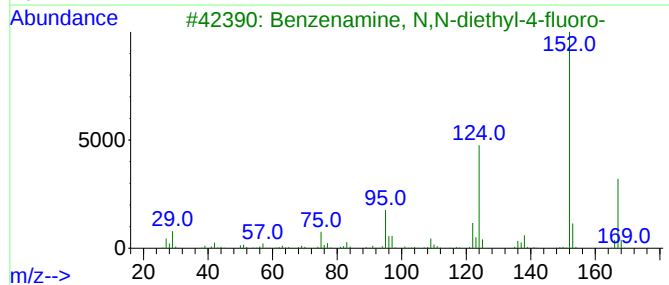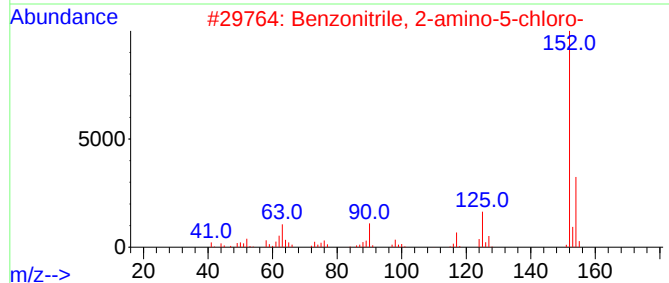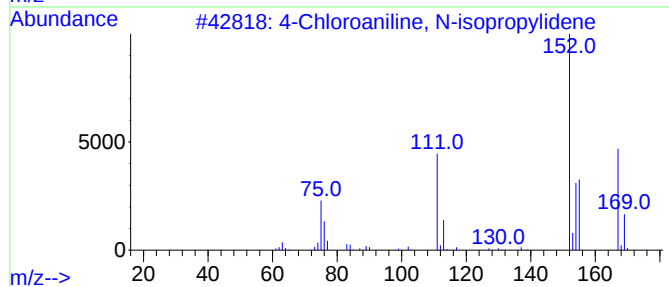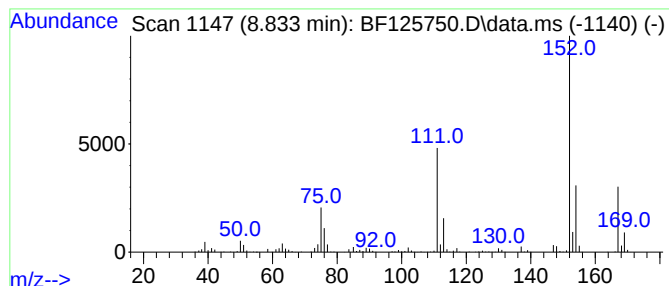

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100121\
Data File : BF125750.D
Acq On : 1 Oct 2021 13:42
Operator : JU/CG
Sample : PB139528BS
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB139528BS










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF092421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 4 Hexanedioic acid, bis(2-eth... Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
13.533	7.67 ng	2655770	Chrysene-d12	14.051

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Hexanedioic acid, bis(2-ethylhex...	370	C22H42O4	000103-23-1	91
2			Adipic acid, 2-ethylhexyl octyl ...	370	C22H42O4	1000324-48-6	90
3			Hexanedioic acid, dioctyl ester	370	C22H42O4	000123-79-5	76
4			Adipic acid, octyl 2-octyl ester	370	C22H42O4	1000324-45-0	64
5			Hexanedioic acid, mono(2-ethylhe...	258	C14H26O4	004337-65-9	62

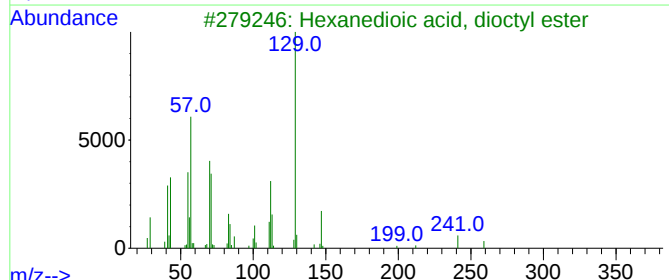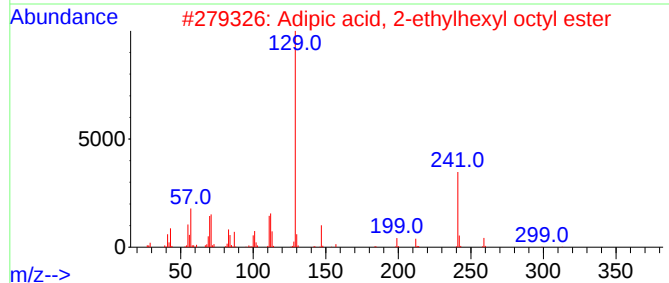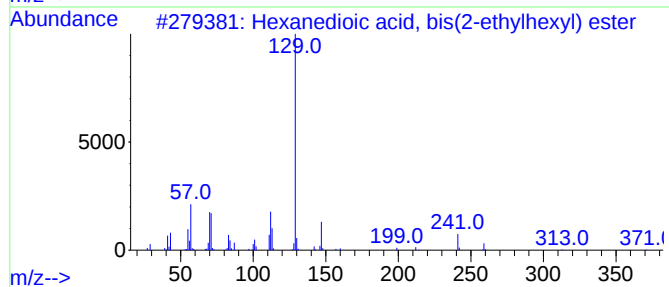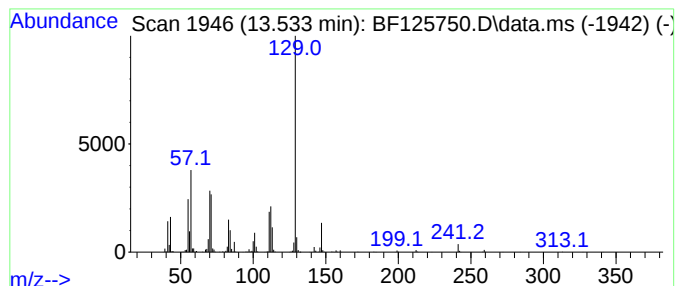

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100121\
Data File : BF125750.D
Acq On : 1 Oct 2021 13:42
Operator : JU/CG
Sample : PB139528BS
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB139528BS










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF092421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 5 Eicosane Concentration Rank 5

R.T.	EstConc	Area	Relative to ISTD	R.T.
15.998	5.02 ng	359448	Perylene-d12	15.521

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Eicosane	282	C20H42	000112-95-8	97
2			Heneicosane	296	C21H44	000629-94-7	91
3			Octacosane, 2-methyl-	408	C29H60	001560-98-1	91
4			Hexacosane	366	C26H54	000630-01-3	90
5			4-Methylheneicosane	310	C22H46	025117-29-7	90

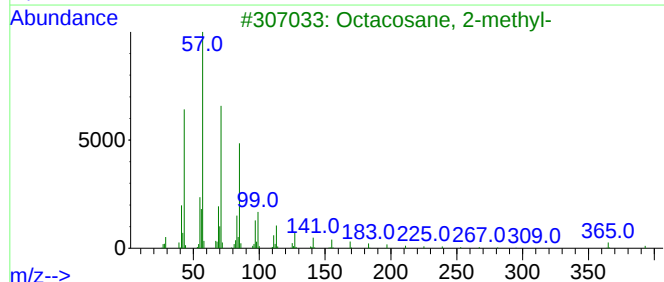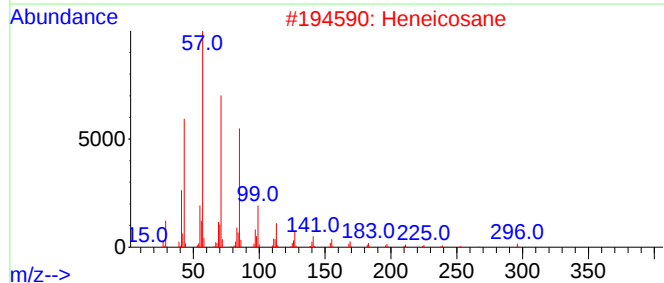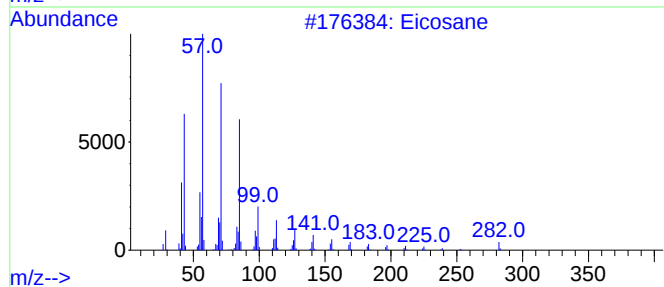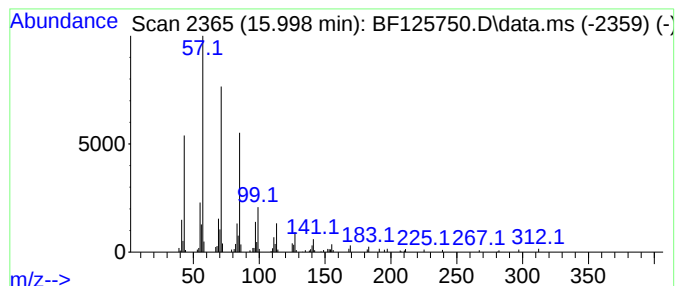

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100121\
Data File : BF125750.D
Acq On : 1 Oct 2021 13:42
Operator : JU/CG
Sample : PB139528BS
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB139528BS










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF092421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 6 Octacosane, 2-methyl- Concentration Rank 4

R.T.	EstConc	Area	Relative to ISTD	R.T.
16.515	5.33 ng	381577	Perylene-d12	15.521

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Octacosane, 2-methyl-	408	C29H60	001560-98-1	91
2			Dotriacontane, 1-iodo-	576	C32H65I	1000406-32-4	91
3			Pentadecane, 8-hexyl-	296	C21H44	013475-75-7	91
4			Hexacosane	366	C26H54	000630-01-3	90
5			Heneicosane	296	C21H44	000629-94-7	90

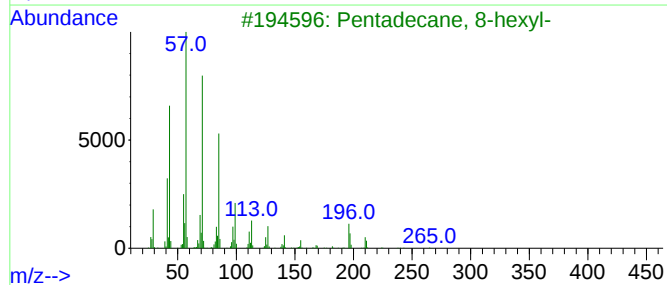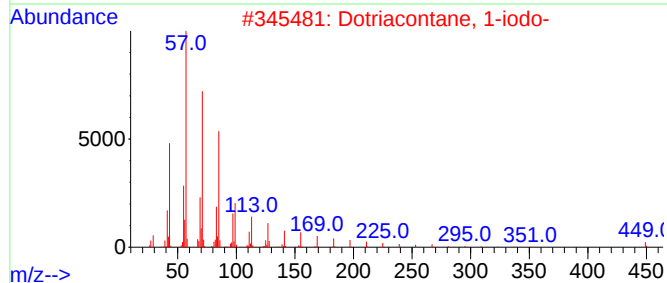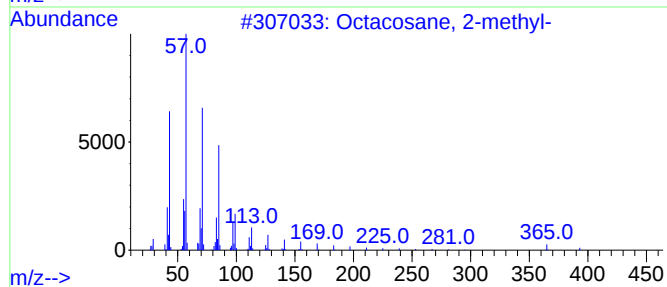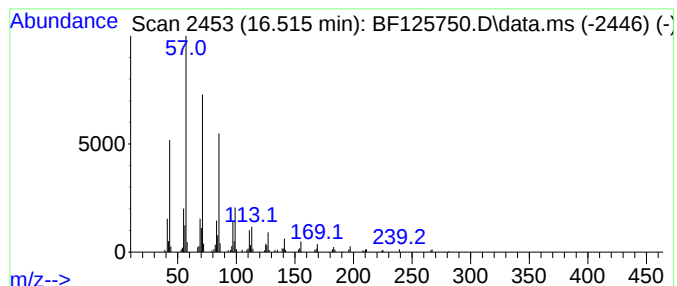

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100121\
Data File : BF125750.D
Acq On : 1 Oct 2021 13:42
Operator : JU/CG
Sample : PB139528BS
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB139528BS










Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF092421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 7 Eicosane Concentration Rank 6

R.T.	EstConc	Area	Relative to ISTD	R.T.
17.115	4.47 ng	320481	Perylene-d12	15.521

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Eicosane	282	C20H42	000112-95-8	94
2			Octacosane, 2-methyl-	408	C29H60	001560-98-1	91
3			Triacontane	422	C30H62	000638-68-6	91
4			Heptadecane, 9-octyl-	352	C25H52	007225-64-1	91
5			Octadecane, 1-iodo-	380	C18H37I	000629-93-6	91

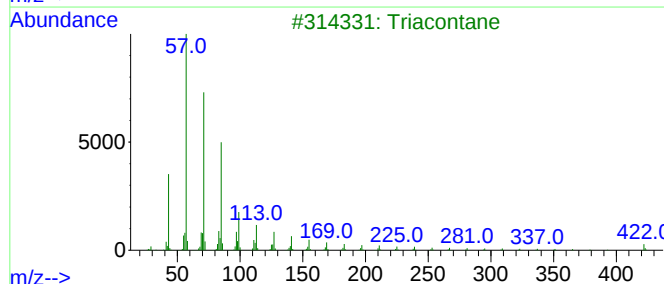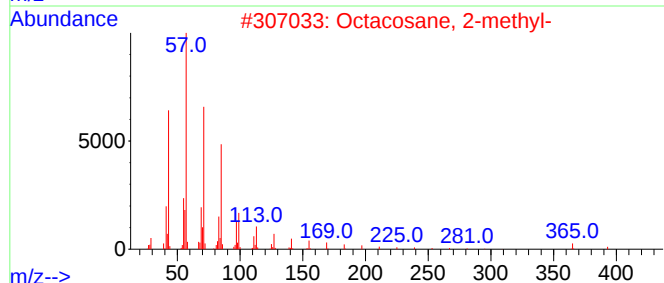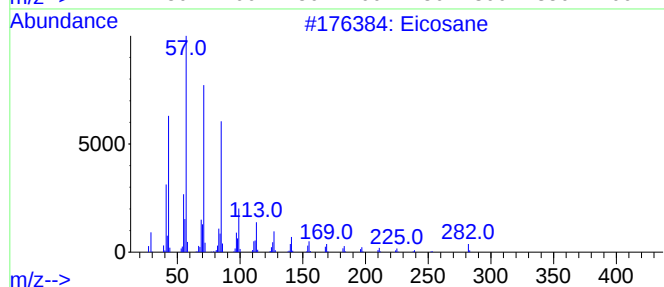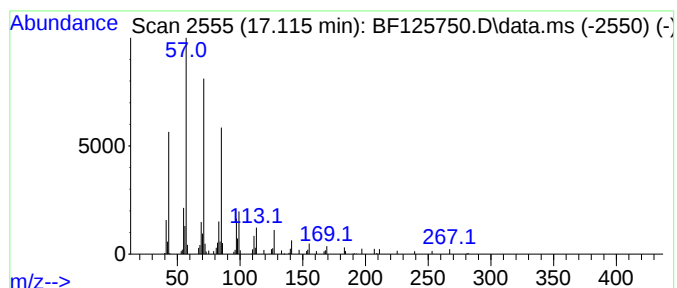

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100121\
Data File : BF125750.D
Acq On : 1 Oct 2021 13:42
Operator : JU/CG
Sample : PB139528BS
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB139528BS

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF092421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	5.134	15.3	ng	1393590	1	6.892	1817120	20.0
3-Nitro-5-[(Z)...	7.563	3.0	ng	373116	2	8.175	2494690	20.0
4-Chloroaniline...	8.833	9.9	ng	1240250	2	8.175	2494690	20.0
Hexanedioic aci...	13.533	7.7	ng	2655770	5	14.051	6928990	20.0
Eicosane	15.998	5.0	ng	359448	6	15.521	1433150	20.0
Octacosane, 2-m...	16.515	5.3	ng	381577	6	15.521	1433150	20.0
Eicosane	17.115	4.5	ng	320481	6	15.521	1433150	20.0