


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100121\
 Data File : BF125742.D
 Acq On : 1 Oct 2021 9:23
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF092421.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Sep 24 15:38:32 2021

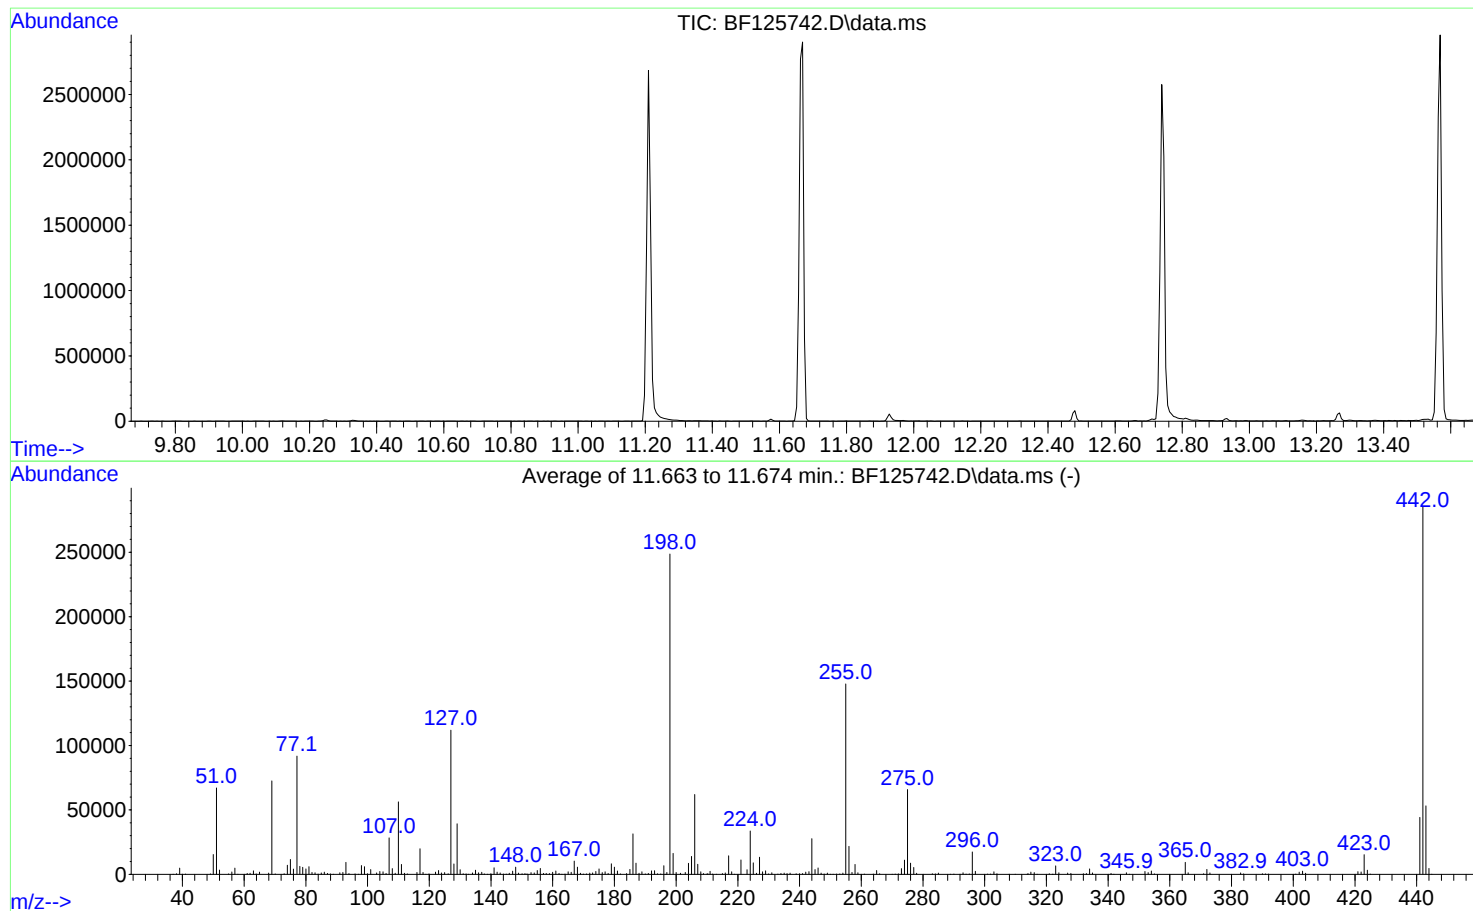




AutoFind: Scans 1628, 1629, 1630; Background Corrected with Scan 1622

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	27.0	67046	PASS
68	69	0.00	2	1.5	1056	PASS
69	198	0.00	100	29.2	72539	PASS
70	69	0.00	2	0.6	435	PASS
127	198	10	80	45.0	111869	PASS
197	198	0.00	2	0.6	1540	PASS
198	198	100	100	100.0	248592	PASS
199	198	5	9	6.5	16260	PASS
275	198	10	60	26.5	65861	PASS
365	198	1	100	3.8	9363	PASS
441	198	0.01	100	17.8	44165	PASS
442	442	50	100	100.0	285525	PASS
443	442	15	24	18.6	53211	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100121\
Data File : BF125742.D
Acq On : 1 Oct 2021 9:23
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 01 10:56:51 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF092421.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Sep 24 15:38:32 2021
Response via : Initial Calibration

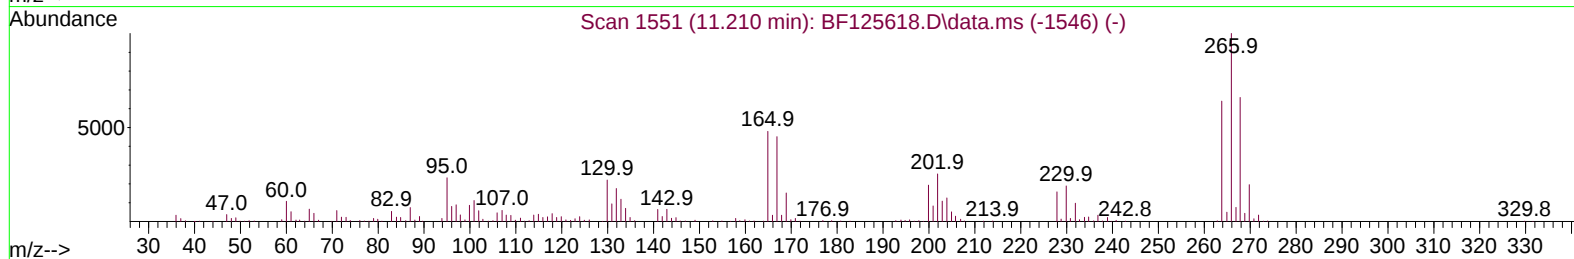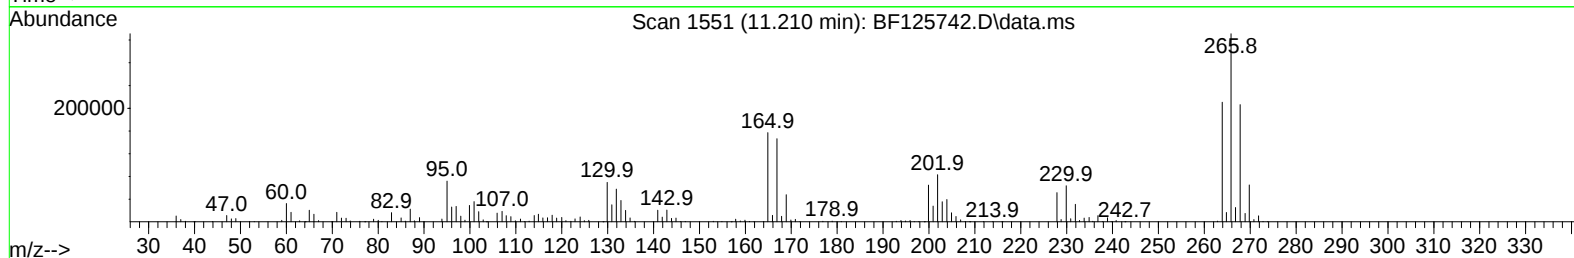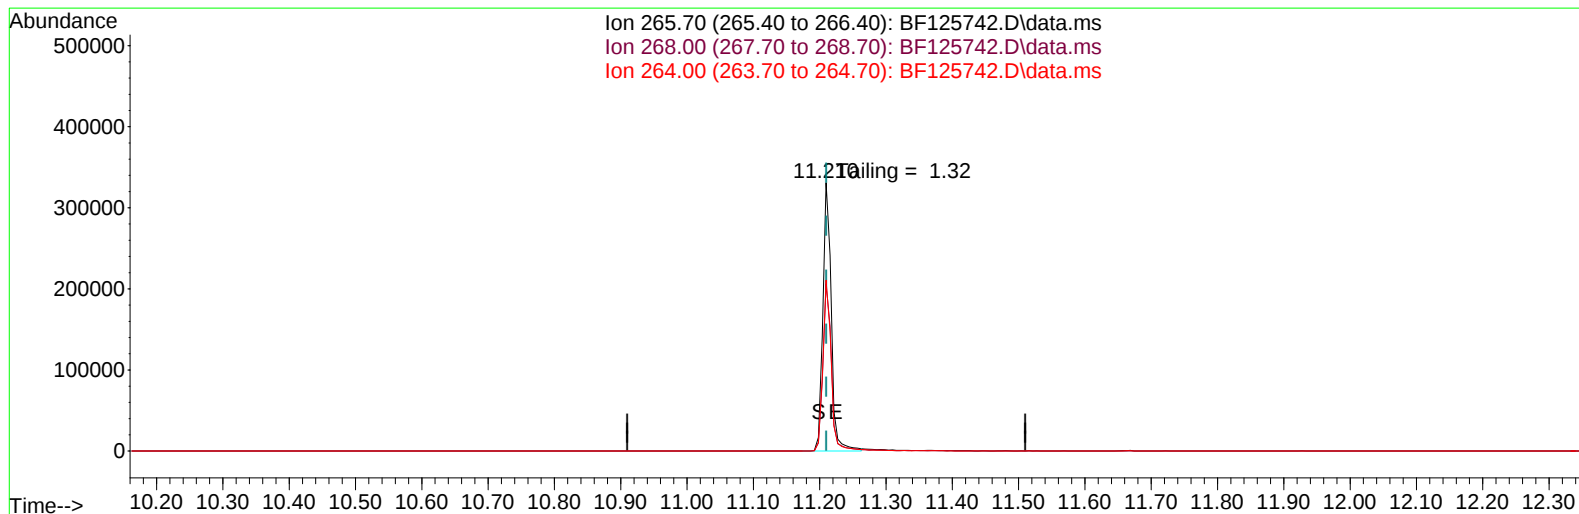

TIC: BF125742.D\data.ms

(70) Pentachlorophenol (C)

11.210min (-0.000) 40264.90 ng




response 298028

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	62.32
264.00	69.90	63.62
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100121\
 Data File : BF125742.D
 Acq On : 1 Oct 2021 9:23
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Oct 01 10:56:51 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF092421.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Sep 24 15:38:32 2021
 Response via : Initial Calibration

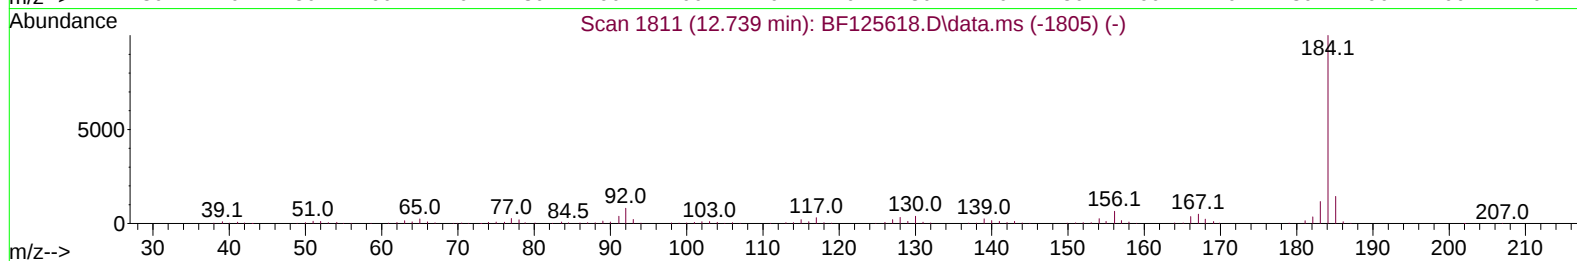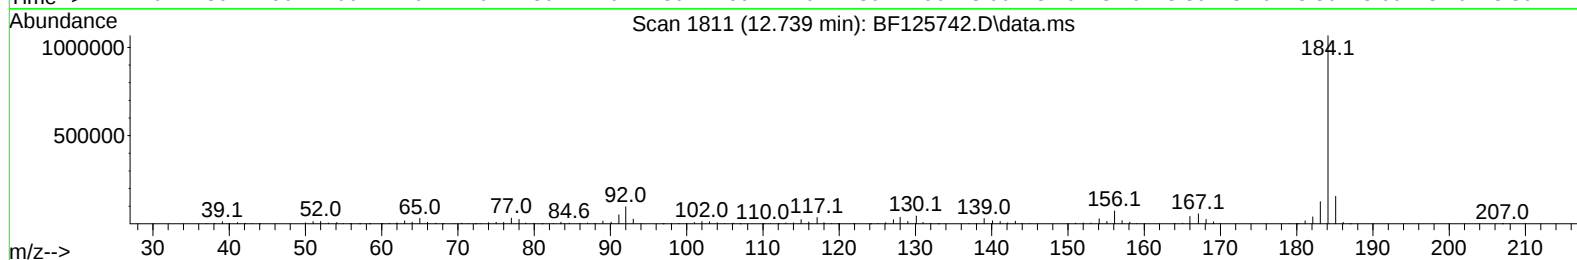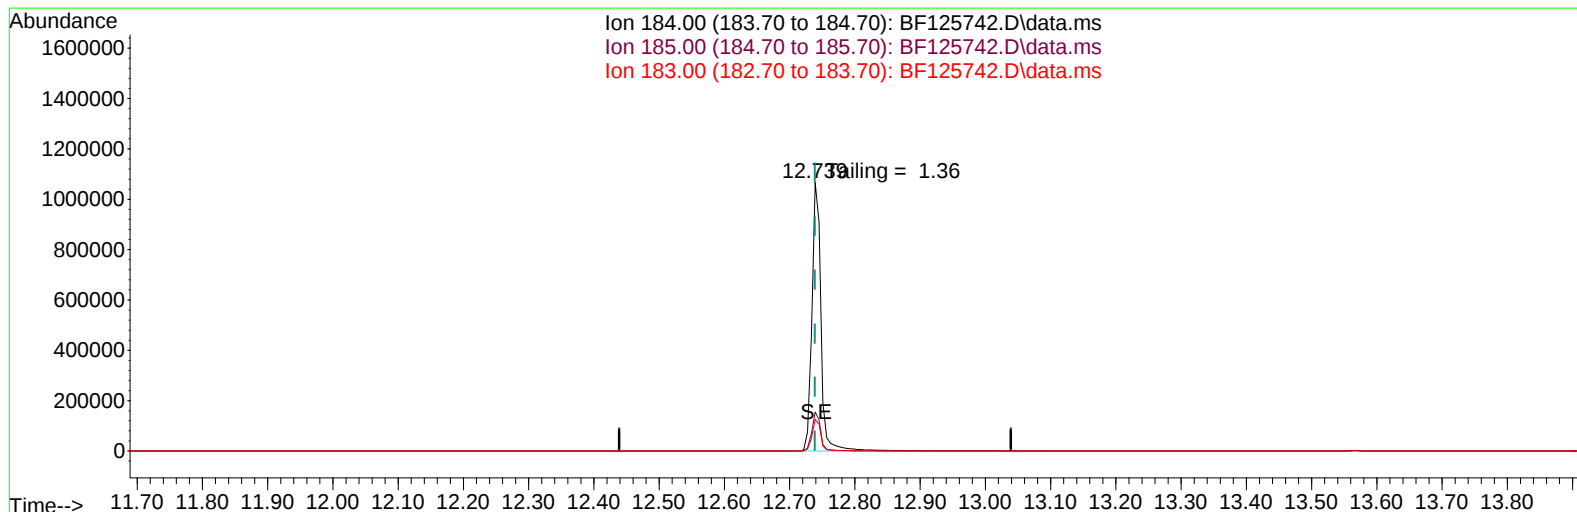

TIC: BF125742.D\data.ms

(77) Benzidine

12.739min (+ 0.000) 0.00 ng

response 1029654

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	14.55
183.00	10.10	11.77
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/1/2021	BNA_F	BF125742.D
Compound Name	Response	Retention Time
DDT	509305	13.56
DDD	12215	13.26
DDE	2922	12.93
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
15137	524442	2.89

Instrument :
BNA_F
ClientSampleId :
DFTPP