


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100219\
 Data File : BF117291.D
 Acq On : 2 Oct 2019 10:46
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF091319.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Sep 13 16:23:17 2019

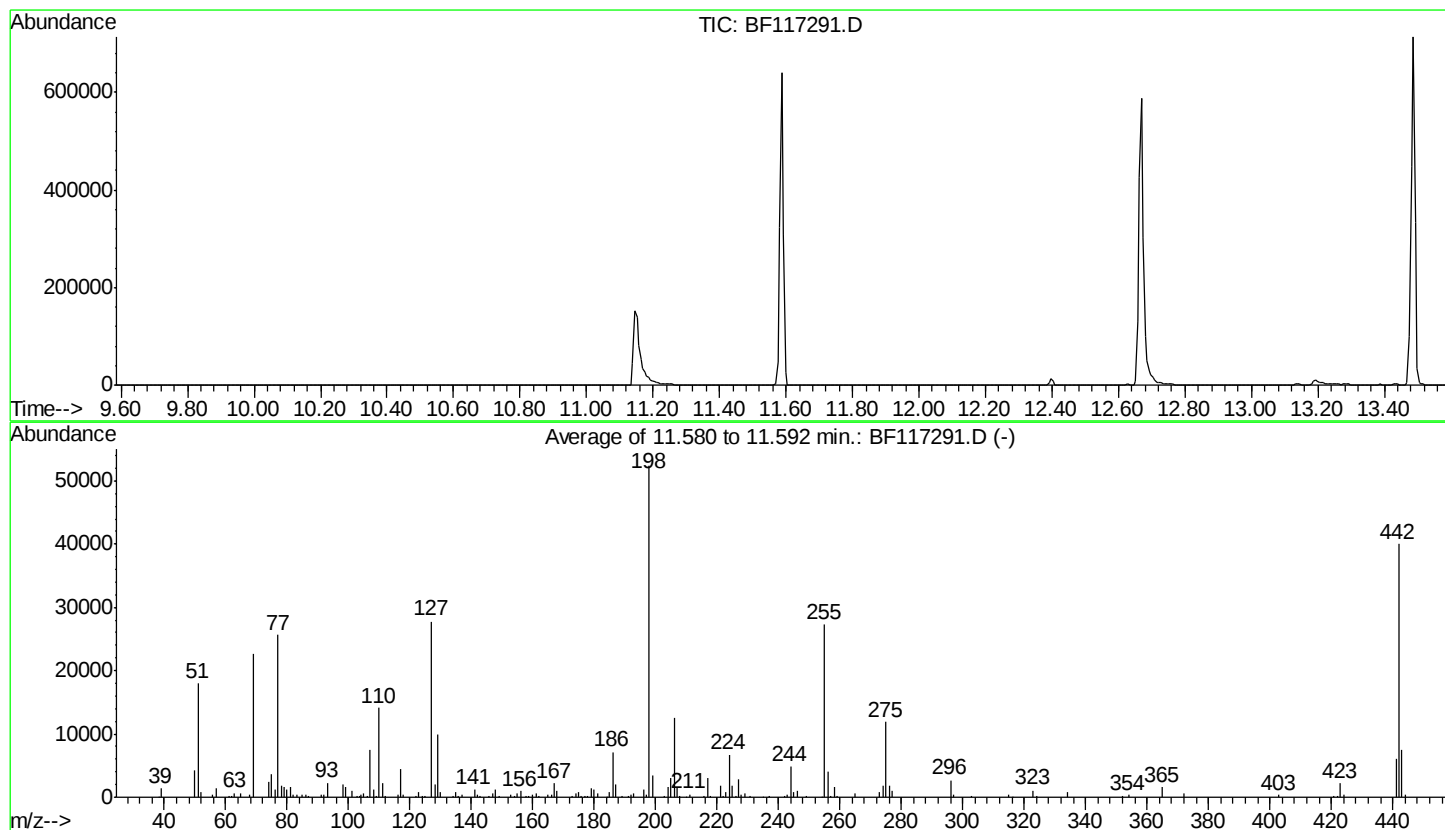

AutoFind: Scans 1614, 1615, 1616; Background Corrected with Scan 1610

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.3	17993	PASS
68	69	0.00	2	1.6	364	PASS
69	198	0.00	100	43.1	22608	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	53.0	27750	PASS
197	198	0.00	2	0.9	481	PASS
198	198	100	100	100.0	52400	PASS
199	198	5	9	6.5	3430	PASS
275	198	10	60	22.7	11910	PASS
365	198	1	100	3.0	1555	PASS
441	198	0.01	100	11.6	6102	PASS
442	198	50	100	76.3	39985	PASS
443	442	15	24	18.7	7495	PASS