
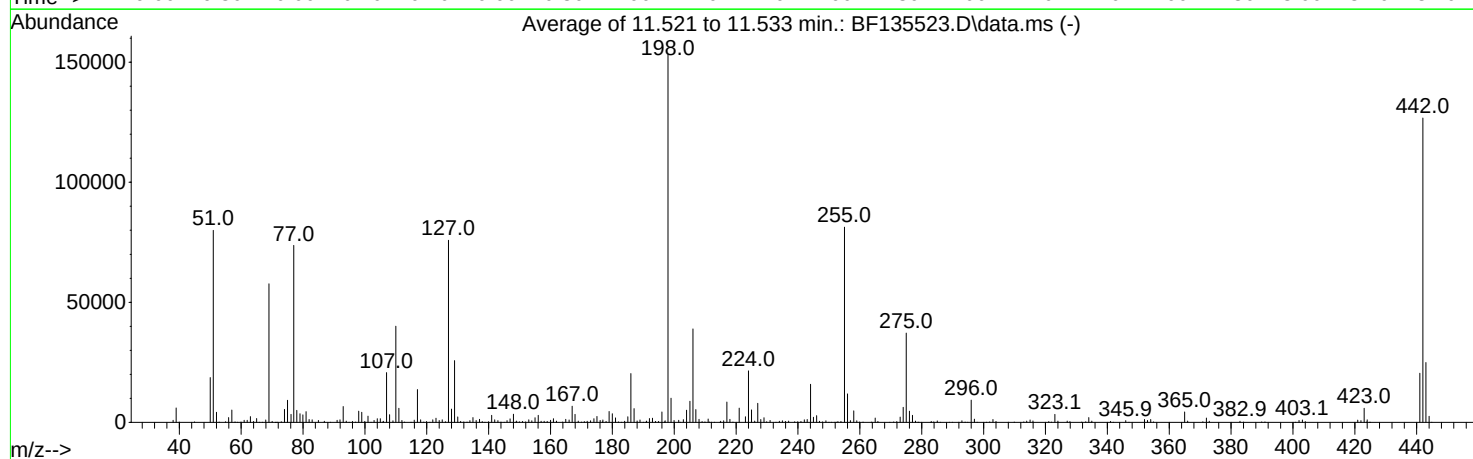


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100223\
Data File : BF135523.D
Acq On : 02 Oct 2023 11:50
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Sat Sep 30 00:12:20 2023

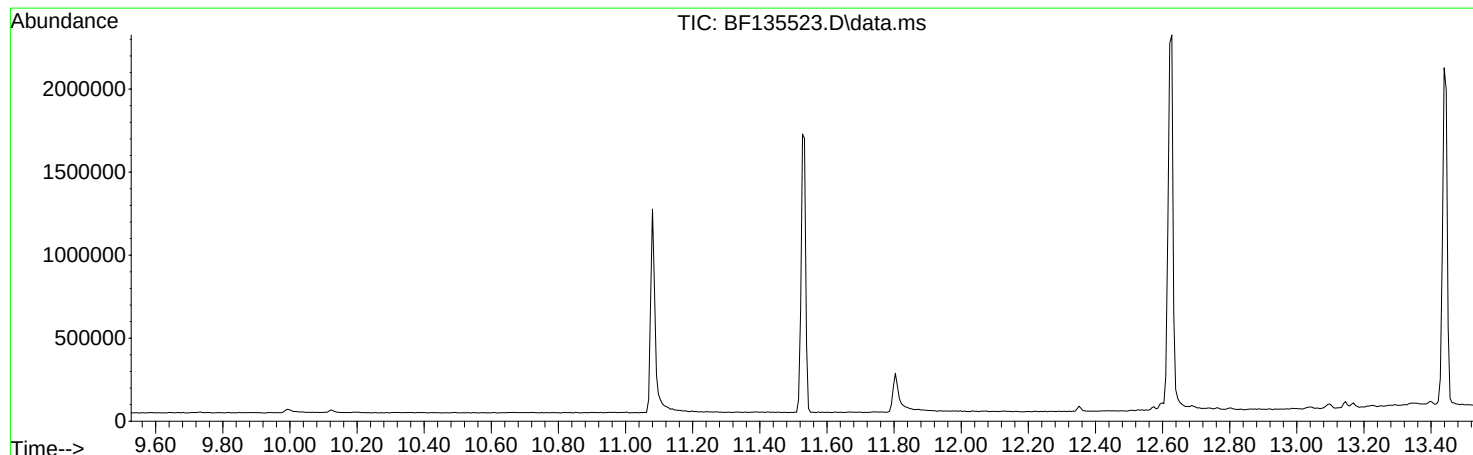




AutoFind: Scans 1604, 1605, 1606; Background Corrected with Scan 1599

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	52.2	79988	PASS
68	69	0.00	2	1.8	1023	PASS
69	198	0.00	100	37.7	57697	PASS
70	69	0.00	2	0.8	433	PASS
127	198	10	80	49.5	75829	PASS
197	198	0.00	2	0.5	699	PASS
198	198	100	100	100.0	153200	PASS
199	198	5	9	6.6	10092	PASS
275	198	10	60	24.3	37161	PASS
365	198	1	100	2.8	4365	PASS
441	198	0.01	100	13.4	20468	PASS
442	442	50	100	100.0	126731	PASS
443	442	15	24	19.7	24938	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100223\
Data File : BF135523.D
Acq On : 02 Oct 2023 11:50
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 02 14:00:54 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 30 00:12:20 2023
Response via : Initial Calibration

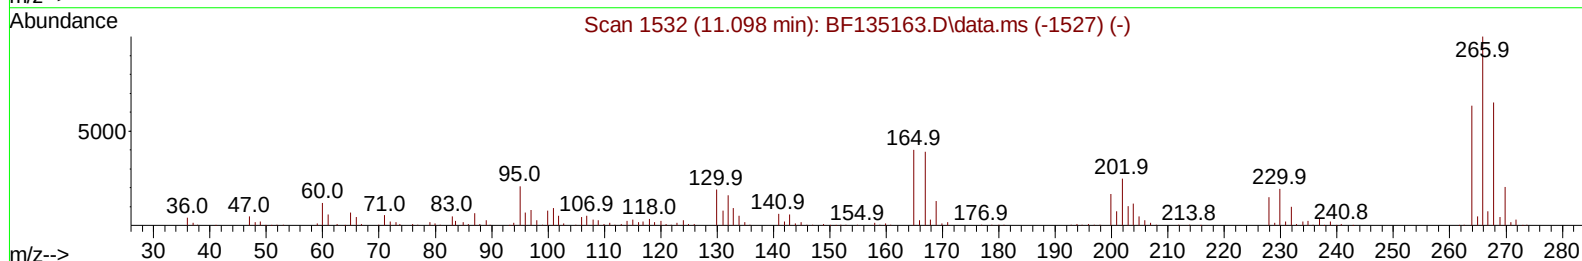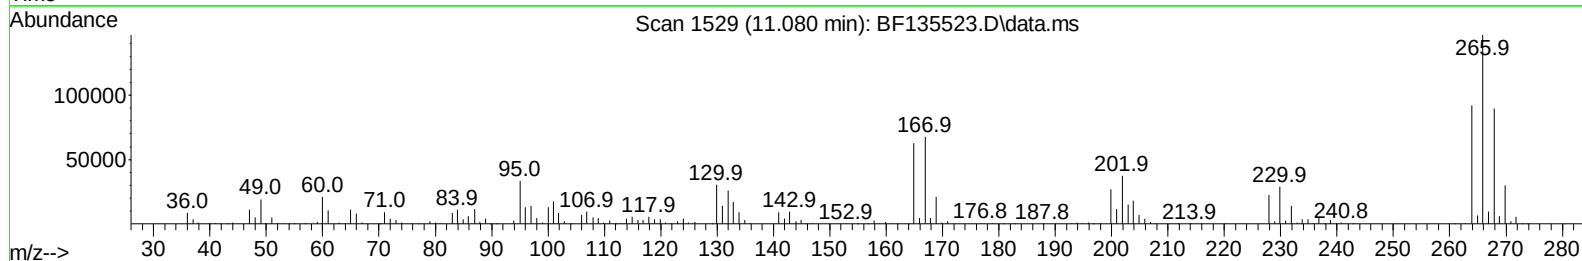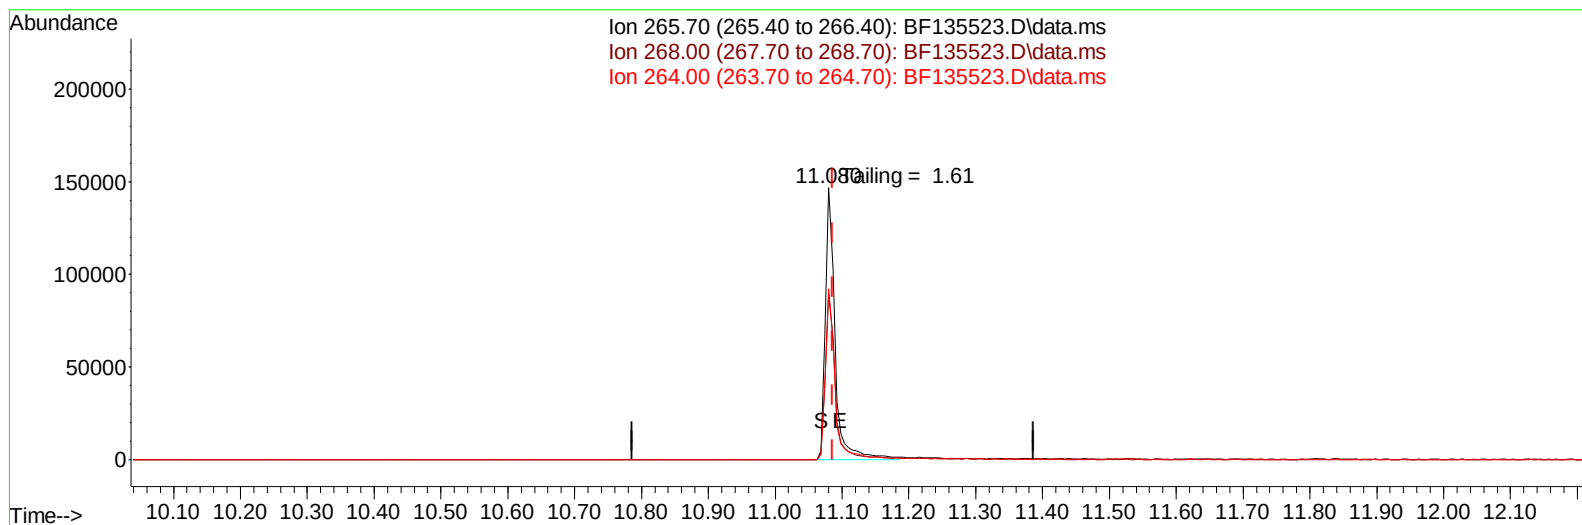

TIC: BF135523.D\data.ms

(70) Pentachlorophenol (C)

11.080min (-0.006) 425416.11 ng




response 147001

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.10	60.97
264.00	63.50	62.76
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100223\
Data File : BF135523.D
Acq On : 02 Oct 2023 11:50
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 02 14:00:54 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 30 00:12:20 2023
Response via : Initial Calibration

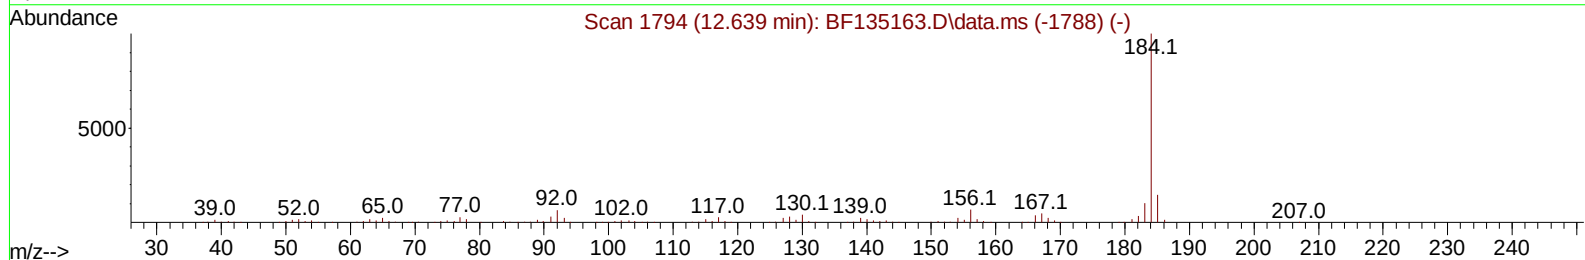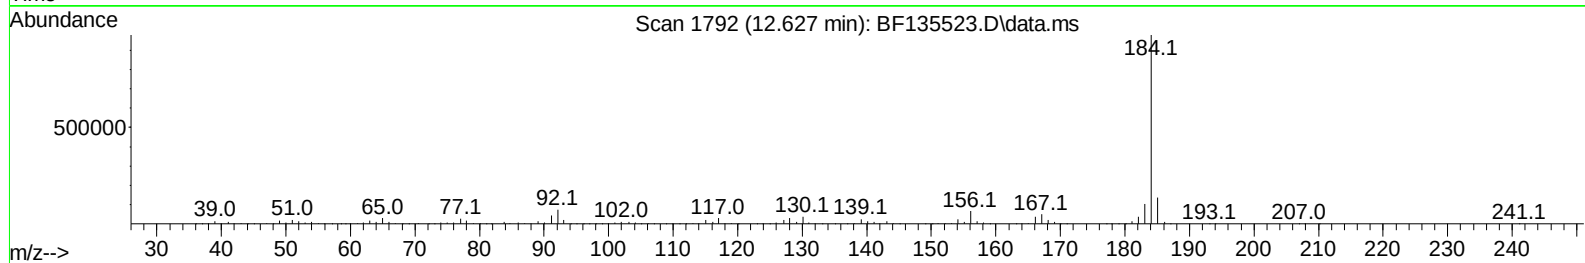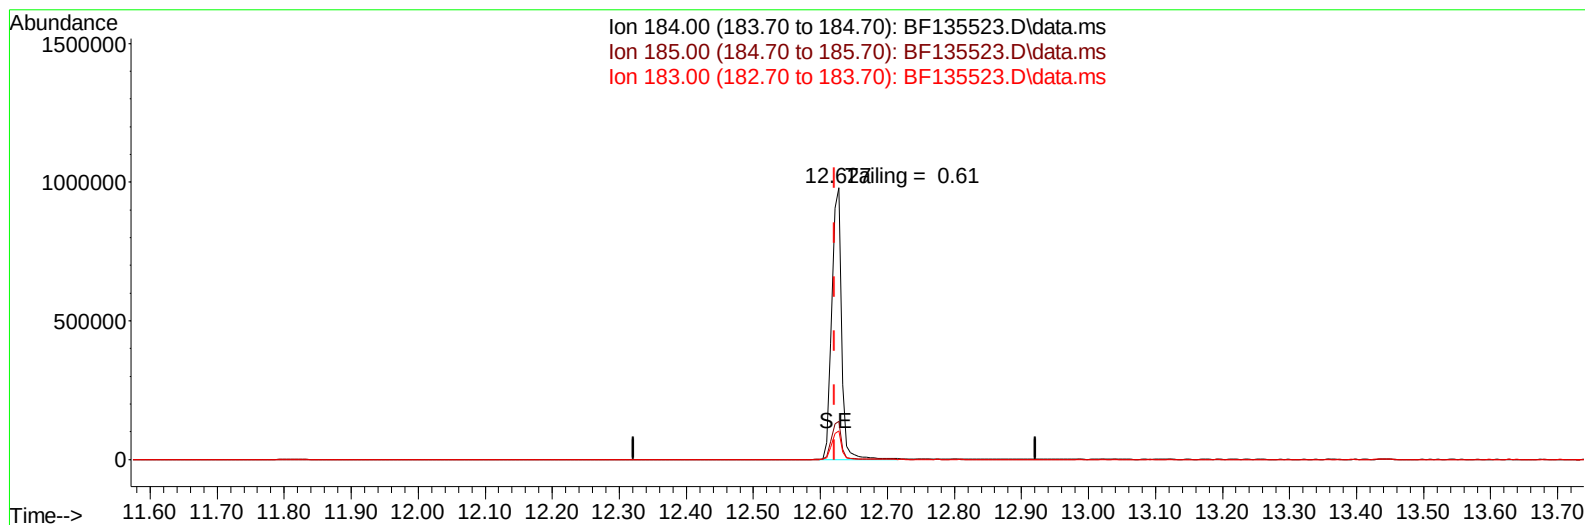

TIC: BF135523.D\data.ms

(77) Benzidine

12.627min (+ 0.006) 66929.03 ng

response 987238

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	13.98
183.00	10.30	10.45
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/2/2023	BNA_F	<u>BF135523.D</u>
Compound Name	Response	Retention Time
DDT	379599	13.445
DDD	10815	13.145
DDE	937	12.804
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
11752	391351	3.00

Instrument :
BNA_F
ClientSampleId :
DFTPP