
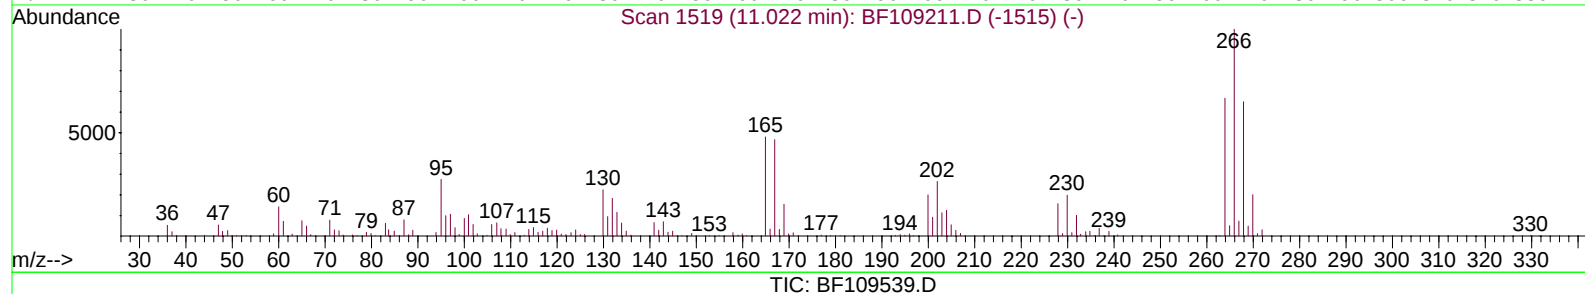
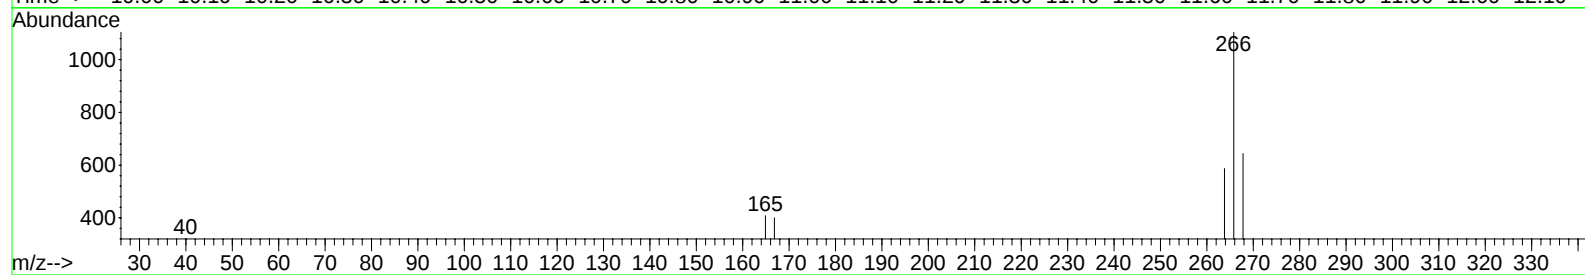


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF100318\
Data File : BF109539.D
Acq On : 3 Oct 2018 12:04
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 03 18:44:42 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF092218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 22 13:32:18 2018
Response via : Initial Calibration

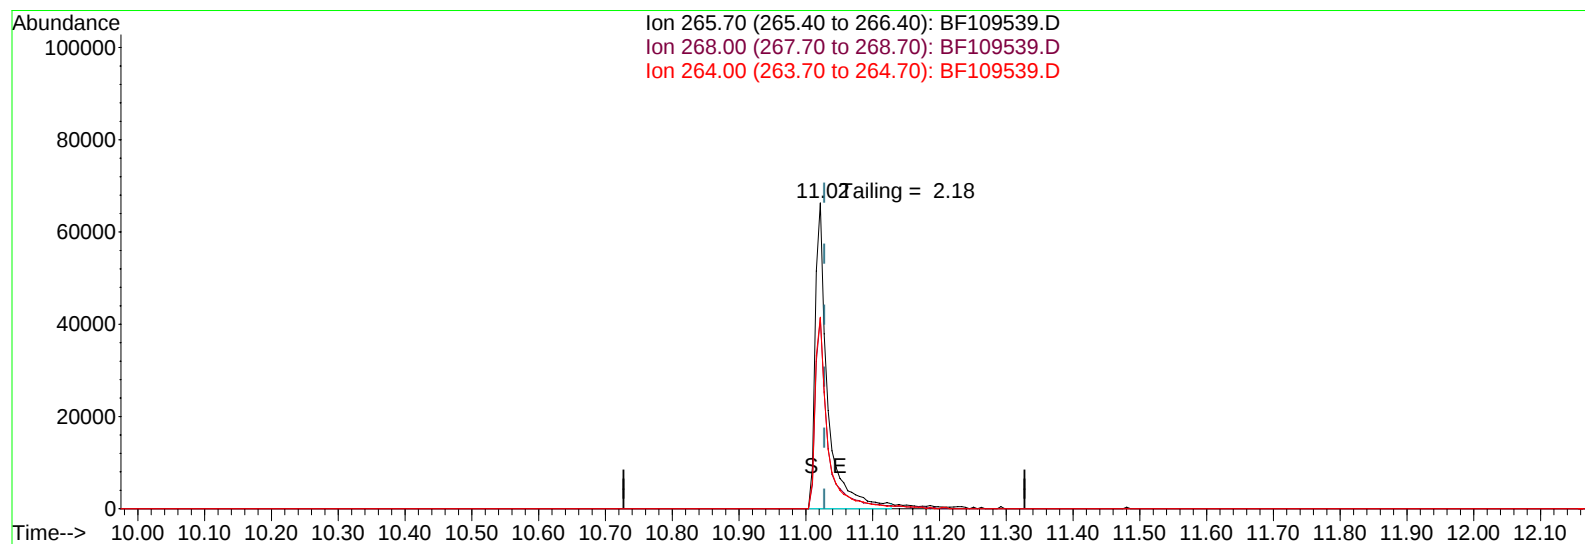

(69) Pentachlorophenol (C)




11.022min (-0.006) 40056.00ng

response 88216

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	62.27
264.00	61.90	62.65
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF100318\
Data File : BF109539.D
Acq On : 3 Oct 2018 12:04
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 03 18:44:42 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF092218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 22 13:32:18 2018
Response via : Initial Calibration

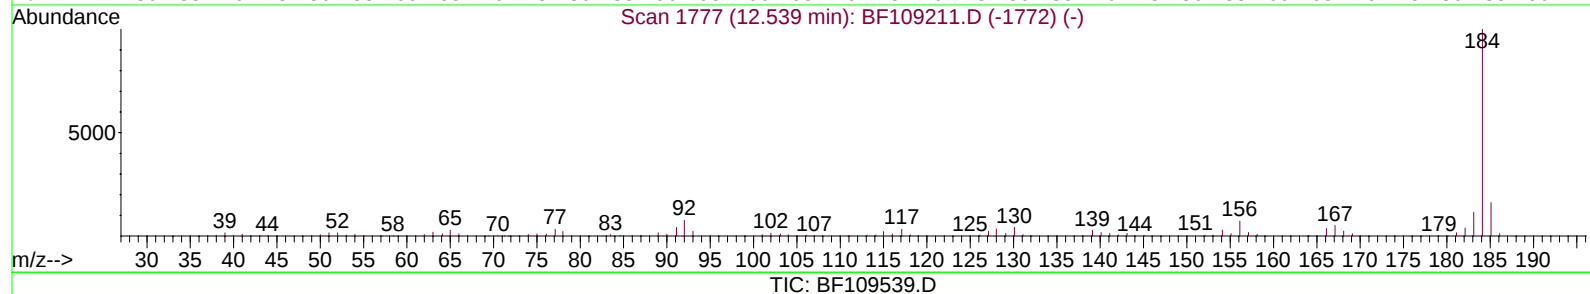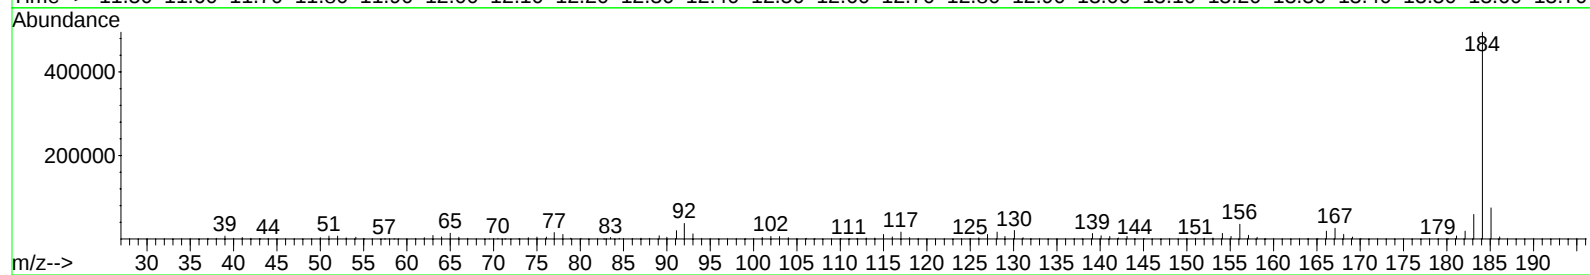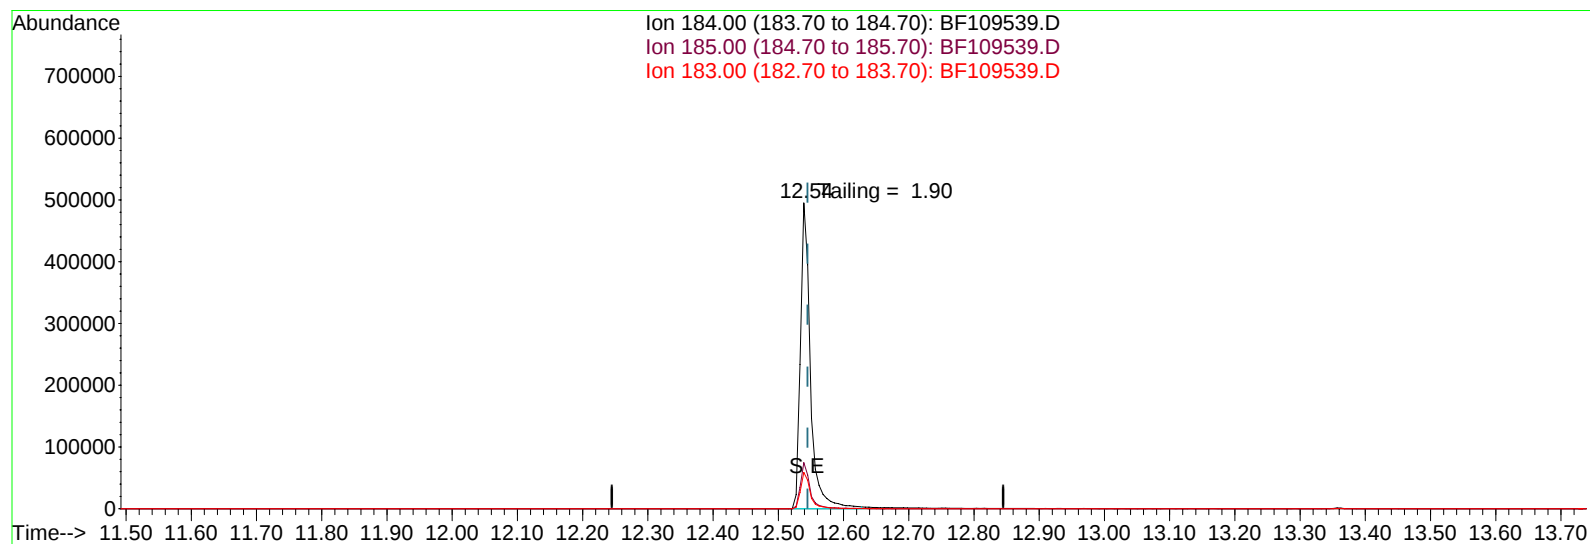

(76) Benzidine

12.539min (-0.006) 0.00ng

response 536899

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	15.05
183.00	11.60	11.90
0.00	0.00	0.00