

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF100318\
 Data File : BF109561.D
 Acq On : 3 Oct 2018 21:48
 Operator : JU/SJ
 Sample : J5221-03
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 100118-JETT-E-U-B

Quant Time: Oct 04 03:24:52 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF092218.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Sep 22 13:32:18 2018
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.70	152	69095	20.00	ng	0.00
21) Naphthalene-d8	7.99	136	224422	20.00	ng	0.00
38) Acenaphthene-d10	9.73	164	97529	20.00	ng	0.00
63) Phenanthrene-d10	11.21	188	209346	20.00	ng	0.00
75) Chrysene-d12	13.84	240	205165	20.00	ng	0.00
86) Perylene-d12	15.24	264	139083	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.32	112	168135	40.08	ng	0.00
7) Phenol-d6	6.35	99	126267	23.59	ng	-0.01
23) Nitrobenzene-d5	7.27	82	424060	111.54	ng	-0.01
41) 2,4,6-Tribromophenol	10.52	330	109840	114.25	ng	-0.01
44) 2-Fluorobiphenyl	9.06	172	714282	110.46	ng	-0.01
78) Terphenyl-d14	12.80	244	897152	107.32	ng	0.00
Target Compounds						
49) Dimethylphthalate	9.45	163	74072	10.442	ng	Qvalue 100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF100318\
Data File : BF109561.D
Acq On : 3 Oct 2018 21:48
Operator : JU/SJ
Sample : J5221-03
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
100118-JETT-E-U-B

Quant Time: Oct 04 03:24:52 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF092218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Sep 22 13:32:18 2018
Response via : Initial Calibration

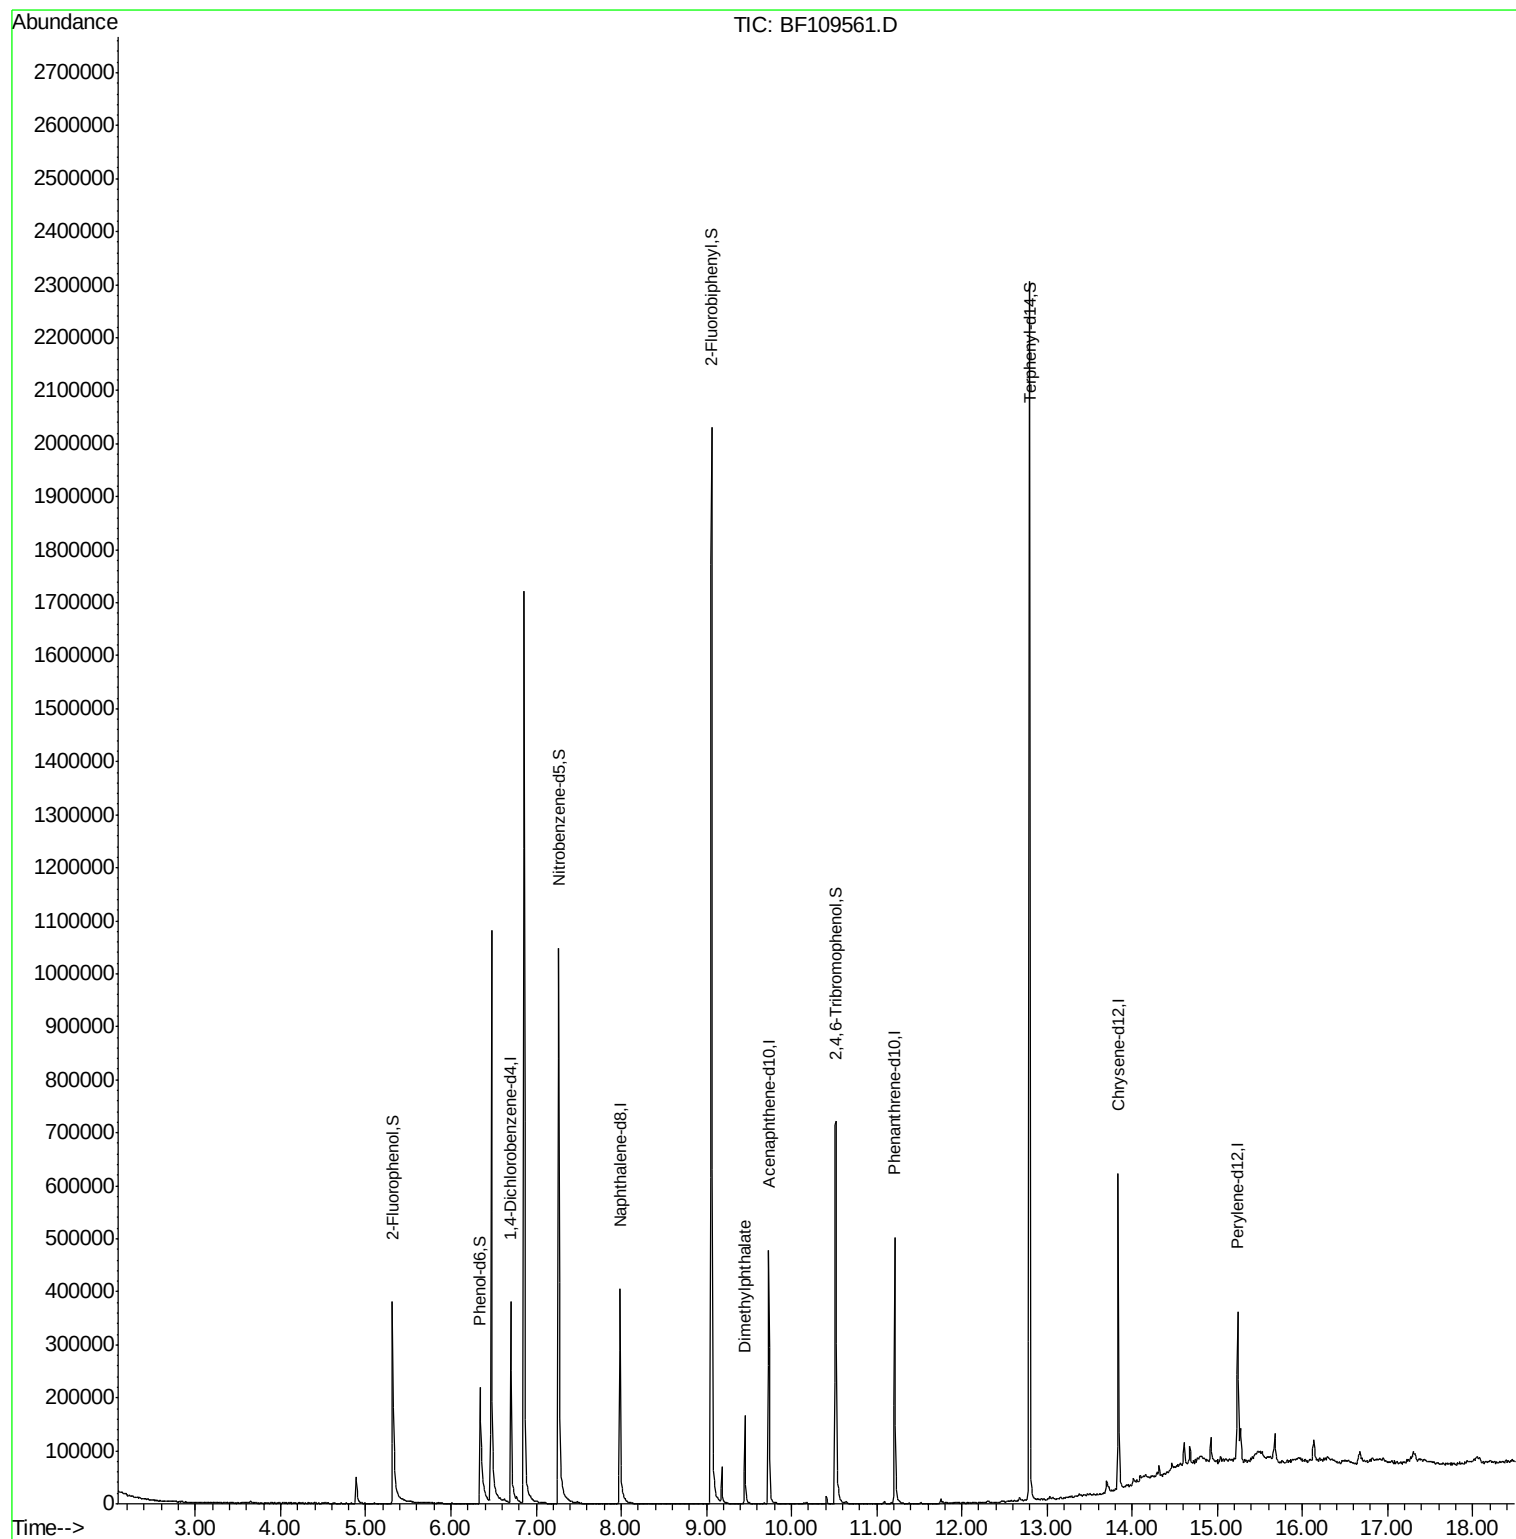

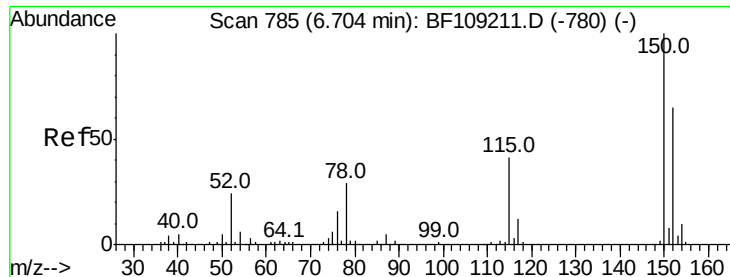


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.70 min Scan# 785
Delta R.T. -0.01 min
Lab File: BF109561.D
Acq: 3 Oct 2018 21:48

Instrument :
BNA_F
ClientSampleId :
100118-JETT-E-U-B

Tot Ion:152 Resp: 69095
Ion Ratio Lower Upper
152 100
150 153.9 124.6 186.8
115 63.1 50.1 75.1

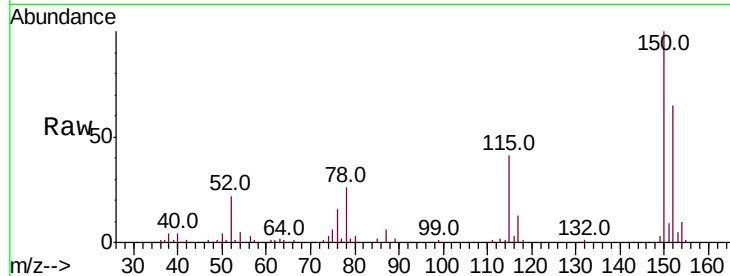


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

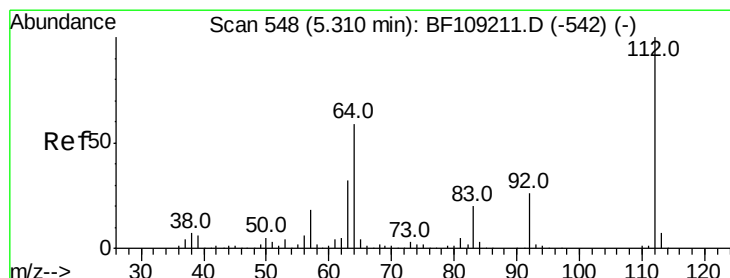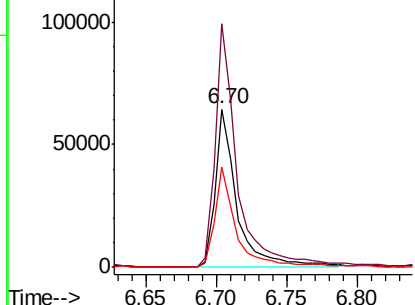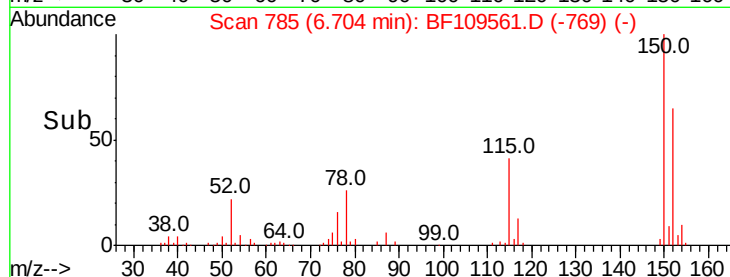



#5


2-Fluorophenol
Concen: 40.080 ng
RT: 5.32 min Scan# 549
Delta R.T. 0.00 min
Lab File: BF109561.D
Acq: 3 Oct 2018 21:48

Tgt Ion:112 Resp: 168135
Ion Ratio Lower Upper
112 100
64 60.3 47.9 71.9
63 30.7 23.7 35.5

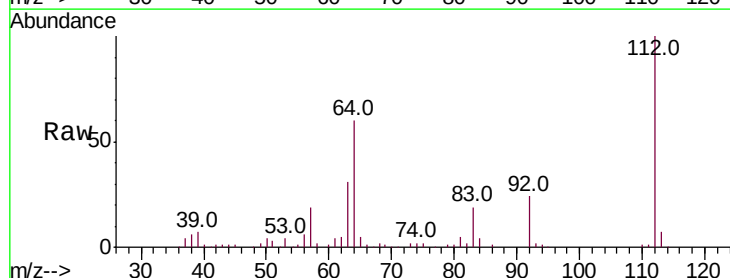

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

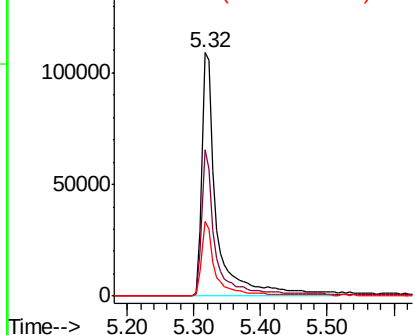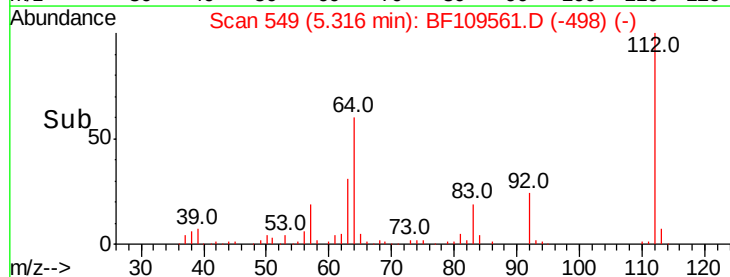

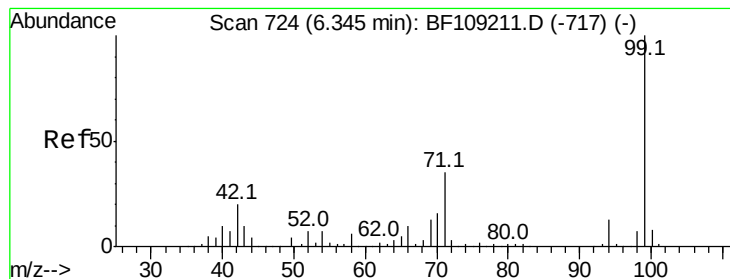

#7

Phenol-d6

Concen: 23.588 ng

RT: 6.35 min Scan# 724

Delta R.T. -0.01 min

Lab File: BF109561.D

Acq: 3 Oct 2018 21:48

Instrument :

BNA_F

ClientSampleId :

100118-JETT-E-U-B





Tot Ion: 99 Resp: 126267

Ion Ratio Lower Upper

99 100

42 17.3 14.5 21.7

71 33.2 25.4 38.0

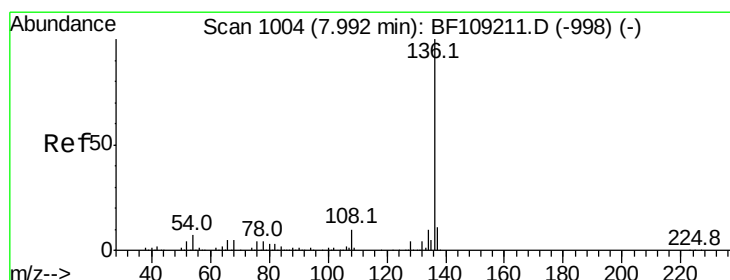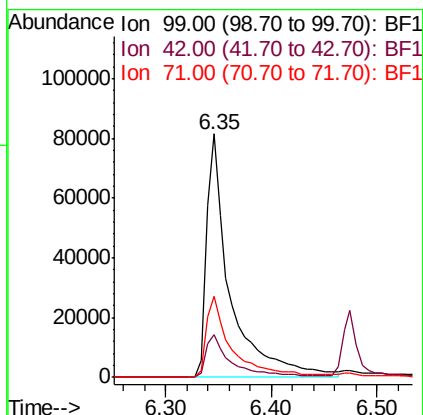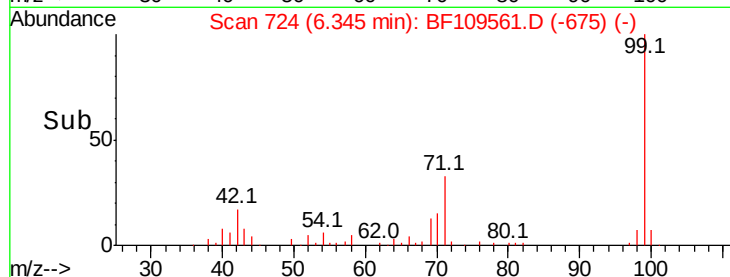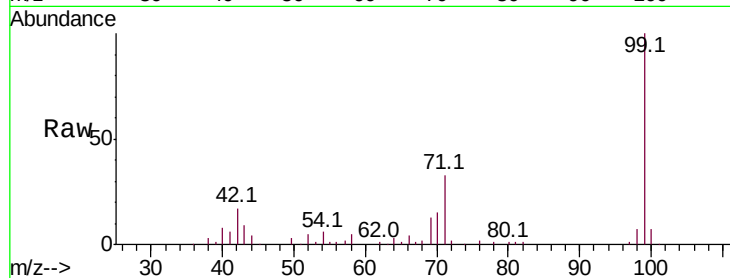

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 7.99 min Scan# 1003

Delta R.T. -0.01 min

Lab File: BF109561.D

Acq: 3 Oct 2018 21:48

Tgt Ion: 136 Resp: 224422




Ion Ratio Lower Upper


136 100

137 10.9 8.9 13.3

54 6.7 6.6 9.8

68 5.4 5.0 7.4

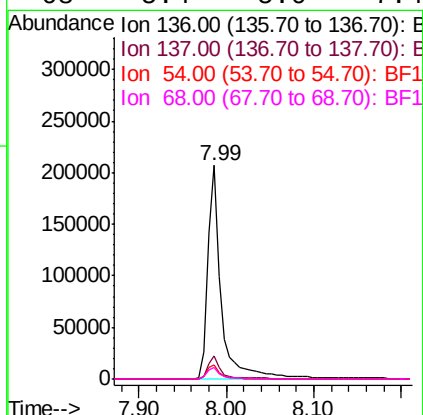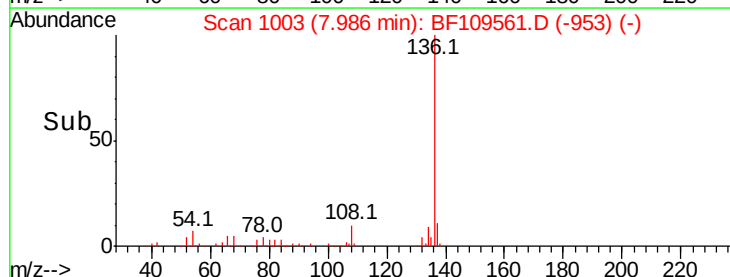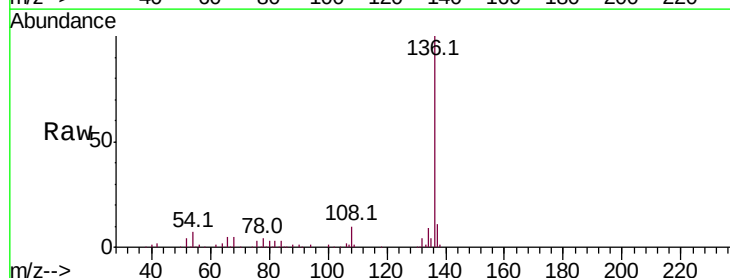


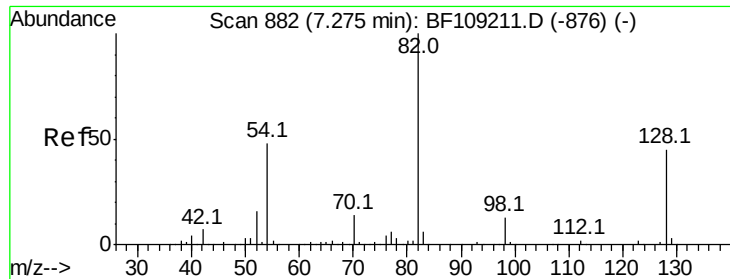




#23
 Nitrobenzene-d5
 Concen: 111.544 ng
 RT: 7.27 min Scan# 881
 Delta R.T. -0.01 min
 Lab File: BF109561.D
 Acq: 3 Oct 2018 21:48

Instrument :
 BNA_F
 ClientSampleId :
 100118-JETT-E-U-B

Tot Ion: 82 Resp: 424060
 Ion Ratio Lower Upper
 82 100
 128 44.5 36.1 54.1
 54 47.2 41.4 62.2

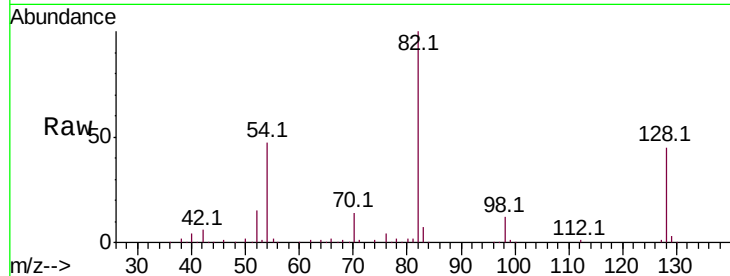


Abundance Ion 82.00 (81.70 to 82.70): BF1
 Ion 128.00 (127.70 to 128.70): E
 Ion 54.00 (53.70 to 54.70): BF1

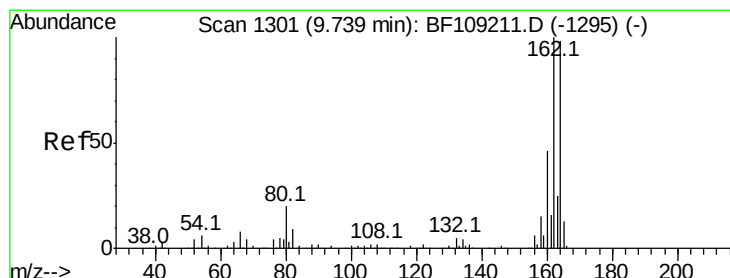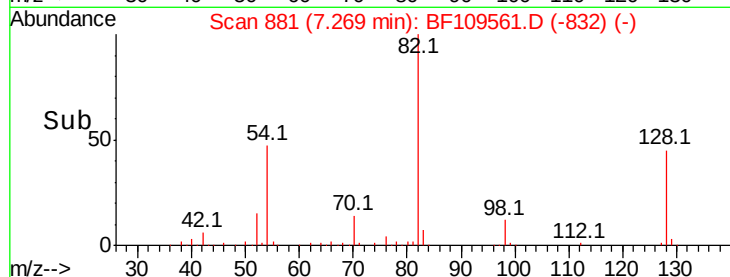
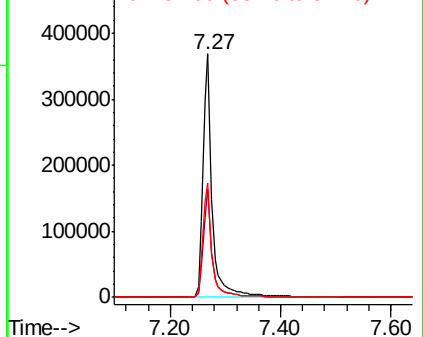



#38
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 9.73 min Scan# 1300
 Delta R.T. -0.01 min
 Lab File: BF109561.D
 Acq: 3 Oct 2018 21:48

Tgt Ion:164 Resp: 97529
 Ion Ratio Lower Upper
 164 100
 162 102.1 86.1 129.1
 160 45.2 38.3 57.5

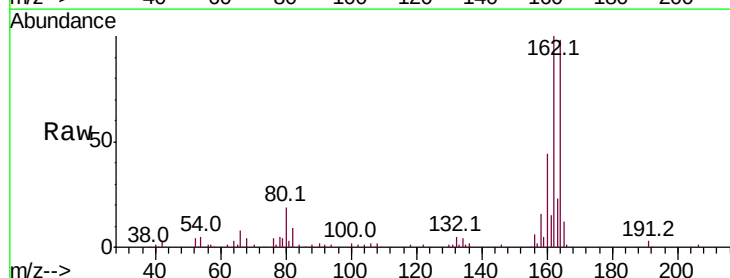

Abundance Ion 164.00 (163.70 to 164.70): E
 Ion 162.00 (161.70 to 162.70): E
 Ion 160.00 (159.70 to 160.70): E

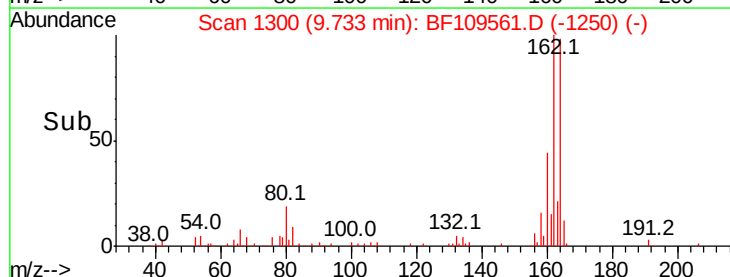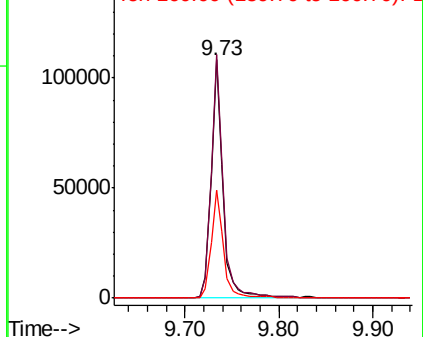


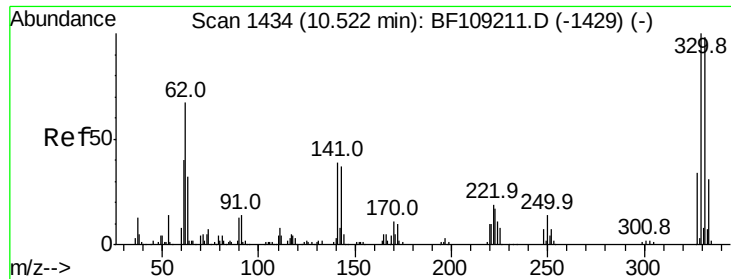

#41
 2,4,6-Tribromophenol
 Concen: 114.246 ng
 RT: 10.52 min Scan# 1434
 Delta R.T. -0.01 min
 Lab File: BF109561.D
 Acq: 3 Oct 2018 21:48

Instrument :
 BNA_F
 ClientSampleId :
 100118-JETT-E-U-B

Tot Ion	Ratio	Lower	Upper
330	100		
332	96.3	77.0	115.6
141	33.2	29.9	44.9



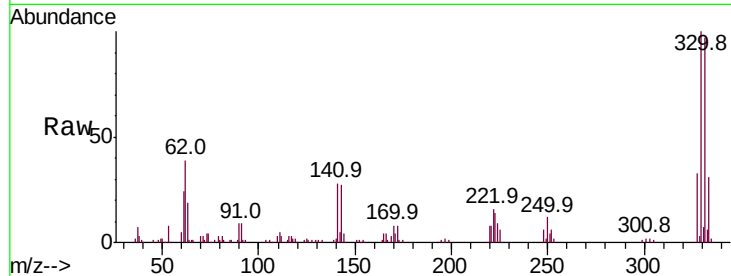


Abundance

Ion 329.80 (329.50 to 330.50): E


Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

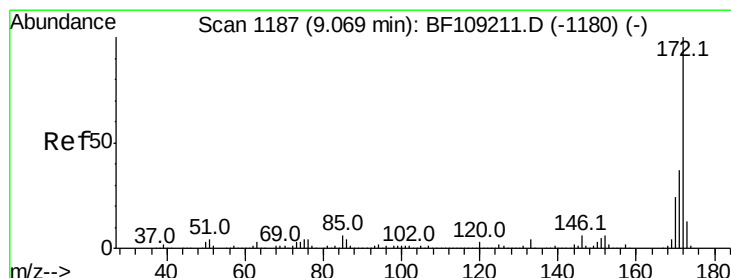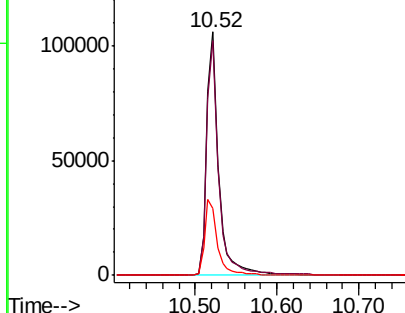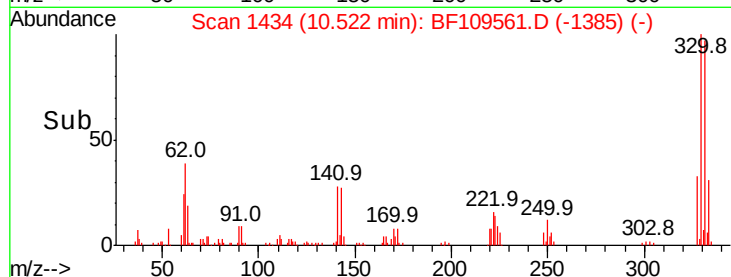

#44
 2-Fluorobiphenyl
 Concen: 110.457 ng
 RT: 9.06 min Scan# 1186
 Delta R.T. -0.01 min
 Lab File: BF109561.D
 Acq: 3 Oct 2018 21:48

Tgt Ion	Ratio	Lower	Upper
172	100		
171	35.3	29.7	44.5
170	23.9	19.6	29.4


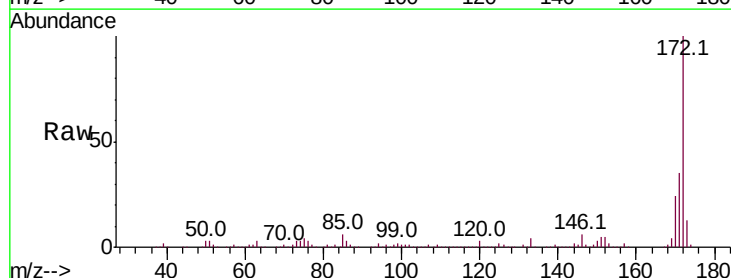



Abundance

Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

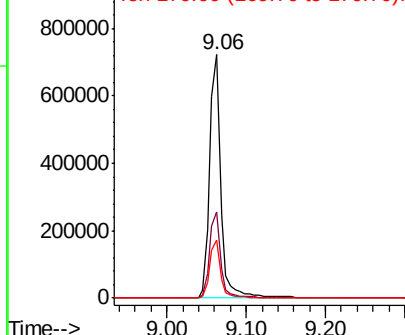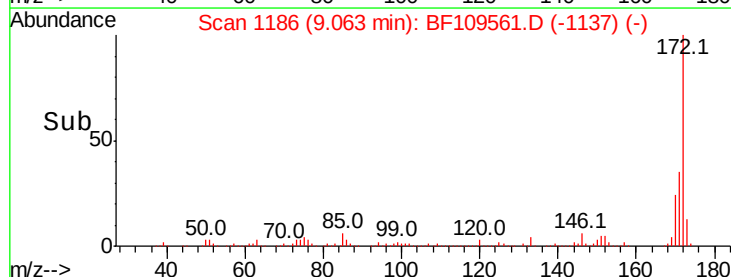


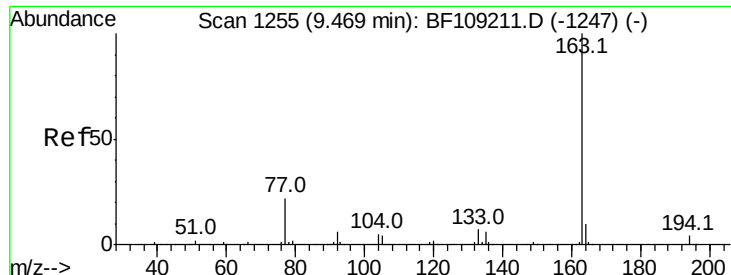




#49
Dimethylphthalate
Concen: 10.442 ng
RT: 9.45 min Scan# 1252
Delta R.T. -0.03 min
Lab File: BF109561.D
Acq: 3 Oct 2018 21:48

Instrument :
BNA_F
ClientSampleId :
100118-JETT-E-U-B

Tot Ion:163 Resp: 74072
Ion Ratio Lower Upper
163 100
194 4.0 2.7 4.1
164 10.2 8.2 12.2

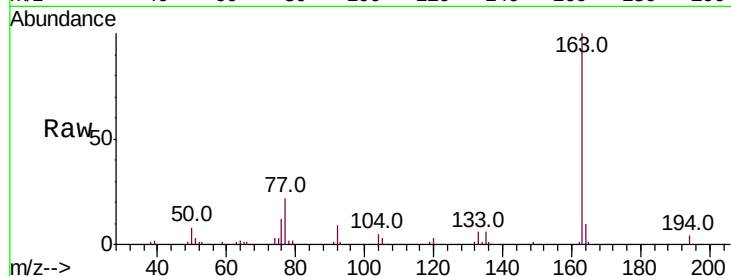


Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

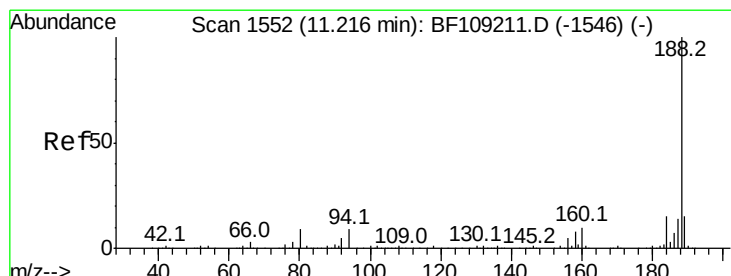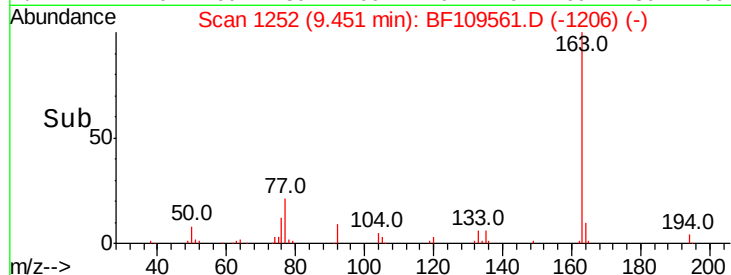
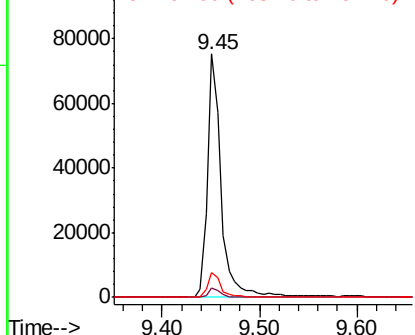



#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.21 min Scan# 1551
Delta R.T. -0.01 min
Lab File: BF109561.D
Acq: 3 Oct 2018 21:48

Tgt Ion:188 Resp: 209346
Ion Ratio Lower Upper
188 100
94 10.0 8.5 12.7
80 10.0 9.2 13.8

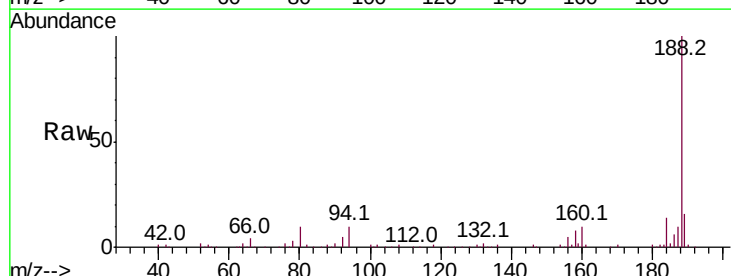

Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF1
Ion 80.00 (79.70 to 80.70): BF1

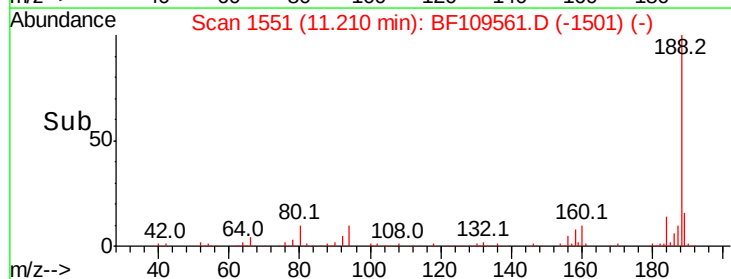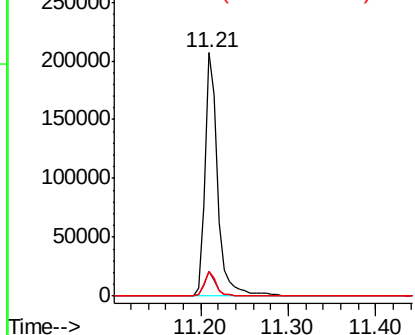

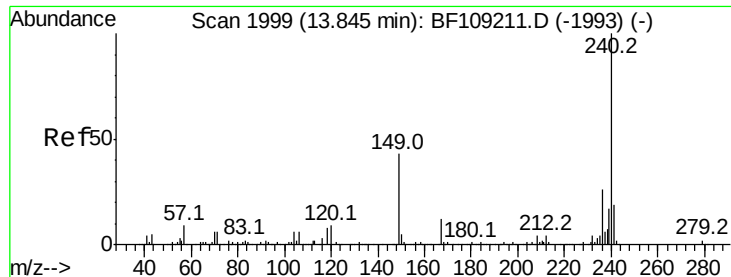

#75

Chrysene-d12

Concen: 20.000 ng

RT: 13.84 min Scan# 1998

Delta R.T. -0.01 min

Lab File: BF109561.D

Acq: 3 Oct 2018 21:48

Instrument :

BNA_F

ClientSampleId :

100118-JETT-E-U-B


Tot Ion:240 Resp: 205165

Ion Ratio Lower Upper

240 100

120 11.0 9.5 14.3




236 26.2 20.7 31.1

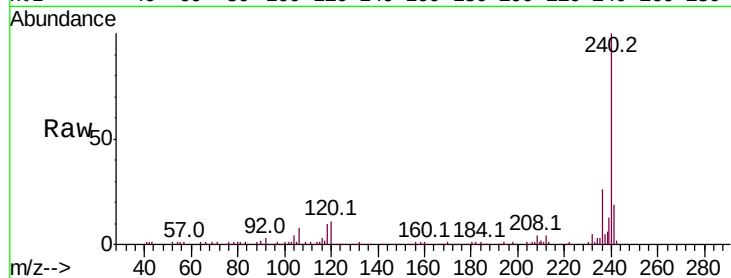

Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

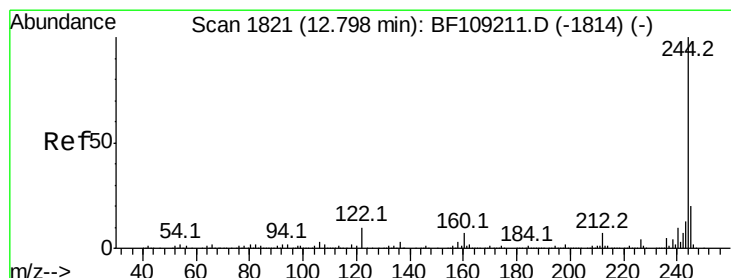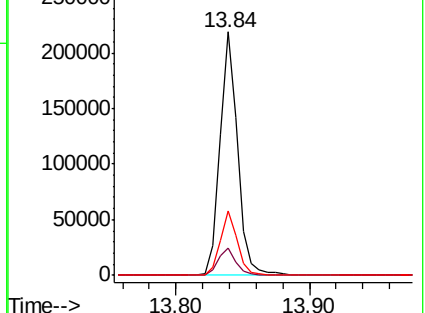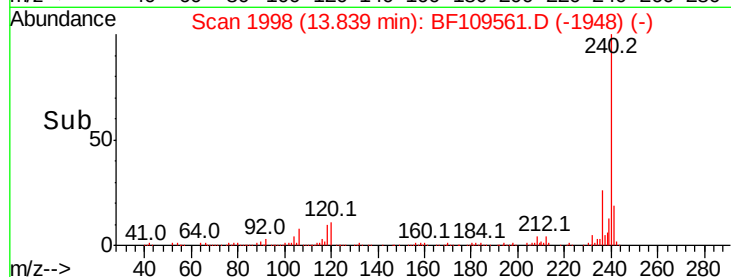

#78

Terphenyl-d14

Concen: 107.316 ng

RT: 12.80 min Scan# 1821

Delta R.T. -0.01 min

Lab File: BF109561.D

Acq: 3 Oct 2018 21:48


Tgt Ion:244 Resp: 897152

Ion Ratio Lower Upper

244 100

212 6.9 5.4 8.0



122 10.3 11.0 16.4#

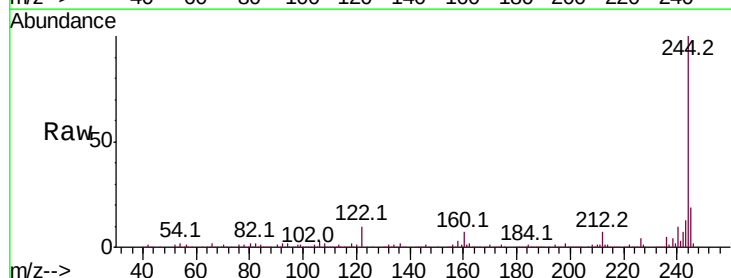


Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

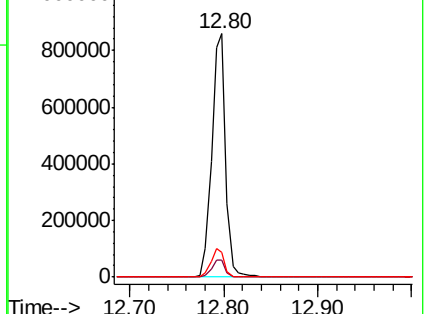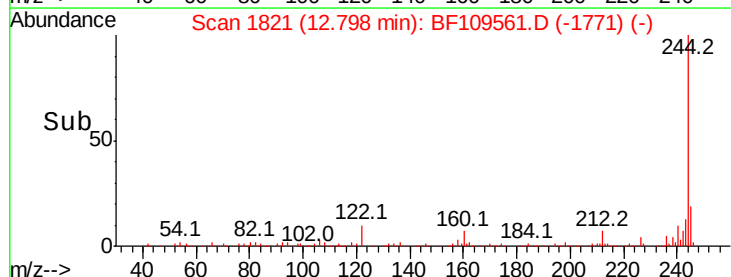

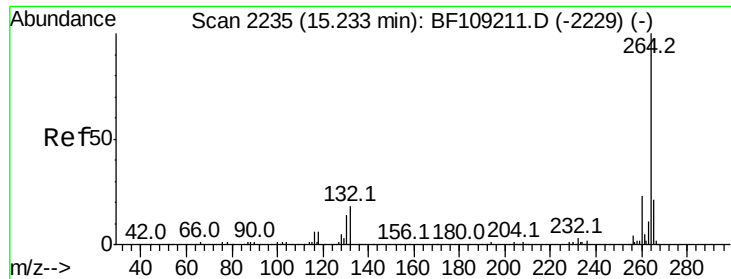

#86
Pervlene-d12
Concen: 20.000 ng
RT: 15.24 min Scan# 2236
Delta R.T. 0.00 min
Lab File: BF109561.D
Acq: 3 Oct 2018 21:48

Instrument :
BNA_F
ClientSampleId :
100118-JETT-E-U-B

Tot Ion	Ratio	Lower	Upper
264	100		
260	23.0	19.2	28.8
265	21.0	17.5	26.3

