

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF100318\
 Data File : BF109556.D
 Acq On : 3 Oct 2018 19:37
 Operator : JU/SJ
 Sample : J5218-05 5X
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 293-230

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF092218.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.887	473	476	482	rBV2	13380	15258	2.49%	0.238%
2	5.316	546	549	559	rBV	165187	232907	38.06%	3.636%
3	6.345	721	724	743	rBV	189755	321395	52.52%	5.017%
4	6.475	743	746	757	rVV	284927	334535	54.67%	5.223%
5	6.551	757	759	768	rVB3	8490	13839	2.26%	0.216%
6	6.704	782	785	802	rBV	432815	458276	74.89%	7.154%
7	6.857	808	811	822	rBV	260838	259024	42.33%	4.044%
8	7.263	877	880	904	rBV	109851	182172	29.77%	2.844%
9	7.987	999	1003	1014	rBV	543320	536438	87.67%	8.375%
10	8.704	1118	1125	1133	rVB4	4406	9202	1.50%	0.144%
11	8.798	1136	1141	1148	rVB2	6329	8078	1.32%	0.126%
12	9.057	1182	1185	1197	rBV	331997	325122	53.13%	5.076%
13	9.151	1197	1201	1205	rVB4	7236	9908	1.62%	0.155%
14	9.451	1249	1252	1259	rBV	104336	87632	14.32%	1.368%
15	9.733	1296	1300	1304	rBV2	540718	501017	81.88%	7.822%
16	9.939	1331	1335	1340	rBV	9629	11845	1.94%	0.185%
17	10.280	1390	1393	1398	rVB	15141	16070	2.63%	0.251%
18	10.522	1430	1434	1446	rBV	165278	195010	31.87%	3.044%
19	10.663	1453	1458	1463	rBV5	8584	14073	2.30%	0.220%
20	10.816	1482	1484	1489	rBV3	5759	7391	1.21%	0.115%
21	11.116	1533	1535	1540	rVB3	7710	11418	1.87%	0.178%
22	11.169	1540	1544	1548	rBV6	5165	8596	1.40%	0.134%
23	11.216	1548	1552	1554	rBV	571983	544599	89.00%	8.502%
24	11.233	1554	1555	1562	rVV	125100	114868	18.77%	1.793%
25	11.292	1562	1565	1567	rVB	19585	21012	3.43%	0.328%
26	11.451	1586	1592	1594	rBV5	6506	10385	1.70%	0.162%
27	11.516	1598	1603	1606	rBV6	6720	8406	1.37%	0.131%
28	11.716	1634	1637	1639	rBV	13902	13415	2.19%	0.209%
29	11.745	1639	1642	1647	rVV2	34102	33224	5.43%	0.519%
30	11.822	1652	1655	1658	rBV	29457	30730	5.02%	0.480%
31	12.010	1685	1687	1689	rBV	13681	12439	2.03%	0.194%
32	12.039	1689	1692	1697	rVB3	13433	17953	2.93%	0.280%
33	12.192	1715	1718	1719	rBV2	9139	8902	1.45%	0.139%
34	12.263	1727	1730	1733	rBV	20079	24640	4.03%	0.385%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF100318\
Data File : BF109556.D
Acq On : 3 Oct 2018 19:37
Operator : JU/SJ
Sample : J5218-05 5X
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
293-230

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF092218.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	12.310	1733	1738	1741	rVV6	12410	24375	3.98%	0.381%
36	12.351	1742	1745	1748	rVV5	10268	13450	2.20%	0.210%
37	12.422	1753	1757	1762	rBV	248828	234169	38.27%	3.656%
38	12.516	1771	1773	1777	rBV3	10707	16422	2.68%	0.256%
39	12.569	1777	1782	1786	rBV6	13286	27255	4.45%	0.425%
40	12.645	1790	1795	1800	rBV	202224	240492	39.30%	3.754%
41	12.792	1817	1820	1828	rVB	434295	391002	63.90%	6.104%
42	12.869	1831	1833	1836	rBV2	14486	14980	2.45%	0.234%
43	12.974	1849	1851	1854	rVB	46166	40599	6.63%	0.634%
44	13.039	1859	1862	1865	rVB2	34768	35752	5.84%	0.558%
45	13.080	1866	1869	1872	rBV2	23820	31797	5.20%	0.496%
46	13.839	1994	1998	2001	rBV	547709	611896	100.00%	9.553%
47	15.245	2234	2237	2241	rBV	269100	323629	52.89%	5.052%


Sum of corrected areas: 6405597

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF100318\
Data File : BF109556.D
Acq On : 3 Oct 2018 19:37
Operator : JU/SJ
Sample : J5218-05 5X
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
293-230

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF092218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

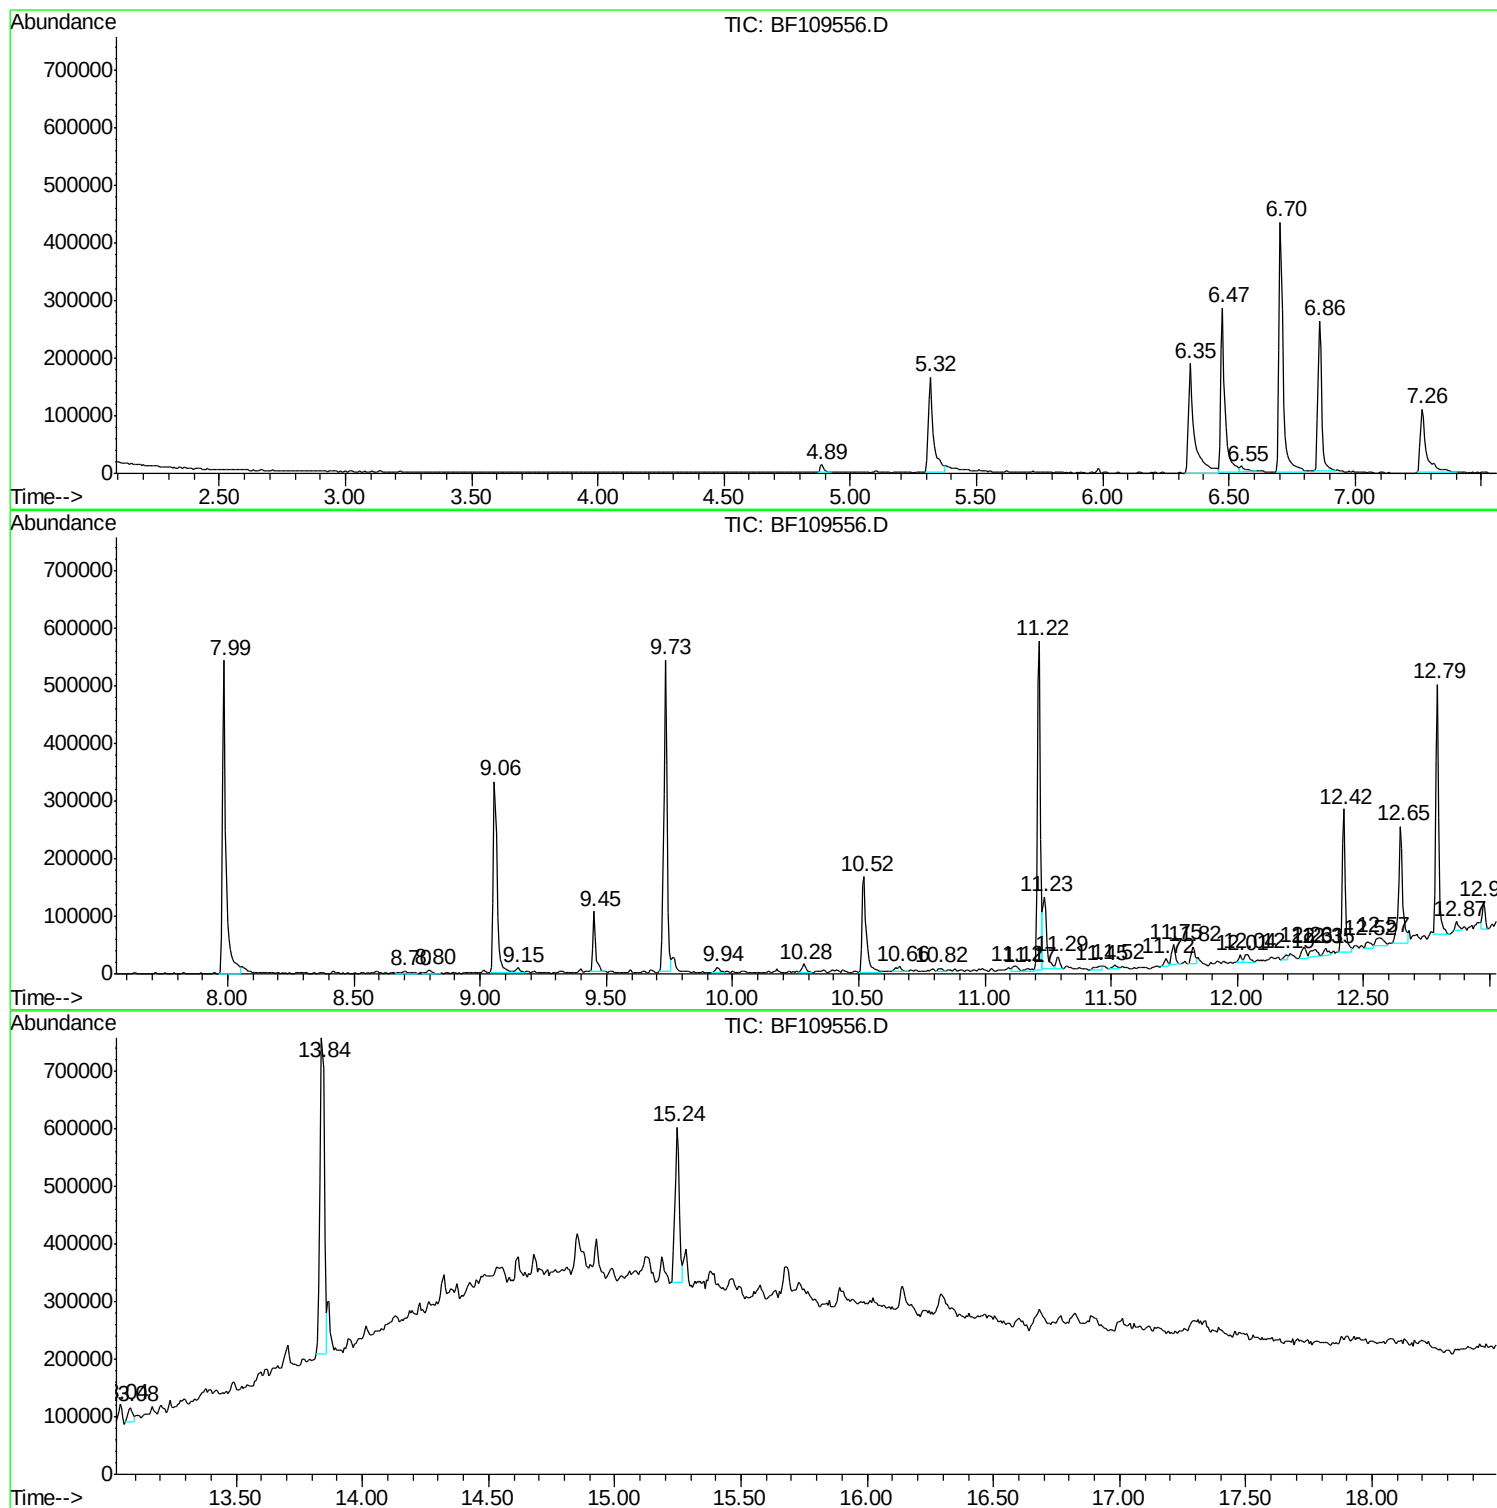

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF100318\
Data File : BF109556.D
Acq On : 3 Oct 2018 19:37
Operator : JU/SJ
Sample : J5218-05 5X
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
293-230










Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF092218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown6.47 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
6.47	14.60 ng	334535	1,4-Dichlorobenzene-d4	6.70

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			3-Chloro-6-fluoro-pyrazine	132	C4H2ClFN2	1000146-10-7	16
2			5-Aminoindole	132	C8H8N2	005192-03-0	12
3			Tranvlcypromine-propionyl	189	C12H15NO	1000123-86-3	10
4			Bicyclo[4.2.0]octa-1,3,5-triene,...	132	C10H12	028749-81-7	9
5			5-Fluoro-2-chloropyrimidine	132	C4H2ClFN2	062802-42-0	9

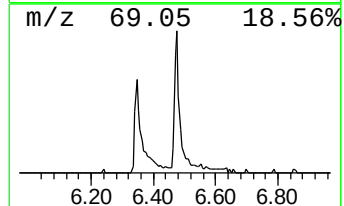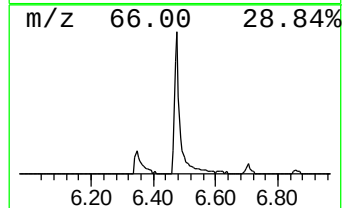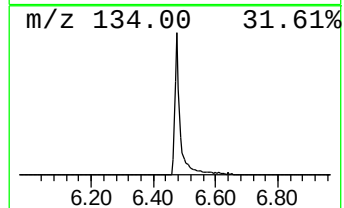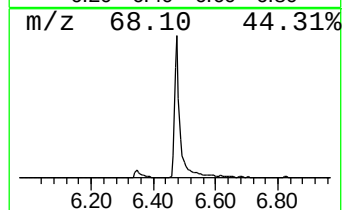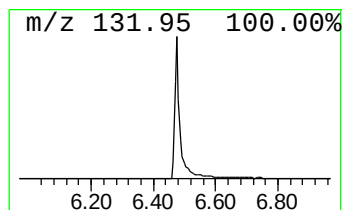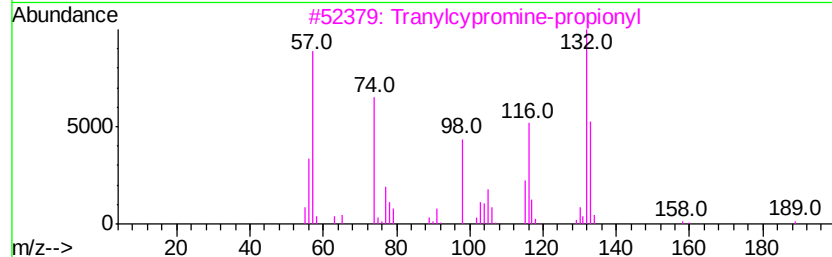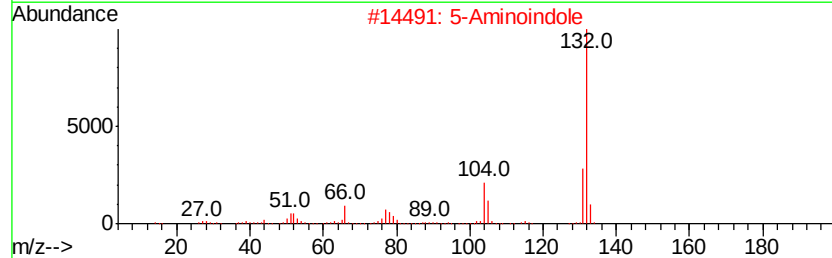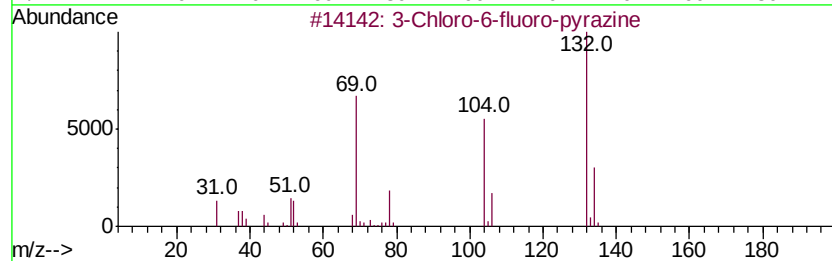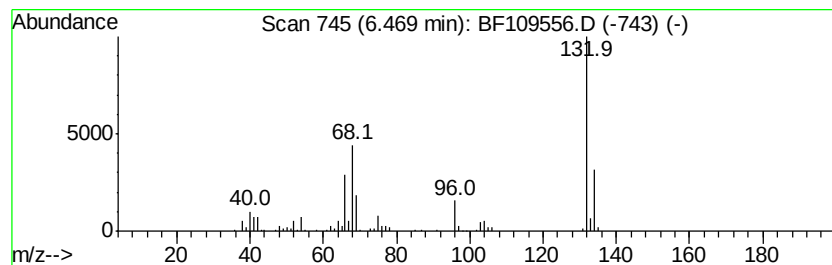

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF100318\
Data File : BF109556.D
Acq On : 3 Oct 2018 19:37
Operator : JU/SJ
Sample : J5218-05 5X
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
293-230

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF092218.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown6.47	6.47	14.6	ng	334535	1	6.70	458276	20.0