


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100318\
 Data File : BF109566.D
 Acq On : 4 Oct 2018 00:59
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF092218.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Sep 22 13:32:18 2018

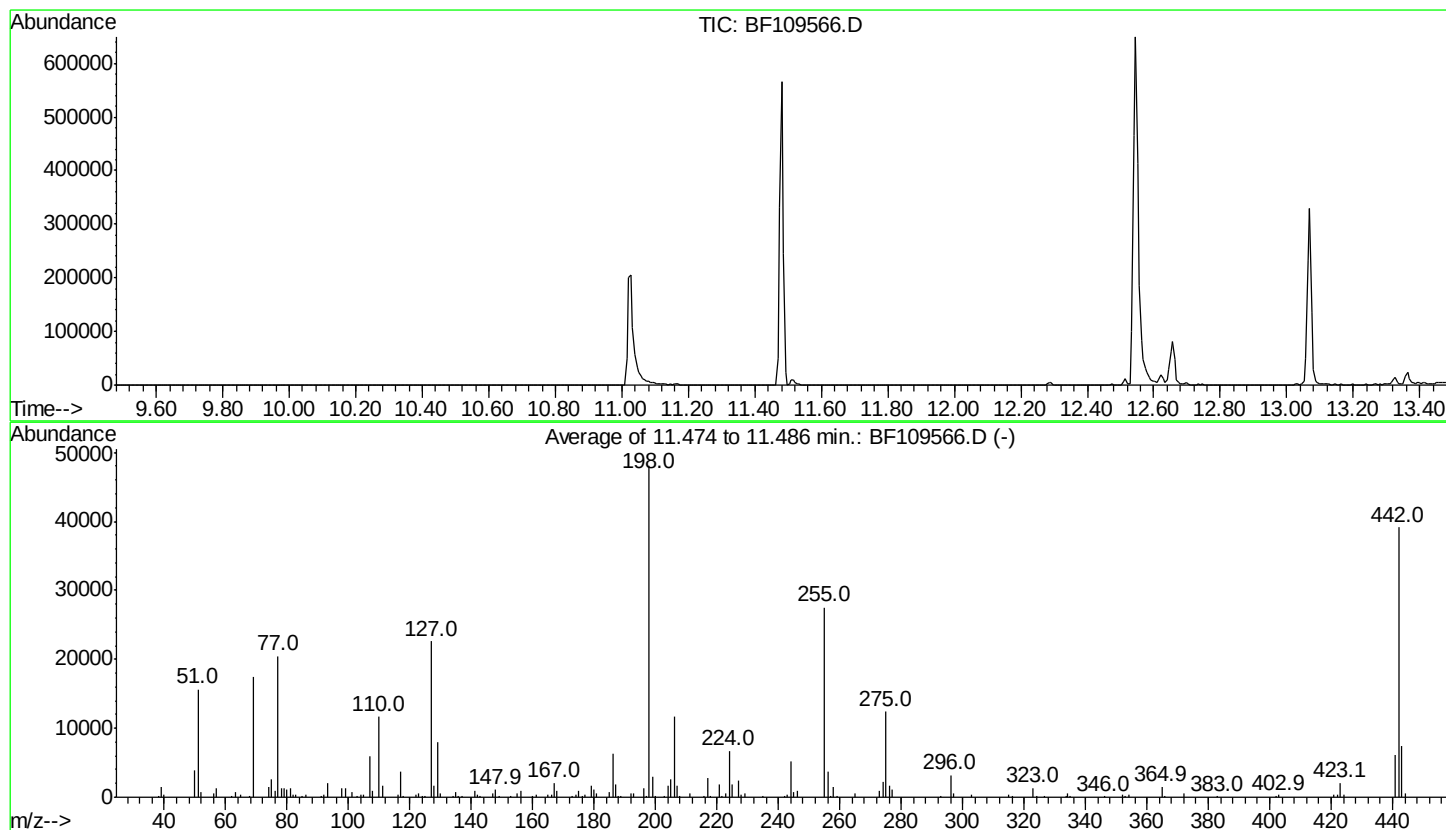

AutoFind: Scans 1596, 1597, 1598; Background Corrected with Scan 1592

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.5	15627	PASS
68	69	0.00	2	0.7	126	PASS
69	198	0.00	100	36.2	17418	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	47.0	22579	PASS
197	198	0.00	2	0.5	263	PASS
198	198	100	100	100.0	48085	PASS
199	198	5	9	6.4	3057	PASS
275	198	10	60	25.8	12402	PASS
365	198	1	100	3.2	1561	PASS
441	198	0.01	100	12.6	6054	PASS
442	198	50	100	81.4	39162	PASS
443	442	15	24	19.0	7434	PASS