

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100322\
 Data File : BF130494.D
 Acq On : 03 Oct 2022 12:51
 Operator : CG\JU
 Sample : PB148034BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB148034BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF130494.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.851	463	470	482	rBV	72484	128101	3.10%	0.494%
2	5.251	533	538	541	rBV	3184341	3438543	83.33%	13.273%
3	6.287	708	714	716	rBV	2998124	3463111	83.93%	13.368%
4	6.634	770	773	777	rBV	841569	670832	16.26%	2.589%
5	7.204	864	870	873	rBV	2077434	2323507	56.31%	8.969%
6	7.916	986	991	999	rBV	930364	909986	22.05%	3.513%
7	8.998	1168	1175	1178	rBV	4379756	4126221	100.00%	15.928%
8	9.669	1283	1289	1299	rBV	1278103	1171913	28.40%	4.524%
9	10.457	1419	1423	1439	rBV	2774754	2838397	68.79%	10.956%
10	11.151	1537	1541	1552	rVB	1348908	1232215	29.86%	4.756%
11	12.739	1806	1811	1814	rBV	4442748	4093860	99.22%	15.803%
12	13.780	1984	1988	1998	rBV	827536	802568	19.45%	3.098%
13	15.168	2220	2224	2238	rVB	382672	571815	13.86%	2.207%
14	16.039	2368	2372	2379	rVB2	30820	47576	1.15%	0.184%
15	16.568	2456	2462	2472	rVB4	21303	45037	1.09%	0.174%
16	17.186	2561	2567	2575	rVB5	17220	42388	1.03%	0.164%




Sum of corrected areas: 25906070

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100322\
Data File : BF130494.D
Acq On : 03 Oct 2022 12:51
Operator : CG\JU
Sample : PB148034BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB148034BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

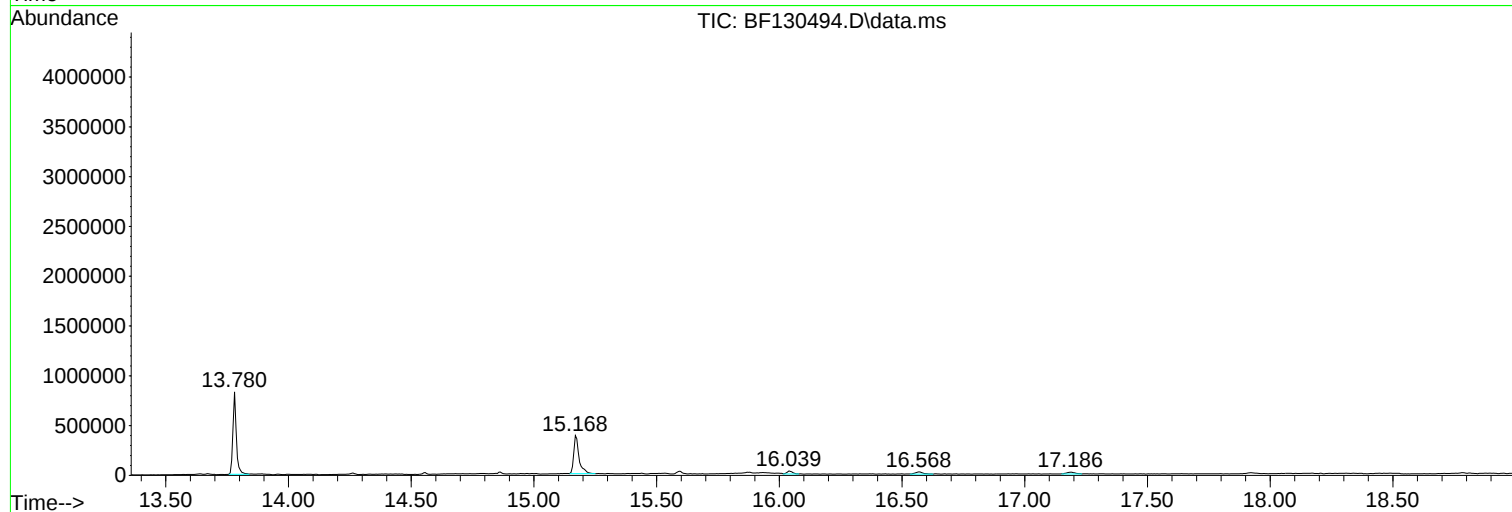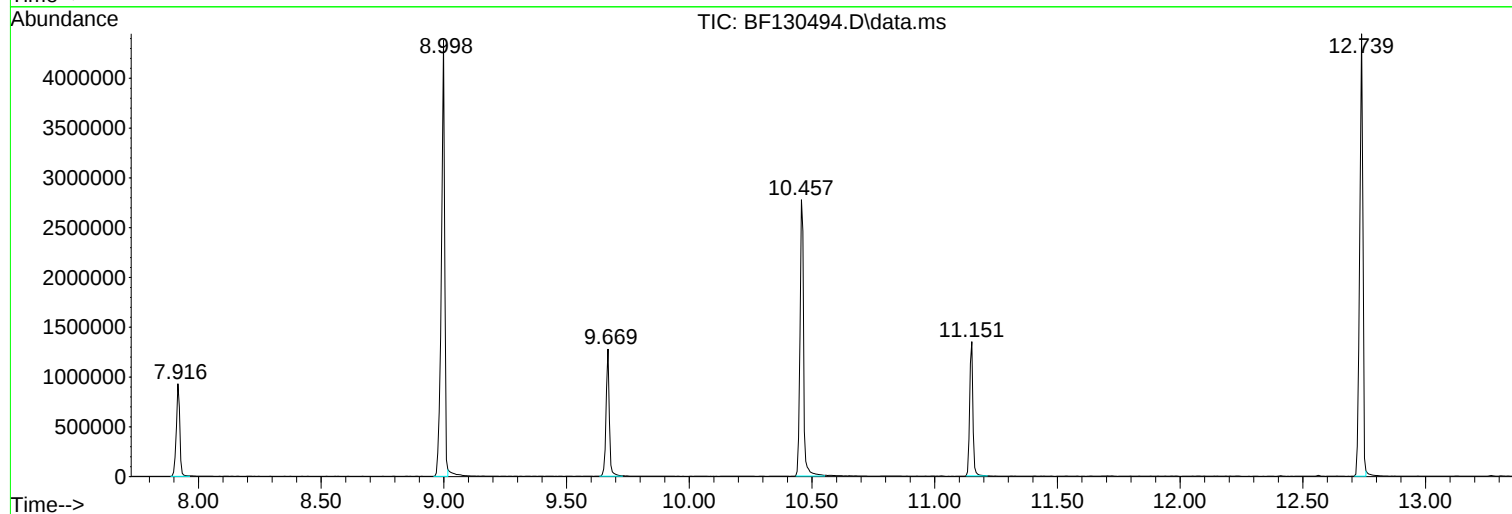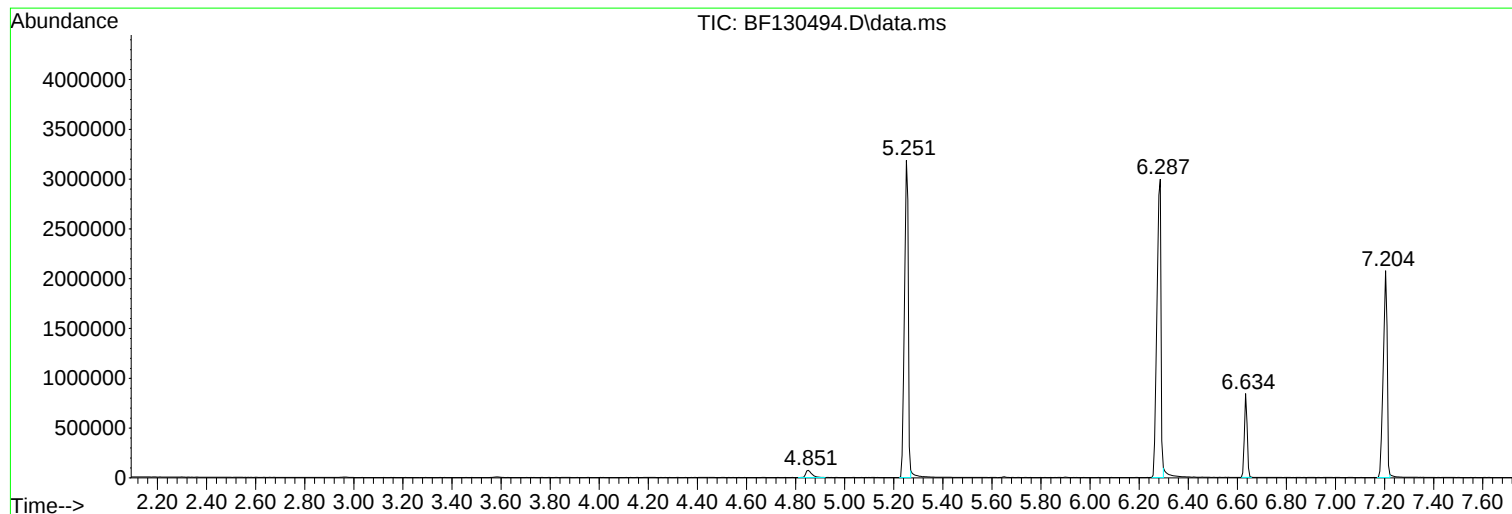

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100322\
Data File : BF130494.D
Acq On : 03 Oct 2022 12:51
Operator : CG\JU
Sample : PB148034BL
Misc :
ALS Vial : 3 Sample Multiplier: 1










Instrument :
BNA_F
ClientSampleId :
PB148034BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD			R.T.
4.851	3.82 ng	128101	1,4-Dichlorobenzene-d4			6.634
Hit# of 5	Tentative ID		MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-		116	C6H12O2	000123-42-2	59
2	Acetic acid, 1,1-dimethylethyl e...		116	C6H12O2	000540-88-5	45
3	1-Propen-2-ol, acetate		100	C5H8O2	000108-22-5	10
4	2,3-Butanedione, monooxime		101	C4H7NO2	000057-71-6	10
5	2-Propyn-1-ol, acetate		98	C5H6O2	000627-09-8	9

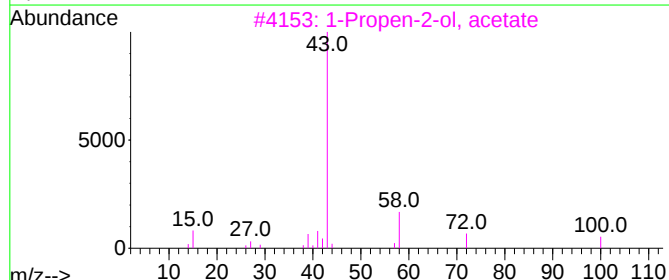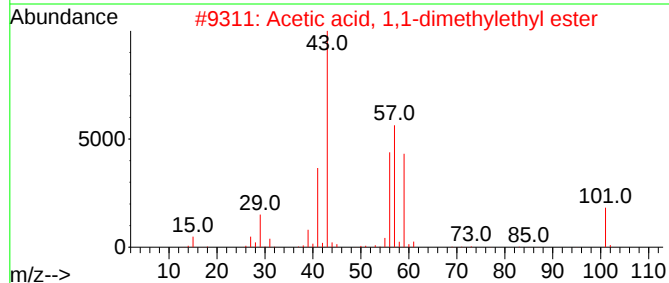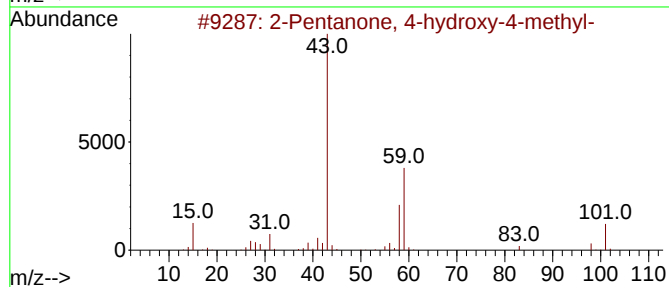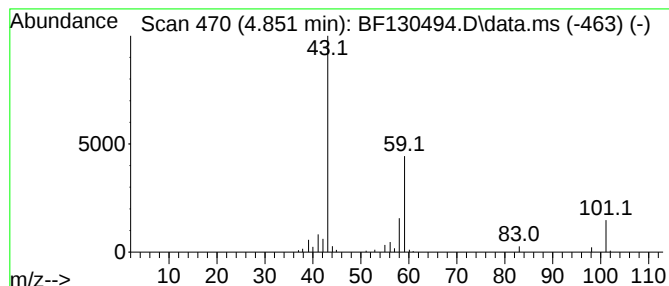

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100322\
Data File : BF130494.D
Acq On : 03 Oct 2022 12:51
Operator : CG\JU
Sample : PB148034BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB148034BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	4.851	3.8	ng	128101	1	6.634	670832	20.0