


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100322\
 Data File : BF130492.D
 Acq On : 03 Oct 2022 11:21
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Sep 28 02:59:31 2022

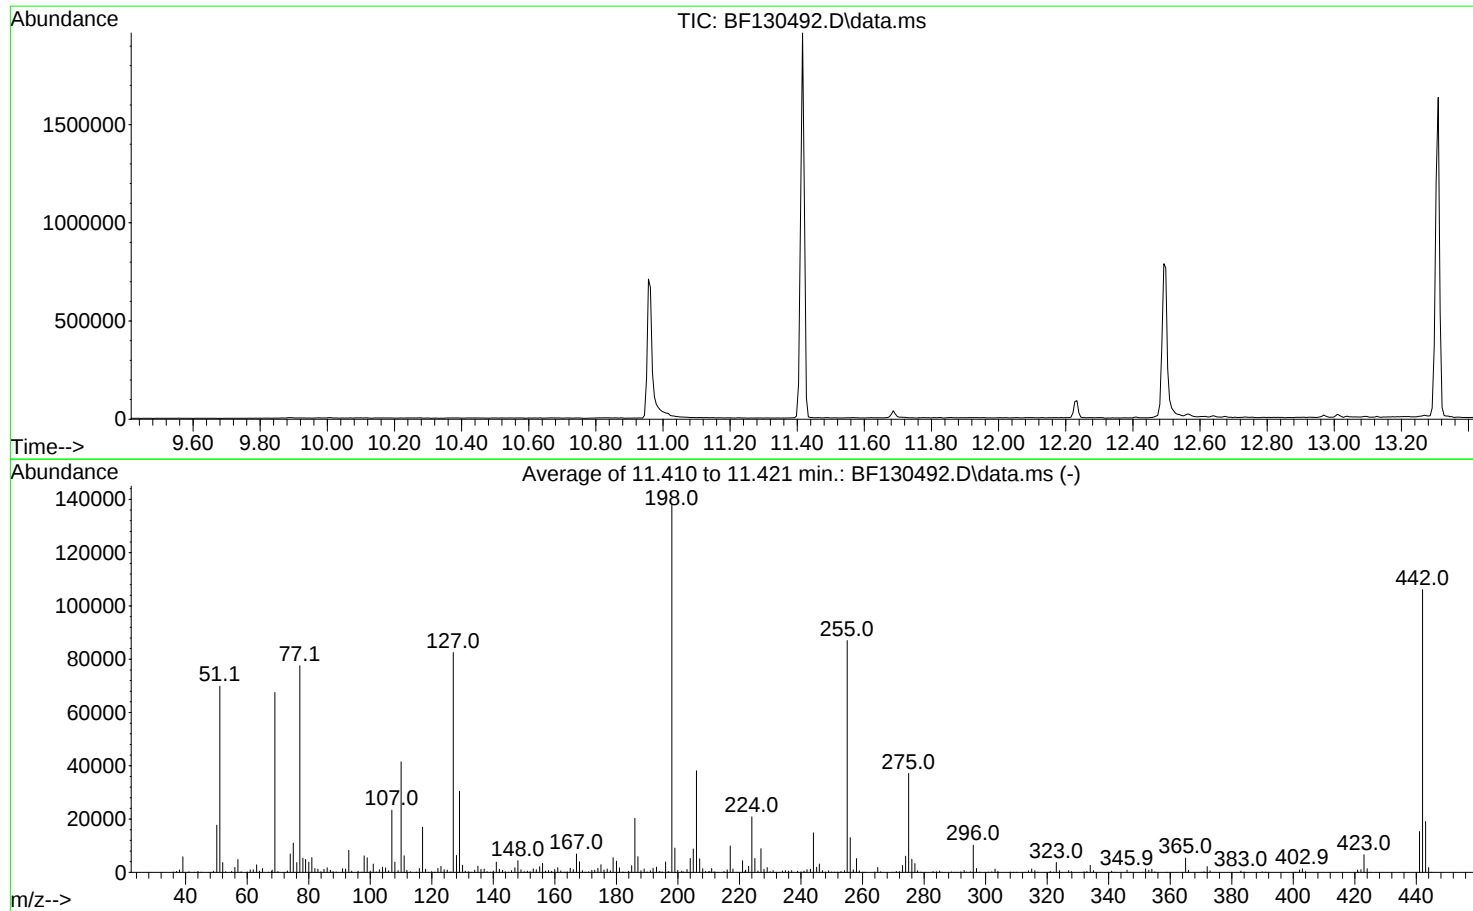




AutoFind: Scans 1585, 1586, 1587; Background Corrected with Scan 1580

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	50.6	69859	PASS
68	69	0.00	2	1.3	902	PASS
69	198	0.00	100	48.9	67515	PASS
70	69	0.00	2	0.4	284	PASS
127	198	10	80	59.7	82501	PASS
197	198	0.00	2	0.2	230	PASS
198	198	100	100	100.0	138077	PASS
199	198	5	9	6.6	9130	PASS
275	198	10	60	26.9	37136	PASS
365	198	1	100	3.9	5366	PASS
441	198	0.01	100	11.1	15315	PASS
442	442	50	100	100.0	106096	PASS
443	442	15	24	18.0	19098	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100322\
 Data File : BF130492.D
 Acq On : 03 Oct 2022 11:21
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Oct 04 06:43:05 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 28 02:59:31 2022
 Response via : Initial Calibration

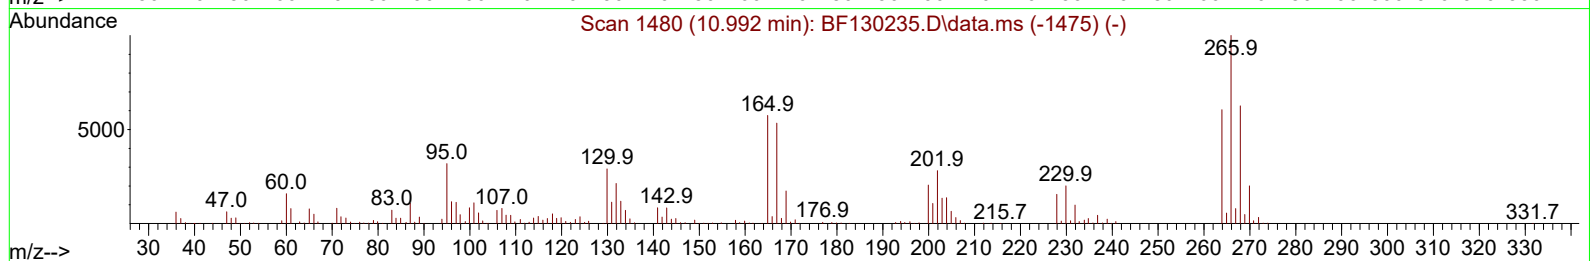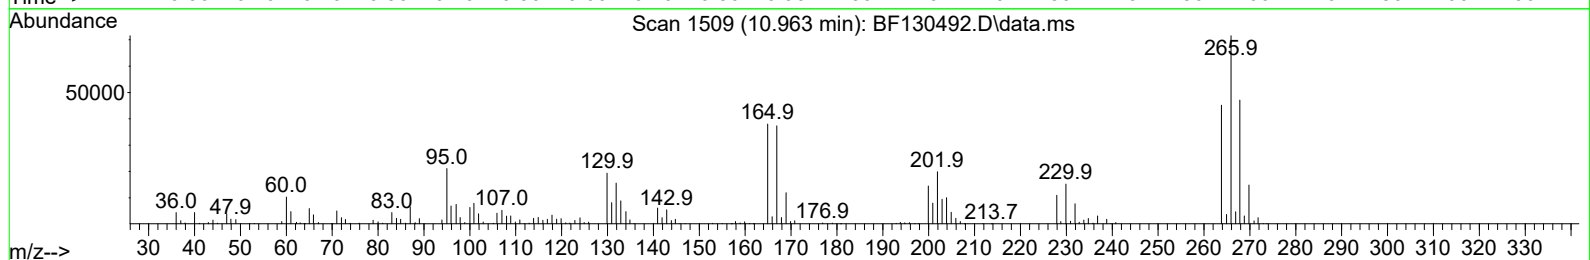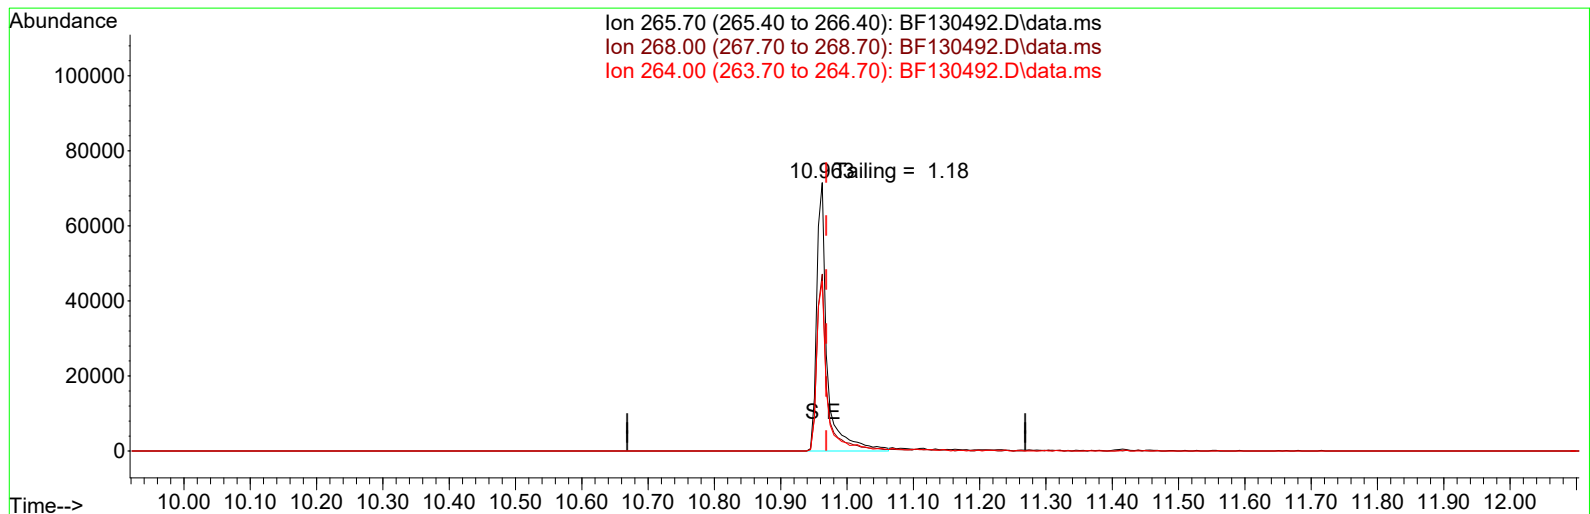

TIC: BF130492.D\data.ms

(70) Pentachlorophenol (C)

10.963min (-0.006) 18241.47 ng




response 79576

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	65.89
264.00	63.10	63.17
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100322\
Data File : BF130492.D
Acq On : 03 Oct 2022 11:21
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 04 06:43:05 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 28 02:59:31 2022
Response via : Initial Calibration

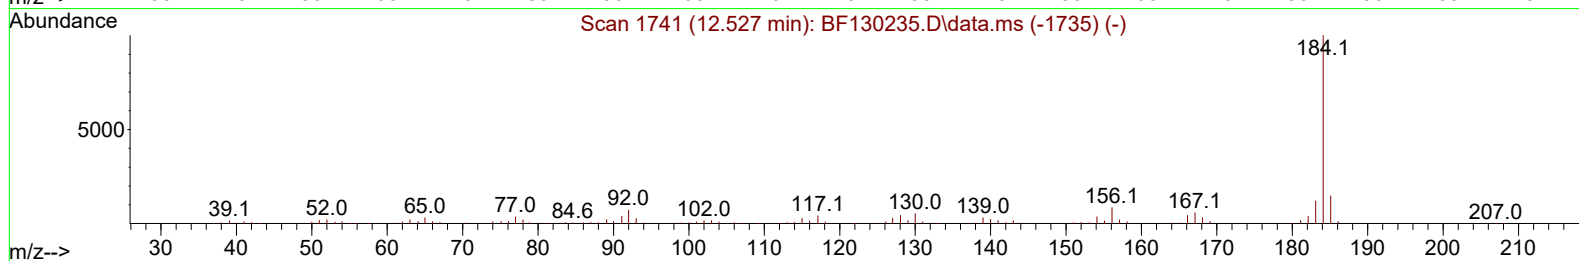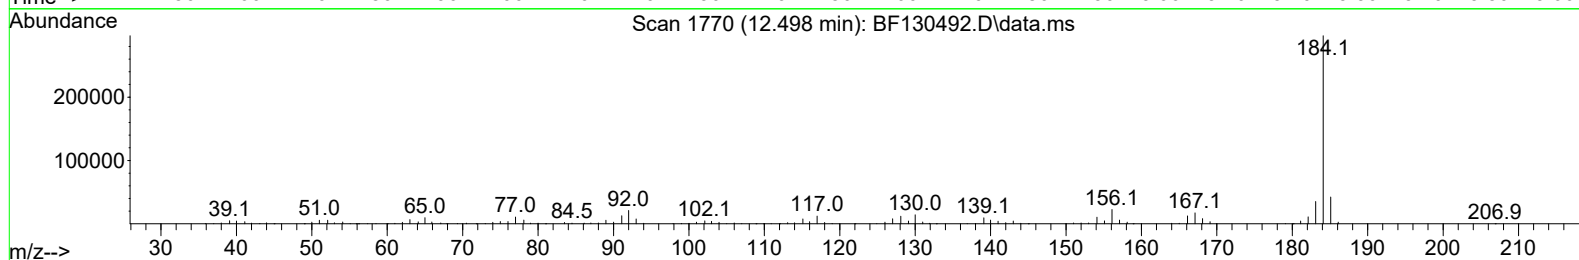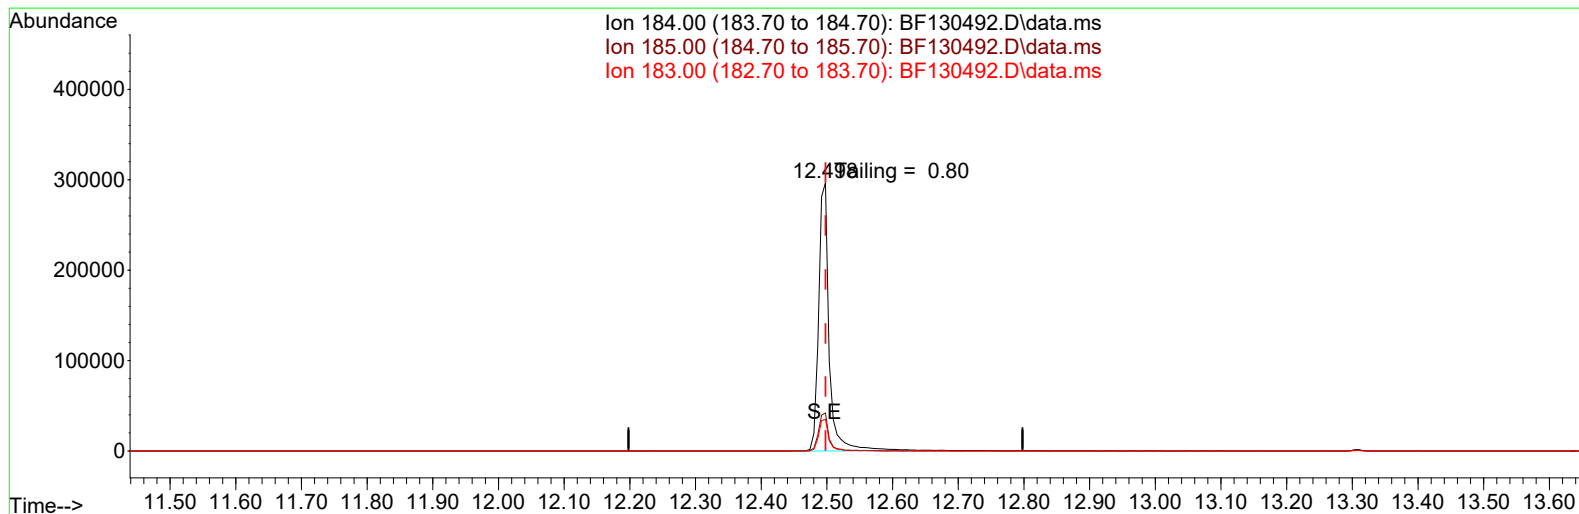

TIC: BF130492.D\data.ms

(77) Benzidine

12.498min (-0.000) 0.00 ng

response 332970

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.22
183.00	11.40	11.90
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/3/2022	BNA_F	<u>BF130492.D</u>
Compound Name	Response	Retention Time
DDT	205563	13.31
DDD	3408	13.01
DDE	706	12.674
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4114	209677	1.96

Instrument :
BNA_F
ClientSampleId :
DFTPP