
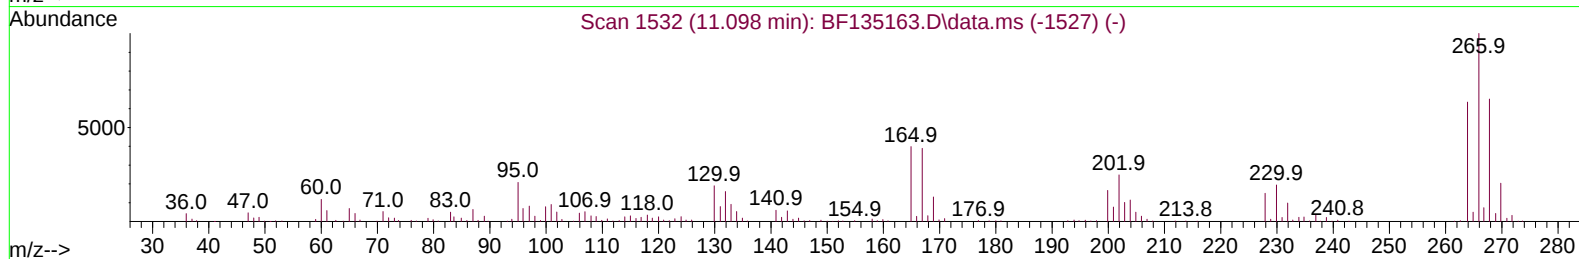
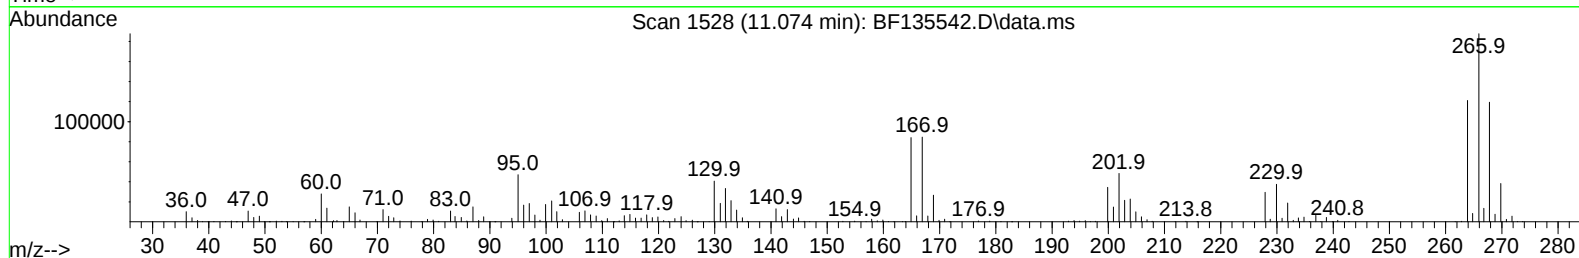


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100323\
Data File : BF135542.D
Acq On : 03 Oct 2023 14:30
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 04 07:55:27 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 04 06:58:43 2023
Response via : Initial Calibration

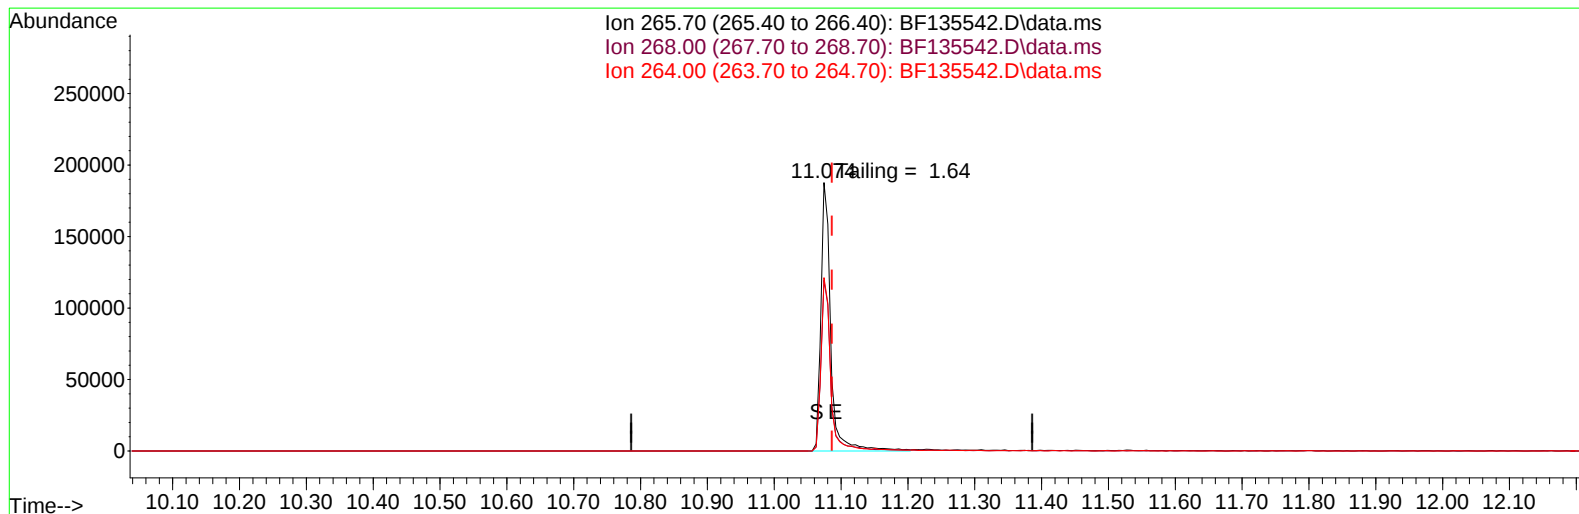

TIC: BF135542.D\data.ms

(70) Pentachlorophenol (C)




11.074min (-0.012) 43895.42 ng

response 192659

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.10	63.64
264.00	63.50	64.55
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100323\
Data File : BF135542.D
Acq On : 03 Oct 2023 14:30
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 04 07:55:27 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 04 06:58:43 2023
Response via : Initial Calibration

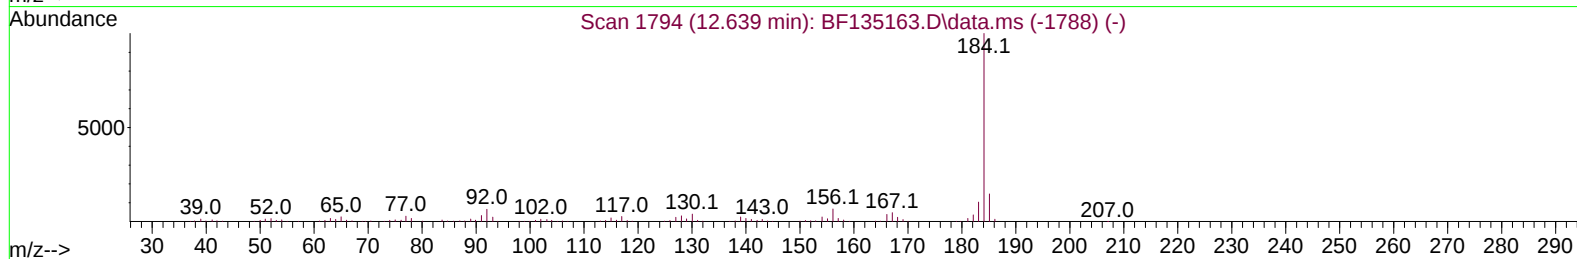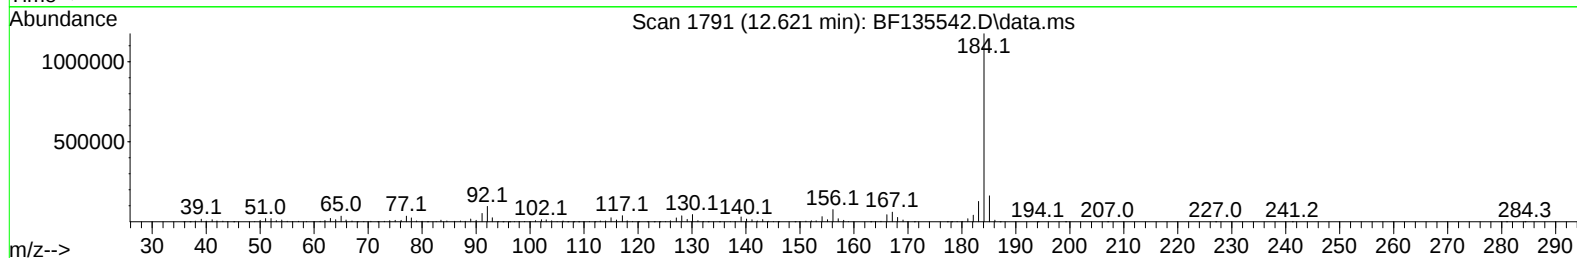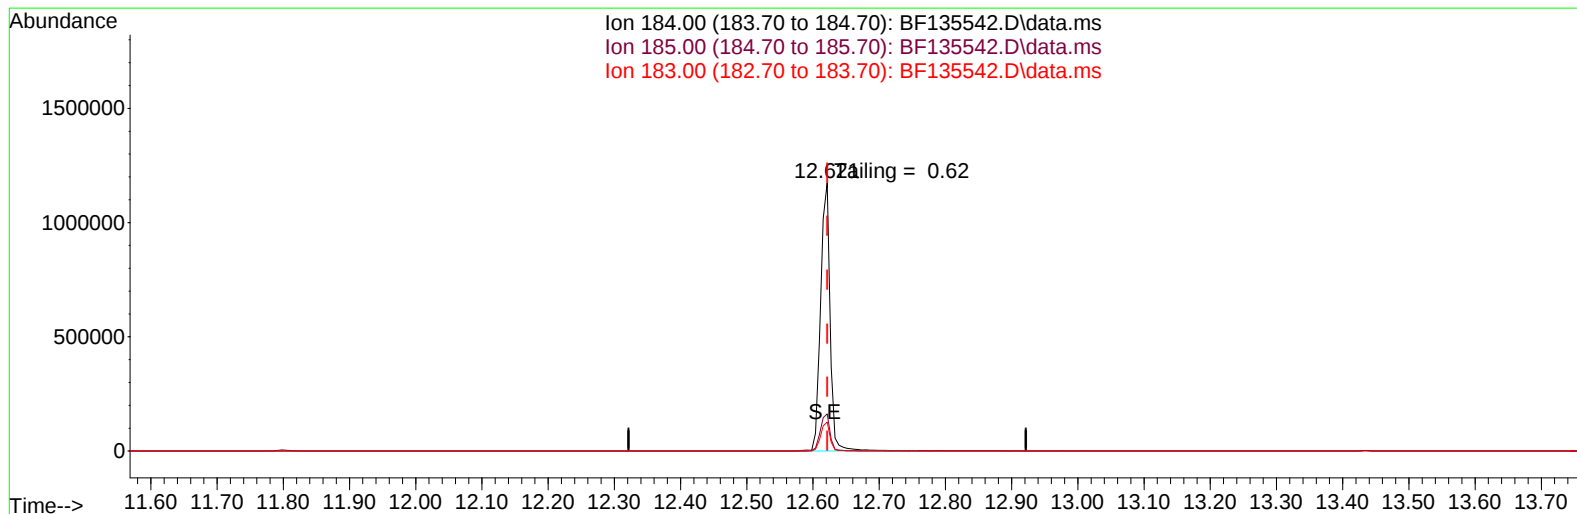

TIC: BF135542.D\data.ms

(77) Benzidine

12.621min (-0.000) 929519.86 ng

response 1161618

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	13.84
183.00	10.30	10.84
0.00	0.00	0.00