


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100323\
Data File : BF135542.D
Acq On : 03 Oct 2023 14:30
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Oct 04 14:41:55 2023

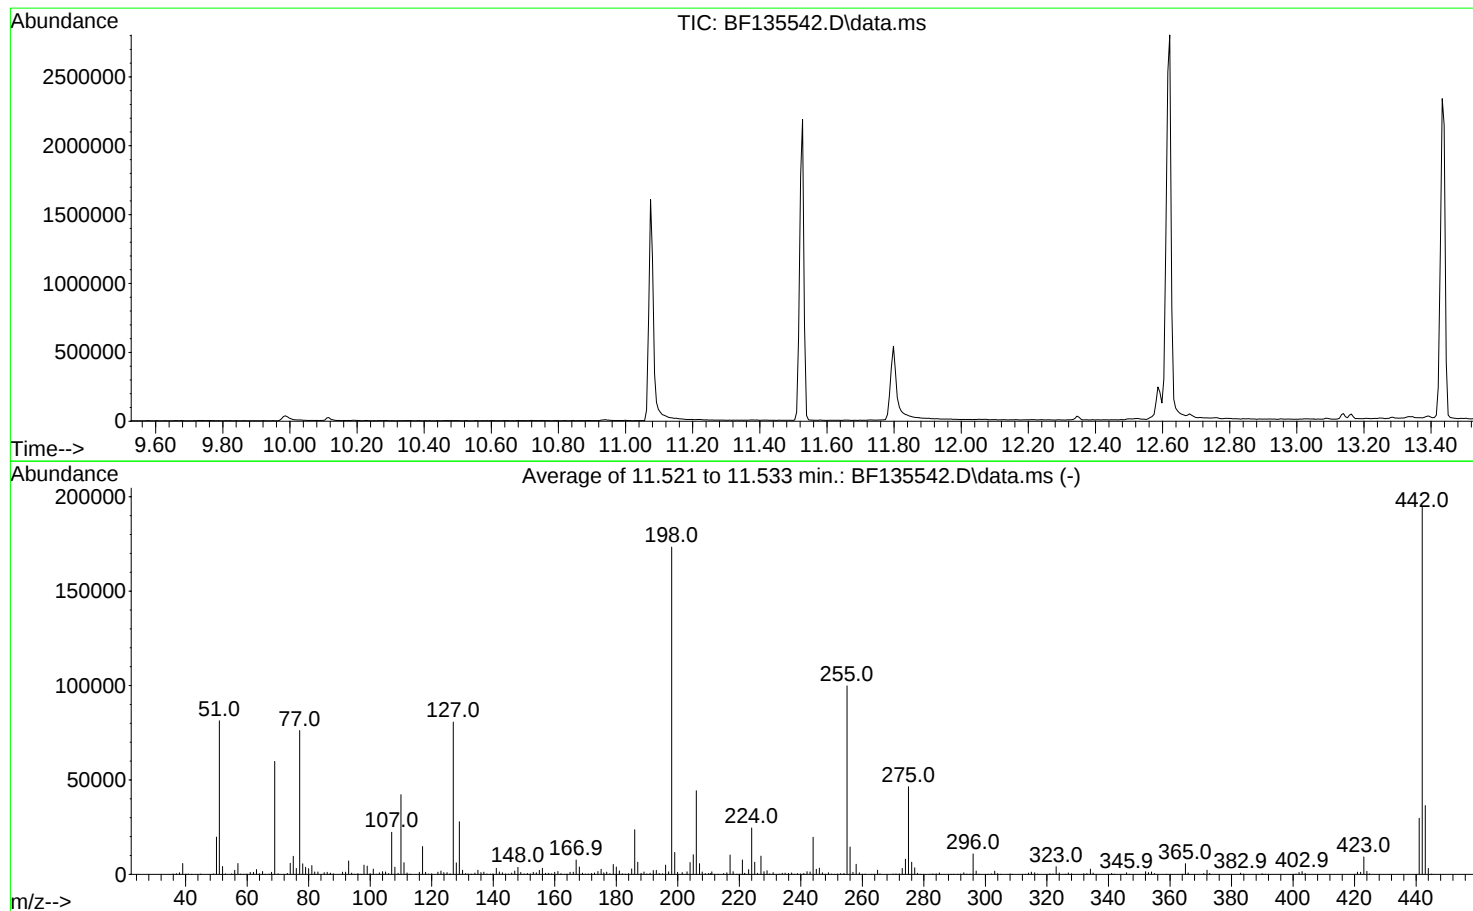




AutoFind: Scans 1604, 1605, 1606; Background Corrected with Scan 1598

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	47.0	81363	PASS
68	69	0.00	2	1.9	1139	PASS
69	198	0.00	100	34.5	59866	PASS
70	69	0.00	2	0.6	341	PASS
127	198	10	80	46.5	80643	PASS
197	198	0.00	2	0.8	1323	PASS
198	198	100	100	100.0	173285	PASS
199	198	5	9	6.7	11639	PASS
275	198	10	60	26.8	46403	PASS
365	198	1	100	3.3	5673	PASS
441	198	0.01	100	17.1	29707	PASS
442	442	50	100	100.0	194816	PASS
443	442	15	24	18.7	36400	PASS

```
Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100323\  
Data File : BF135542.D  
Acq On    : 03 Oct 2023  14:30  
Operator  : CG\JU  
Sample    : DFTPP  
Misc      :  
ALS Vial  : 1    Sample Multiplier: 1
```

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 04 07:55:27 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 04 06:58:43 2023
Response via : Initial Calibration

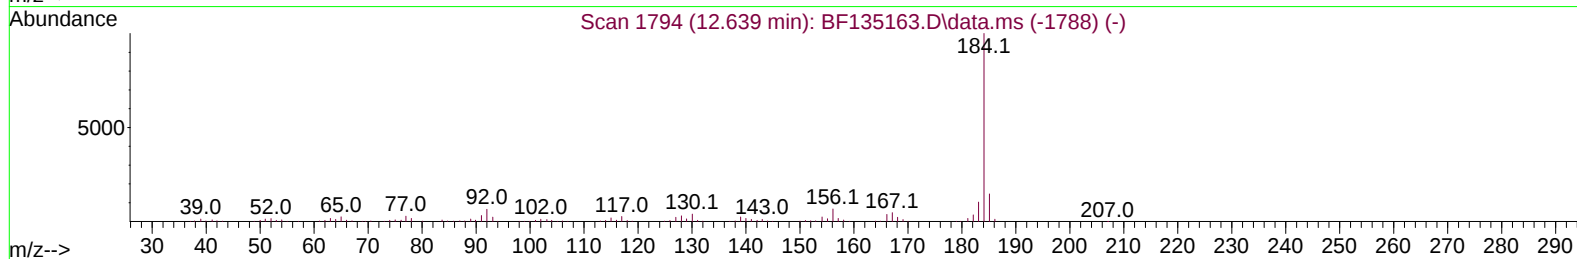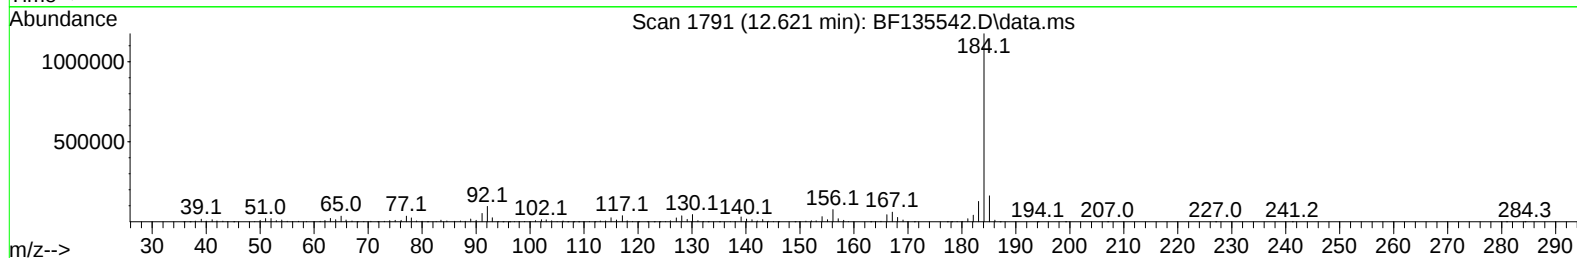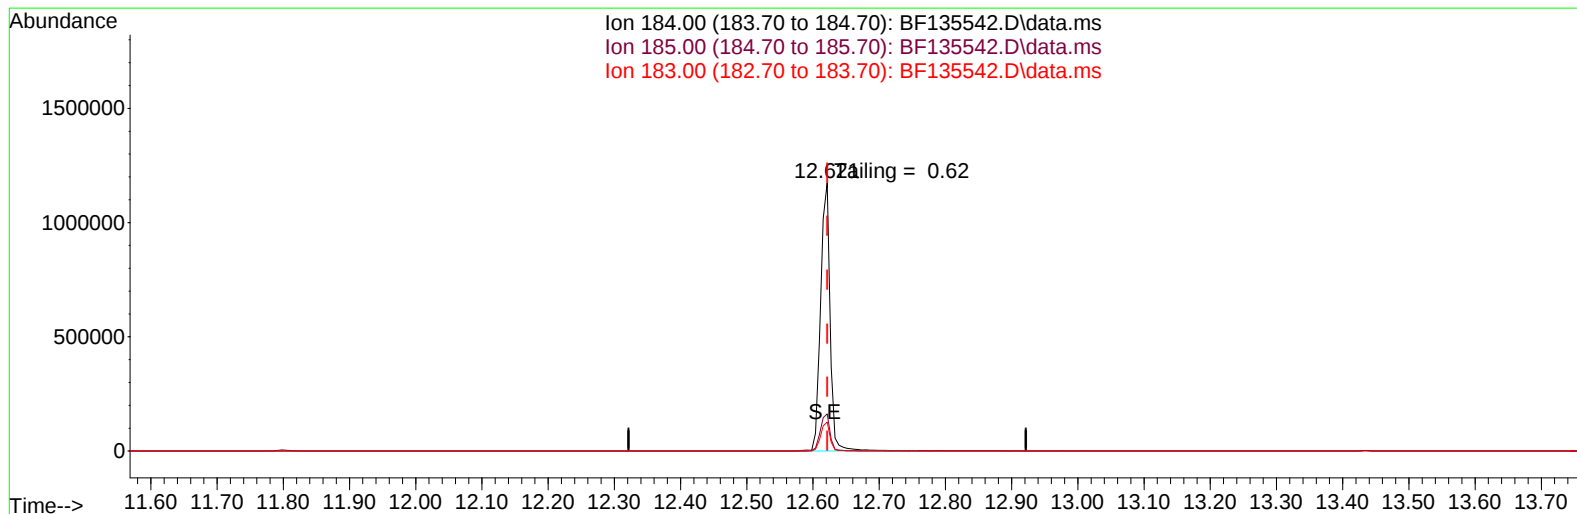

TIC: BF135542.D\data.ms

(77) Benzidine

12.621min (-0.000) 929519.86 ng

response 1161618

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	13.84
183.00	10.30	10.84
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/3/2023	BNA_F	<u>BF135542.D</u>
Compound Name	Response	Retention Time
DDT	451495	13.433
DDD	12447	13.139
DDE	401	12.798
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
12848	464343	2.77

Instrument :
BNA_F
ClientSampleId :
DFTPP