
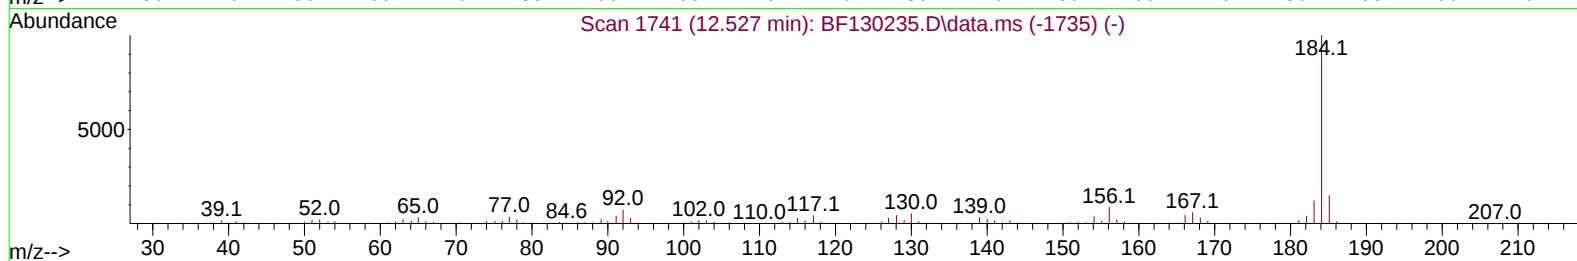
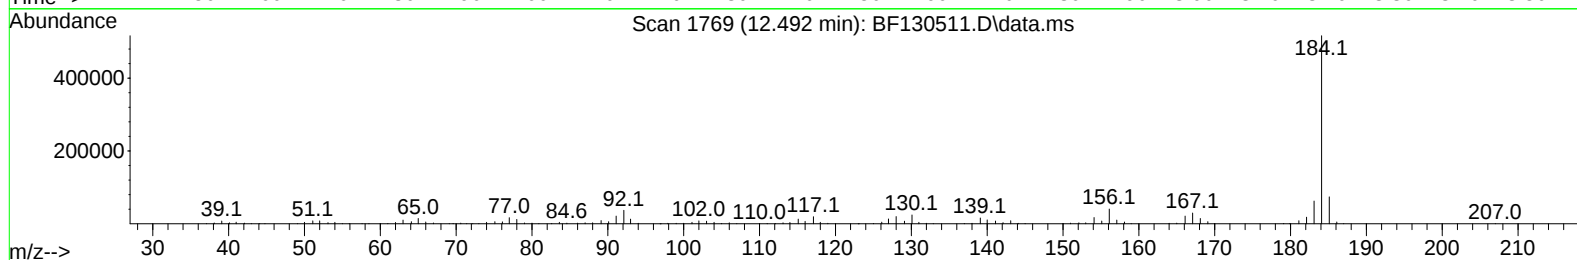


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100422\
 Data File : BF130511.D
 Acq On : 04 Oct 2022 10:58
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 05 03:25:20 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 28 02:59:31 2022
 Response via : Initial Calibration

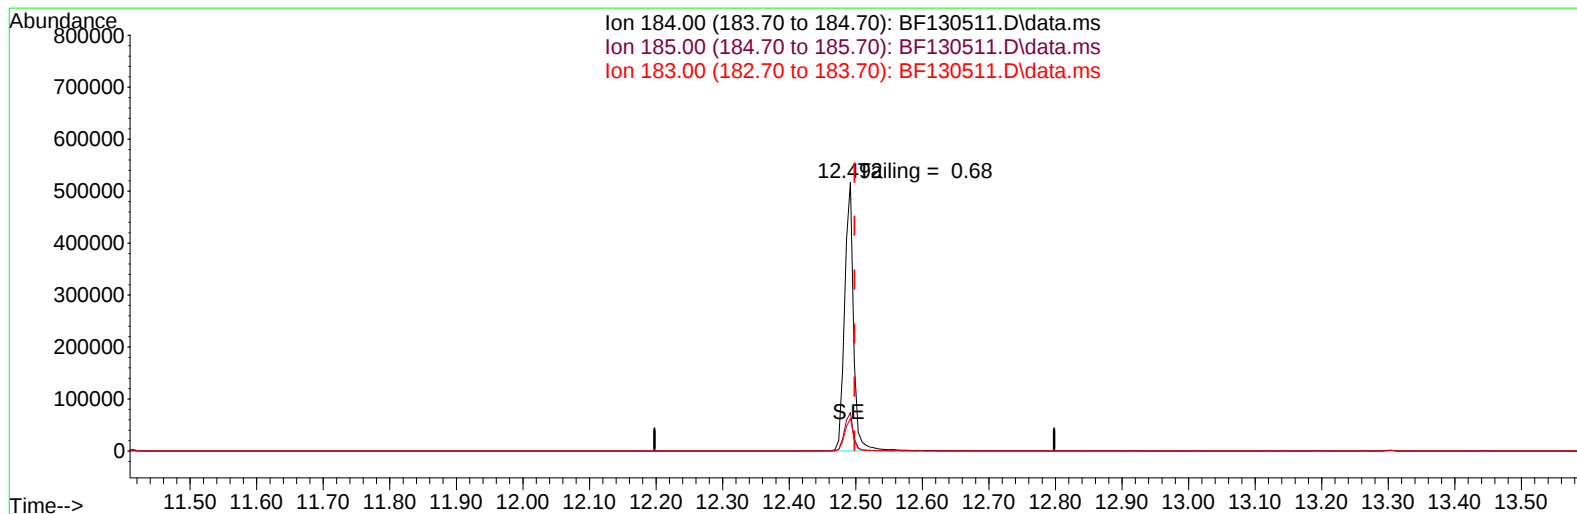

TIC: BF130511.D\data.ms

(77) Benzidine




12.492min (-0.006) 0.00 ng

response 483189

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.29
183.00	11.40	12.11
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100422\
Data File : BF130511.D
Acq On : 04 Oct 2022 10:58
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 05 03:25:20 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 28 02:59:31 2022
Response via : Initial Calibration

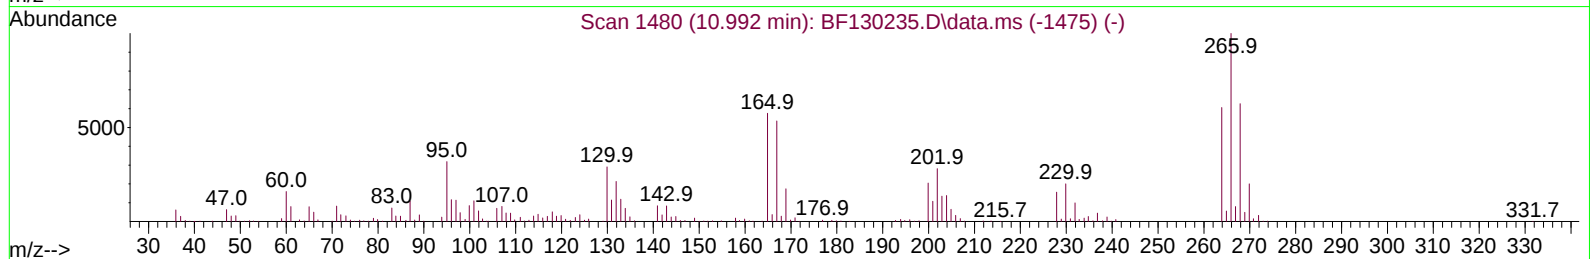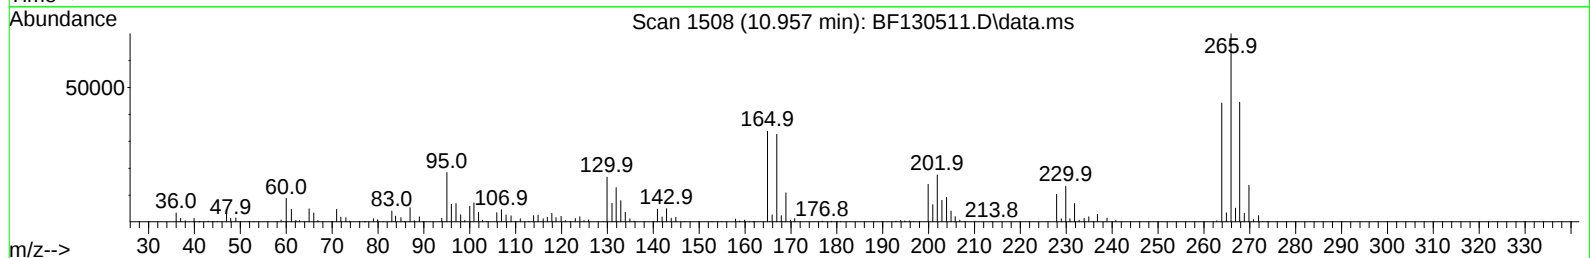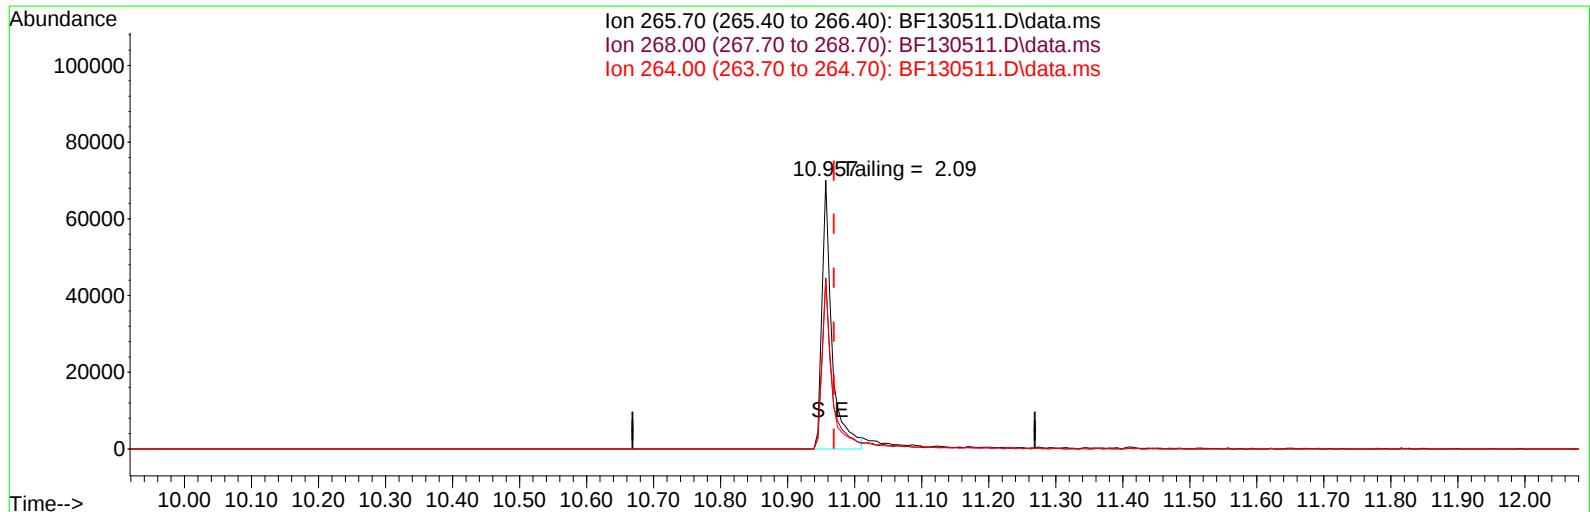

TIC: BF130511.D\data.ms

(70) Pentachlorophenol (C)

10.957min (-0.012) 21826.01 ng

response 79686

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	63.64
264.00	63.10	63.16
0.00	0.00	0.00