

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100422\
 Data File : BF130526.D
 Acq On : 04 Oct 2022 19:17
 Operator : CG\JU
 Sample : N4919-01
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 265393-6

Quant Time: Oct 05 02:21:26 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Sep 28 02:59:31 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	6.634	152	90846	20.000	ng	-0.01
21) Naphthalene-d8	7.916	136	346204	20.000	ng	#-0.01
39) Acenaphthene-d10	9.663	164	166162	20.000	ng	-0.02
64) Phenanthrene-d10	11.145	188	235115	20.000	ng	-0.01
76) Chrysene-d12	13.774	240	152406	20.000	ng	-0.02
86) Perylene-d12	15.163	264	182694	20.000	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.234	112	349996	66.822	ng	-0.01
7) Phenol-d6	6.275	99	272327	41.554	ng	-0.02
23) Nitrobenzene-d5	7.204	82	614610	90.697	ng	-0.01
42) 2,4,6-Tribromophenol	10.451	330	223010	140.069	ng	-0.02
45) 2-Fluorobiphenyl	8.992	172	1095895	96.041	ng	-0.02
79) Terphenyl-d14	12.727	244	848838	92.260	ng	-0.02


Target Compounds	Qvalue
-----	-----

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100422\
Data File : BF130526.D
Acq On : 04 Oct 2022 19:17
Operator : CG\JU
Sample : N4919-01
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
265393-6

Quant Time: Oct 05 02:21:26 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 28 02:59:31 2022
Response via : Initial Calibration




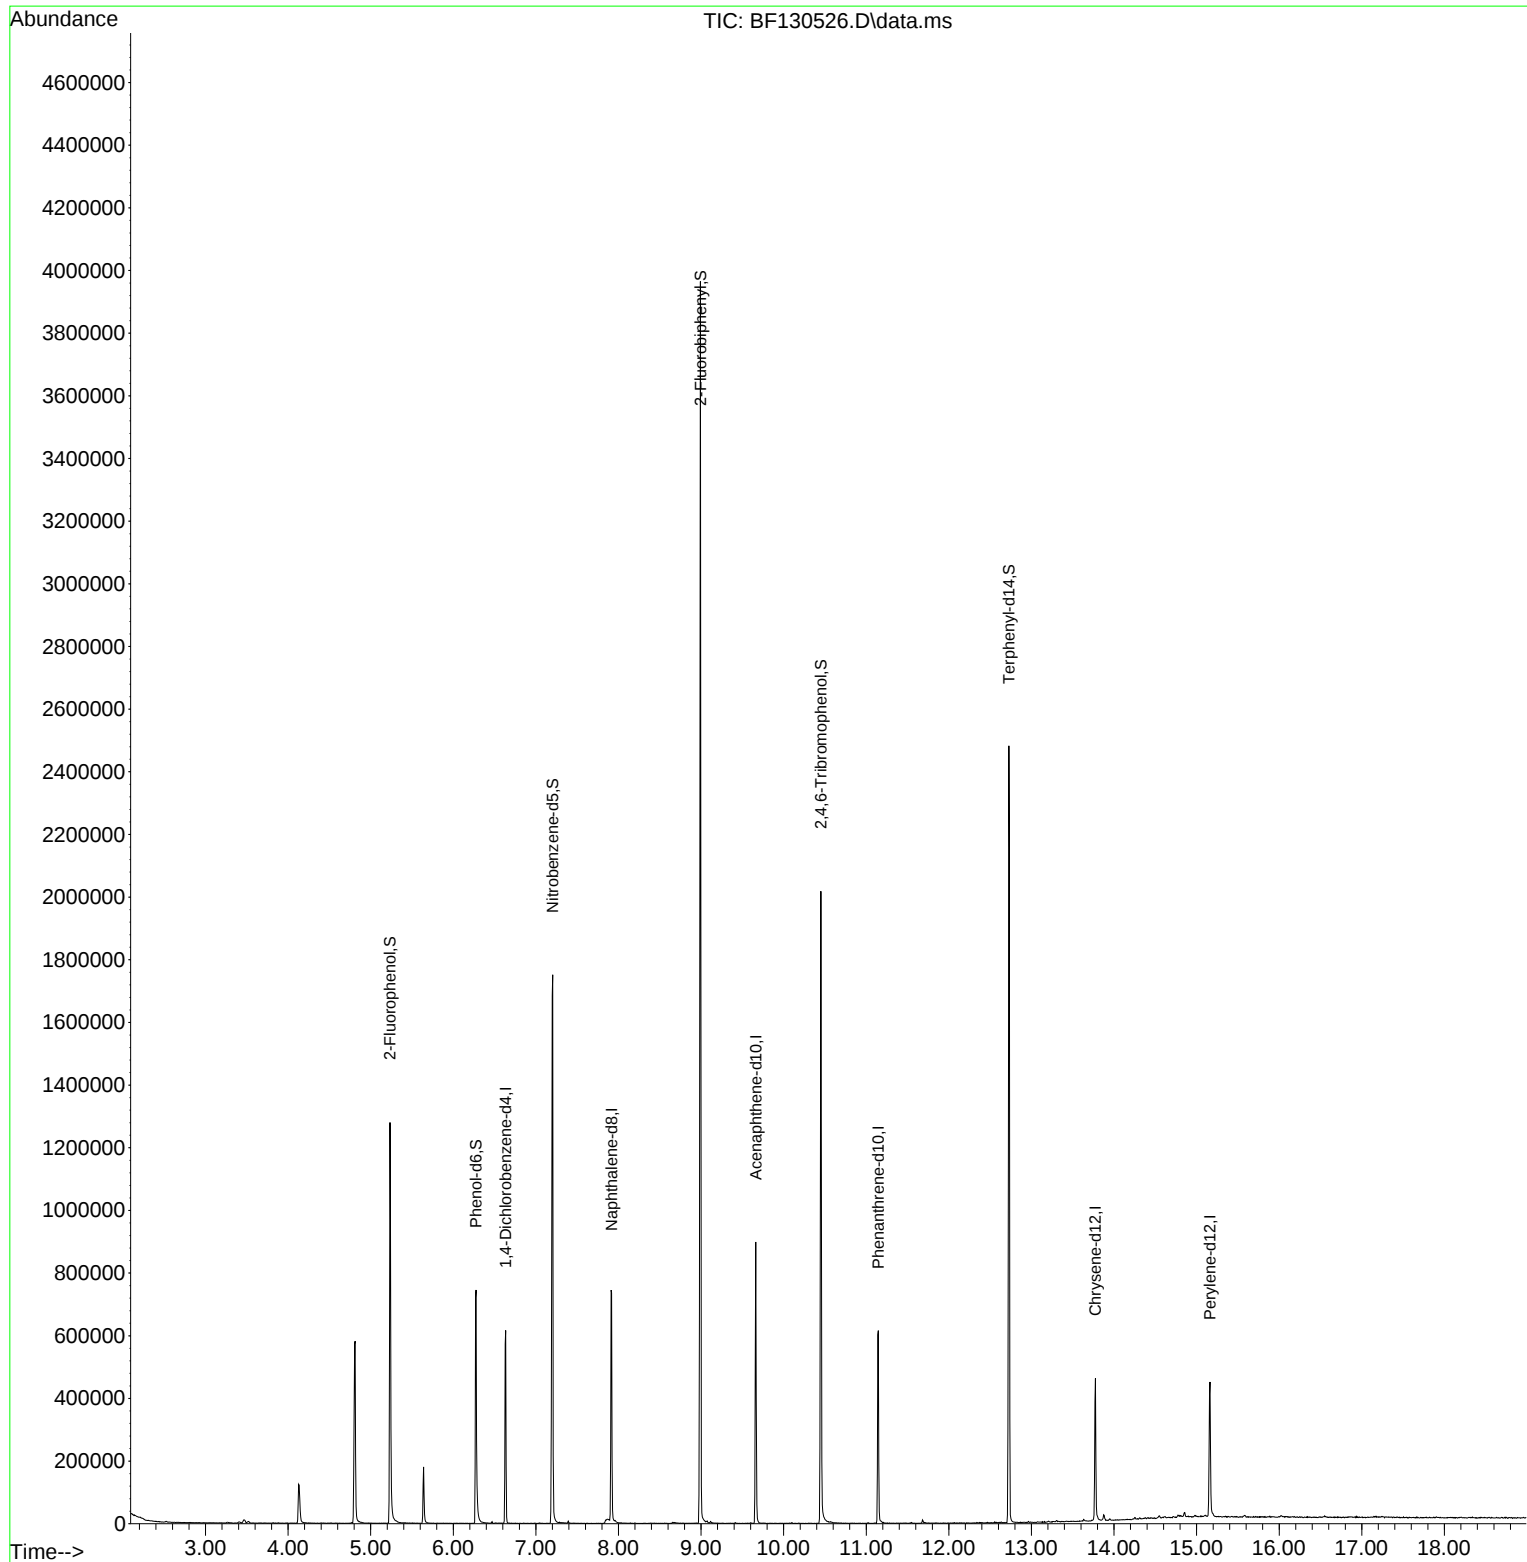




#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.634 min Scan# 71
Delta R.T. -0.011 min
Lab File: BF130526.D
Acq: 04 Oct 2022 19:17




Instrument :
BNA_F
ClientSampleId :
265393-6


Tgt Ion:152 Resp: 90846
Ion Ratio Lower Upper
152 100
150 154.2 122.8 184.2
115 61.5 53.8 80.8

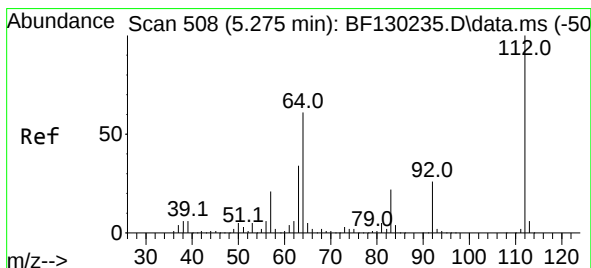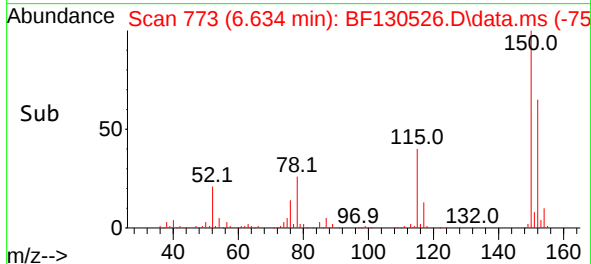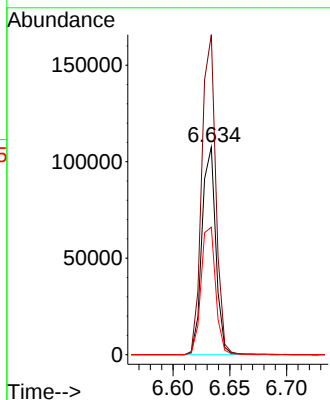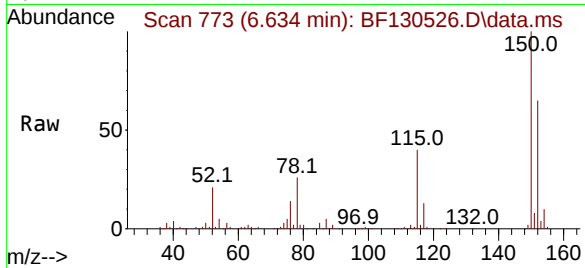

#5
2-Fluorophenol
Concen: 66.822 ng
RT: 5.234 min Scan# 535
Delta R.T. -0.012 min
Lab File: BF130526.D
Acq: 04 Oct 2022 19:17

Tgt Ion:112 Resp: 349996
Ion Ratio Lower Upper
112 100
64 62.1 51.4 77.0
63 32.7 28.8 43.2


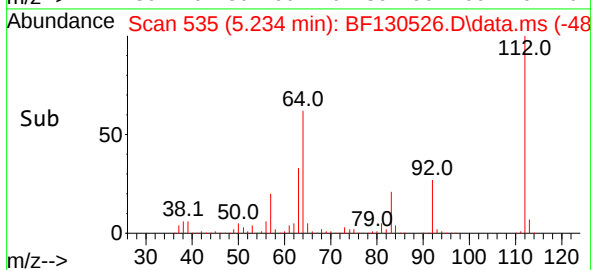
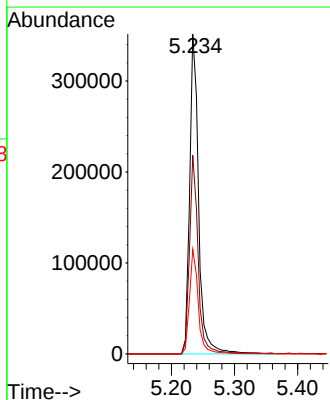
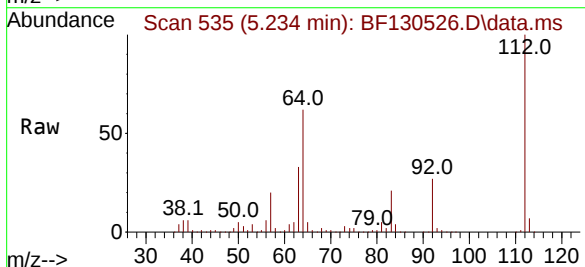


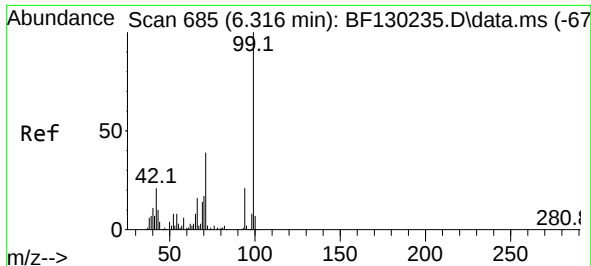

#7
Phenol-d6
Concen: 41.554 ng
RT: 6.275 min Scan# 71
Delta R.T. -0.018 min
Lab File: BF130526.D
Acq: 04 Oct 2022 19:17




Instrument :
BNA_F
ClientSampleId :
265393-6


Tgt Ion: 99 Resp: 272327
Ion Ratio Lower Upper
99 100
42 17.6 17.0 25.6
71 35.5 32.3 48.5

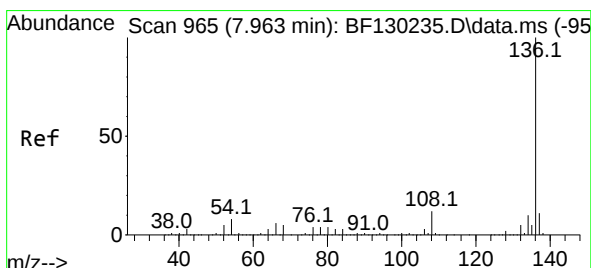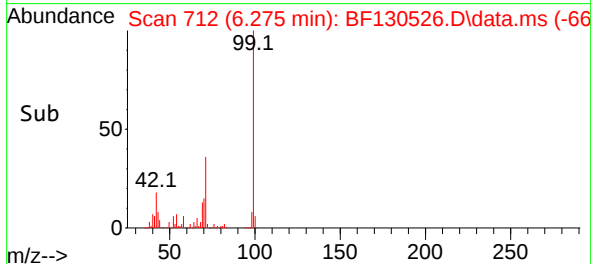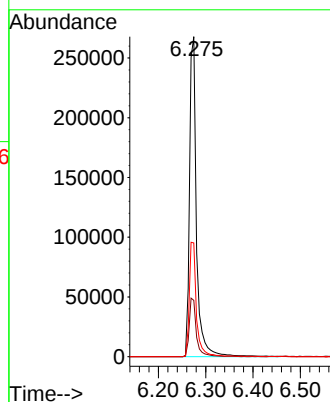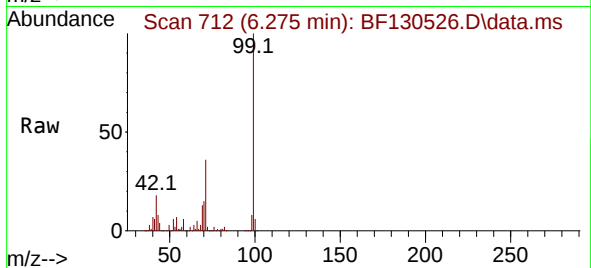

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 7.916 min Scan# 991
Delta R.T. -0.012 min
Lab File: BF130526.D
Acq: 04 Oct 2022 19:17

Tgt Ion: 136 Resp: 346204
Ion Ratio Lower Upper
136 100
137 10.4 9.1 13.7
54 6.6 7.1 10.7#
68 4.4 4.5 6.7#

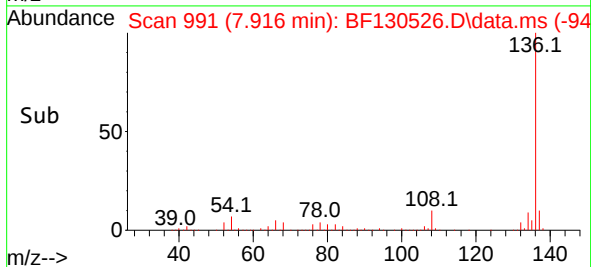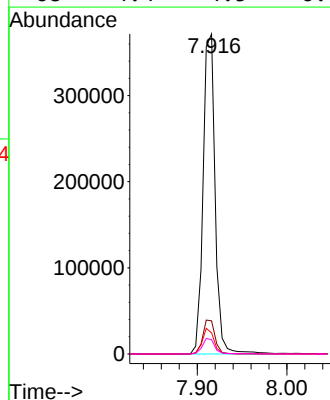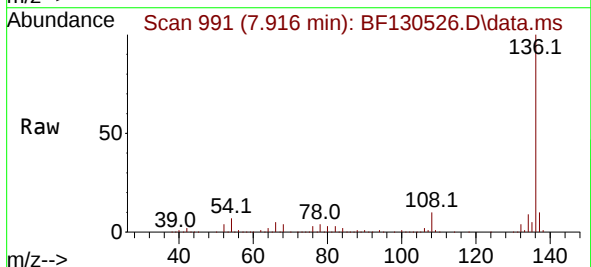

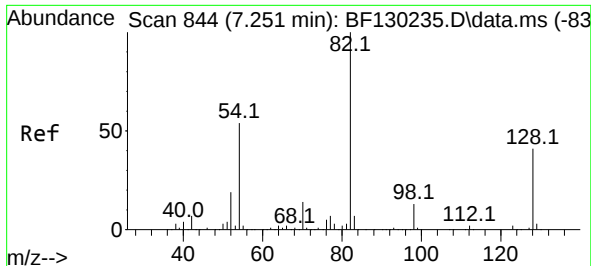

#23

Nitrobenzene-d5

Concen: 90.697 ng

RT: 7.204 min Scan# 81

Delta R.T. -0.012 min

Lab File: BF130526.D

Acq: 04 Oct 2022 19:17

Instrument :

BNA_F

ClientSampleId :

265393-6





Tgt Ion: 82 Resp: 614610

Ion Ratio Lower Upper

82 100

128 45.7 32.6 49.0

54 48.4 43.8 65.6

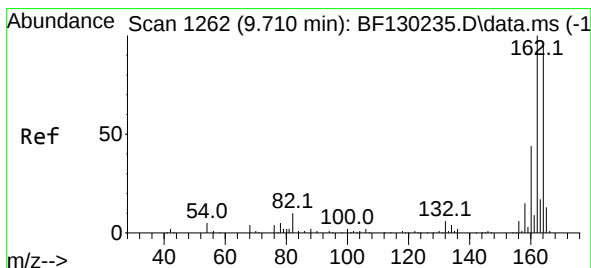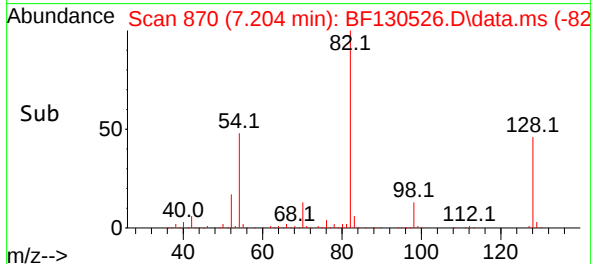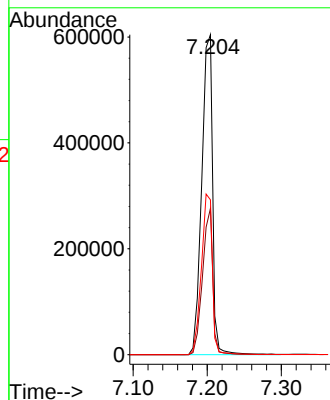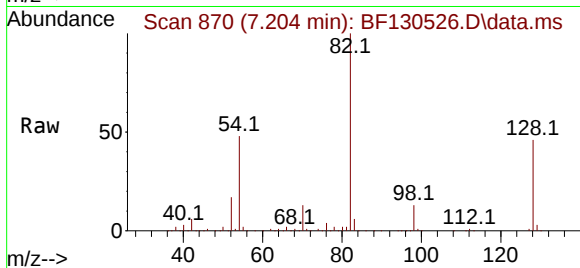

#39

Acenaphthene-d10

Concen: 20.000 ng

RT: 9.663 min Scan# 1288

Delta R.T. -0.018 min

Lab File: BF130526.D

Acq: 04 Oct 2022 19:17




Tgt Ion:164 Resp: 166162


Ion Ratio Lower Upper

164 100

162 101.1 81.4 122.0

160 43.5 36.2 54.4


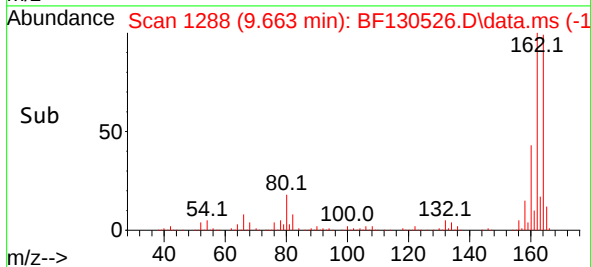
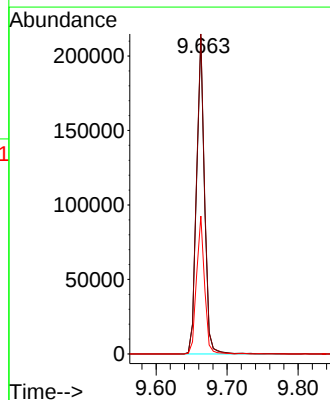
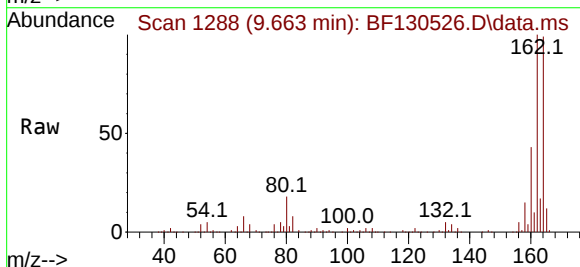


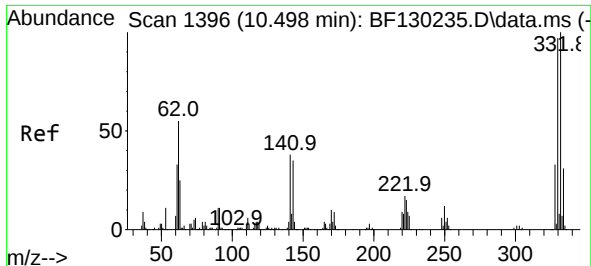

#42
2,4,6-Tribromophenol
Concen: 140.069 ng
RT: 10.451 min Scan# 1422
Delta R.T. -0.018 min
Lab File: BF130526.D
Acq: 04 Oct 2022 19:17




Instrument :
BNA_F
ClientSampleId :
265393-6


Tgt Ion:330 Resp: 223010
Ion Ratio Lower Upper
330 100
332 103.9 83.4 125.2
141 35.8 34.0 51.0

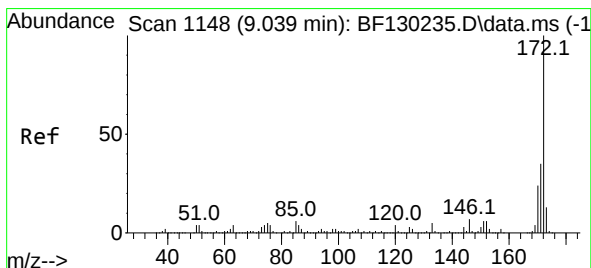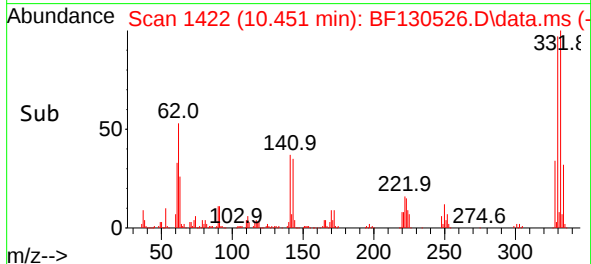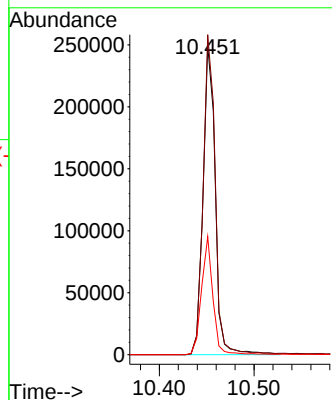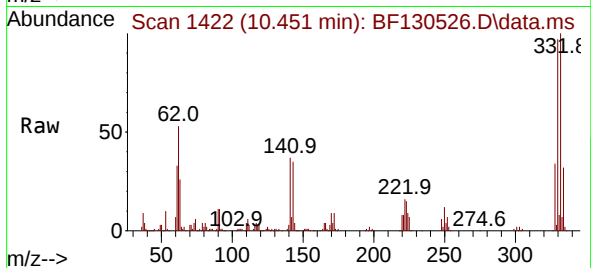

#45
2-Fluorobiphenyl
Concen: 96.041 ng
RT: 8.992 min Scan# 1174
Delta R.T. -0.018 min
Lab File: BF130526.D
Acq: 04 Oct 2022 19:17

Tgt Ion:172 Resp: 1095895
Ion Ratio Lower Upper
172 100
171 35.5 28.3 42.5
170 23.3 18.7 28.1

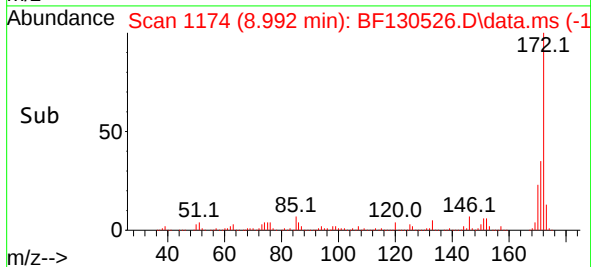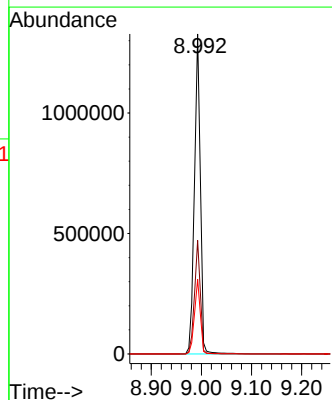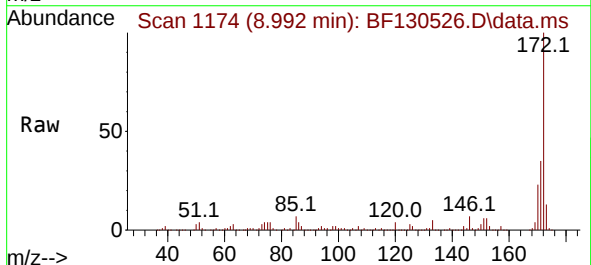

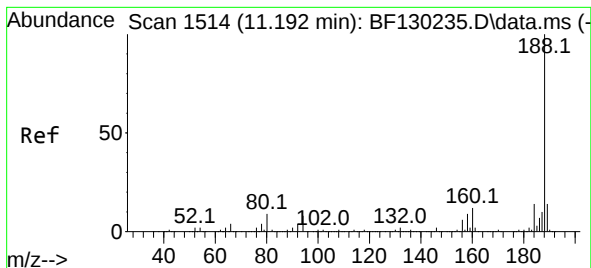

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 11.145 min Scan# 1

Delta R.T. -0.012 min

Lab File: BF130526.D

Acq: 04 Oct 2022 19:17

Instrument :

BNA_F

ClientSampleId :

265393-6





Tgt Ion:188 Resp: 235115

Ion Ratio Lower Upper

188 100

94 8.7 7.4 11.2

80 9.2 7.9 11.9

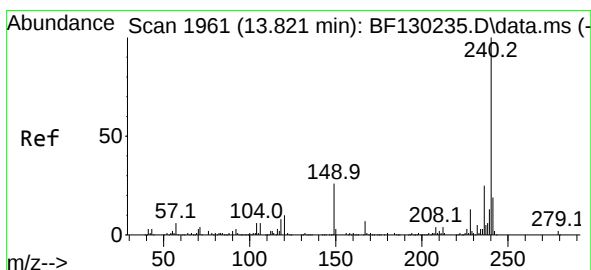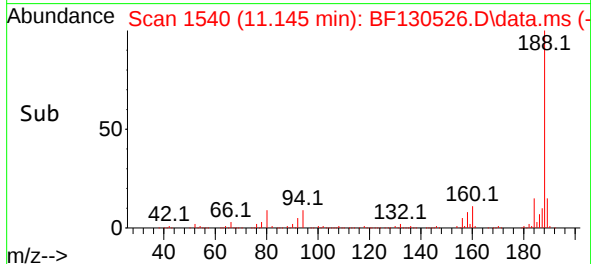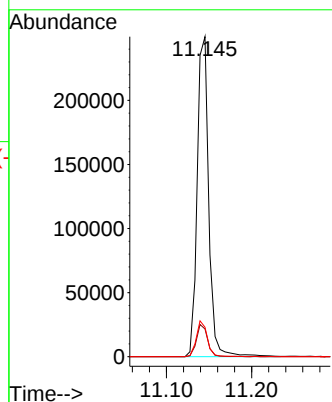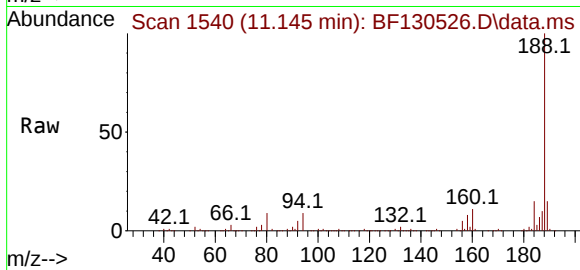

#76

Chrysene-d12

Concen: 20.000 ng

RT: 13.774 min Scan# 1987

Delta R.T. -0.018 min

Lab File: BF130526.D

Acq: 04 Oct 2022 19:17




Tgt Ion:240 Resp: 152406


Ion Ratio Lower Upper

240 100

120 9.9 8.7 13.1

236 25.5 20.9 31.3


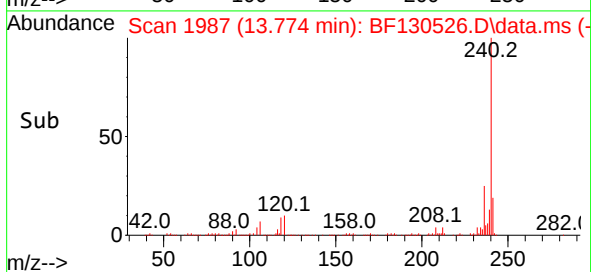
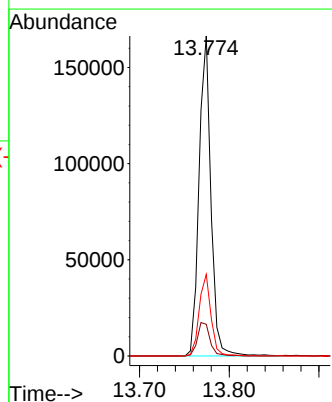
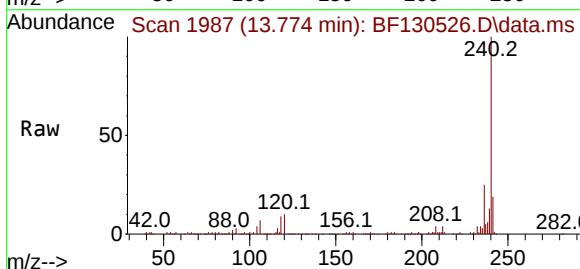


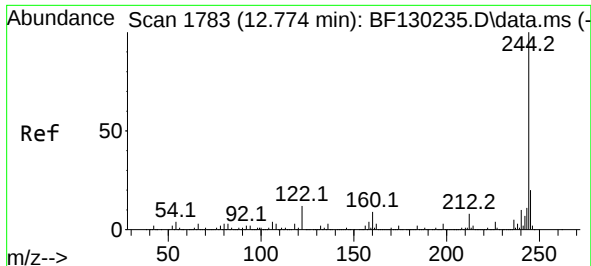

#79
 Terphenyl-d14
 Concen: 92.260 ng
 RT: 12.727 min Scan# 1809
 Delta R.T. -0.018 min
 Lab File: BF130526.D
 Acq: 04 Oct 2022 19:17

Instrument :
 BNA_F
 ClientSampleId :
 265393-6

Tgt Ion:244 Resp: 848838
 Ion Ratio Lower Upper
 244 100
 212 7.3 5.9 8.9
 122 12.7 8.5 12.7#

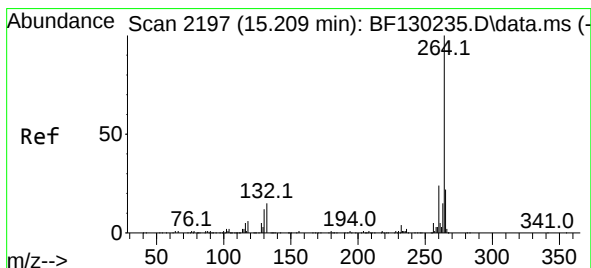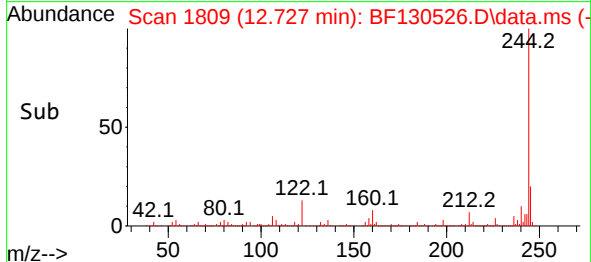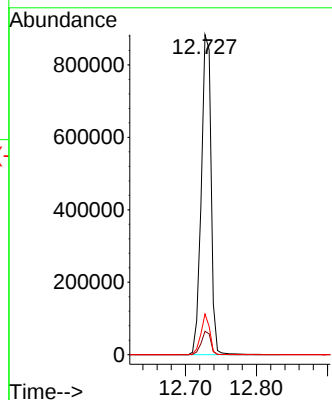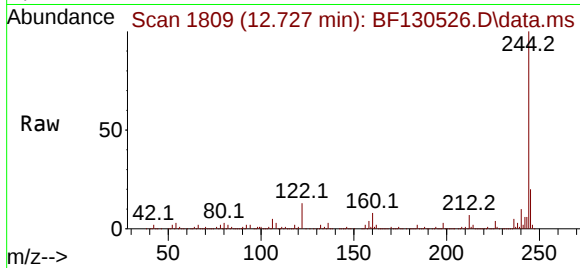

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 15.163 min Scan# 2223
 Delta R.T. -0.012 min
 Lab File: BF130526.D
 Acq: 04 Oct 2022 19:17

Tgt Ion:264 Resp: 182694
 Ion Ratio Lower Upper
 264 100
 260 23.2 19.3 28.9
 265 21.6 17.0 25.4

