


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100422\
 Data File : BF130511.D
 Acq On : 04 Oct 2022 10:58
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Oct 06 01:07:05 2022

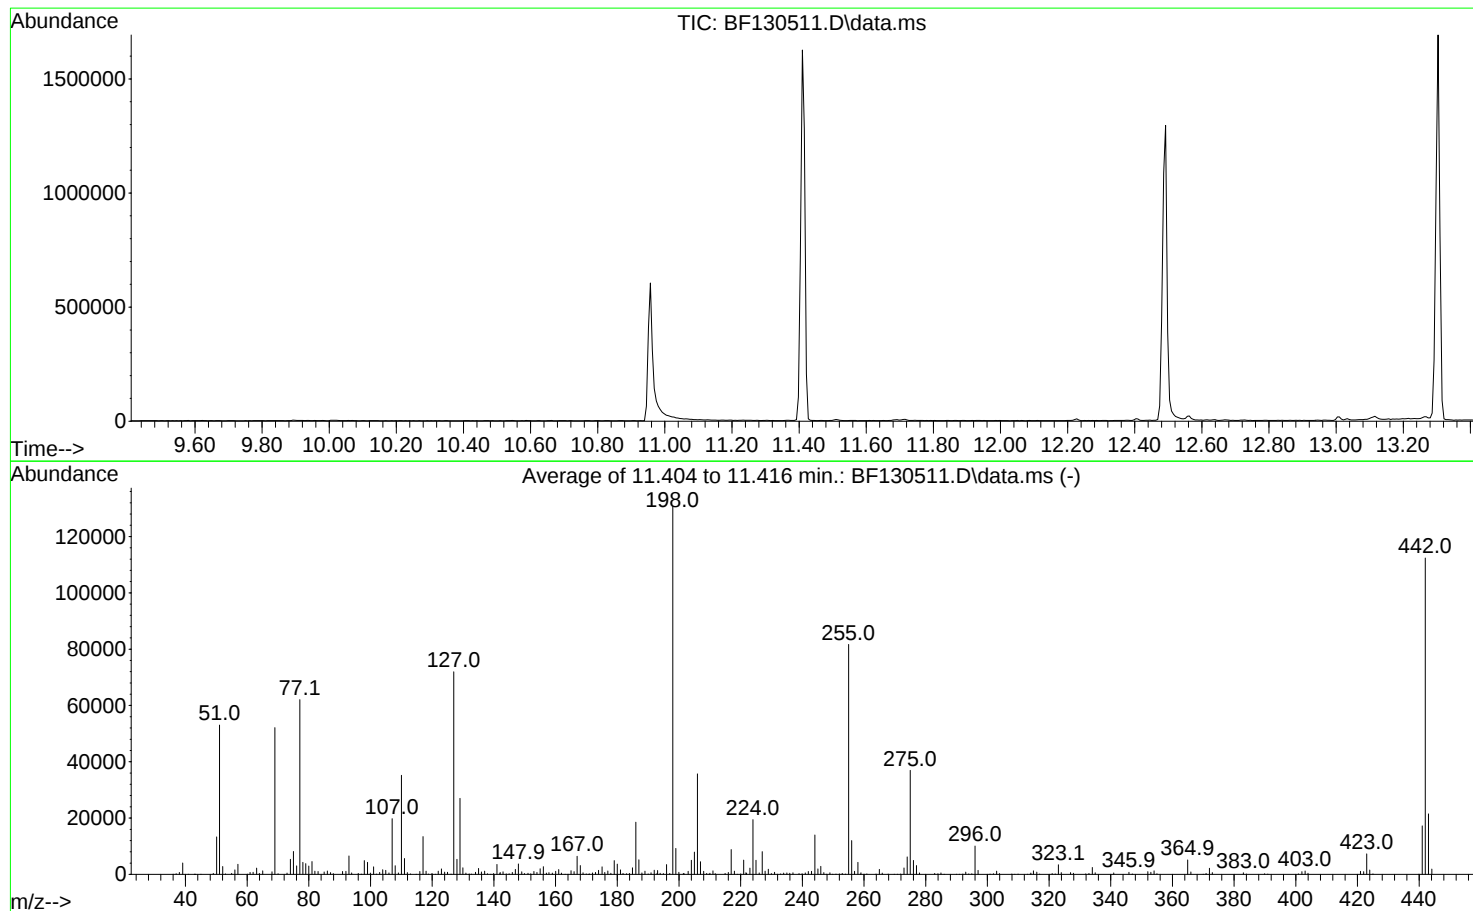




AutoFind: Scans 1584, 1585, 1586; Background Corrected with Scan 1579

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.6	53011	PASS
68	69	0.00	2	1.8	923	PASS
69	198	0.00	100	39.9	52104	PASS
70	69	0.00	2	0.5	256	PASS
127	198	10	80	55.1	71979	PASS
197	198	0.00	2	0.3	362	PASS
198	198	100	100	100.0	130677	PASS
199	198	5	9	7.1	9230	PASS
275	198	10	60	28.3	36941	PASS
365	198	1	100	3.9	5139	PASS
441	198	0.01	100	13.2	17222	PASS
442	442	50	100	100.0	112363	PASS
443	442	15	24	19.1	21464	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100422\
Data File : BF130511.D
Acq On : 04 Oct 2022 10:58
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 05 03:25:20 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 28 02:59:31 2022
Response via : Initial Calibration

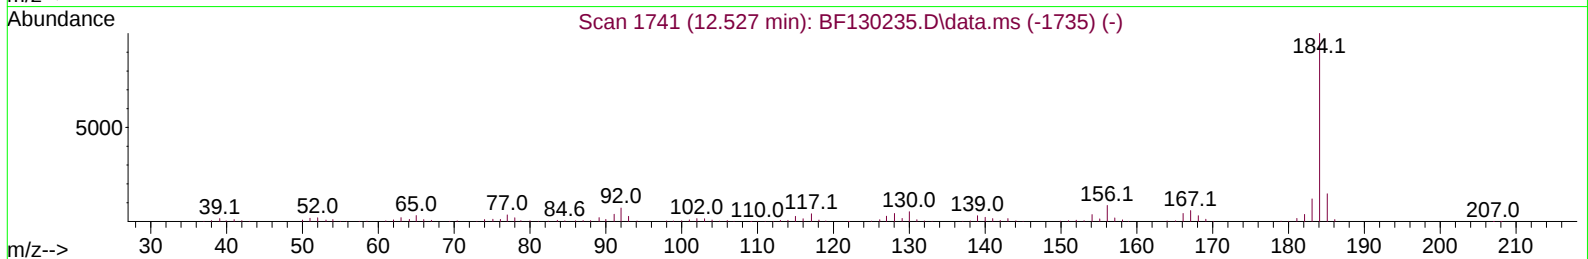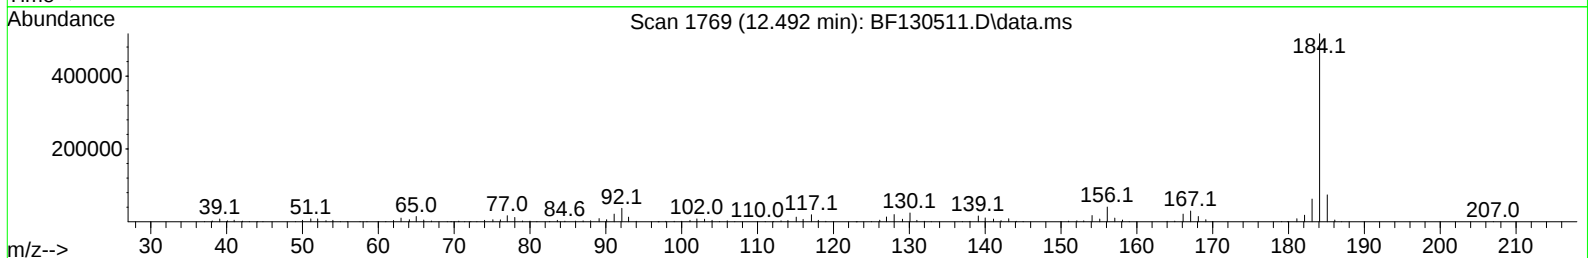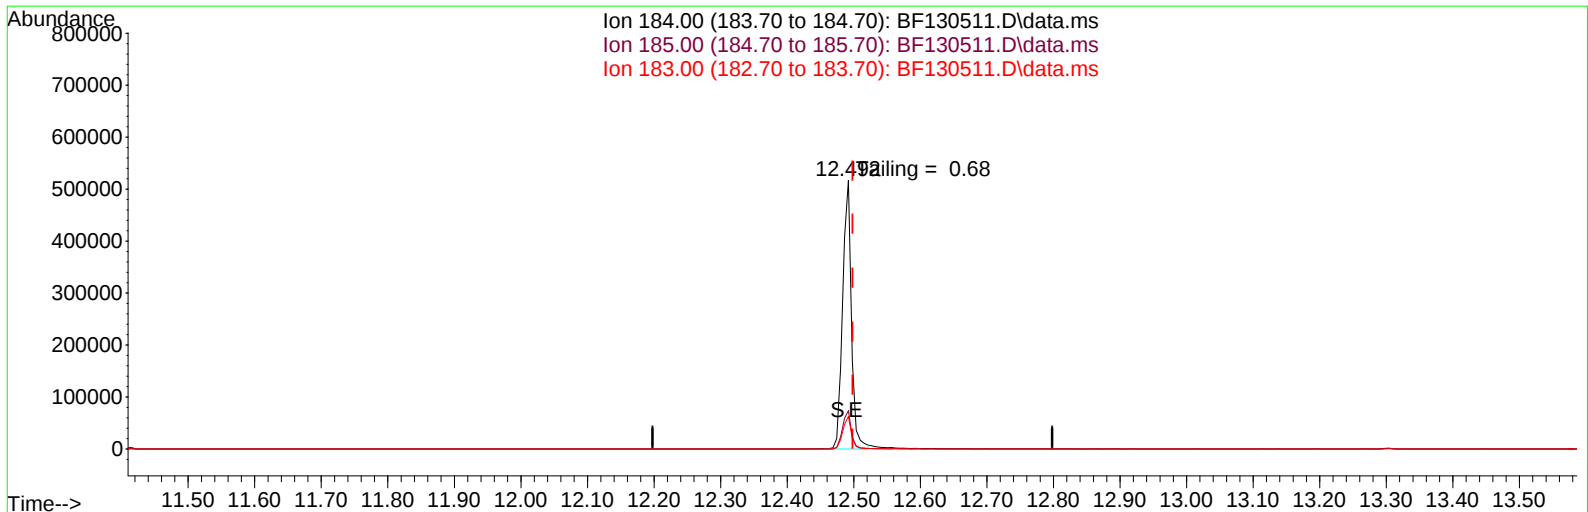

TIC: BF130511.D\data.ms

(77) Benzidine

12.492min (-0.006) 0.00 ng




response 483189

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.29
183.00	11.40	12.11
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100422\
Data File : BF130511.D
Acq On : 04 Oct 2022 10:58
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 05 03:25:20 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Sep 28 02:59:31 2022
Response via : Initial Calibration

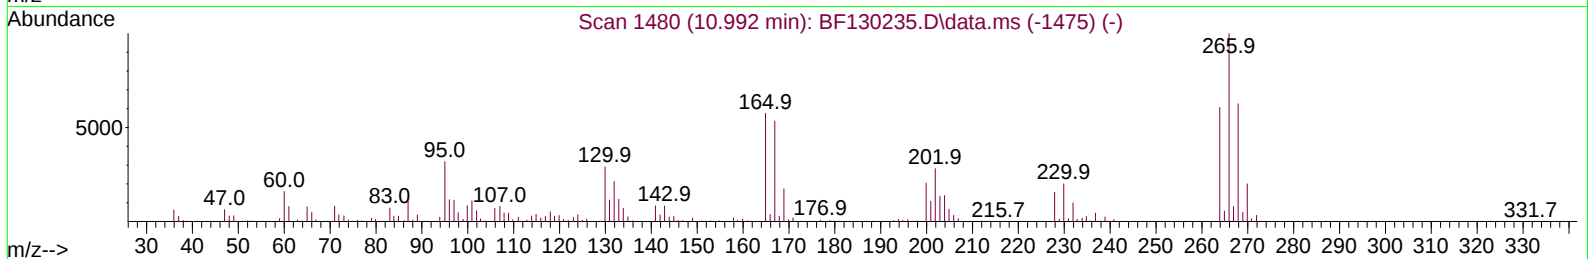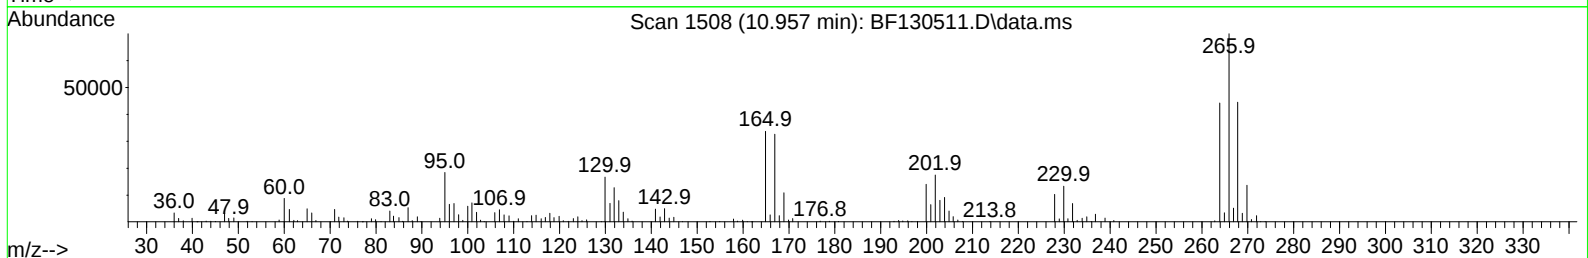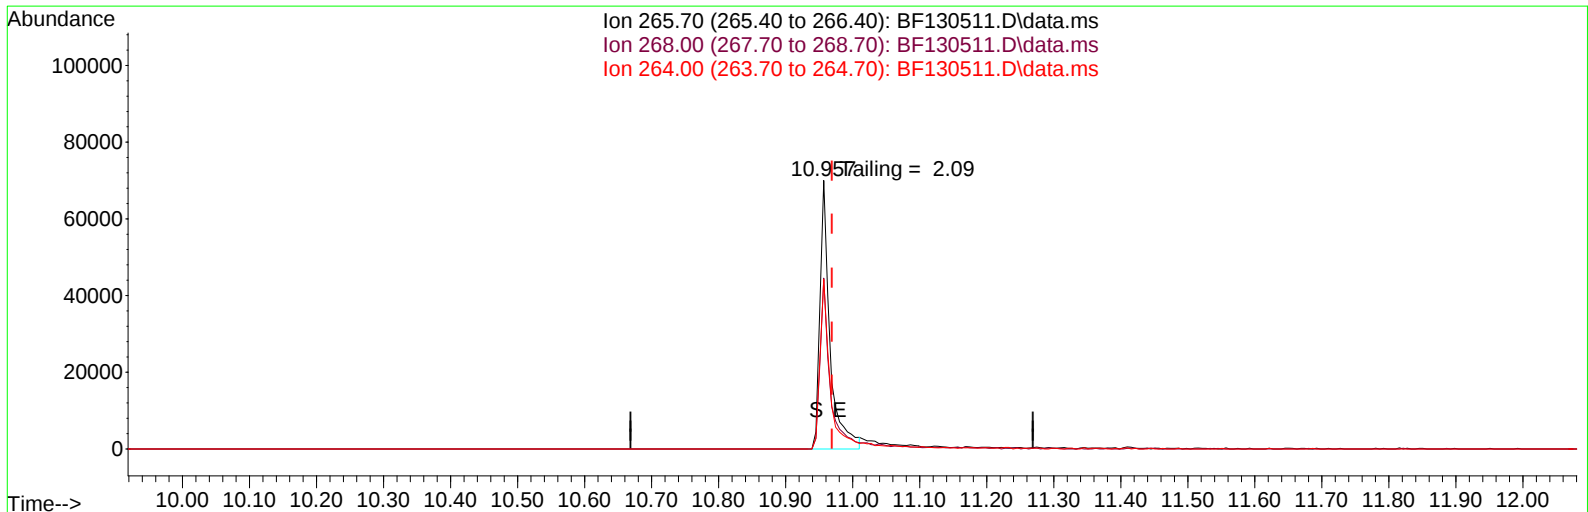

TIC: BF130511.D\data.ms

(70) Pentachlorophenol (C)

10.957min (-0.012) 21826.01 ng

response 79686

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	63.64
264.00	63.10	63.16
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/4/2022	BNA_F	<u>BF130511.D</u>
Compound Name	Response	Retention Time
DDT	256723	13.304
DDD	4141	13.01
DDE	592	12.668
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4733	261456	1.81

Instrument :
BNA_F
ClientSampleId :
DFTPP