
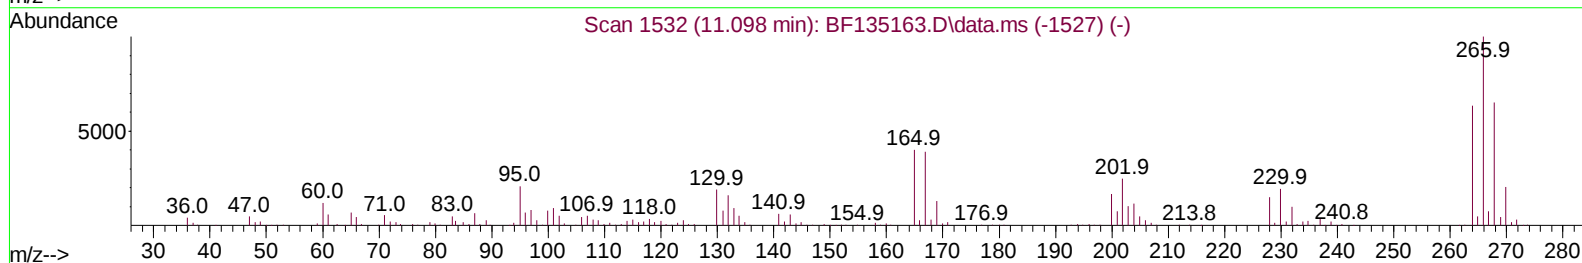
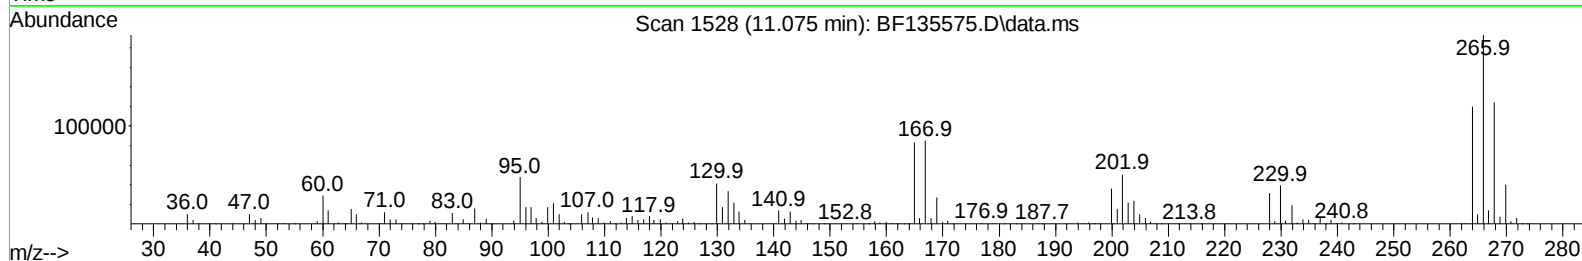


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100423\
Data File : BF135575.D
Acq On : 04 Oct 2023 17:57
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 05 08:23:05 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 04 17:06:20 2023
Response via : Initial Calibration

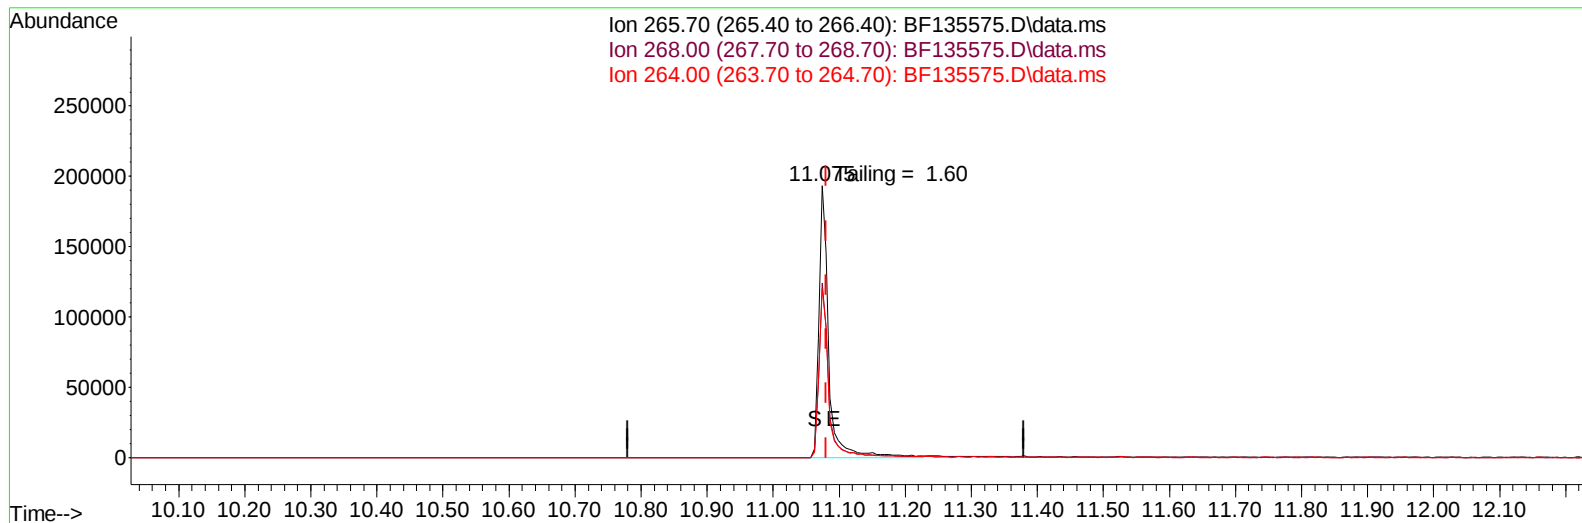

TIC: BF135575.D\data.ms

(70) Pentachlorophenol (C)




11.075min (-0.006) 258173.25 ng

response 198768

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.10	64.36
264.00	63.50	62.19
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100423\
Data File : BF135575.D
Acq On : 04 Oct 2023 17:57
Operator : CG\JU
Sample : DFTTP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 05 08:23:05 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 04 17:06:20 2023
Response via : Initial Calibration

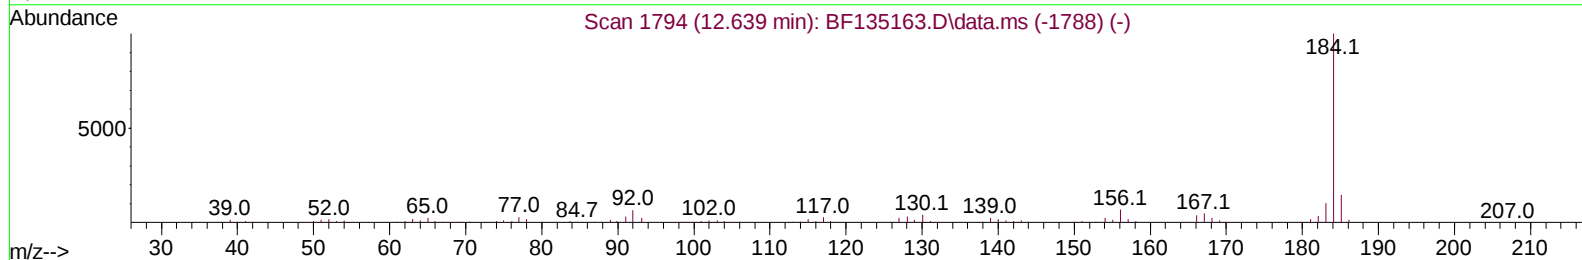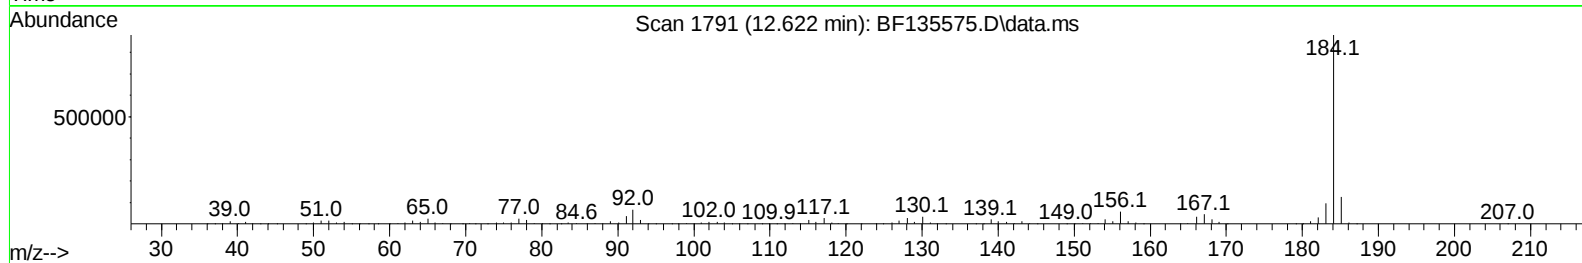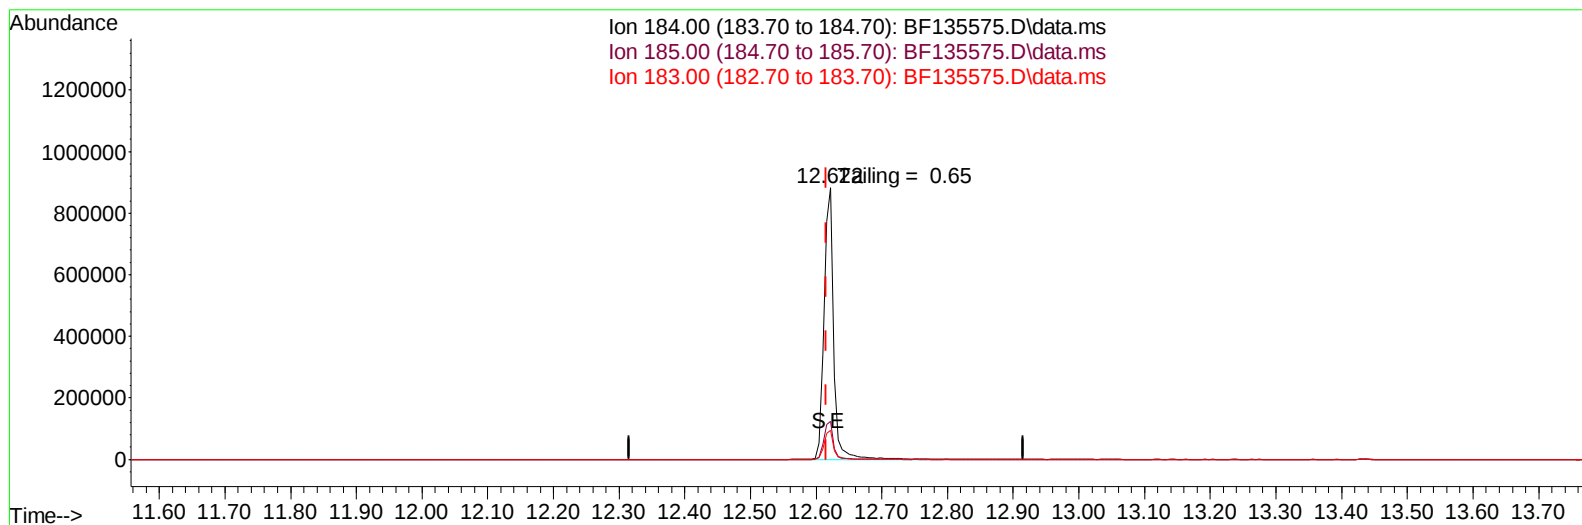

TIC: BF135575.D\data.ms

(77) Benzidine

12.622min (+ 0.006) 315311.14 ng

response 897902

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.15
183.00	10.30	10.86
0.00	0.00	0.00