

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100423\
Data File : BF135564.D
Acq On : 04 Oct 2023 11:13
Operator : CG\JU
Sample : PB156015BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB156015BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF135564.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.381	556	560	581	rBV	3962226	4236109	99.00%	15.122%
2	6.387	727	731	753	rBV	3552388	4239653	99.08%	15.135%
3	6.740	787	791	802	rBV	931324	856254	20.01%	3.057%
4	7.304	882	887	890	rBV	2771564	2755940	64.41%	9.838%
5	8.016	1004	1008	1024	rBV	1199362	1101085	25.73%	3.931%
6	9.098	1186	1192	1195	rBV	4087102	4278892	100.00%	15.275%
7	9.769	1302	1306	1317	rBV	1233884	1192541	27.87%	4.257%
8	10.569	1438	1442	1445	rBV	2651967	2543510	59.44%	9.080%
9	11.263	1557	1560	1568	rBV	1299756	1212134	28.33%	4.327%
10	12.863	1827	1832	1836	rBV	3885369	4109269	96.04%	14.669%
11	13.921	2008	2012	2021	rBV	949172	880599	20.58%	3.144%
12	15.386	2255	2261	2272	rVB	466831	607145	14.19%	2.167%




Sum of corrected areas: 28013131

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100423\
Data File : BF135564.D
Acq On : 04 Oct 2023 11:13
Operator : CG\JU
Sample : PB156015BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB156015BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

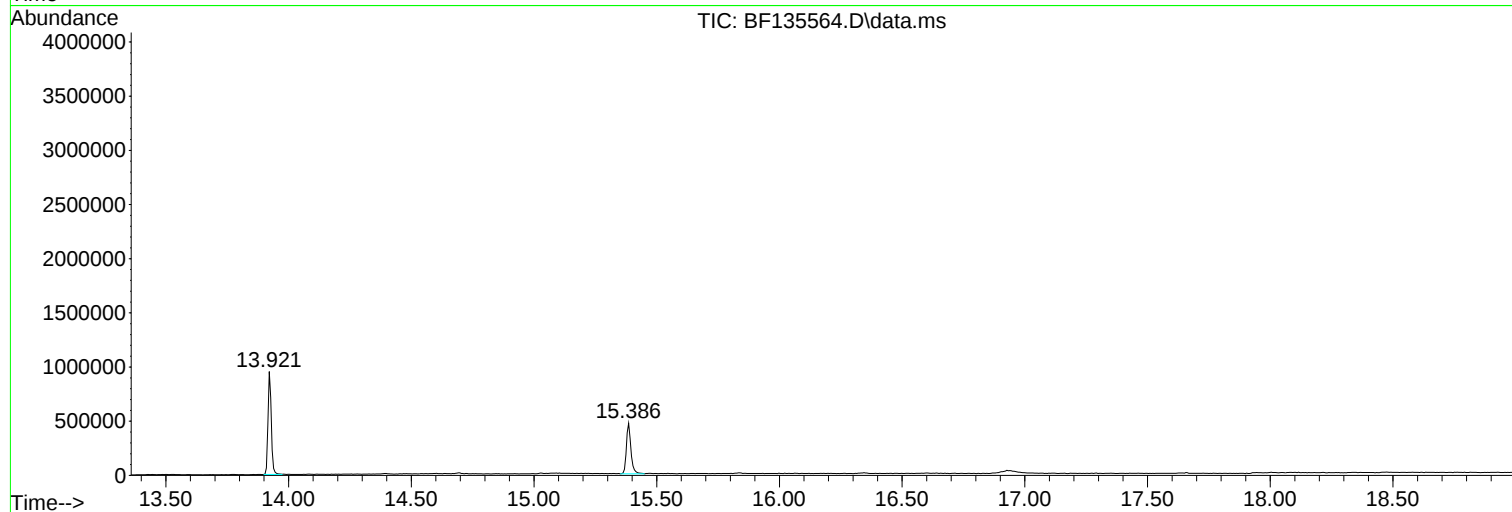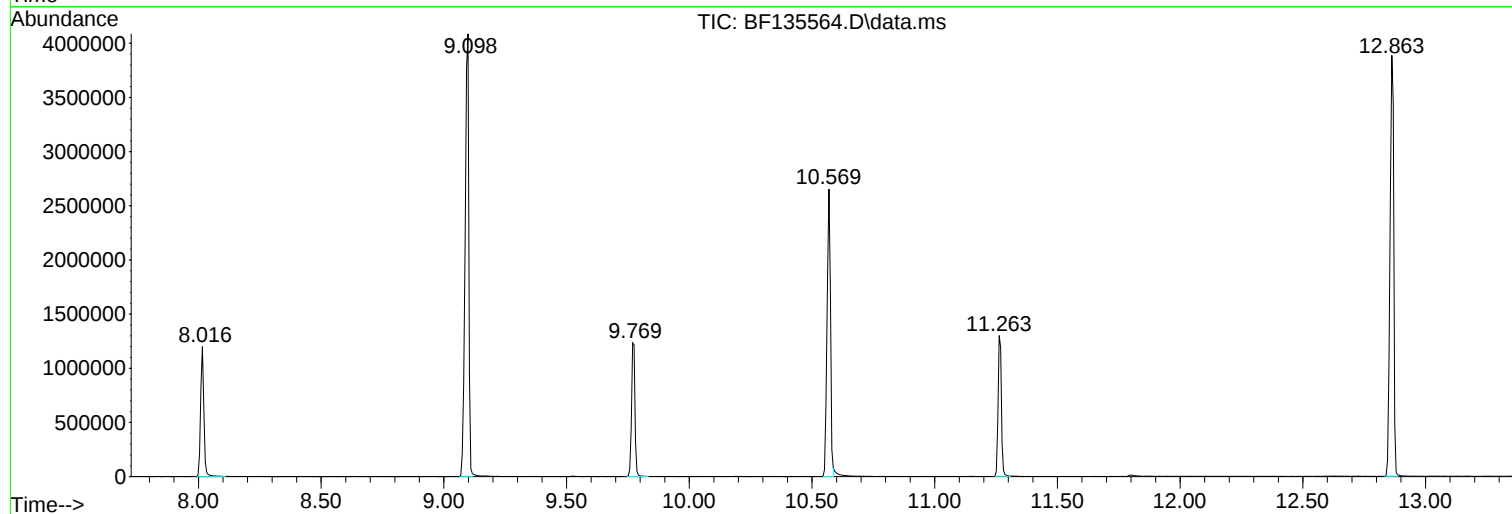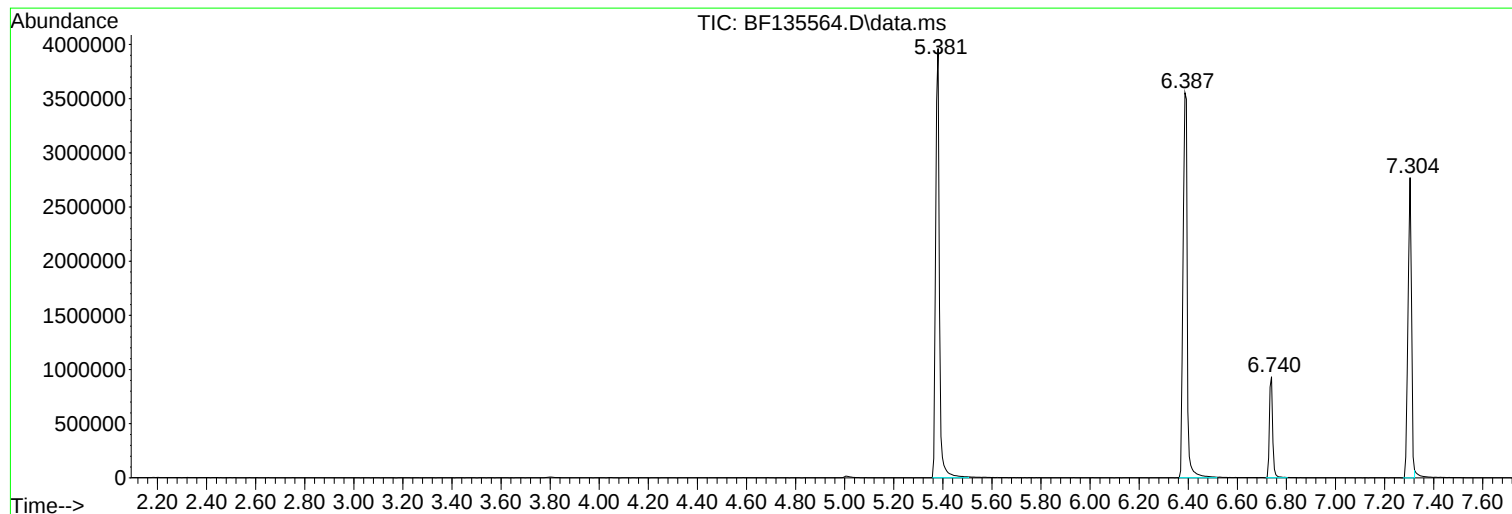

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100423\
Data File : BF135564.D
Acq On : 04 Oct 2023 11:13
Operator : CG\JU
Sample : PB156015BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB156015BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100423\
Data File : BF135564.D
Acq On : 04 Oct 2023 11:13
Operator : CG\JU
Sample : PB156015BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB156015BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------