

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100423\
Data File : BF135577.D
Acq On : 04 Oct 2023 19:03
Operator : CG\JU
Sample : PB156015BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB156015BL

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF135577.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.381	556	560	579	rBV	4200684	4383697	93.13%	14.465%
2	6.392	727	732	760	rBV	3642878	4398868	93.46%	14.515%
3	6.734	787	790	802	rBV	917581	865928	18.40%	2.857%
4	7.304	882	887	890	rBV	2682782	2854735	60.65%	9.420%
5	8.016	1004	1008	1023	rBV	1228937	1160740	24.66%	3.830%
6	9.098	1186	1192	1195	rBV	4271832	4706931	100.00%	15.531%
7	9.769	1301	1306	1310	rBV	1396863	1296856	27.55%	4.279%
8	10.569	1438	1442	1460	rBV	2853158	2958516	62.85%	9.762%
9	11.263	1557	1560	1569	rBV	1581354	1386082	29.45%	4.574%
10	12.863	1827	1832	1835	rBV	4181377	4576084	97.22%	15.100%
11	13.921	2008	2012	2019	rBV	1022507	933909	19.84%	3.082%
12	15.386	2256	2261	2272	rBV	599602	783846	16.65%	2.586%




Sum of corrected areas: 30306192

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100423\
Data File : BF135577.D
Acq On : 04 Oct 2023 19:03
Operator : CG\JU
Sample : PB156015BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB156015BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

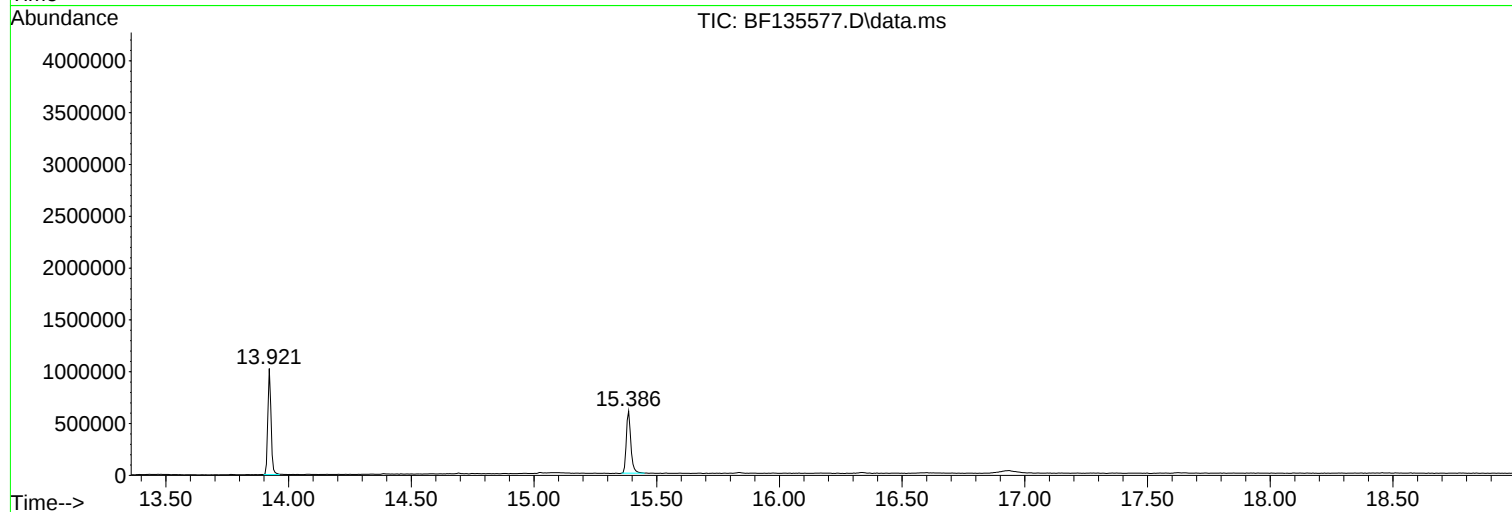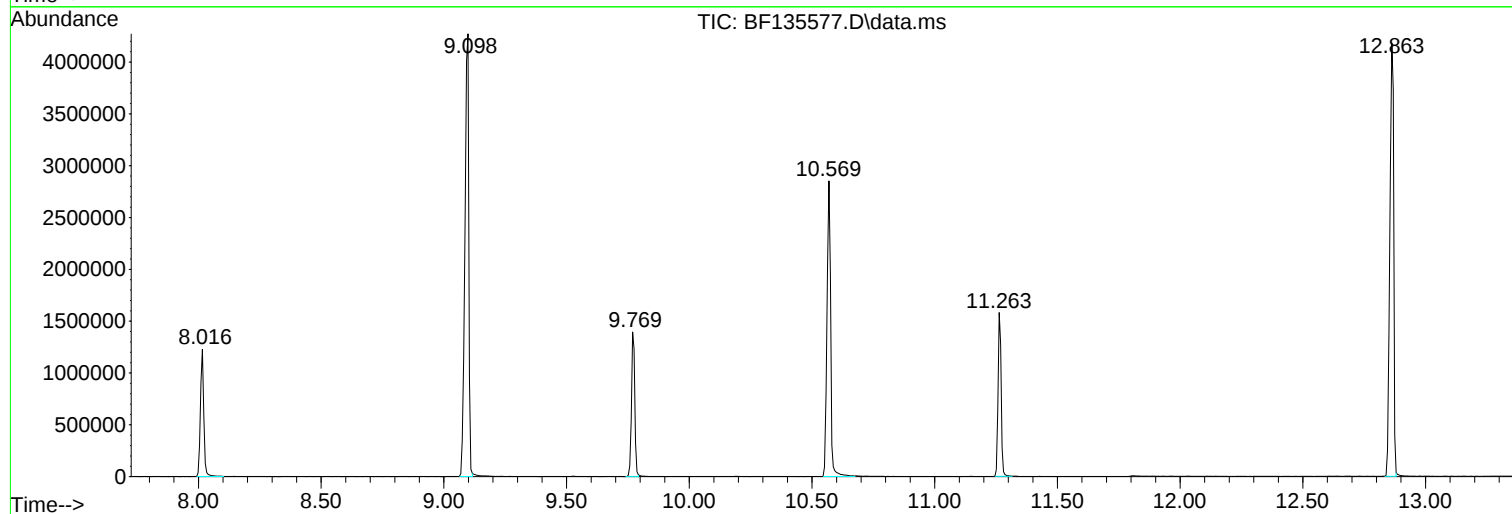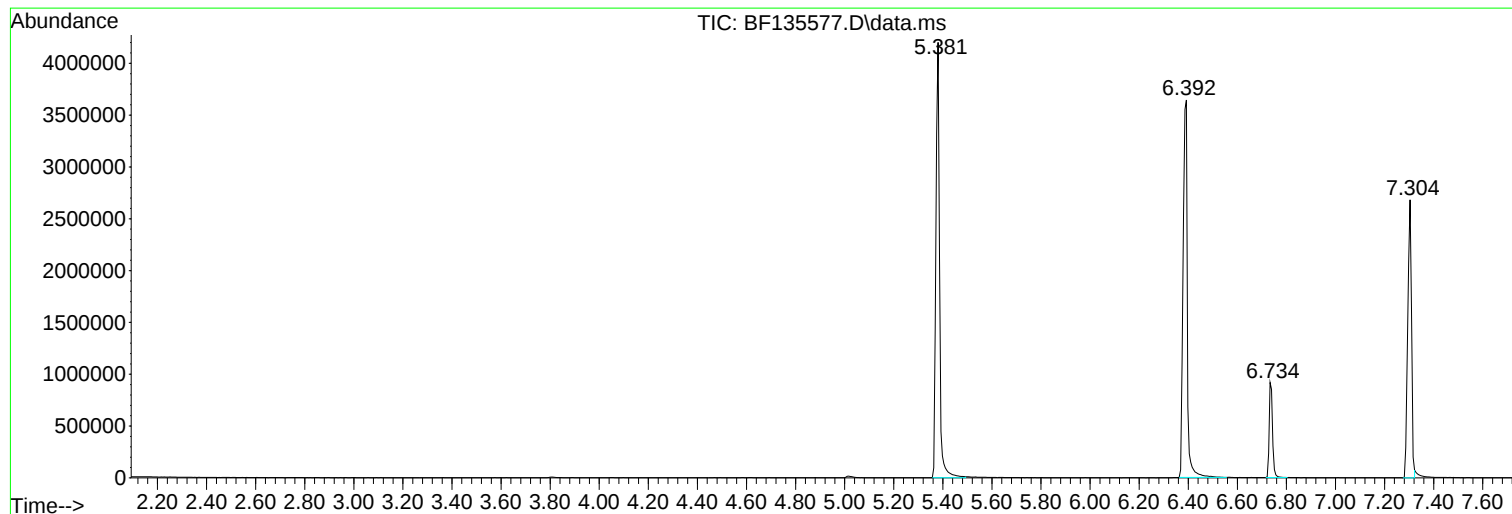

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100423\
Data File : BF135577.D
Acq On : 04 Oct 2023 19:03
Operator : CG\JU
Sample : PB156015BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB156015BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100423\
Data File : BF135577.D
Acq On : 04 Oct 2023 19:03
Operator : CG\JU
Sample : PB156015BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB156015BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------