


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100423\
Data File : BF135562.D
Acq On : 04 Oct 2023 10:11
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Oct 04 17:06:20 2023

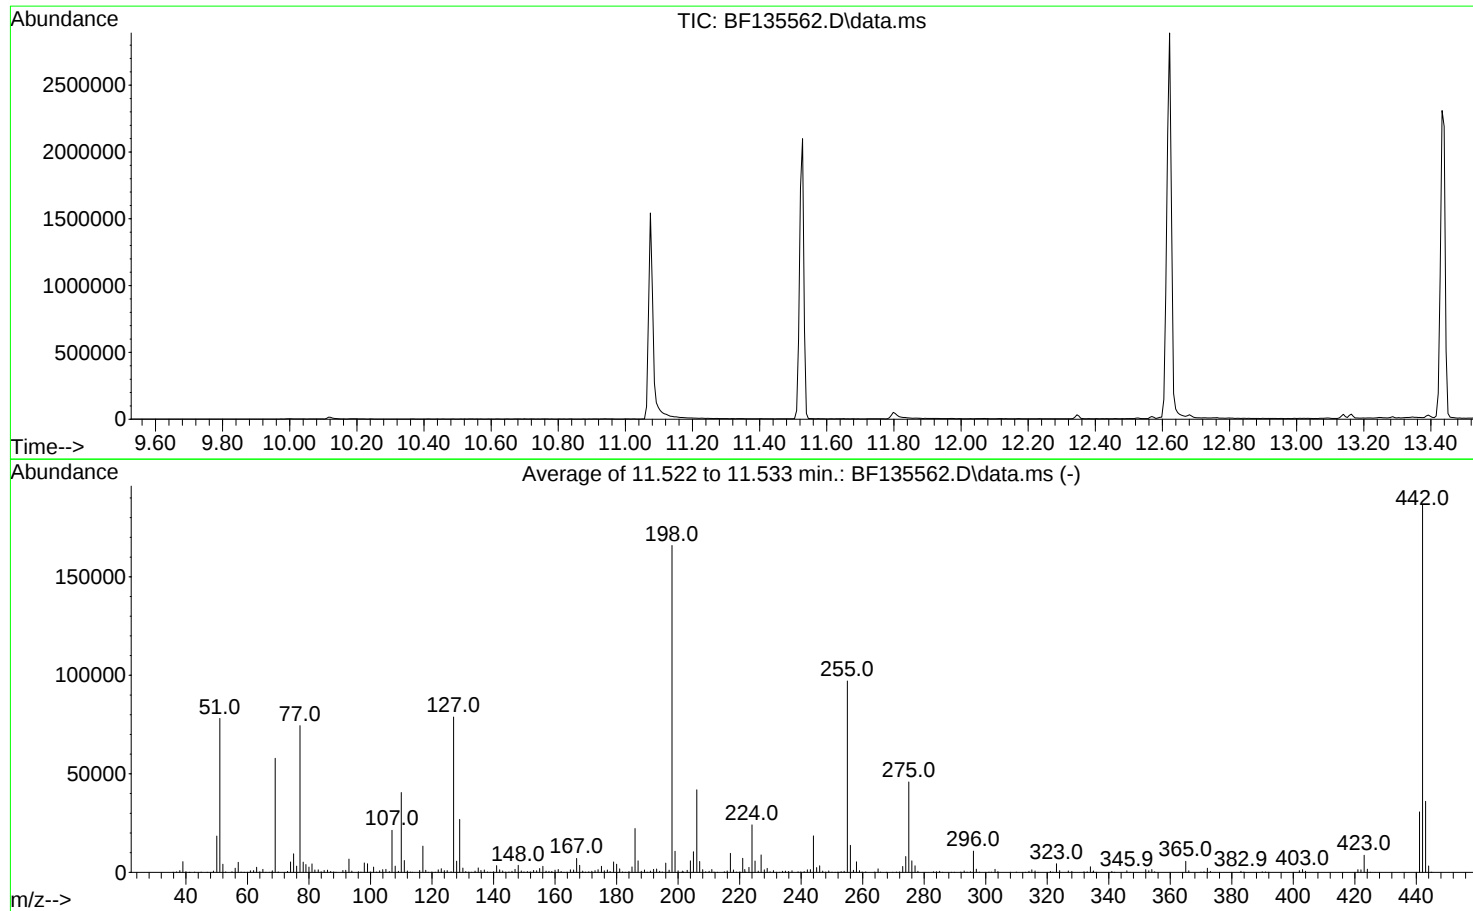




AutoFind: Scans 1604, 1605, 1606; Background Corrected with Scan 1598

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	47.1	78101	PASS
68	69	0.00	2	1.5	852	PASS
69	198	0.00	100	34.9	57918	PASS
70	69	0.00	2	0.2	133	PASS
127	198	10	80	47.6	78891	PASS
197	198	0.00	2	0.7	1109	PASS
198	198	100	100	100.0	165904	PASS
199	198	5	9	6.5	10735	PASS
275	198	10	60	27.7	45917	PASS
365	198	1	100	3.4	5634	PASS
441	198	0.01	100	18.5	30717	PASS
442	442	50	100	100.0	186688	PASS
443	442	15	24	19.3	36083	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100423\
Data File : BF135562.D
Acq On : 04 Oct 2023 10:11
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 05 08:17:56 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 04 17:06:20 2023
Response via : Initial Calibration

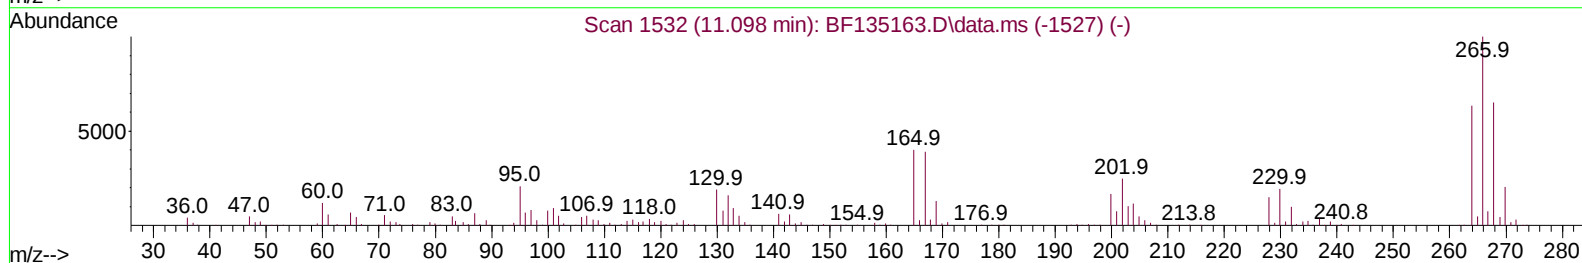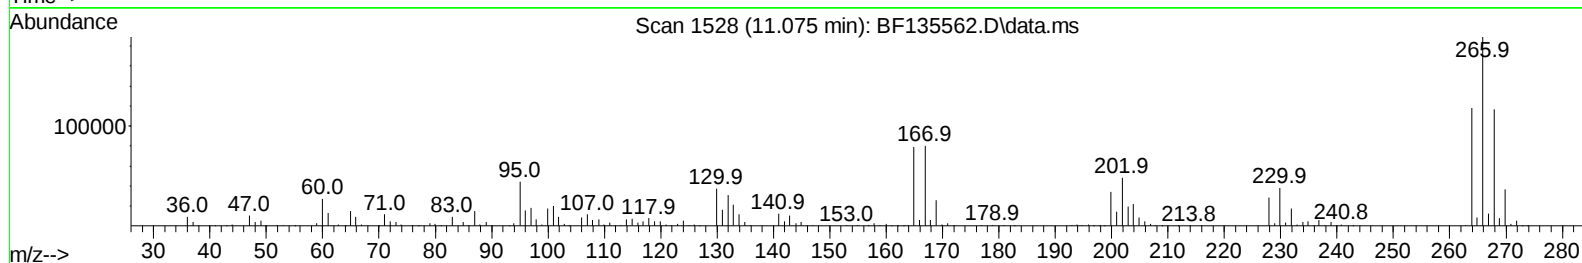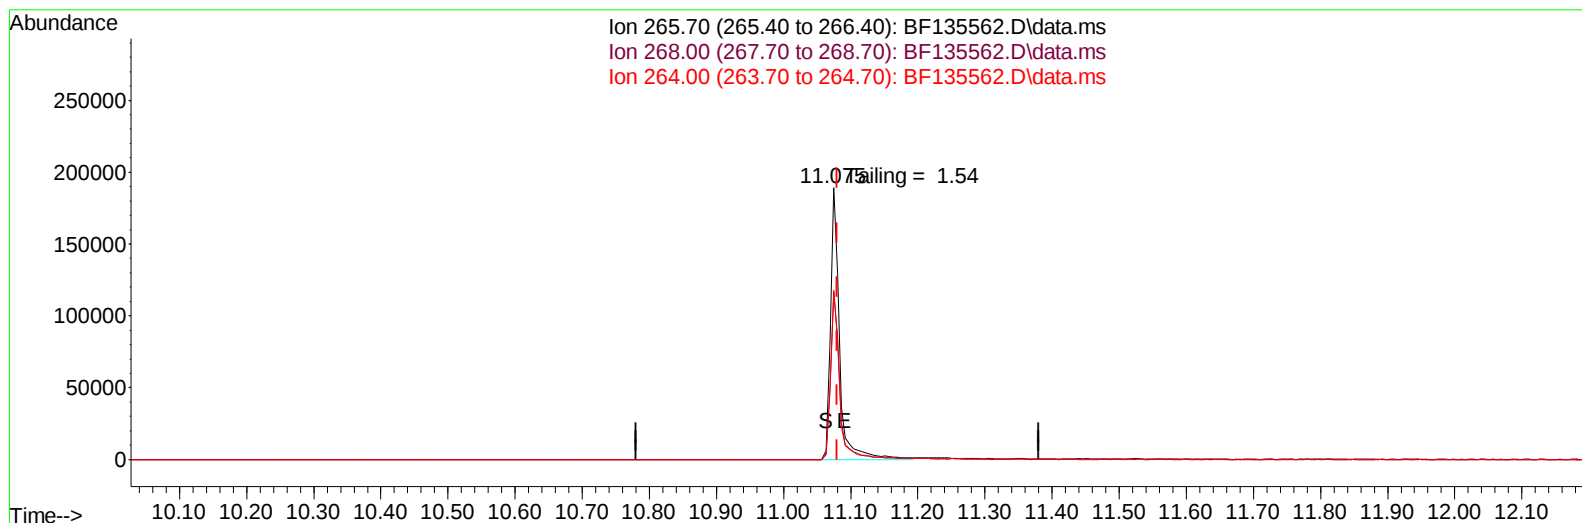

TIC: BF135562.D\data.ms

(70) Pentachlorophenol (C)

11.075min (-0.006) 48153.09 ng




response 180987

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.10	61.68
264.00	63.50	62.29
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100423\
Data File : BF135562.D
Acq On : 04 Oct 2023 10:11
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 05 08:17:56 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 04 17:06:20 2023
Response via : Initial Calibration

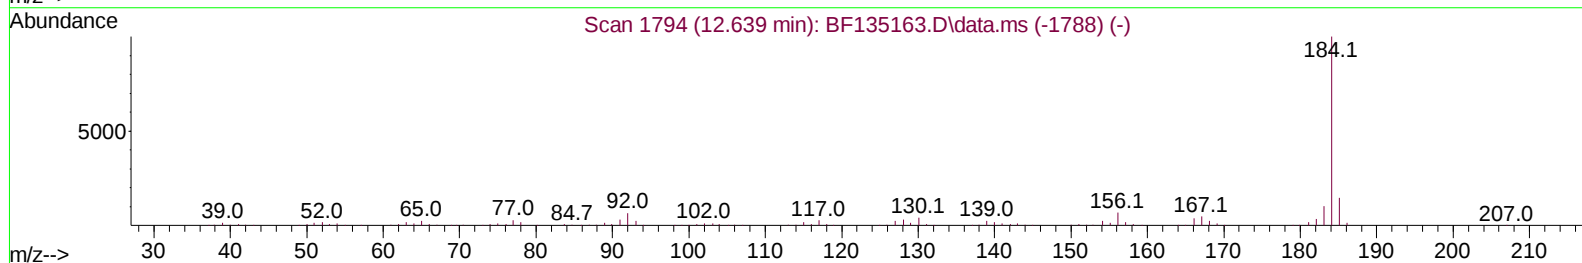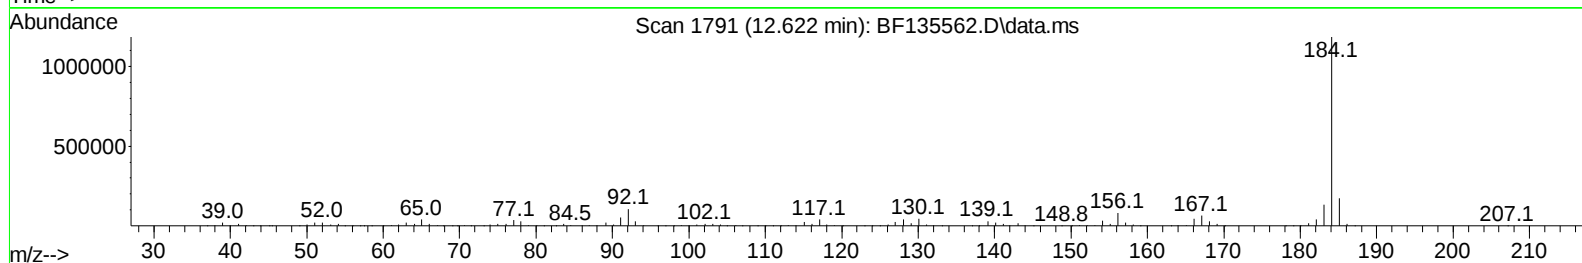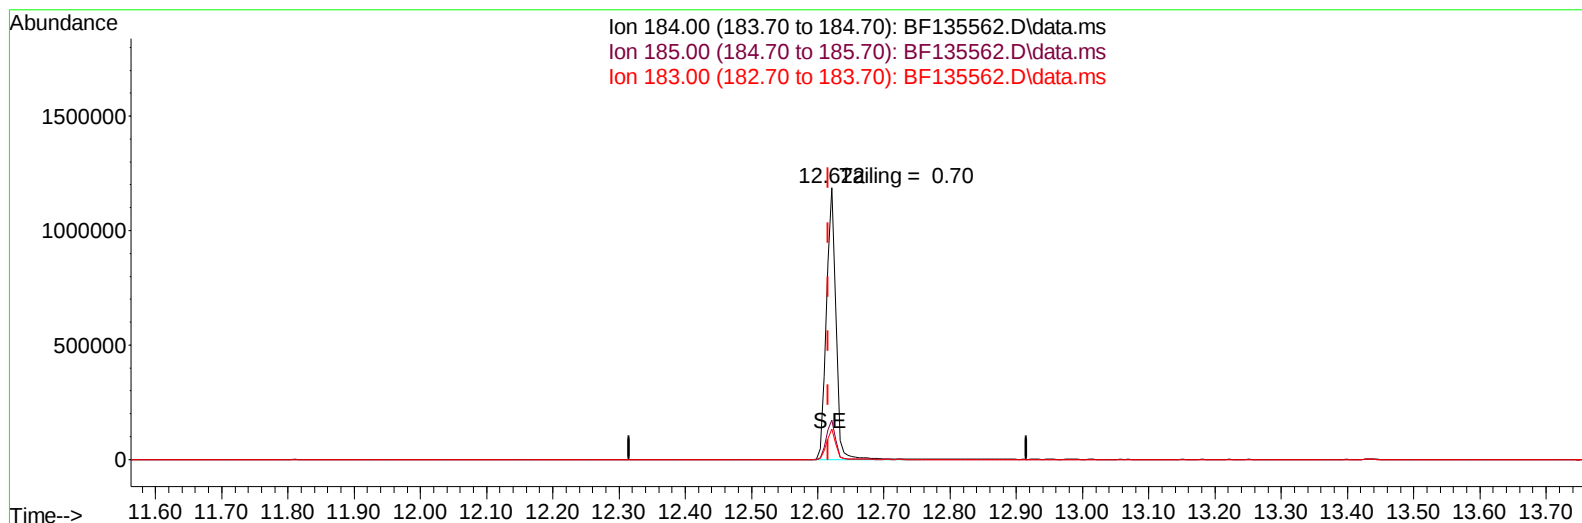

TIC: BF135562.D\data.ms

(77) Benzidine

12.622min (+ 0.006) 0.00 ng

response 1178051

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.44
183.00	10.30	11.23
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/4/2023	BNA_F	<u>BF135562.D</u>
Compound Name	Response	Retention Time
DDT	451659	13.439
DDD	10289	13.139
DDE	495	12.804
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
10784	462443	2.33

Instrument :
BNA_F
ClientSampleId :
DFTPP