


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100423\
Data File : BF135575.D
Acq On : 04 Oct 2023 17:57
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Oct 04 17:06:20 2023

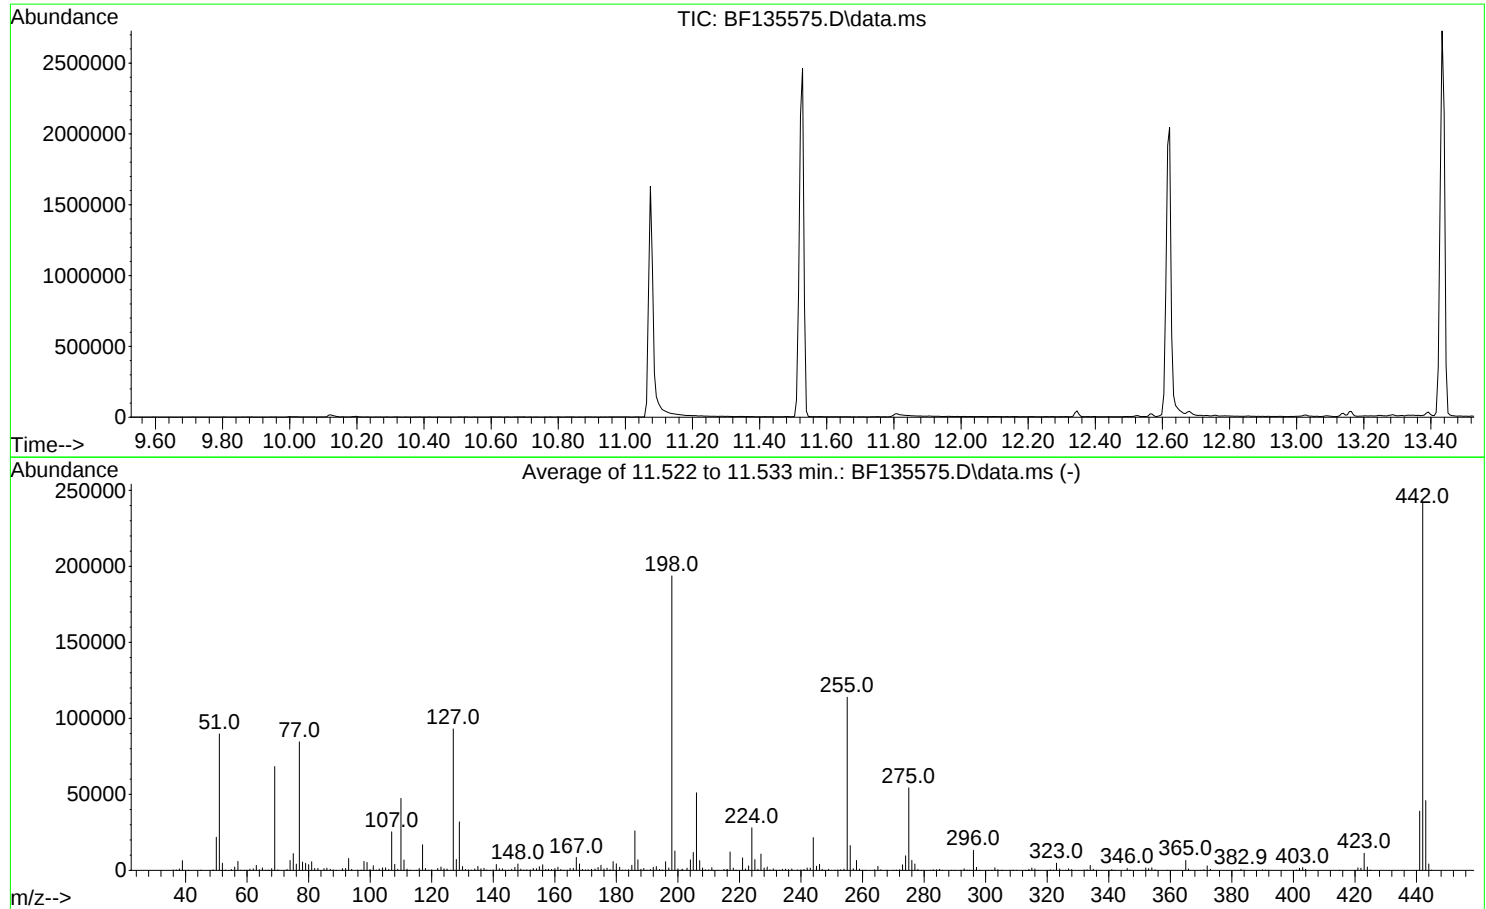




AutoFind: Scans 1604, 1605, 1606; Background Corrected with Scan 1598

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.4	89821	PASS
68	69	0.00	2	1.7	1172	PASS
69	198	0.00	100	35.3	68336	PASS
70	69	0.00	2	0.4	305	PASS
127	198	10	80	48.0	93011	PASS
197	198	0.00	2	0.8	1587	PASS
198	198	100	100	100.0	193709	PASS
199	198	5	9	6.6	12732	PASS
275	198	10	60	28.0	54333	PASS
365	198	1	100	3.4	6542	PASS
441	198	0.01	100	20.1	38928	PASS
442	442	50	100	100.0	241984	PASS
443	442	15	24	18.9	45853	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100423\
Data File : BF135575.D
Acq On : 04 Oct 2023 17:57
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 05 08:23:05 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 04 17:06:20 2023
Response via : Initial Calibration

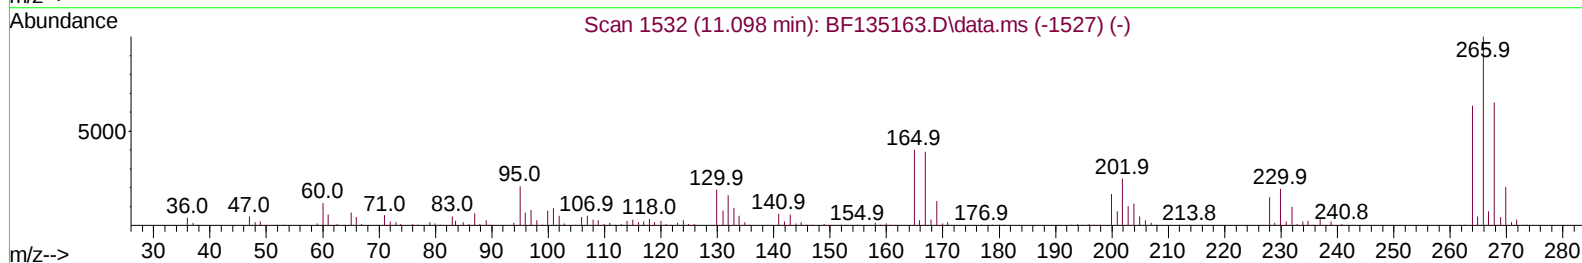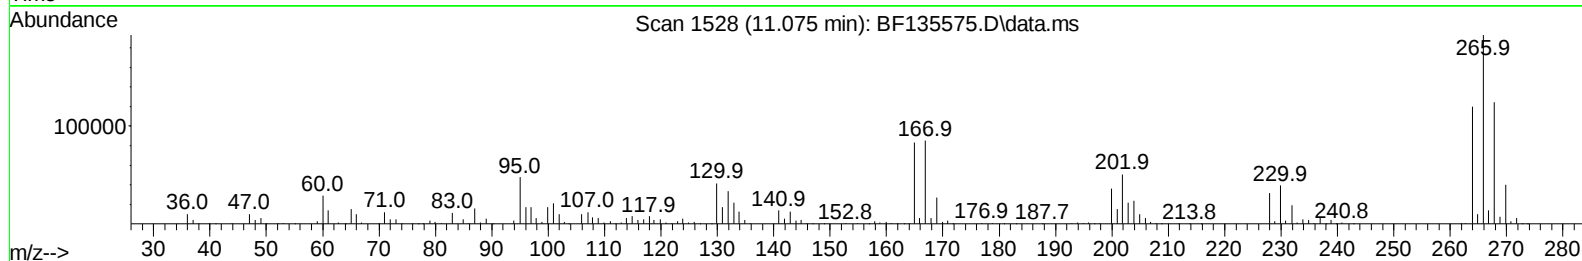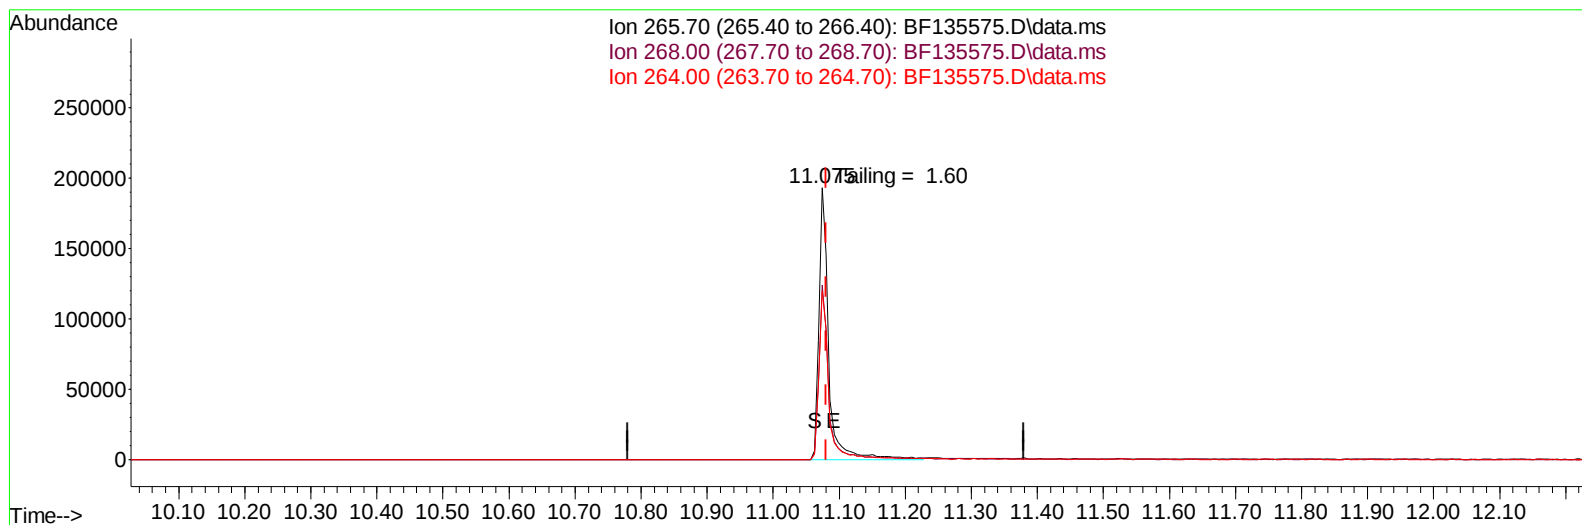

TIC: BF135575.D\data.ms

(70) Pentachlorophenol (C)

11.075min (-0.006) 258173.25 ng




response 198768

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.10	64.36
264.00	63.50	62.19
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100423\
Data File : BF135575.D
Acq On : 04 Oct 2023 17:57
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 05 08:23:05 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 04 17:06:20 2023
Response via : Initial Calibration

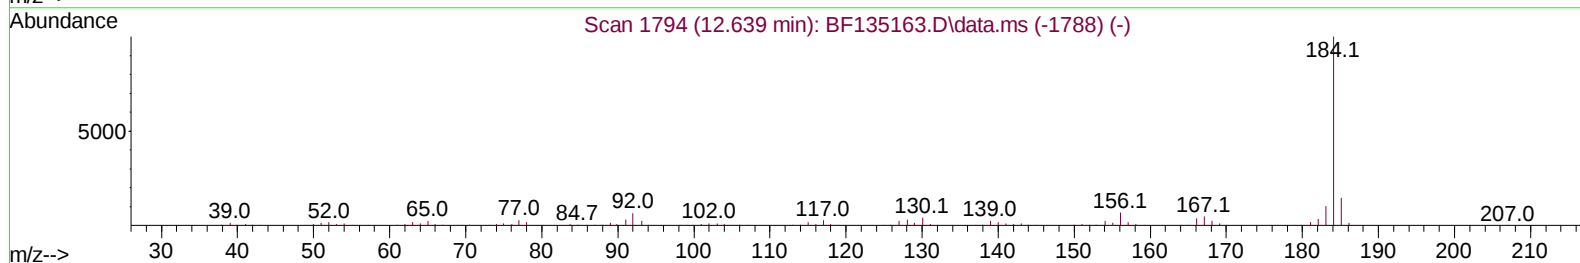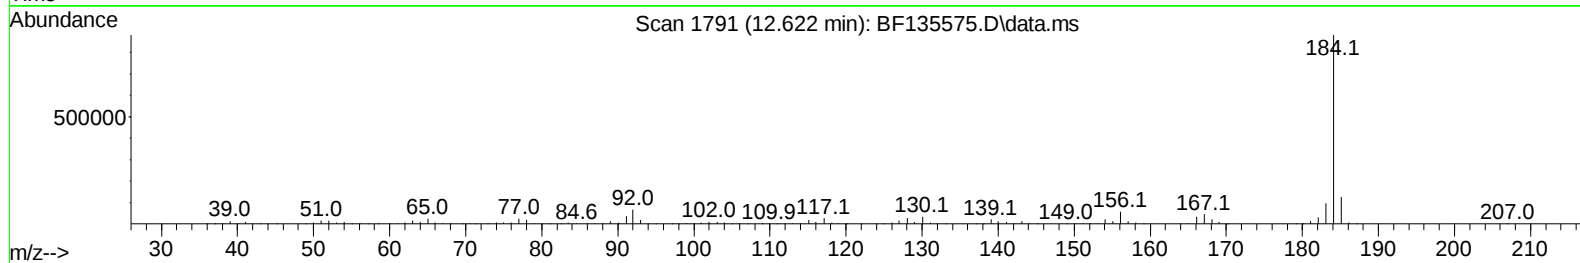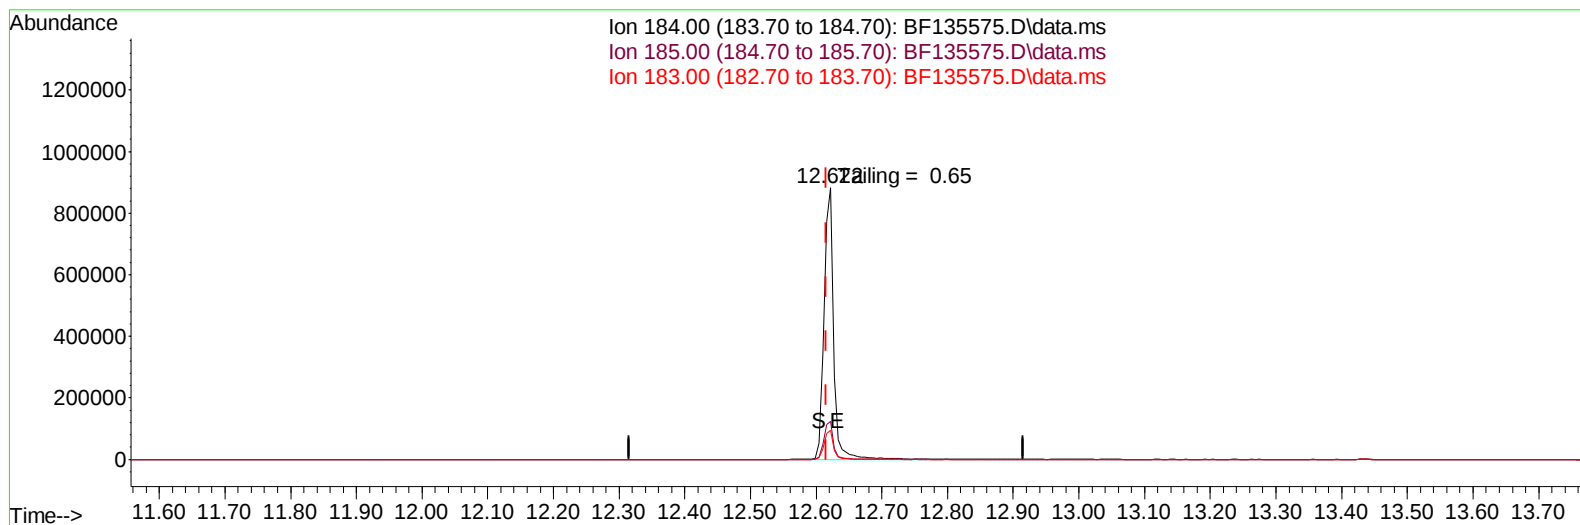

TIC: BF135575.D\data.ms

(77) Benzidine

12.622min (+ 0.006) 315311.14 ng

response 897902

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.15
183.00	10.30	10.86
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/4/2023	BNA_F	<u>BF135575.D</u>
Compound Name	Response	Retention Time
DDT	510679	13.433
DDD	11192	13.163
DDE	270	12.792
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
11462	522141	2.20

Instrument :
BNA_F
ClientSampleId :
DFTPP