

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100522\
 Data File : BF130529.D
 Acq On : 05 Oct 2022 13:21
 Operator : CG\JU
 Sample : PB148087BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB148087BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF130529.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.840	464	468	485	rBV	88220	146190	3.34%	0.559%
2	5.245	532	537	540	rBV	3676217	3806298	86.90%	14.547%
3	6.281	707	713	716	rBV	3088182	3306027	75.48%	12.635%
4	6.628	769	772	776	rBV	799859	703034	16.05%	2.687%
5	7.204	864	870	872	rBV	1979989	2234753	51.02%	8.541%
6	7.916	986	991	994	rBV	922661	936167	21.37%	3.578%
7	8.992	1168	1174	1177	rBV	4476688	4230161	96.57%	16.167%
8	9.663	1282	1288	1296	rBV	1282862	1064485	24.30%	4.068%
9	10.457	1417	1423	1426	rBV	2896339	2631137	60.07%	10.056%
10	11.145	1536	1540	1548	rBV	1238829	1033626	23.60%	3.950%
11	12.733	1803	1810	1813	rBV	4456517	4380223	100.00%	16.740%
12	13.774	1983	1987	1997	rBV	849832	785418	17.93%	3.002%
13	15.162	2218	2223	2227	rBV	536161	621595	14.19%	2.376%
14	15.192	2227	2228	2237	rVB	54577	64020	1.46%	0.245%
15	15.586	2289	2295	2300	rBV	39486	59647	1.36%	0.228%
16	16.033	2365	2371	2377	rBV	34257	59755	1.36%	0.228%
17	16.551	2455	2459	2467	rVB4	24135	45934	1.05%	0.176%
18	17.168	2558	2564	2575	rBV2	23219	57491	1.31%	0.220%




Sum of corrected areas: 26165961

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100522\
Data File : BF130529.D
Acq On : 05 Oct 2022 13:21
Operator : CG\JU
Sample : PB148087BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB148087BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

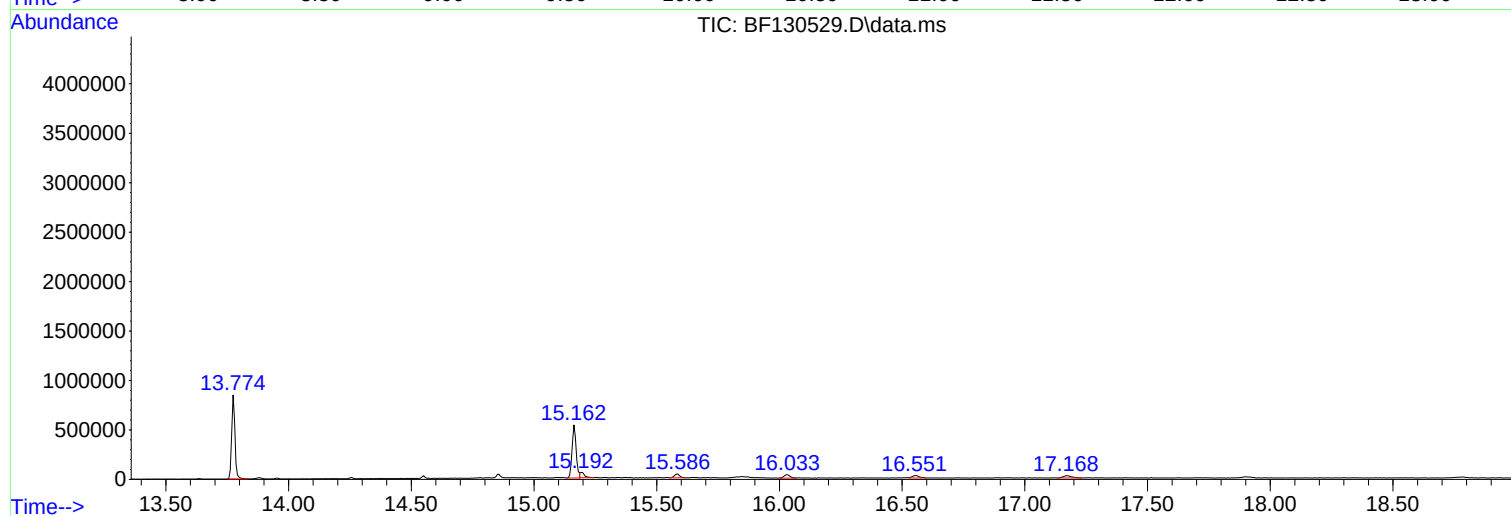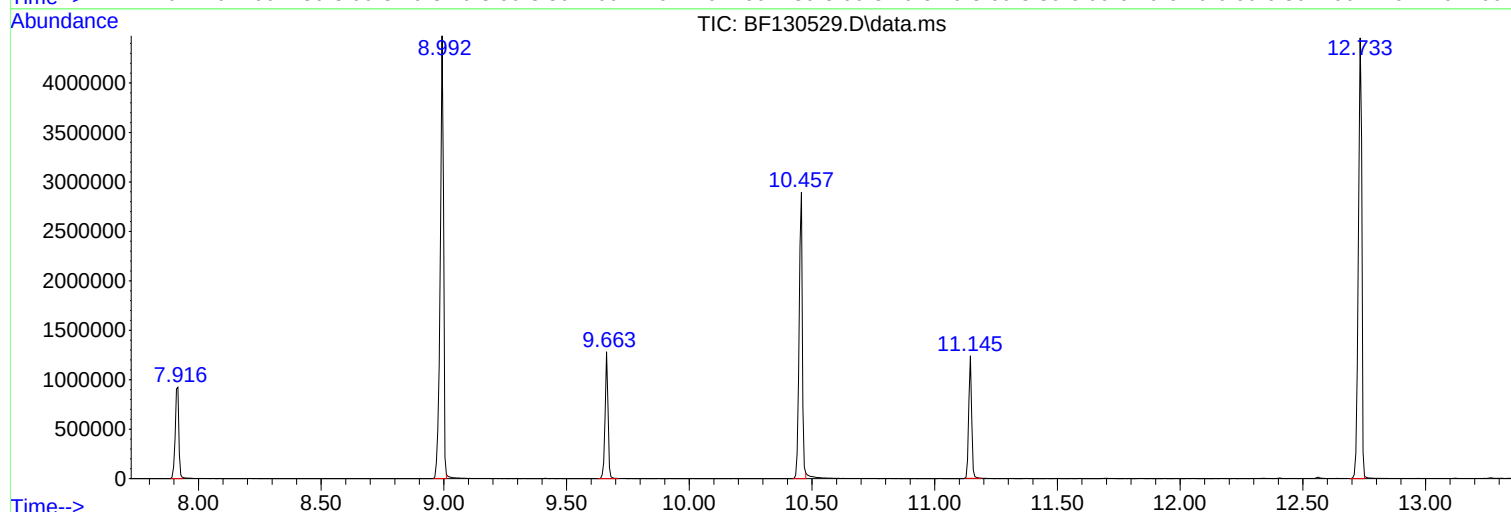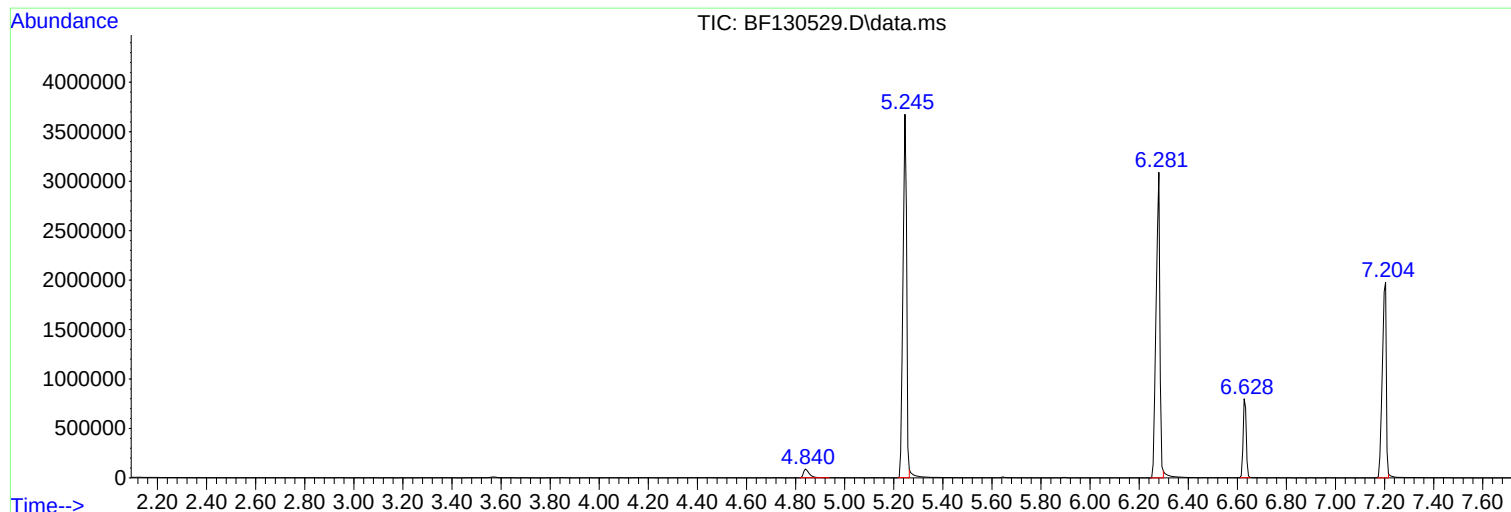

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100522\
Data File : BF130529.D
Acq On : 05 Oct 2022 13:21
Operator : CG\JU
Sample : PB148087BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB148087BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
4.840	4.16 ng	146190	1,4-Dichlorobenzene-d4	6.628

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	64		
2	Acetic acid, cyano-, 1,1-dimethy...	141	C7H11NO2	001116-98-9	23		
3	1-Propen-2-ol, acetate	100	C5H8O2	000108-22-5	10		
4	2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	9		
5	5-Hexen-2-one	98	C6H10O	000109-49-9	9		

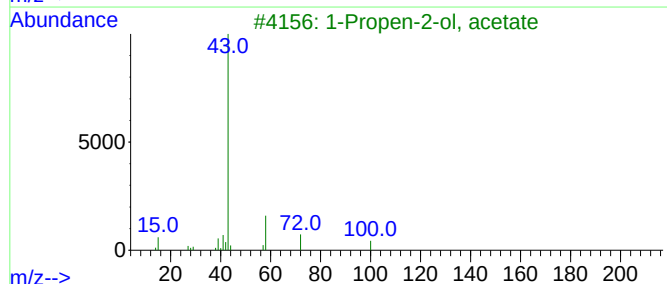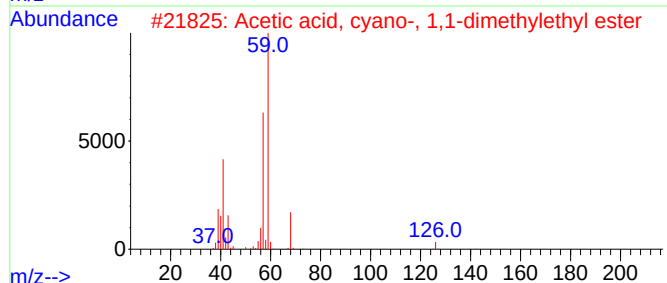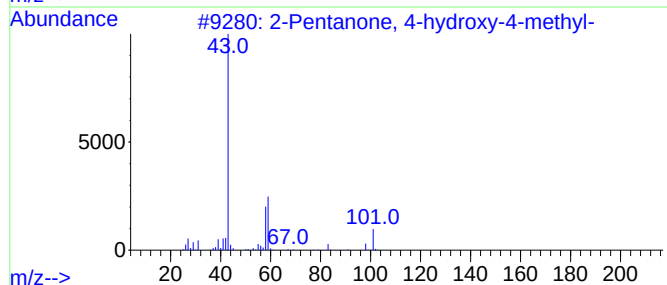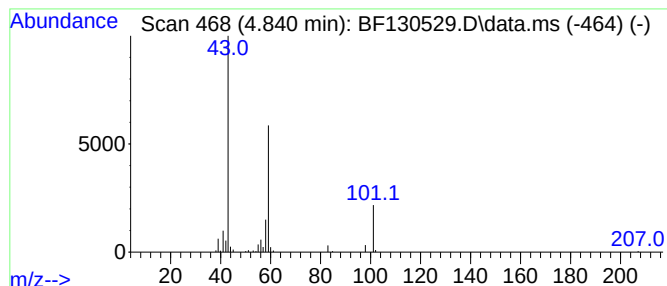

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100522\
Data File : BF130529.D
Acq On : 05 Oct 2022 13:21
Operator : CG\JU
Sample : PB148087BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB148087BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	4.840	4.2	ng	146190	1	6.628	703034	20.0