


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100522\
 Data File : BF130527.D
 Acq On : 05 Oct 2022 11:56
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Oct 07 02:06:46 2022

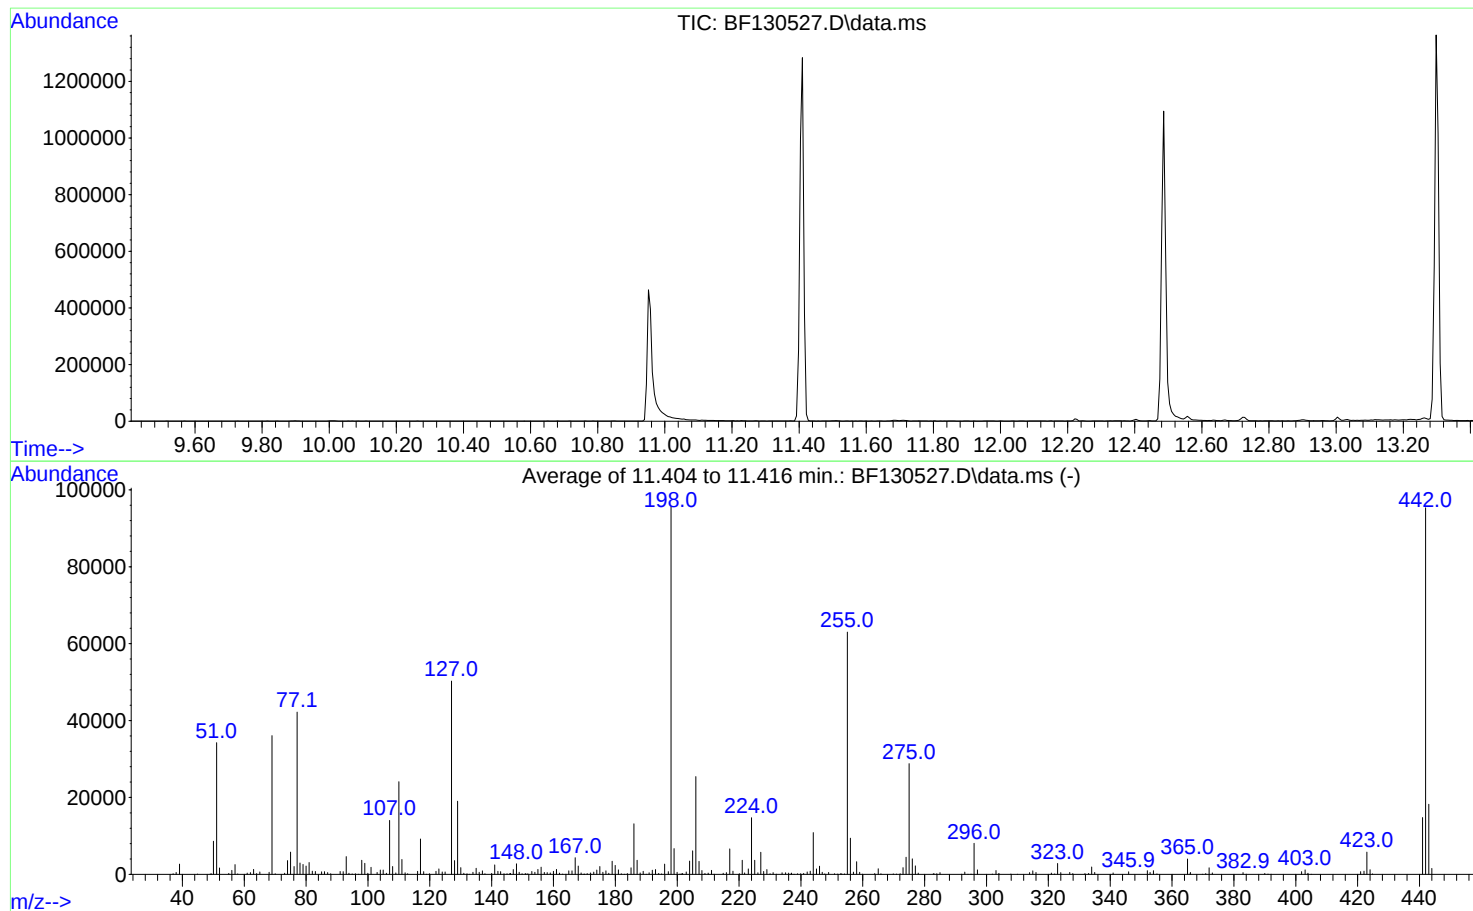




AutoFind: Scans 1584, 1585, 1586; Background Corrected with Scan 1579

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.8	34266	PASS
68	69	0.00	2	1.5	546	PASS
69	198	0.00	100	37.7	36102	PASS
70	69	0.00	2	0.4	159	PASS
127	198	10	80	52.6	50279	PASS
197	198	0.00	2	0.7	690	PASS
198	198	100	100	100.0	95672	PASS
199	198	5	9	7.0	6685	PASS
275	198	10	60	30.1	28806	PASS
365	198	1	100	4.2	3994	PASS
441	198	0.01	100	15.4	14769	PASS
442	442	50	100	100.0	95352	PASS
443	442	15	24	19.1	18248	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100522\
Data File : BF130527.D
Acq On : 05 Oct 2022 11:56
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 06 04:25:59 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 06 01:07:05 2022
Response via : Initial Calibration

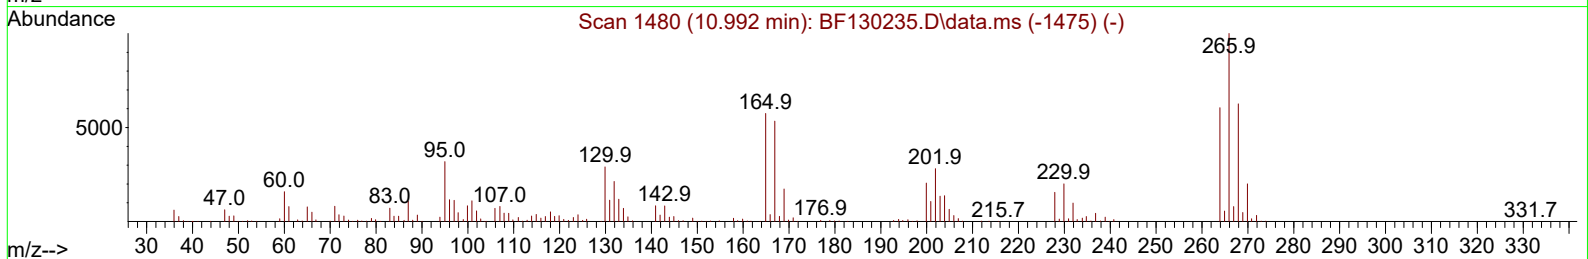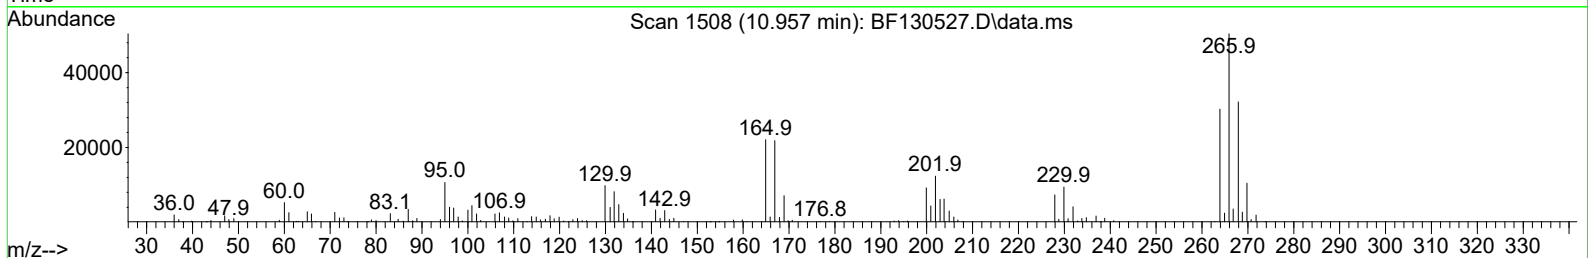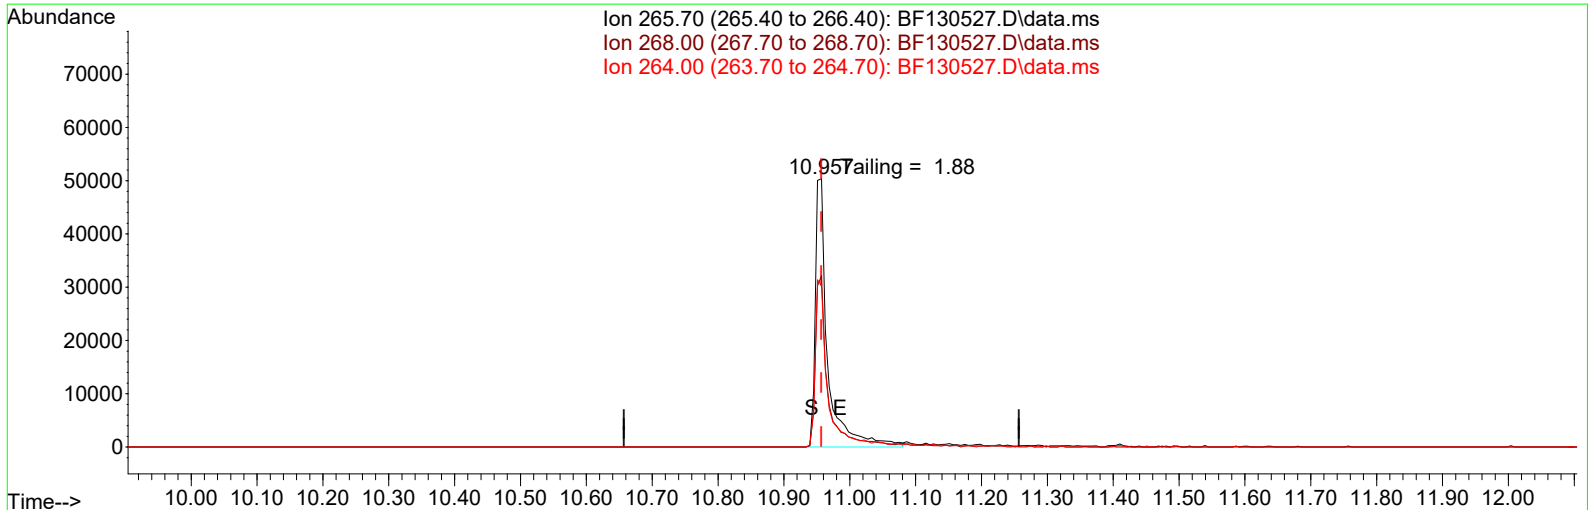

TIC: BF130527.D\data.ms

(70) Pentachlorophenol (C)

10.957min (+ 0.000) 24718.90 ng




response 67520

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.10	63.85
264.00	63.10	60.02
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100522\
Data File : BF130527.D
Acq On : 05 Oct 2022 11:56
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Oct 06 04:25:59 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091422.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Oct 06 01:07:05 2022
Response via : Initial Calibration

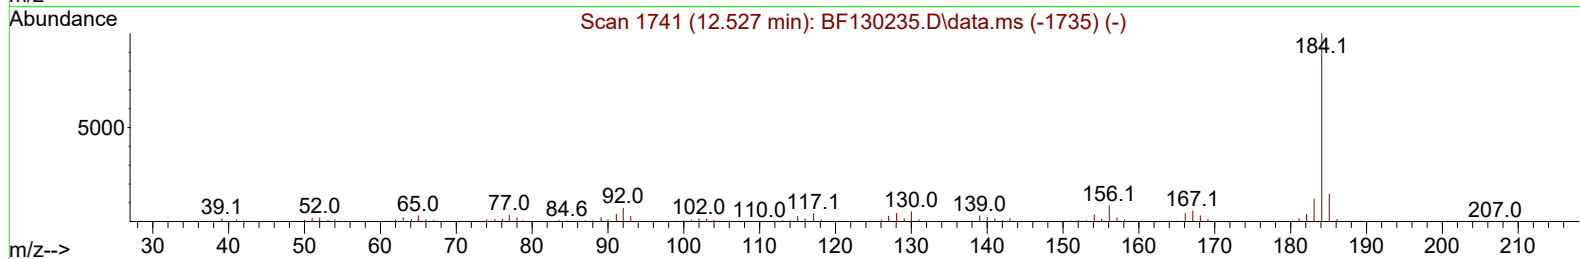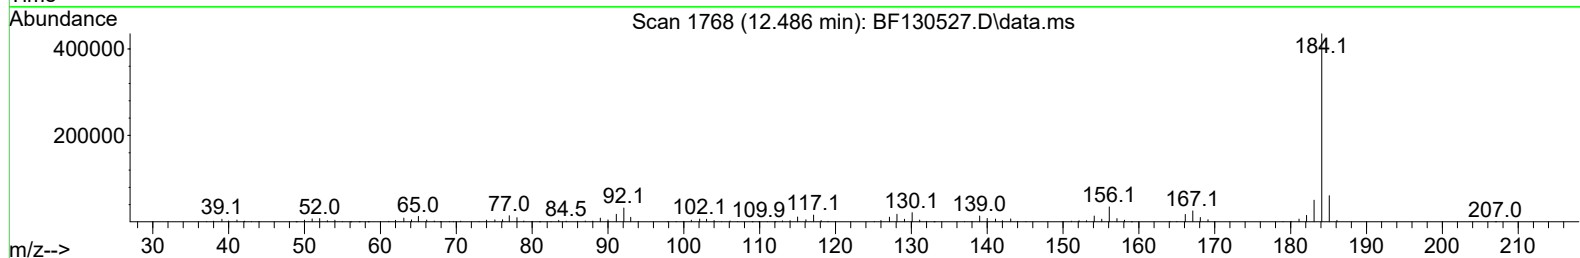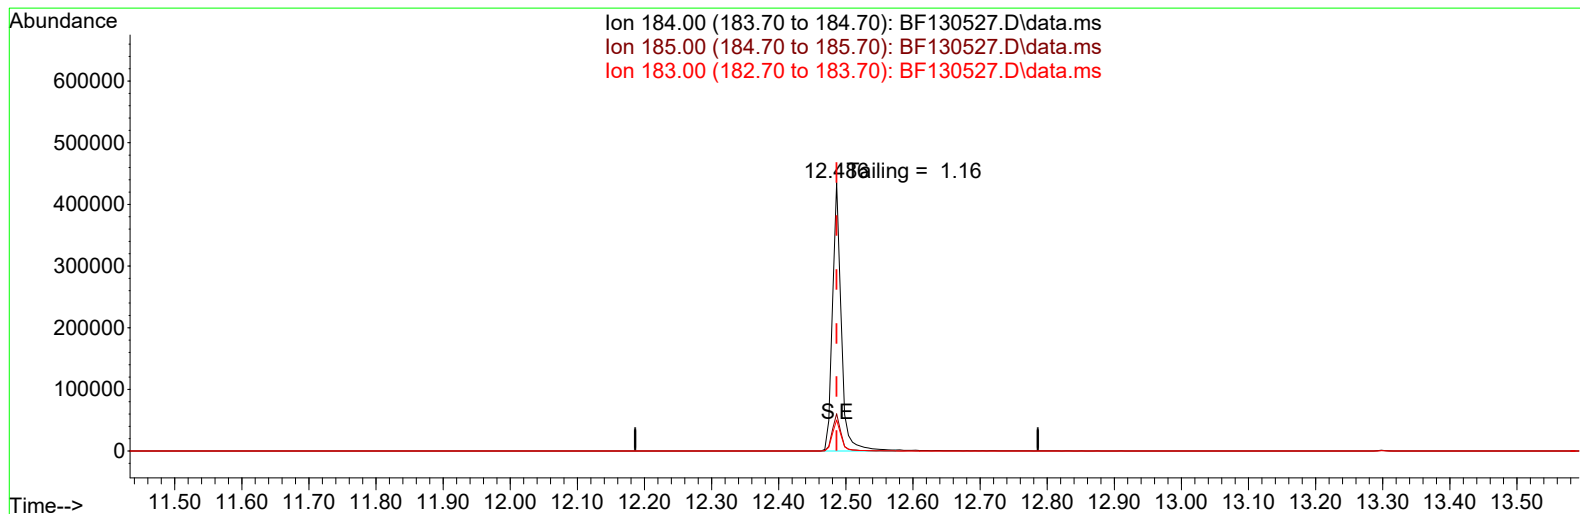

TIC: BF130527.D\data.ms

(77) Benzidine

12.486min (+ 0.000) 0.00 ng

response 398021

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	13.91
183.00	11.40	11.56
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
10/5/2022	BNA_F	<u>BF130527.D</u>
Compound Name	Response	Retention Time
DDT	214424	13.298
DDD	4038	13.004
DDE	738	12.669
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4776	219200	2.18

Instrument :
BNA_F
ClientSampleId :
DFTPP