
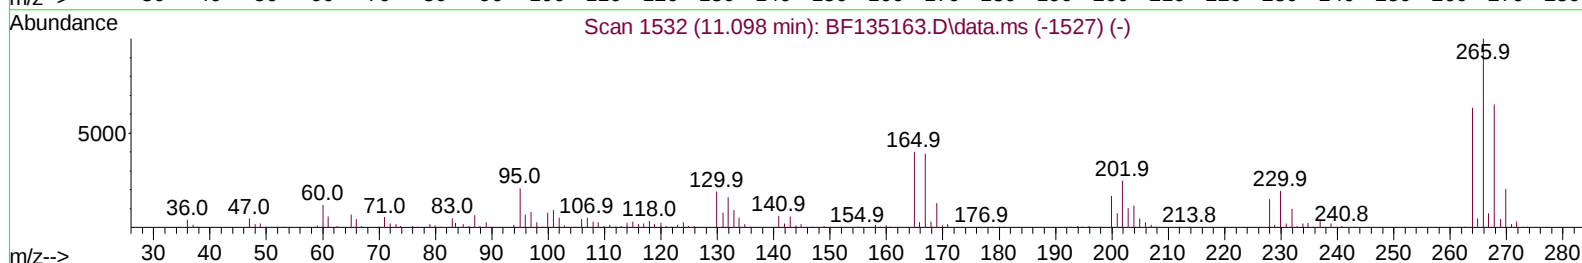
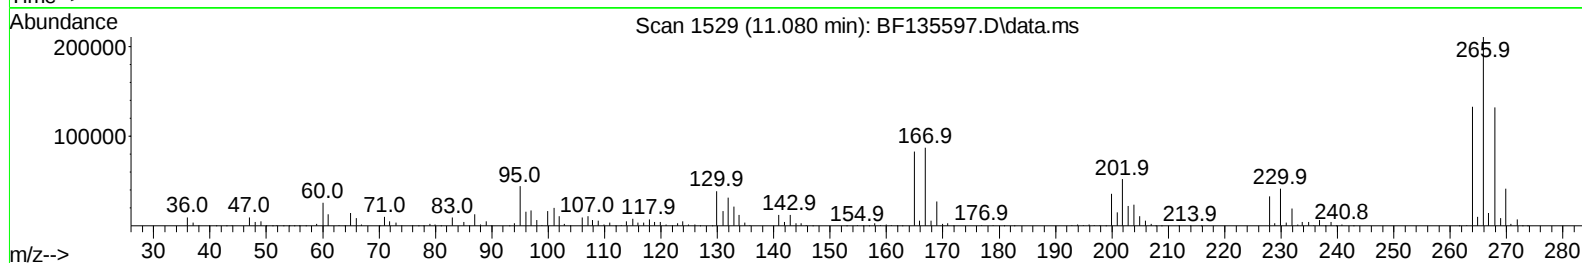


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100523\
Data File : BF135597.D
Acq On : 05 Oct 2023 13:49
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 06 08:22:17 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 04 17:06:20 2023
Response via : Initial Calibration

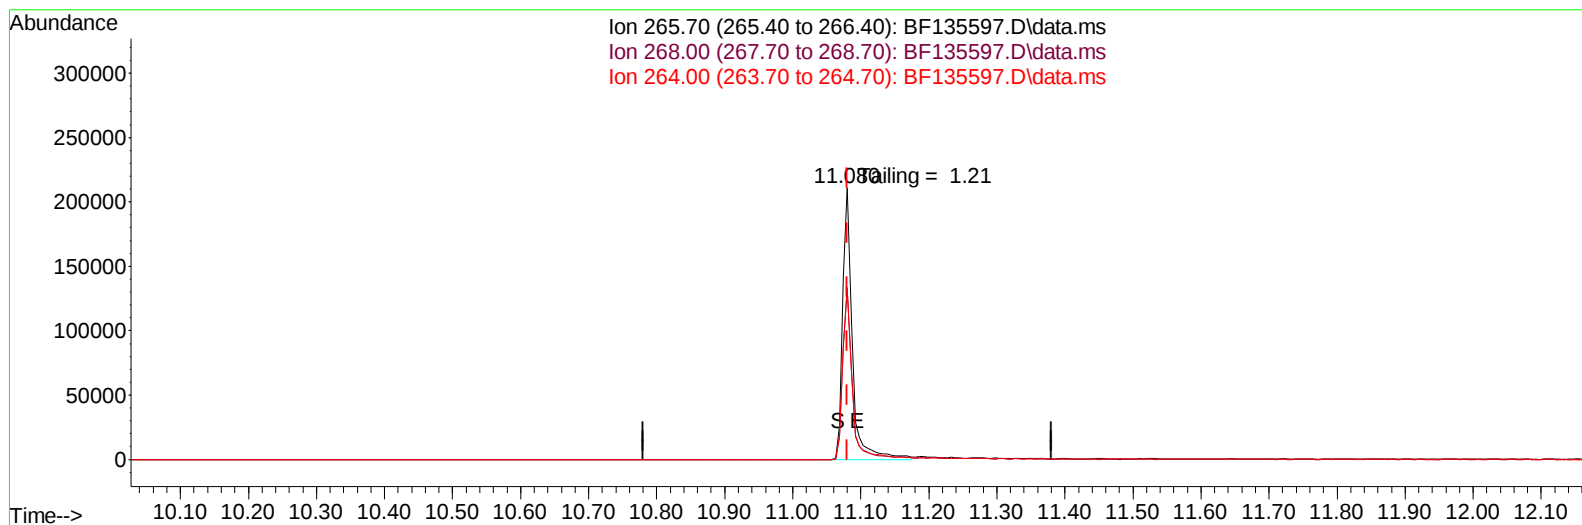

TIC: BF135597.D\data.ms

(70) Pentachlorophenol (C)




11.080min (-0.000) 525857.35 ng

response 207211

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.10	62.70
264.00	63.50	63.25
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100523\
Data File : BF135597.D
Acq On : 05 Oct 2023 13:49
Operator : CG\JU
Sample : DFTTP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Oct 06 08:22:17 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Oct 04 17:06:20 2023
Response via : Initial Calibration

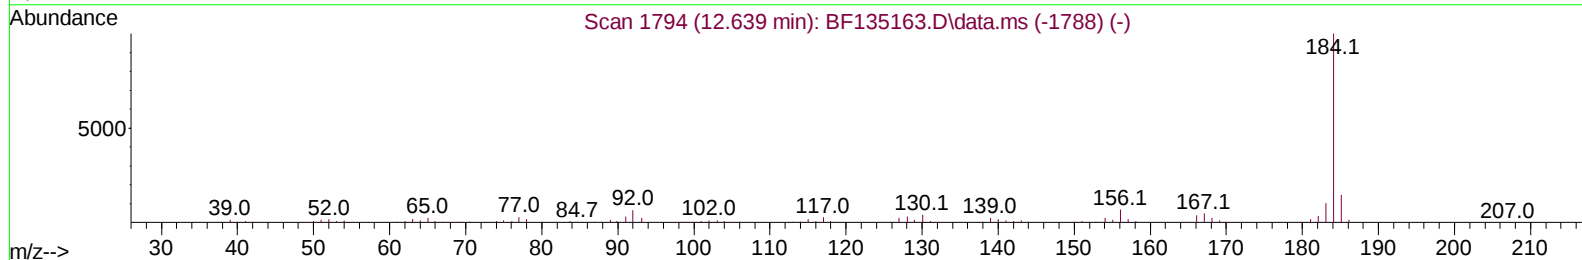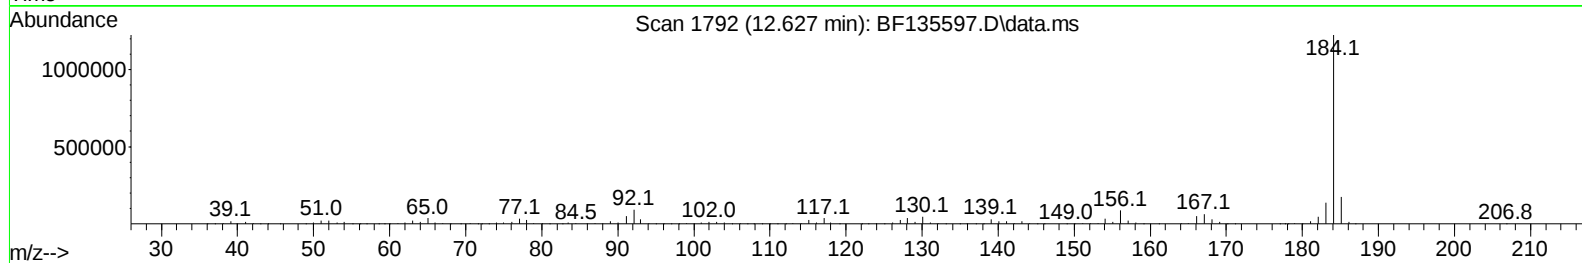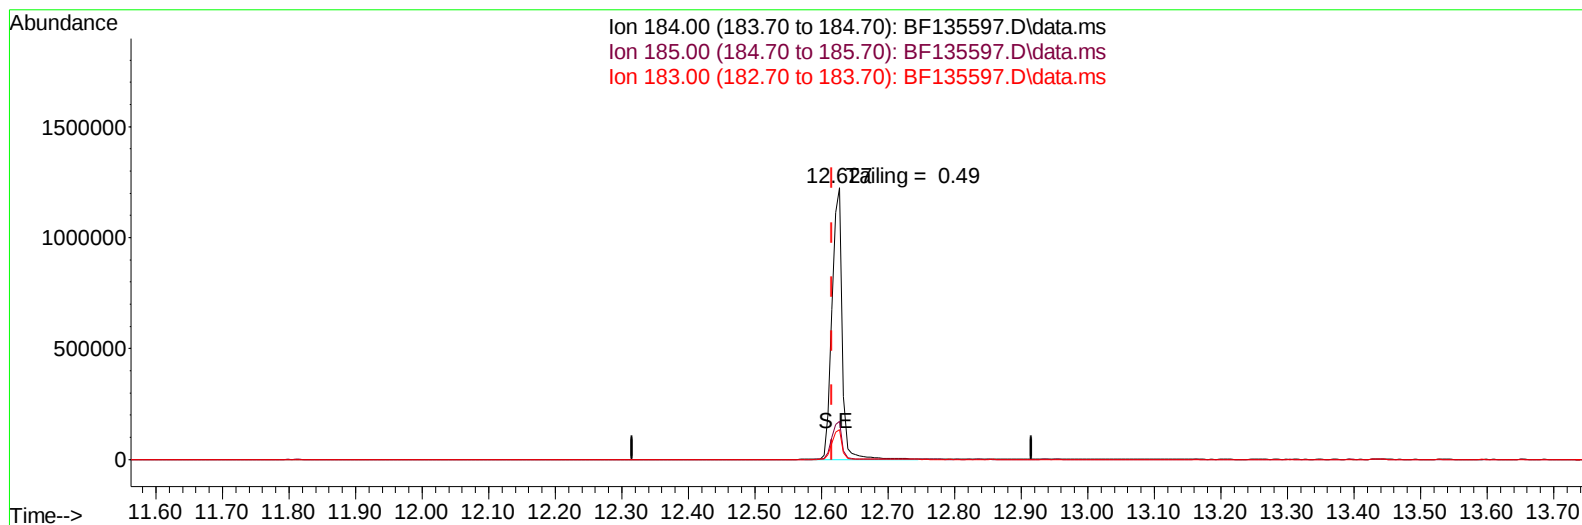

TIC: BF135597.D\data.ms

(77) Benzidine

12.627min (+ 0.012) 7798.62 ng m

response 1316177

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.10
183.00	10.30	11.05
0.00	0.00	0.00