

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100523\
Data File : BF135599.D
Acq On : 05 Oct 2023 14:53
Operator : CG\JU
Sample : PB156098BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB156098BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF135599.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.381	556	560	585	rBV	3776110	4265677	93.13%	14.044%
2	6.393	727	732	760	rBV	3792375	4324146	94.41%	14.236%
3	6.734	787	790	800	rBV	956925	935651	20.43%	3.080%
4	7.304	882	887	890	rBV	2708199	2836555	61.93%	9.339%
5	8.016	1003	1008	1020	rBV	1345967	1271050	27.75%	4.185%
6	9.098	1185	1192	1195	rBV	4078836	4580160	100.00%	15.079%
7	9.775	1301	1307	1310	rBV	1487859	1364033	29.78%	4.491%
8	10.569	1438	1442	1446	rBV	2576687	2804733	61.24%	9.234%
9	11.269	1557	1561	1569	rBV	1636760	1461189	31.90%	4.811%
10	12.869	1828	1833	1836	rBV	4364306	4566599	99.70%	15.034%
11	13.927	2009	2013	2023	rBV	1291510	1187302	25.92%	3.909%
12	15.392	2257	2262	2271	rBV	573463	777321	16.97%	2.559%




Sum of corrected areas: 30374416

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100523\
Data File : BF135599.D
Acq On : 05 Oct 2023 14:53
Operator : CG\JU
Sample : PB156098BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB156098BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

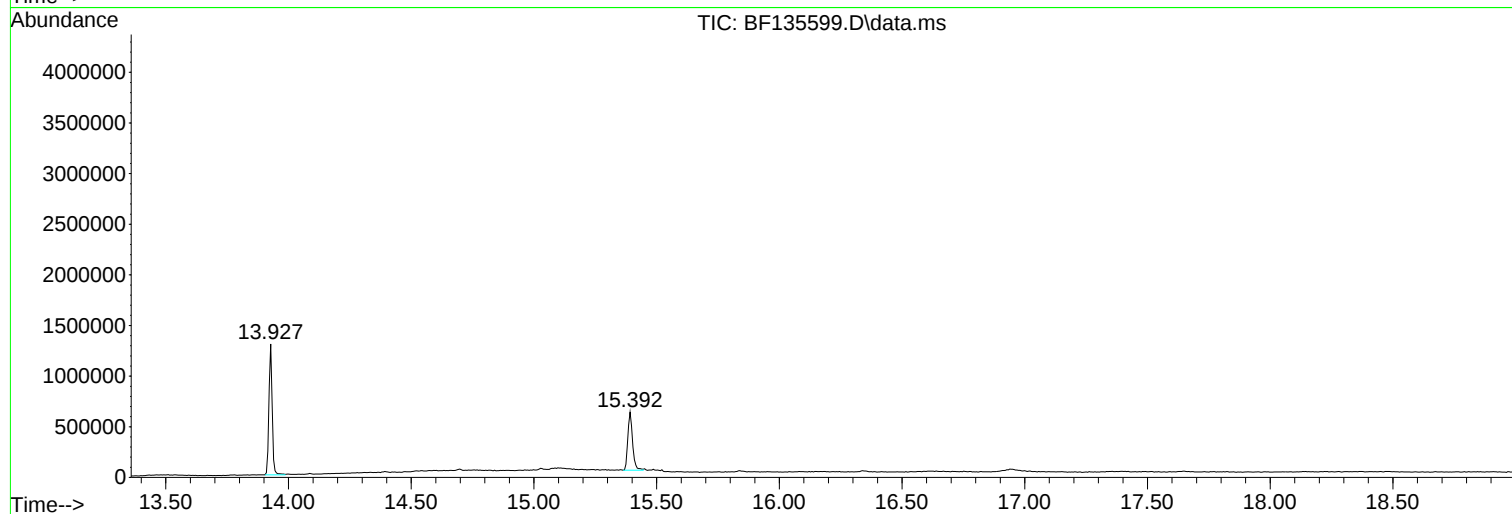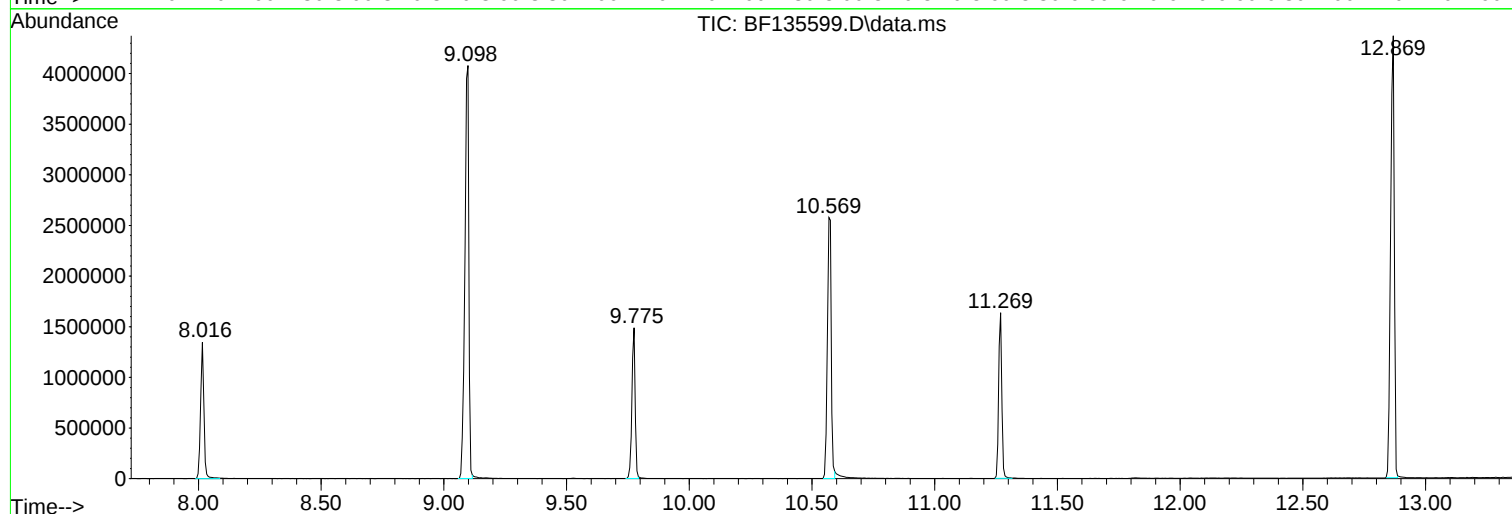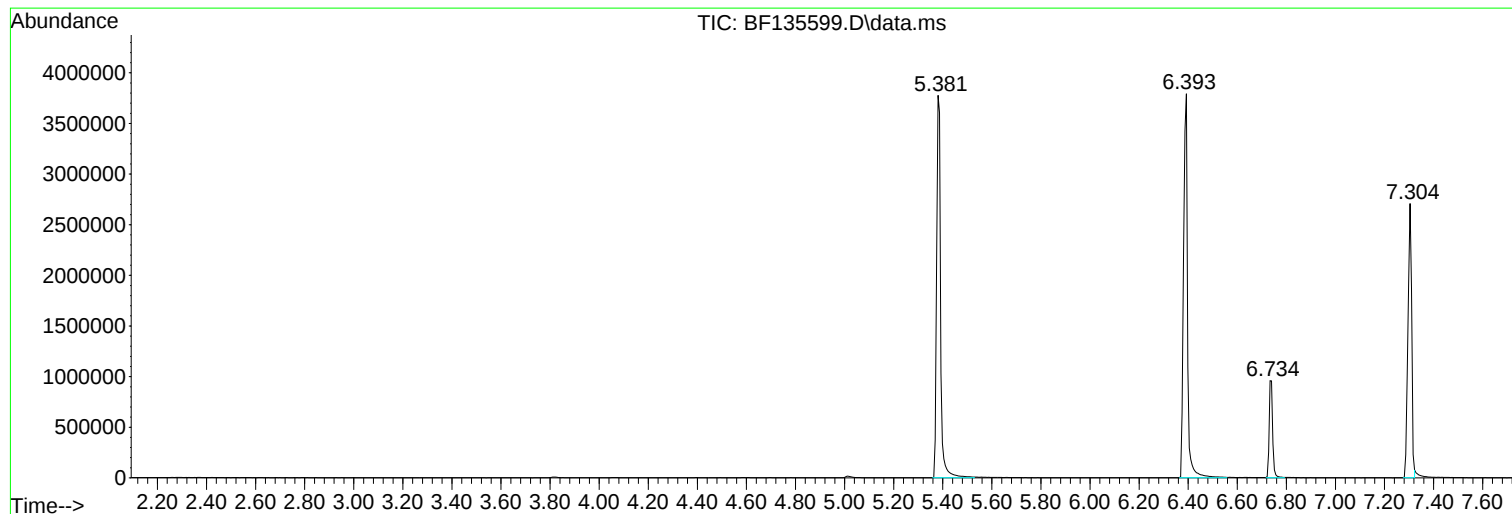

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100523\
Data File : BF135599.D
Acq On : 05 Oct 2023 14:53
Operator : CG\JU
Sample : PB156098BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB156098BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100523\
Data File : BF135599.D
Acq On : 05 Oct 2023 14:53
Operator : CG\JU
Sample : PB156098BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB156098BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------