

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100523\
 Data File : BF135617.D
 Acq On : 06 Oct 2023 00:28
 Operator : CG\JU
 Sample : 04702-01 10X
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 OK-02-100223

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF135617.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.381	557	560	573	rBV	109733	165761	23.89%	2.562%
2	5.981	659	662	667	rVB3	7601	8508	1.23%	0.131%
3	6.398	730	733	742	rBV	101272	145286	20.94%	2.245%
4	6.569	758	762	768	rVB2	23495	24240	3.49%	0.375%
5	6.739	787	791	798	rBV	634649	560282	80.75%	8.658%
6	6.875	811	814	818	rVB2	8982	9437	1.36%	0.146%
7	7.010	830	837	840	rVB7	11145	11544	1.66%	0.178%
8	7.122	853	856	860	rVB2	15953	16052	2.31%	0.248%
9	7.269	875	881	884	rBV4	13997	14964	2.16%	0.231%
10	7.304	884	887	890	rVV	90743	96041	13.84%	1.484%
11	7.328	890	891	895	rVV	49286	37978	5.47%	0.587%
12	7.381	895	900	903	rVB6	10845	18074	2.60%	0.279%
13	7.533	924	926	929	rVB2	20525	16435	2.37%	0.254%
14	7.651	936	946	948	rBV7	11280	28411	4.09%	0.439%
15	7.698	951	954	956	rVB3	10029	11735	1.69%	0.181%
16	7.733	956	960	961	rBV3	10760	10133	1.46%	0.157%
17	7.757	961	964	968	rVV5	9872	12339	1.78%	0.191%
18	7.969	995	1000	1002	rBV6	9586	17505	2.52%	0.271%
19	8.016	1005	1008	1011	rVV	843400	693875	100.00%	10.723%
20	8.039	1011	1012	1014	rVV	56033	35116	5.06%	0.543%
21	8.075	1017	1018	1021	rVB	22603	13015	1.88%	0.201%
22	8.210	1039	1041	1044	rVB3	15468	13565	1.95%	0.210%
23	8.304	1052	1057	1064	rBV5	16101	32947	4.75%	0.509%
24	8.357	1064	1066	1070	rBV3	9024	10818	1.56%	0.167%
25	8.398	1070	1073	1076	rVB3	14562	15119	2.18%	0.234%
26	8.433	1076	1079	1081	rBV2	26652	23177	3.34%	0.358%
27	8.522	1089	1094	1096	rBV2	21673	23107	3.33%	0.357%
28	8.604	1106	1108	1112	rBV	55714	51238	7.38%	0.792%
29	8.675	1117	1120	1122	rVV4	15016	17248	2.49%	0.267%
30	8.704	1123	1125	1128	rVB4	10873	9358	1.35%	0.145%
31	8.733	1128	1130	1134	rBV2	14394	11783	1.70%	0.182%
32	8.839	1144	1148	1150	rVB3	20656	21287	3.07%	0.329%
33	8.975	1166	1171	1174	rBV5	10065	15621	2.25%	0.241%
34	9.033	1179	1181	1184	rBV	21312	17676	2.55%	0.273%
35	9.092	1188	1191	1195	rBV	231336	172801	24.90%	2.670%
36	9.175	1200	1205	1208	rBV	60448	58222	8.39%	0.900%

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100523\
 Data File : BF135617.D
 Acq On : 06 Oct 2023 00:28
 Operator : CG\JU
 Sample : 04702-01 10X
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 OK-02-100223

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	9.239	1214	1216	1219	rVB3	12309	12354	1.78%	0.191%
38	9.363	1234	1237	1240	rVB3	11600	11044	1.59%	0.171%
39	9.433	1245	1249	1250	rBV2	18456	16419	2.37%	0.254%
40	9.492	1255	1259	1261	rVV	29839	32420	4.67%	0.501%
41	9.516	1261	1263	1266	rVV2	16157	14585	2.10%	0.225%
42	9.551	1266	1269	1272	rVB4	18094	15358	2.21%	0.237%
43	9.633	1280	1283	1287	rVB	21747	21538	3.10%	0.333%
44	9.674	1287	1290	1292	rBV3	8074	8365	1.21%	0.129%
45	9.704	1292	1295	1299	rVB	63616	46611	6.72%	0.720%
46	9.774	1303	1307	1310	rVV	669437	612740	88.31%	9.469%
47	9.804	1310	1312	1315	rVB	20501	16446	2.37%	0.254%
48	9.874	1322	1324	1329	rVB6	8464	11157	1.61%	0.172%
49	9.933	1329	1334	1337	rBV5	7772	15940	2.30%	0.246%
50	9.980	1340	1342	1346	rVB3	14848	18536	2.67%	0.286%
51	10.027	1346	1350	1353	rBV3	17330	23055	3.32%	0.356%
52	10.092	1358	1361	1363	rBV3	9066	9075	1.31%	0.140%
53	10.174	1373	1375	1377	rBV3	8409	8512	1.23%	0.132%
54	10.204	1377	1380	1383	rVB	59850	46415	6.69%	0.717%
55	10.321	1397	1400	1409	rVB2	18523	26575	3.83%	0.411%
56	10.427	1414	1418	1423	rVV	25495	35873	5.17%	0.554%
57	10.480	1424	1427	1429	rVB4	8293	8440	1.22%	0.130%
58	10.545	1435	1438	1440	rBV3	9467	10973	1.58%	0.170%
59	10.569	1440	1442	1448	rVB	74261	70977	10.23%	1.097%
60	10.680	1458	1461	1470	rVB	64510	77323	11.14%	1.195%
61	10.869	1491	1493	1497	rBV4	9525	14604	2.10%	0.226%
62	10.904	1497	1499	1502	rVB3	12582	10302	1.48%	0.159%
63	11.127	1534	1537	1540	rBV	43204	39094	5.63%	0.604%
64	11.163	1540	1543	1547	rVB2	28526	31581	4.55%	0.488%
65	11.263	1557	1560	1563	rBV	582609	545369	78.60%	8.428%
66	11.292	1563	1565	1570	rVV	69238	66285	9.55%	1.024%
67	11.345	1572	1574	1578	rVB	18809	18425	2.66%	0.285%
68	11.510	1599	1602	1606	rVB6	13413	15576	2.24%	0.241%
69	11.557	1607	1610	1613	rVB	45378	39528	5.70%	0.611%
70	11.604	1616	1618	1621	rVV4	7574	9181	1.32%	0.142%
71	11.663	1625	1628	1630	rBV4	11373	8960	1.29%	0.138%
72	11.774	1644	1647	1649	rBV2	11204	10830	1.56%	0.167%
73	11.804	1649	1652	1657	rVV3	21740	28270	4.07%	0.437%
74	11.880	1662	1665	1668	rBV	27733	26281	3.79%	0.406%
75	11.968	1677	1680	1682	rBV	48139	35325	5.09%	0.546%
76	12.068	1695	1697	1701	rBV4	8408	10356	1.49%	0.160%

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100523\
 Data File : BF135617.D
 Acq On : 06 Oct 2023 00:28
 Operator : CG\JU
 Sample : 04702-01 10X
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 OK-02-100223

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

77	12.245	1725	1727	1730	rBV4	15253	17169	2.47%	0.265%
78	12.321	1738	1740	1743	rBV2	22520	22455	3.24%	0.347%
79	12.357	1743	1746	1752	rVV3	62021	88986	12.82%	1.375%
80	12.486	1765	1768	1773	rBV	105730	90003	12.97%	1.391%
81	12.639	1792	1794	1796	rBV3	17374	17350	2.50%	0.268%
82	12.715	1804	1807	1813	rVB2	97741	135151	19.48%	2.089%
83	12.857	1828	1831	1834	rBV	166455	143047	20.62%	2.211%
84	13.092	1868	1871	1873	rBV	67036	55813	8.04%	0.863%
85	13.115	1873	1875	1877	rVB	24221	16592	2.39%	0.256%
86	13.439	1927	1930	1933	rVB	73380	73227	10.55%	1.132%
87	13.768	1984	1986	1991	rBV2	67608	74831	10.78%	1.156%
88	13.927	2009	2013	2016	rBV	556728	531784	76.64%	8.218%
89	14.086	2038	2040	2045	rVB	81861	77817	11.21%	1.203%
90	14.392	2090	2092	2097	rBV	79270	75777	10.92%	1.171%
91	14.698	2142	2144	2148	rVB	73661	63442	9.14%	0.980%
92	15.392	2259	2262	2274	rVB2	301082	466182	67.19%	7.204%




Sum of corrected areas: 6471022

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100523\
Data File : BF135617.D
Acq On : 06 Oct 2023 00:28
Operator : CG\JU
Sample : 04702-01 10X
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OK-02-100223

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

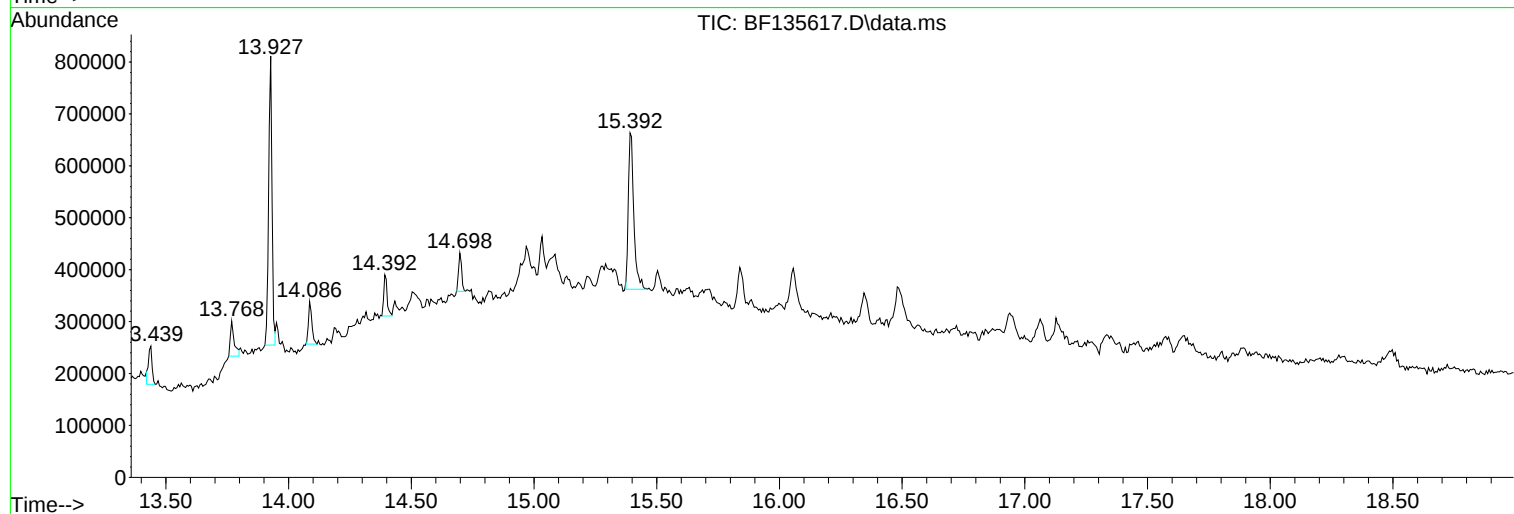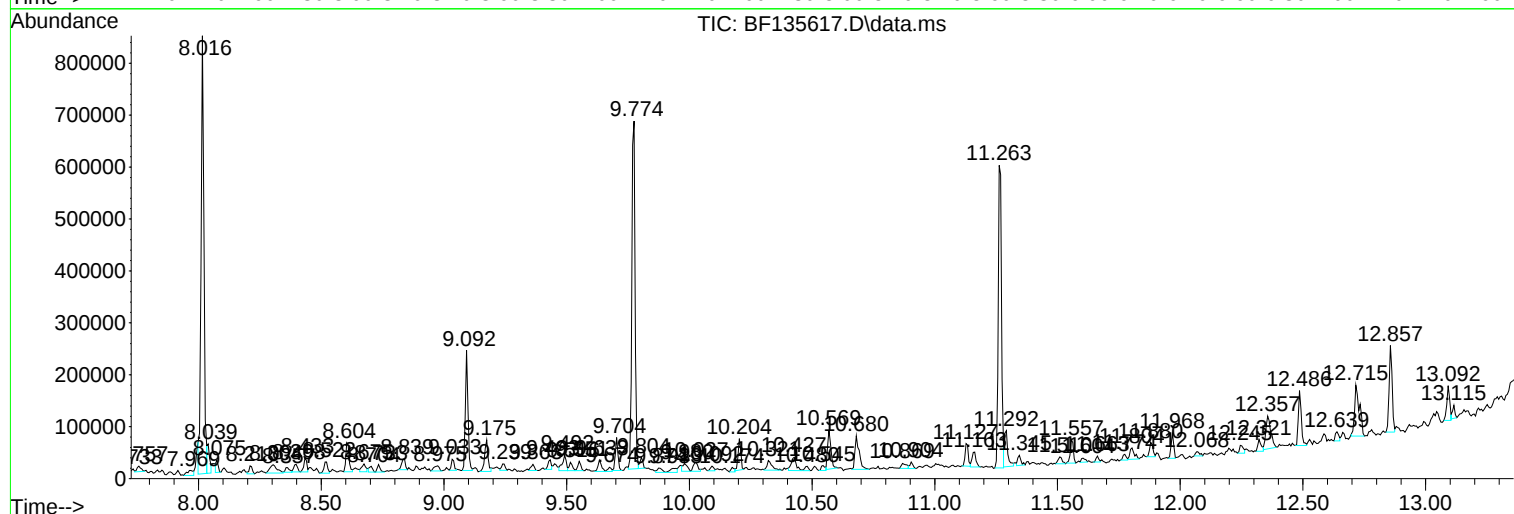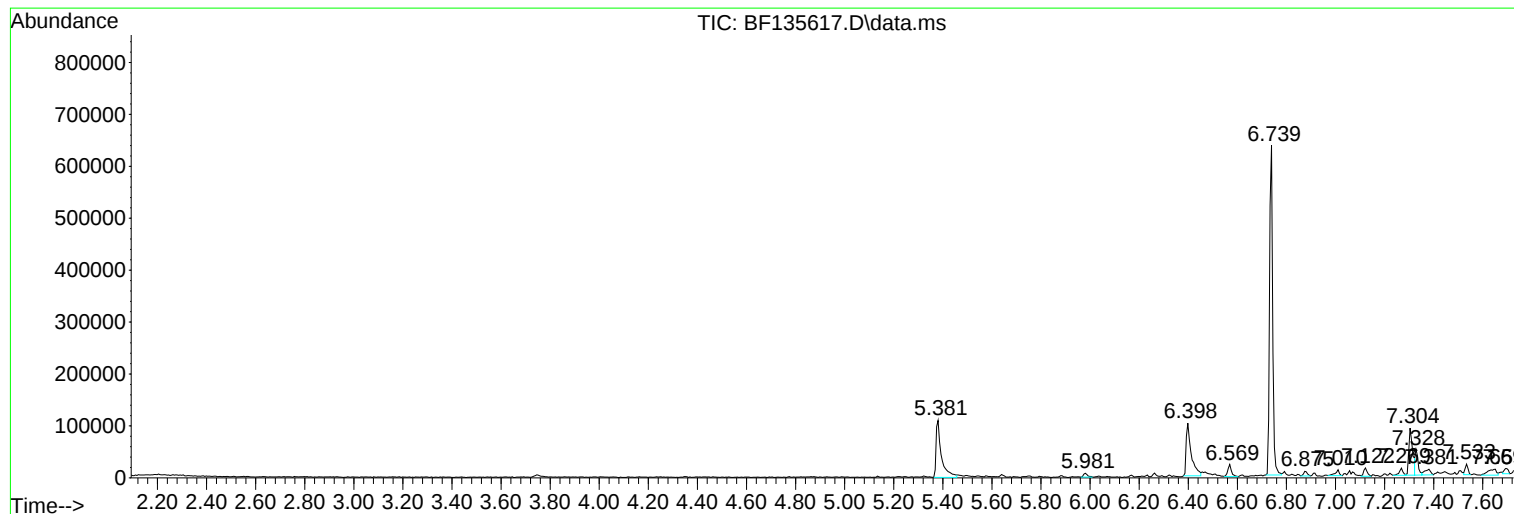

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100523\
Data File : BF135617.D
Acq On : 06 Oct 2023 00:28
Operator : CG\JU
Sample : 04702-01 10X
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OK-02-100223










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 1-Iodo-2-methylundecane Concentration Rank 4

R.T.	EstConc	Area	Relative to ISTD	R.T.
10.680	2.84 ng	77323	Phenanthrene-d10	11.269

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			1-Iodo-2-methylundecane	296	C12H25I	073105-67-6	90
2			Heptadecane	240	C17H36	000629-78-7	86
3			Eicosane	282	C20H42	000112-95-8	86
4			Dodecane, 2-methyl-6-propyl-	226	C16H34	055045-08-4	86
5			Hexadecane	226	C16H34	000544-76-3	80

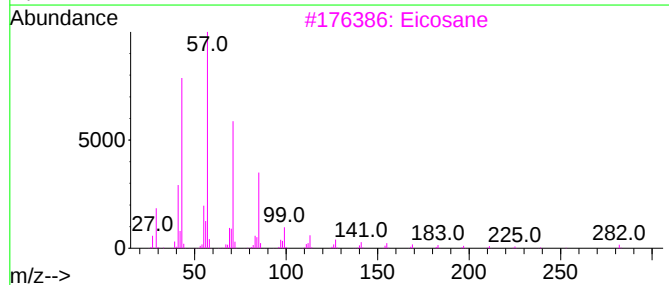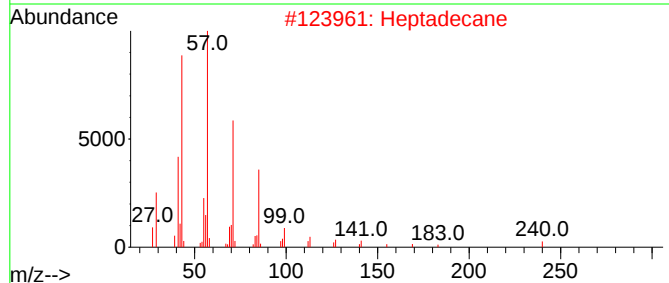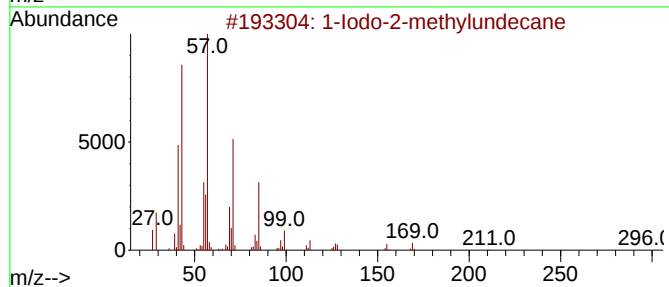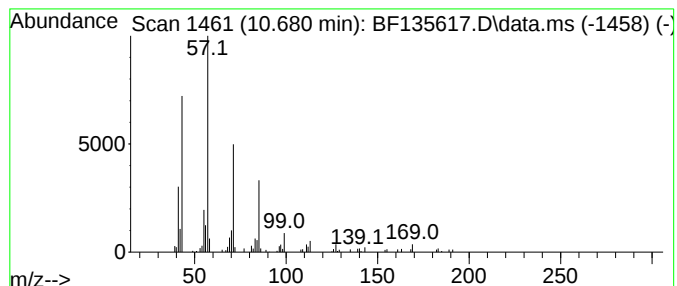

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100523\
Data File : BF135617.D
Acq On : 06 Oct 2023 00:28
Operator : CG\JU
Sample : 04702-01 10X
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OK-02-100223










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 2 Heptadecane Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
12.357	3.26 ng	88986	Phenanthrene-d10	11.269

Hit#	of 5	Tentative ID	MW	MolForm	CAS#	Qual
1		Heptadecane	240	C17H36	000629-78-7	74
2		Hexadecane	226	C16H34	000544-76-3	72
3		Tridecane, 1-iodo-	310	C13H27I	035599-77-0	72
4		2-Bromo dodecane	248	C12H25Br	013187-99-0	72
5		Hentriacontane	437	C31H64	000630-04-6	72

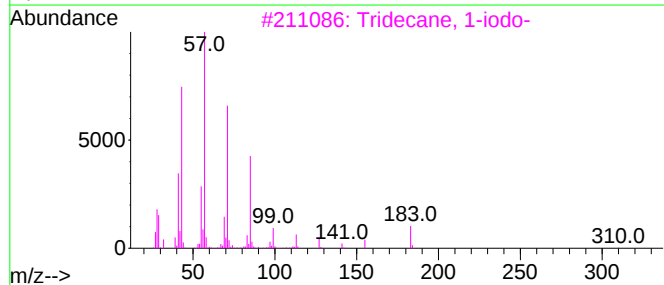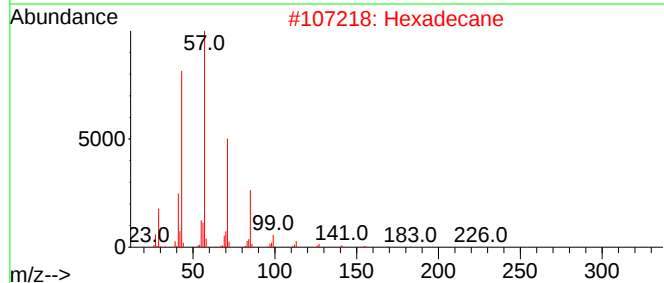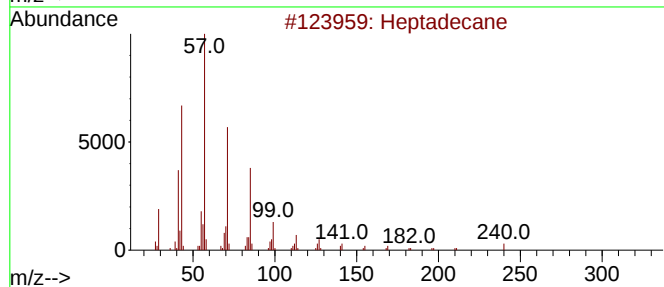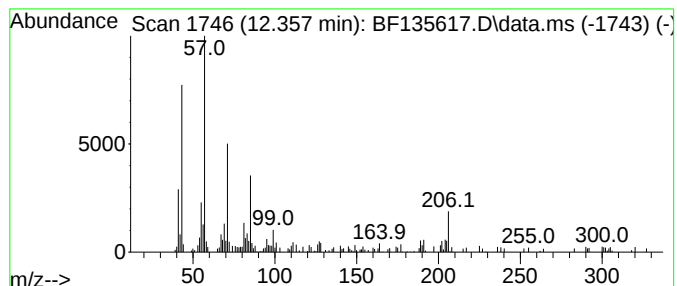

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100523\
Data File : BF135617.D
Acq On : 06 Oct 2023 00:28
Operator : CG\JU
Sample : 04702-01 10X
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OK-02-100223










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 3 Tricosane Concentration Rank 8

R.T.	EstConc	Area	Relative to ISTD	R.T.
13.092	2.10 ng	55813	Chrysene-d12	13.927

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Tricosane	324	C23H48	000638-67-5	87
2			Heneicosane	296	C21H44	000629-94-7	74
3			Decane, 3,8-dimethyl-	170	C12H26	017312-55-9	74
4			Eicosane	282	C20H42	000112-95-8	72
5			Nonadecane	268	C19H40	000629-92-5	72

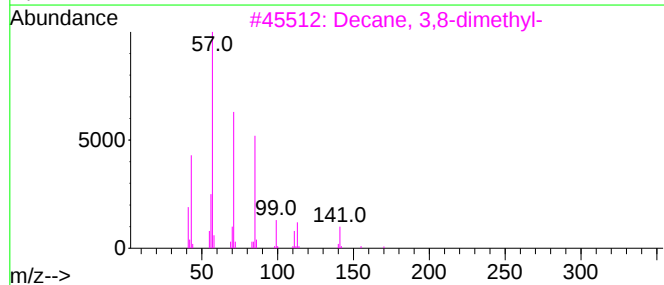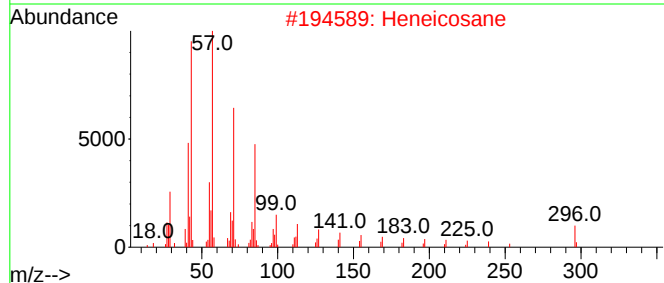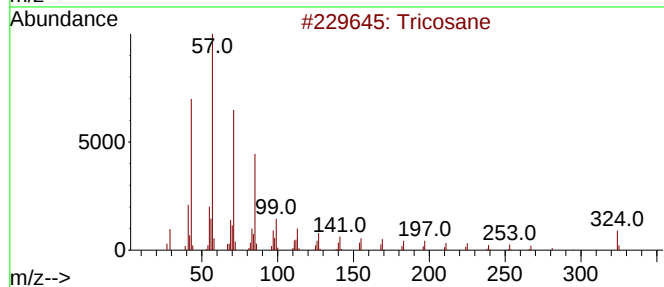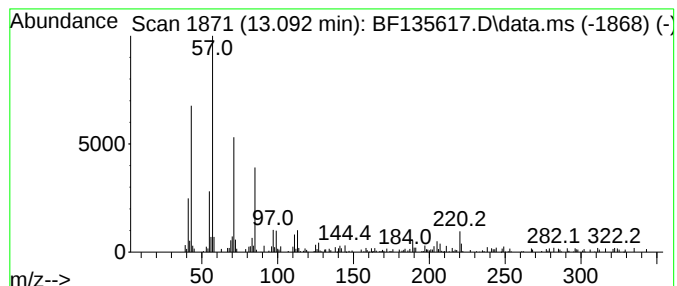

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100523\
Data File : BF135617.D
Acq On : 06 Oct 2023 00:28
Operator : CG\JU
Sample : 04702-01 10X
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OK-02-100223










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 4 Tetracosane Concentration Rank 6

R.T.	EstConc	Area	Relative to ISTD	R.T.
13.439	2.75 ng	73227	Chrysene-d12	13.927

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Tricosane	324	C23H48	000638-67-5	87
2			Tetracosane	338	C24H50	000646-31-1	83
3			Heneicosane	296	C21H44	000629-94-7	74
4			10-Methylnonadecane	282	C20H42	056862-62-5	74
5			Eicosane	282	C20H42	000112-95-8	72

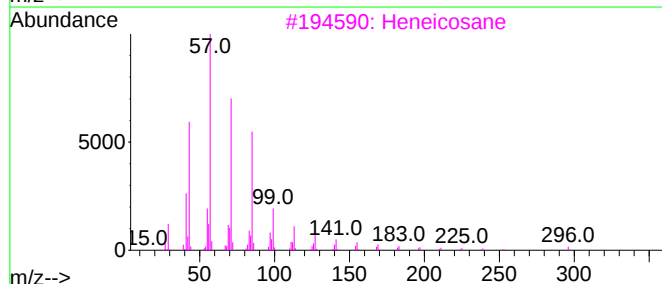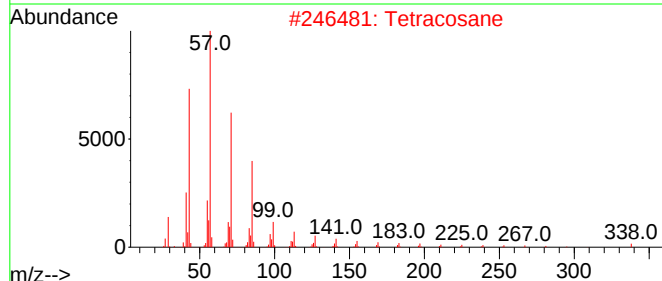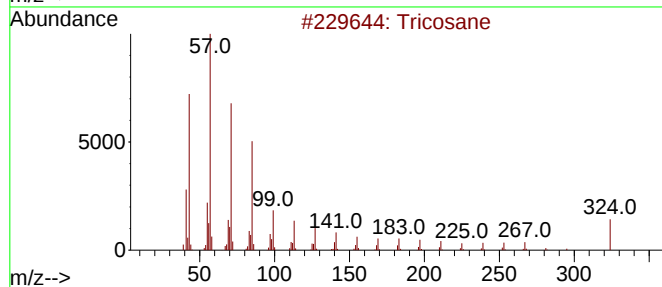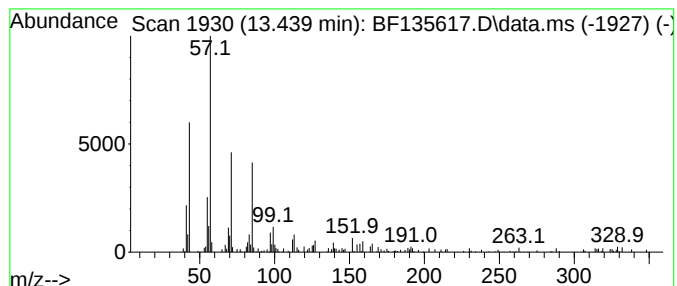

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100523\
Data File : BF135617.D
Acq On : 06 Oct 2023 00:28
Operator : CG\JU
Sample : 04702-01 10X
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OK-02-100223










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 5 Heneicosane Concentration Rank 5

R.T.	EstConc	Area	Relative to ISTD	R.T.
13.768	2.81 ng	74831	Chrysene-d12	13.927

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Heneicosane	296	C21H44	000629-94-7	89
2			Heptadecane, 2,6,10,15-tetramethyl-	296	C21H44	054833-48-6	70
3			Nonadecane	268	C19H40	000629-92-5	64
4			Heptadecane	240	C17H36	000629-78-7	62
5			10-Methylnonadecane	282	C20H42	056862-62-5	59

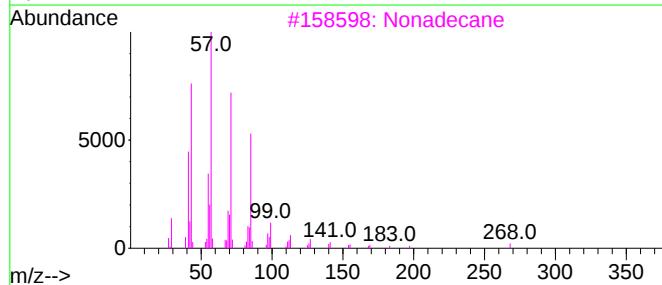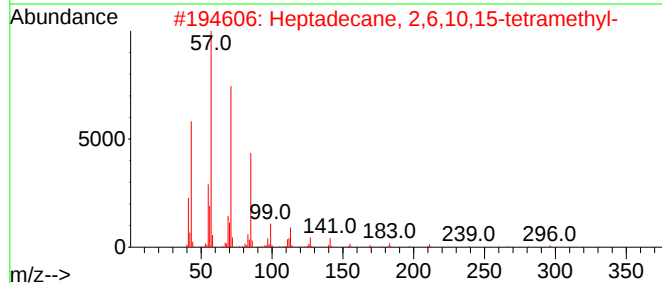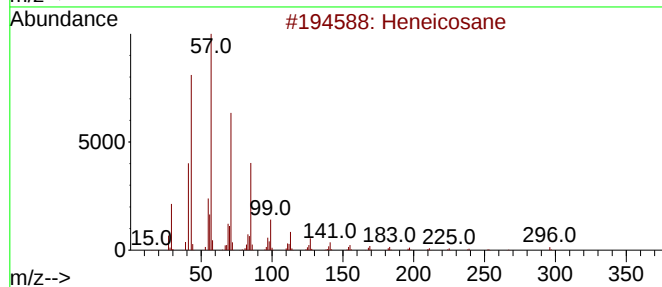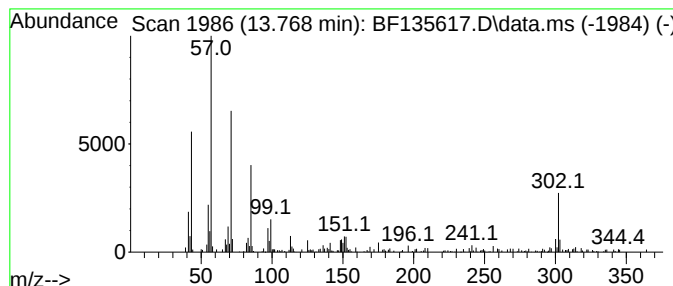

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100523\
Data File : BF135617.D
Acq On : 06 Oct 2023 00:28
Operator : CG\JU
Sample : 04702-01 10X
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OK-02-100223










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 6 Pentacosane Concentration Rank 2

R.T.	EstConc	Area	Relative to ISTD	R.T.
14.086	2.93 ng	77817	Chrysene-d12	13.927

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Pentacosane	352	C25H52	000629-99-2	86
2			Tetracosane	338	C24H50	000646-31-1	74
3			Heptacosane	380	C27H56	000593-49-7	72
4			Tricosane, 2-methyl-	338	C24H50	001928-30-9	72
5			Heneicosane	296	C21H44	000629-94-7	70

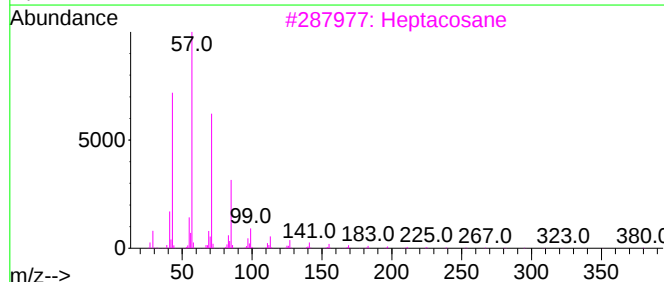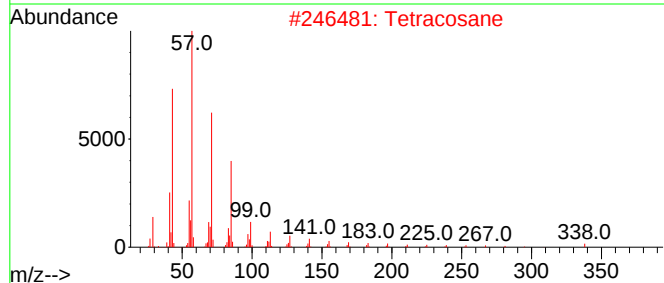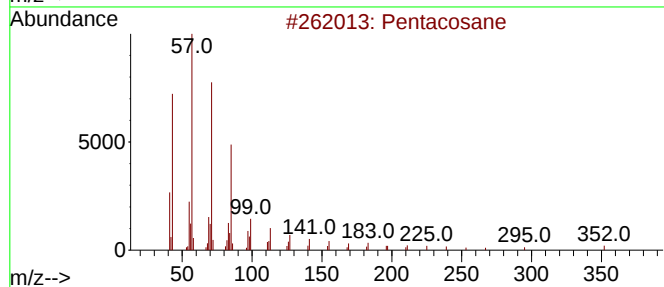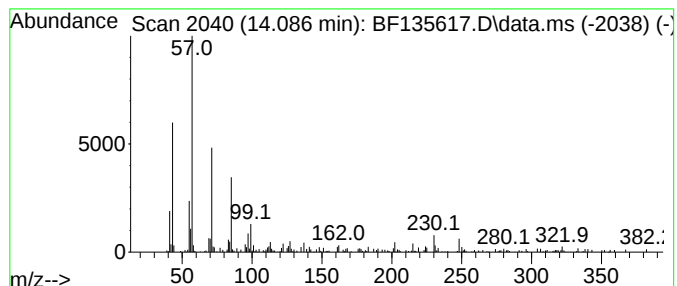

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100523\
Data File : BF135617.D
Acq On : 06 Oct 2023 00:28
Operator : CG\JU
Sample : 04702-01 10X
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OK-02-100223










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 7 Octadecane Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
14.392	2.85 ng	75777	Chrysene-d12	13.927

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Octadecane	254	C18H38	000593-45-3	93
2			Heptadecane, 2,6,10,15-tetramethyl-	296	C21H44	054833-48-6	89
3			Hexadecane	226	C16H34	000544-76-3	89
4			Heptadecane	240	C17H36	000629-78-7	87
5			10-Methylnonadecane	282	C20H42	056862-62-5	83

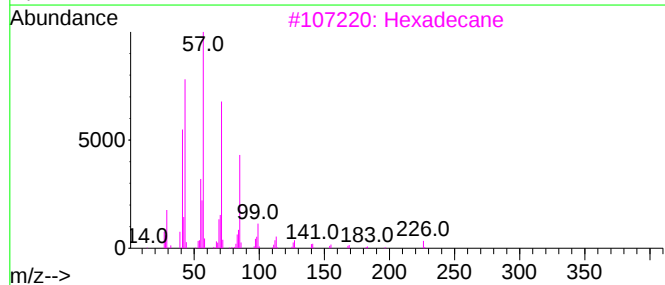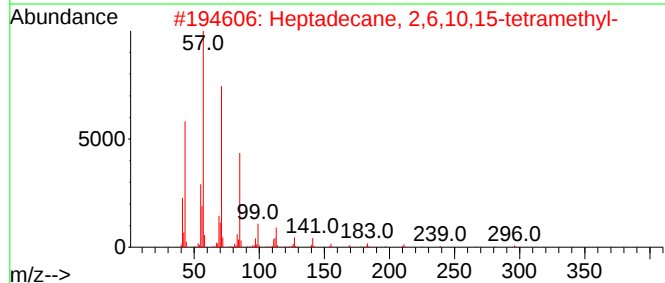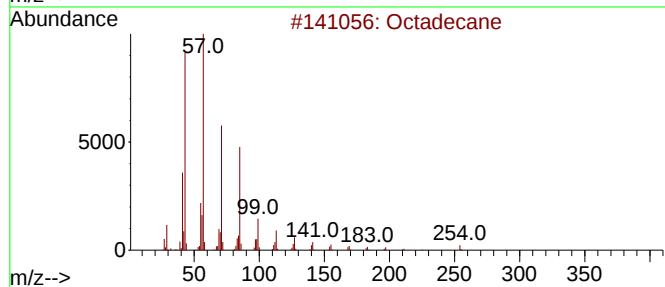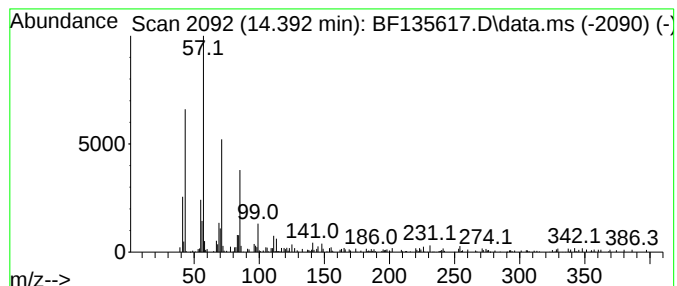

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100523\
Data File : BF135617.D
Acq On : 06 Oct 2023 00:28
Operator : CG\JU
Sample : 04702-01 10X
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OK-02-100223










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 8 Heptadecane, 8-methyl- Concentration Rank 7

R.T.	EstConc	Area	Relative to ISTD	R.T.
14.698	2.72 ng	63442	Perylene-d12	15.392

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Heptadecane, 8-methyl-	254	C18H38	013287-23-5	93
2			Octadecane	254	C18H38	000593-45-3	91
3			Docosane	310	C22H46	000629-97-0	91
4			Heptadecane, 2,6,10,15-tetramethyl-	296	C21H44	054833-48-6	91
5			Pentacosane	352	C25H52	000629-99-2	83

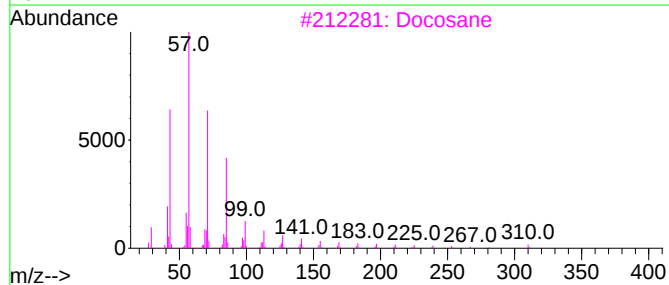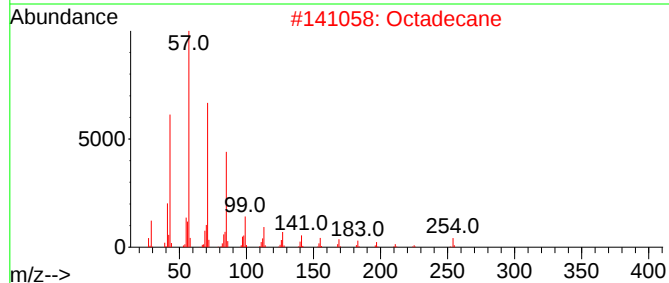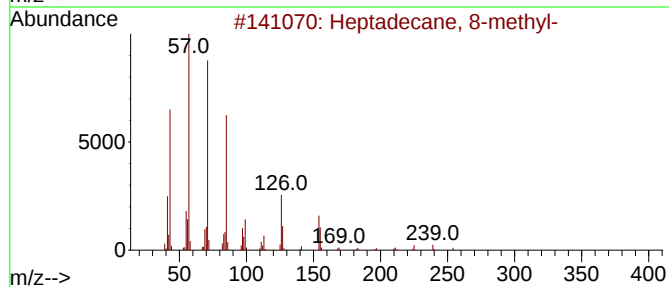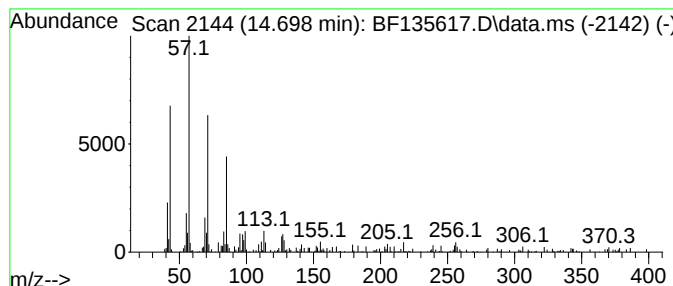

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF100523\
Data File : BF135617.D
Acq On : 06 Oct 2023 00:28
Operator : CG\JU
Sample : 04702-01 10X
Misc :
ALS Vial : 21 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
OK-02-100223

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF091123.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
1-Iodo-2-methyl...	10.680	2.8	ng	77323	4	11.269	545369	20.0
Heptadecane	12.357	3.3	ng	88986	4	11.269	545369	20.0
Tricosane	13.092	2.1	ng	55813	5	13.927	531784	20.0
Tetracosane	13.439	2.8	ng	73227	5	13.927	531784	20.0
Heneicosane	13.768	2.8	ng	74831	5	13.927	531784	20.0
Pentacosane	14.086	2.9	ng	77817	5	13.927	531784	20.0
Octadecane	14.392	2.9	ng	75777	5	13.927	531784	20.0
Heptadecane, 8-...	14.698	2.7	ng	63442	6	15.392	466182	20.0